
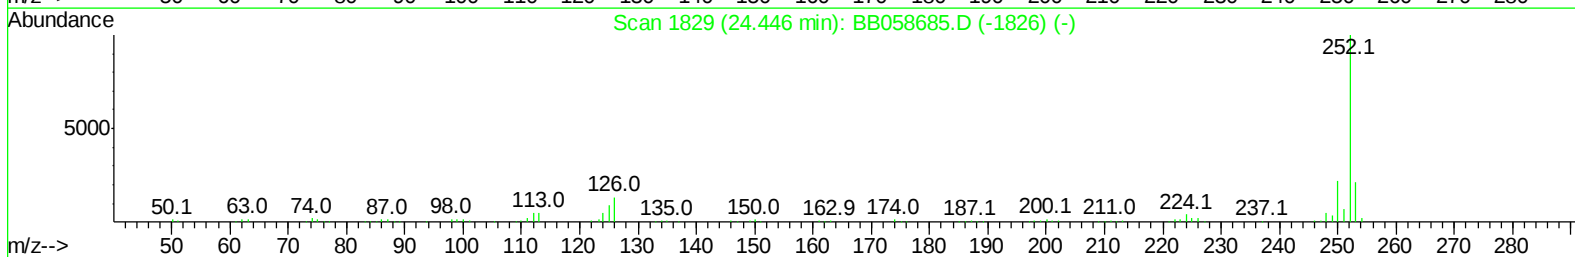
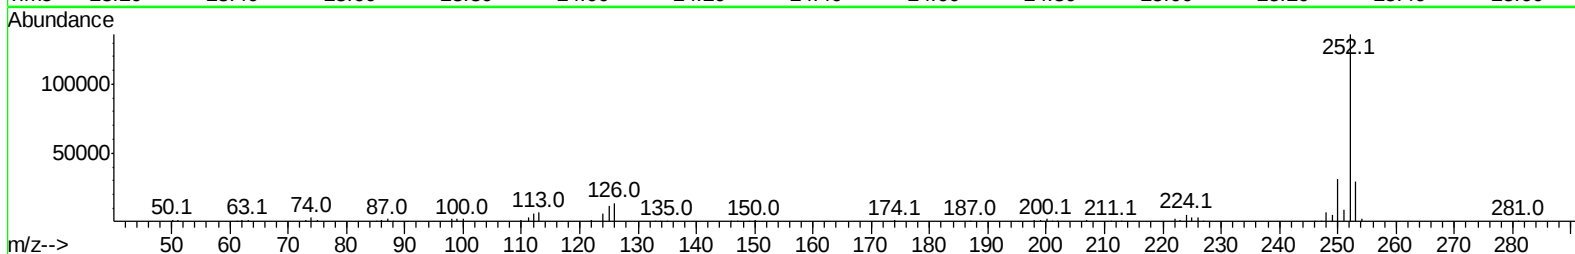


Data Path : Z:\HPCHEM1\BNA B\DATA\BB030317\
Data File : BB058684.D
Acq On : 3 Mar 2017 13:13
Operator : UM/SJ
Sample : SST01077
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Mar 03 15:23:52 2017
Quant Method : Z:\HPCHEM1\BNA B\METHOD\SOM-EPA-BB030317-PAH.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 03 14:56:52 2017
Response via : Initial Calibration

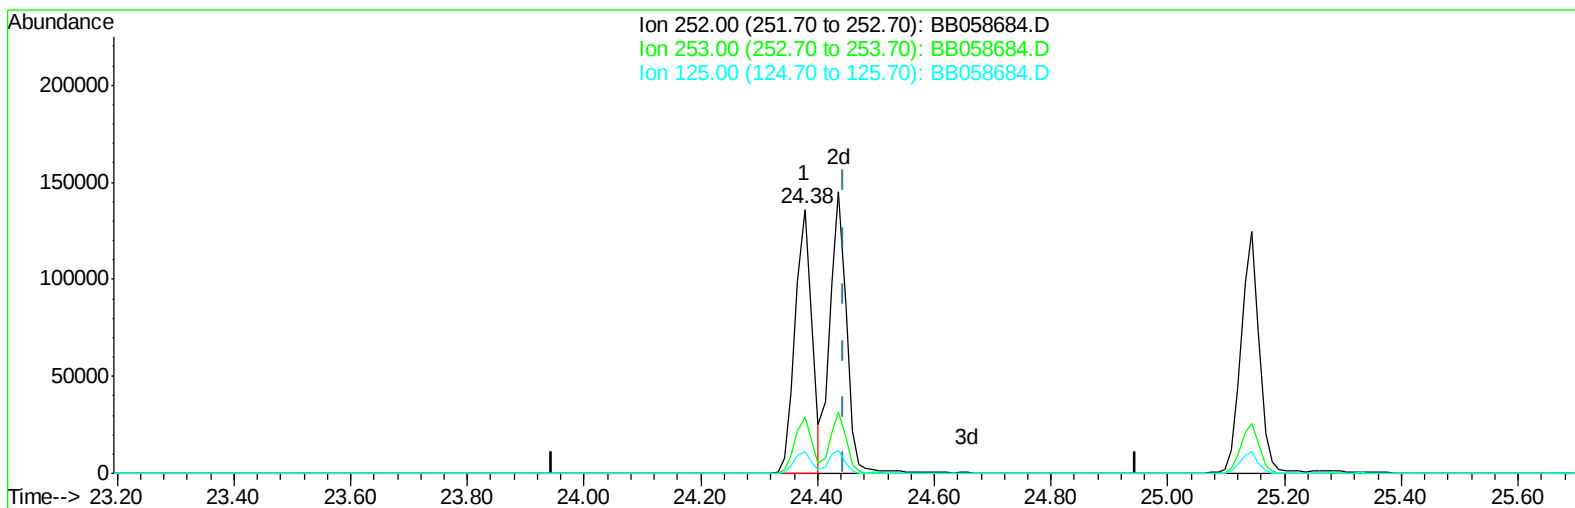

TIC: BB058684.D

(23) Benzo(k)fluoranthene




24.378min (-0.068) 9.83ng/ul

response 272018

Ion	Exp%	Act%
252.00	100	100
253.00	22.50	21.49
125.00	10.10	8.45
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA B\DATA\BB030317\
Data File : BB058684.D
Acq On : 3 Mar 2017 13:13
Operator : UM/SJ
Sample : SSTD01077
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Mar 03 15:23:52 2017
Quant Method : Z:\HPCHEM1\BNA B\METHOD\SOM-EPA-BB030317-PAH.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 03 14:56:52 2017
Response via : Initial Calibration

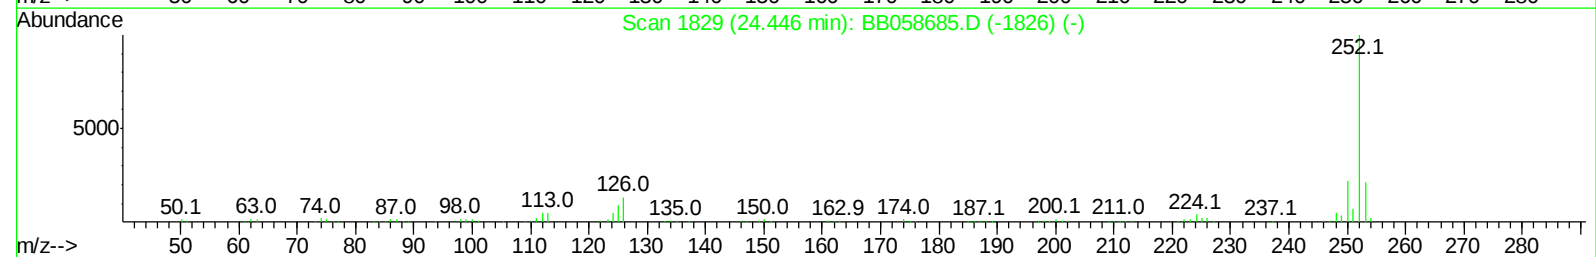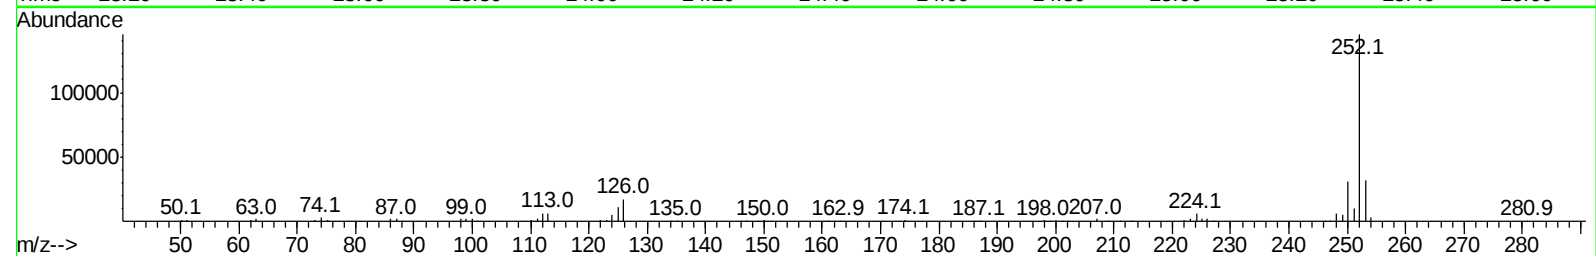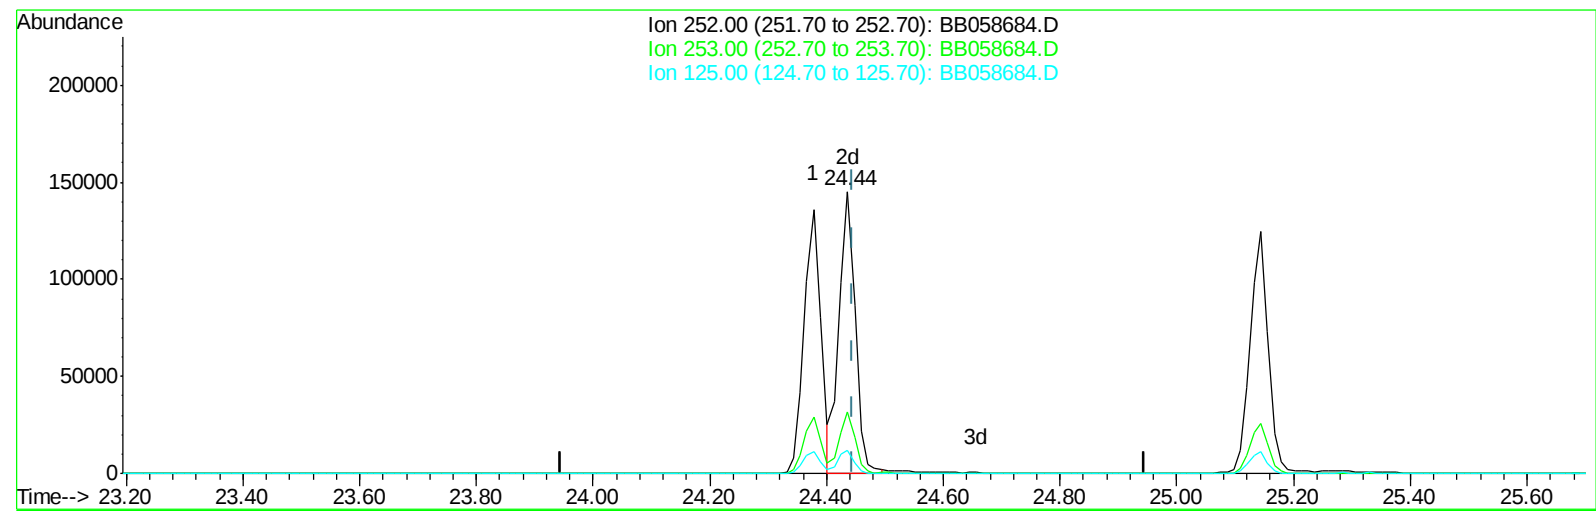

TIC: BB058684.D

(23) Benzo(k)fluoranthene

24.436min (-0.010) 10.01ng/ul m

response 276966

Ion	Exp%	Act%
252.00	100	100
253.00	22.50	22.02
125.00	10.10	7.98#
0.00	0.00	0.00