
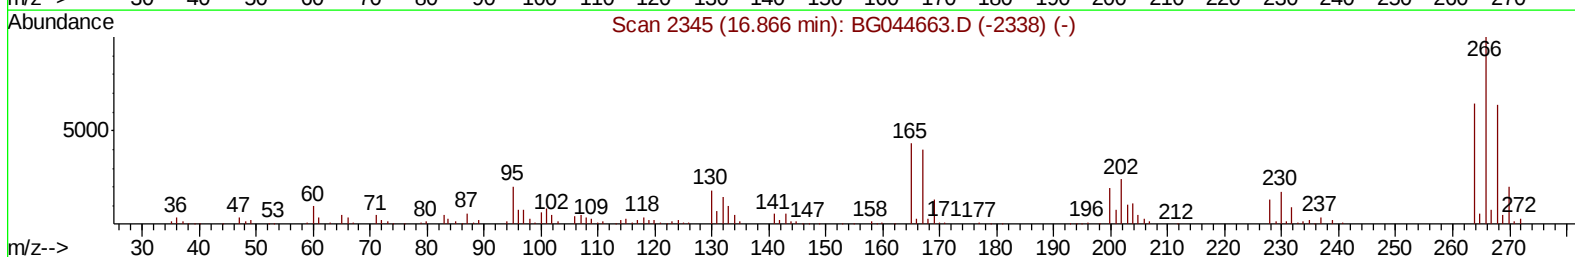
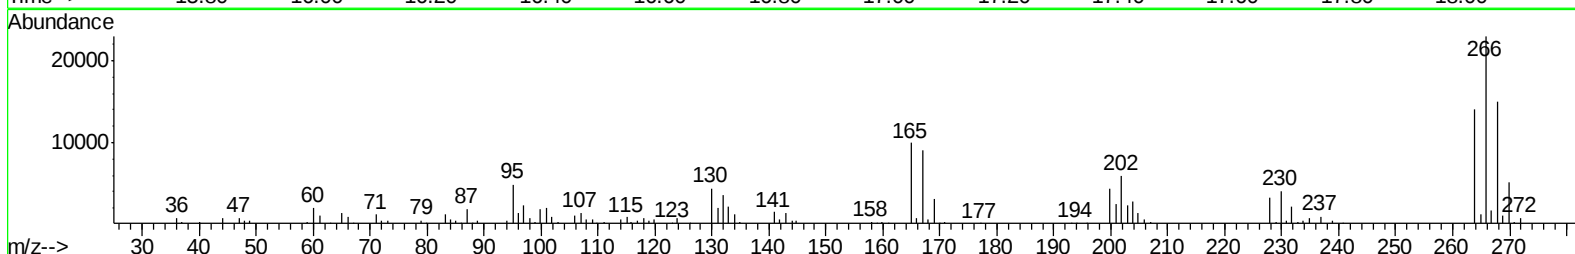


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG030320\
Data File : BG044662.D
Acq On : 3 Mar 2020 14:01
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 04 05:32:06 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 24 16:11:23 2020
Response via : Initial Calibration

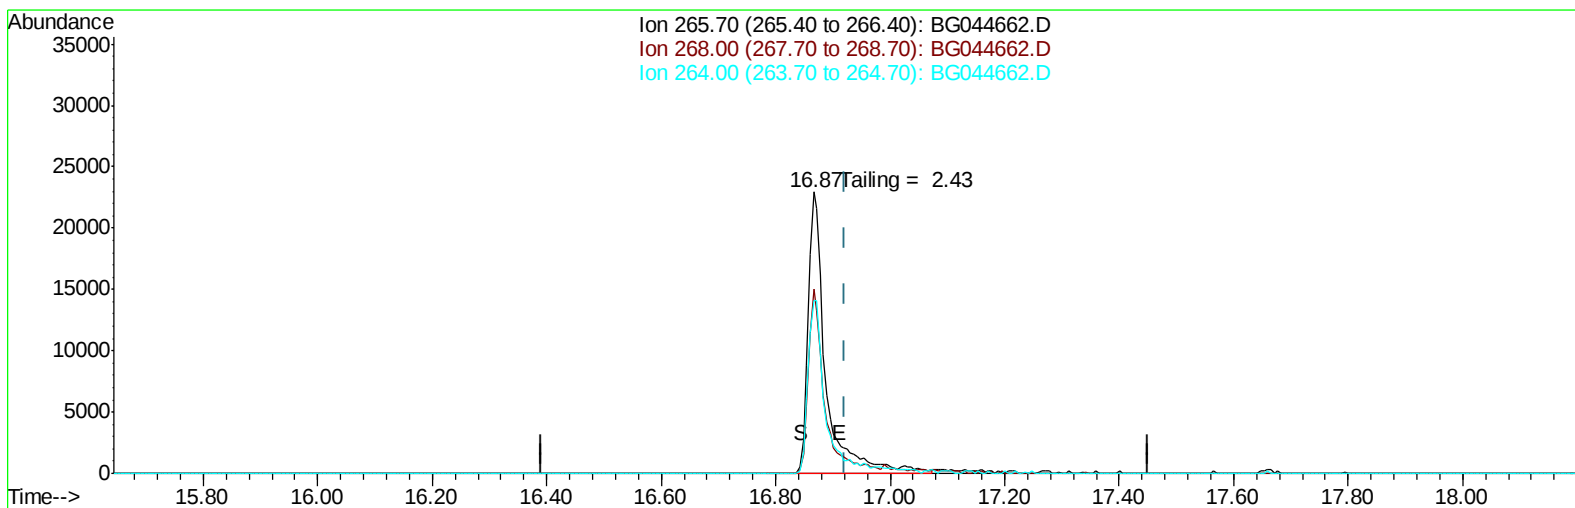

TIC: BG044662.D

(70) Pentachlorophenol (C)




16.866min (-0.055) 18321.53ng

response 48284

Ion	Exp%	Act%
265.70	100	100
268.00	66.70	65.62
264.00	66.20	61.55
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG030320\
 Data File : BG044662.D
 Acq On : 3 Mar 2020 14:01
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 04 05:32:06 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG022420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 24 16:11:23 2020
 Response via : Initial Calibration

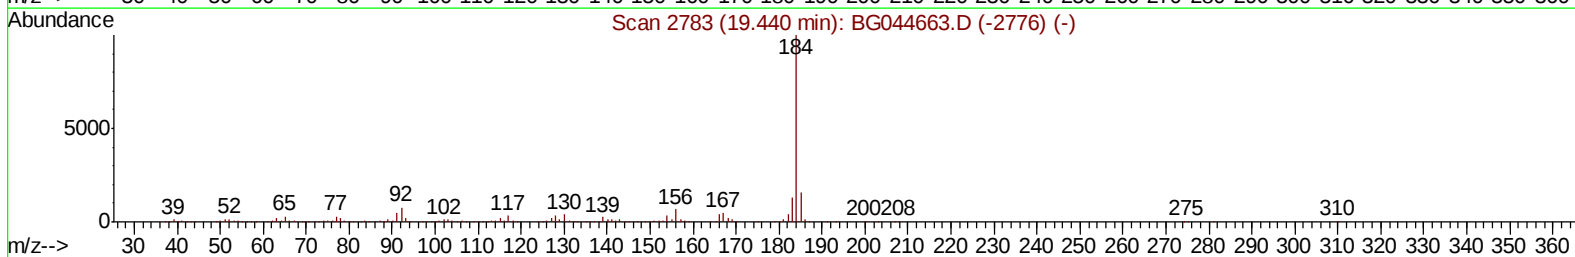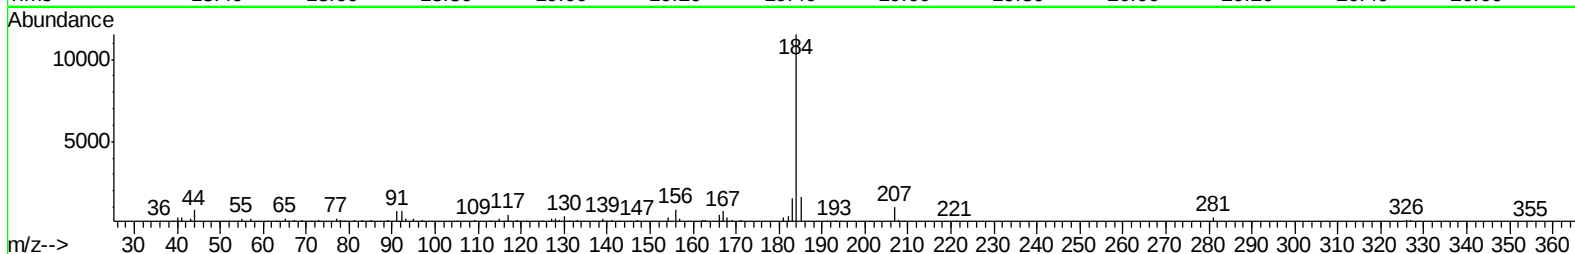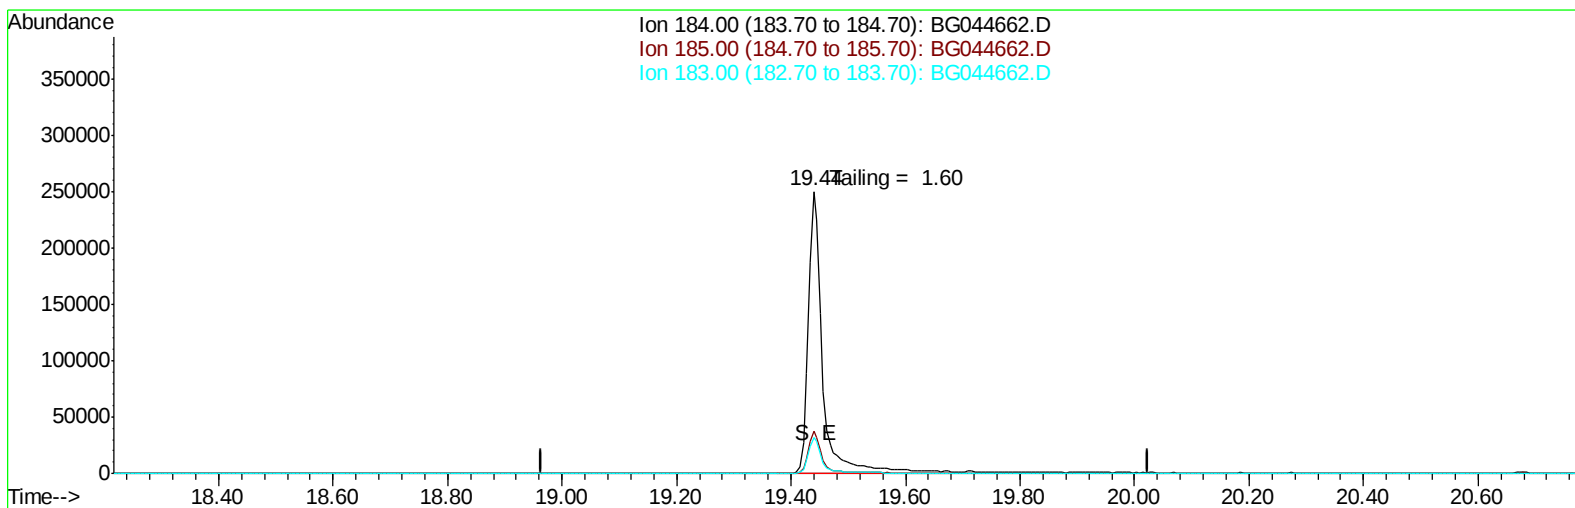

TIC: BG044662.D

(77) Benzidine

19.495min (-19.495) 0.00ng

response 0

Ion	Exp%	Act%
184.00	100	0.00
185.00	15.30	0.00#
183.00	12.40	0.00#
0.00	0.00	0.00