

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG030320\
 Data File : BG044665.D
 Acq On : 3 Mar 2020 16:51
 Operator : CG/JU
 Sample : L1369-06
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PL-02-022820

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG022420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.246	24	27	42	rVB	67217	90895	1.81%	0.450%
2	4.292	200	205	216	rVB2	55817	84630	1.69%	0.419%
3	4.897	299	308	316	rBV2	87064	158256	3.16%	0.784%
4	5.379	383	390	404	rBV	815132	1306438	26.05%	6.471%
5	6.983	656	663	679	rBV	711658	1241624	24.76%	6.150%
6	7.806	796	803	812	rVB	151301	251214	5.01%	1.244%
7	8.129	850	858	871	rBV	727317	1228288	24.49%	6.084%
8	8.963	992	1000	1018	rBV	520361	953340	19.01%	4.722%
9	10.608	1272	1280	1295	rBV	185635	346312	6.91%	1.715%
10	13.076	1693	1700	1711	rBV	1499287	2348865	46.84%	11.634%
11	14.457	1928	1935	1943	rBV	335132	525493	10.48%	2.603%
12	15.949	2182	2189	2204	rBV	1420471	2238571	44.64%	11.088%
13	17.201	2396	2402	2416	rBV	518742	798248	15.92%	3.954%
14	19.827	2843	2849	2862	rBV	3777140	5014960	100.00%	24.839%
15	20.191	2906	2911	2920	rVB3	31213	75285	1.50%	0.373%
16	21.125	3065	3070	3081	rBV	72709	188096	3.75%	0.932%
17	21.437	3117	3123	3141	rBV	624094	1020980	20.36%	5.057%
18	21.642	3154	3158	3162	rBV	63887	90178	1.80%	0.447%
19	22.218	3249	3256	3265	rVB	119811	230561	4.60%	1.142%
20	22.870	3360	3367	3375	rBV	145312	260677	5.20%	1.291%
21	23.622	3488	3495	3504	rVB	136228	291412	5.81%	1.443%
22	24.463	3628	3638	3654	rBV3	299579	1103799	22.01%	5.467%
23	25.555	3815	3824	3835	rVB2	73065	213254	4.25%	1.056%
24	26.807	4029	4037	4049	rVB4	35901	128496	2.56%	0.636%


Sum of corrected areas: 20189872

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG030320\
Data File : BG044665.D
Acq On : 3 Mar 2020 16:51
Operator : CG/JU
Sample : L1369-06
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PL-02-022820

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

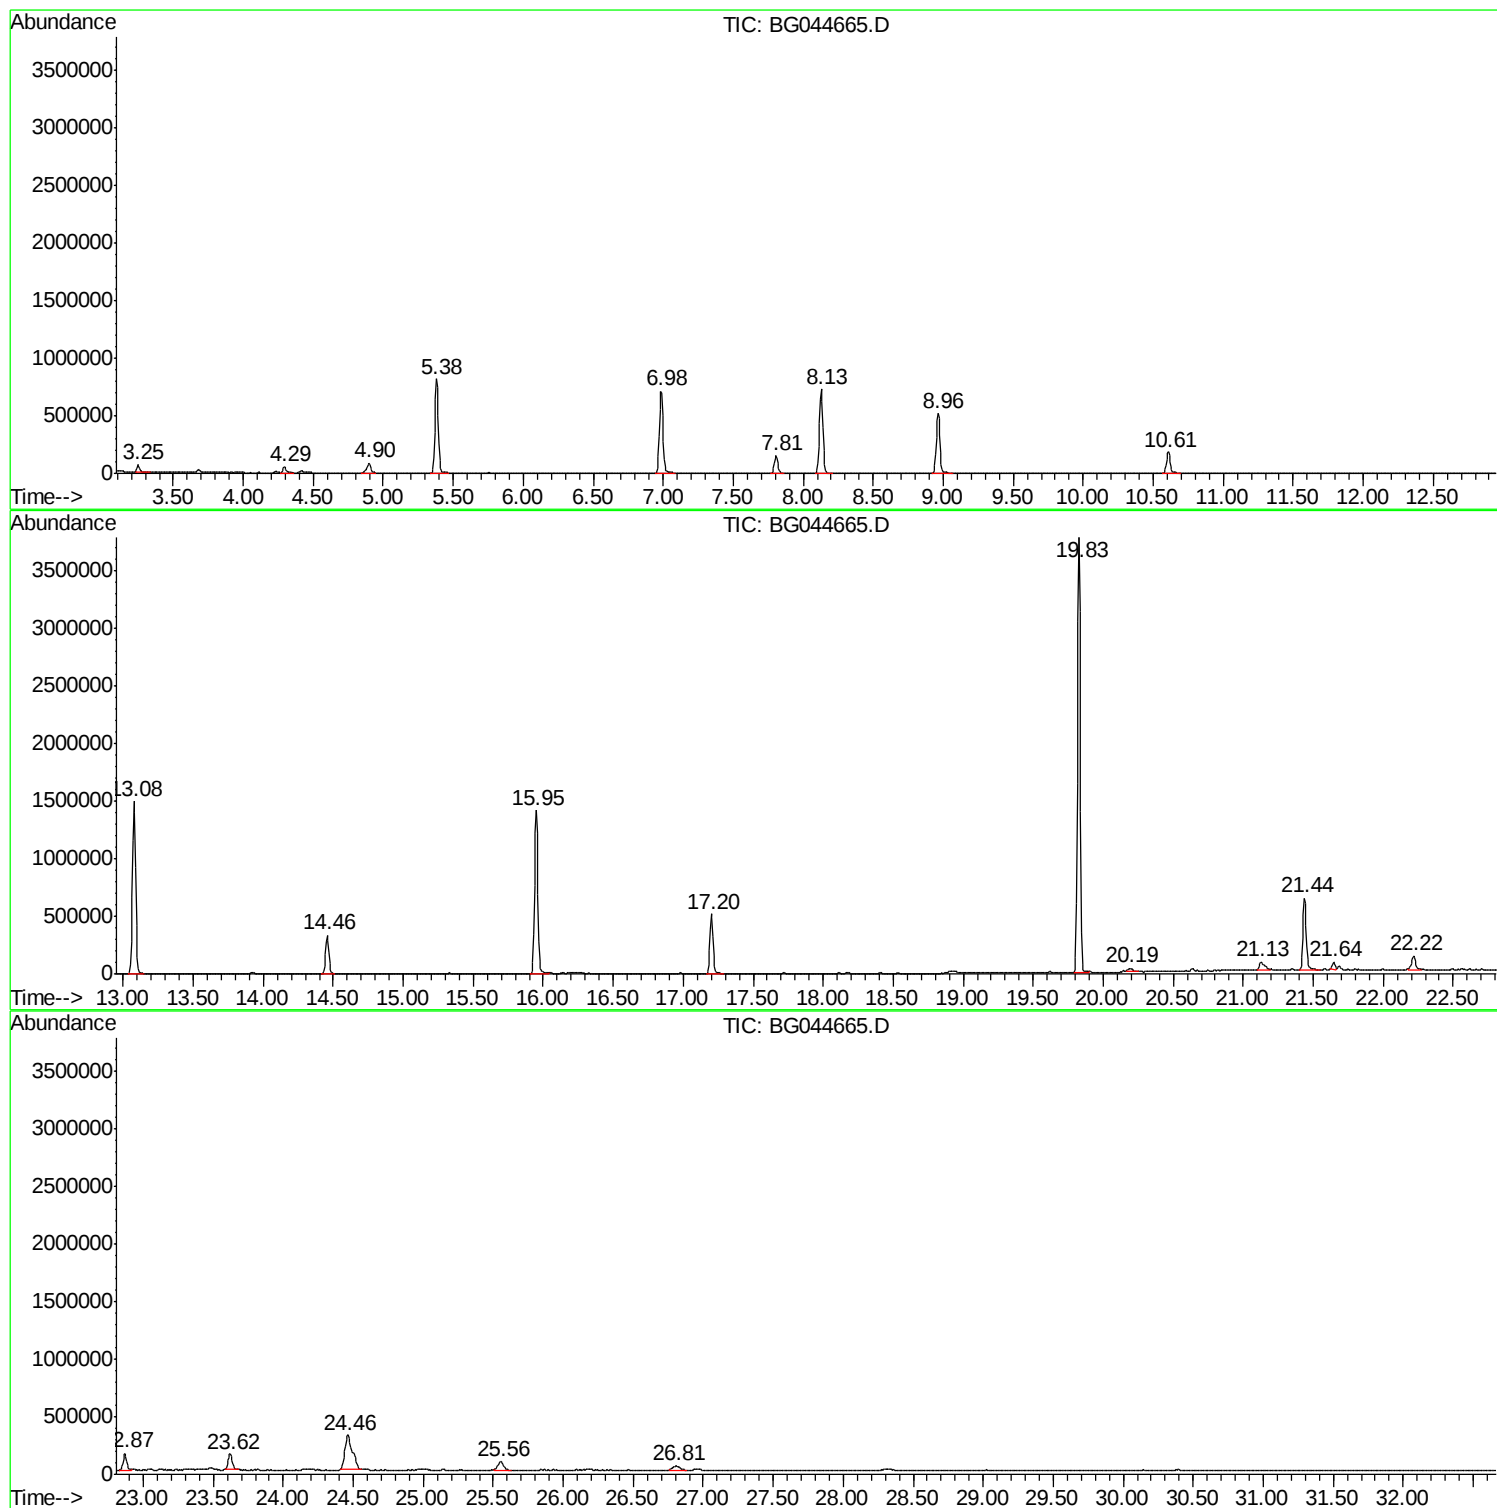

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG030320\
Data_File : BG044665.D
Acq_On : 3-Mar-2020 16:511
Operator : CG/JUU
Sample : L1369-066
Misc :
ALS_Vial : 4 Sample_Multiplier: 11

Instrument :
BNA_G
ClientSampleId :
PL-02-022820

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG022420.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\Database\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
