
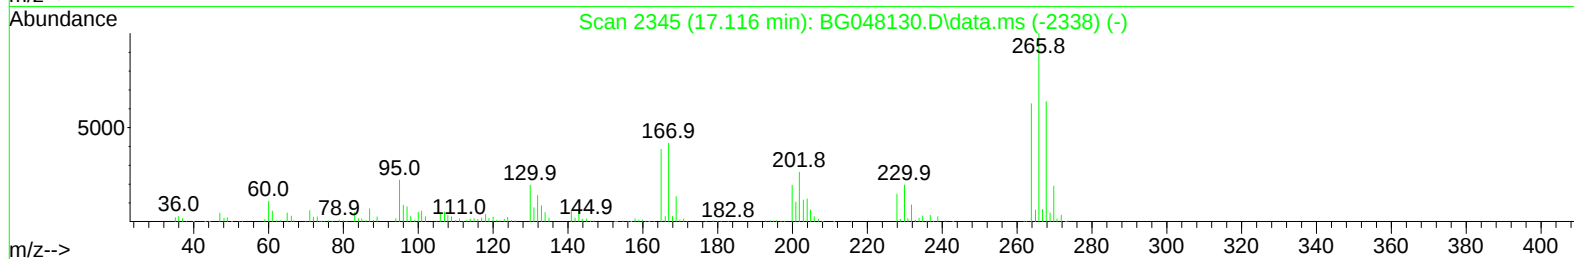
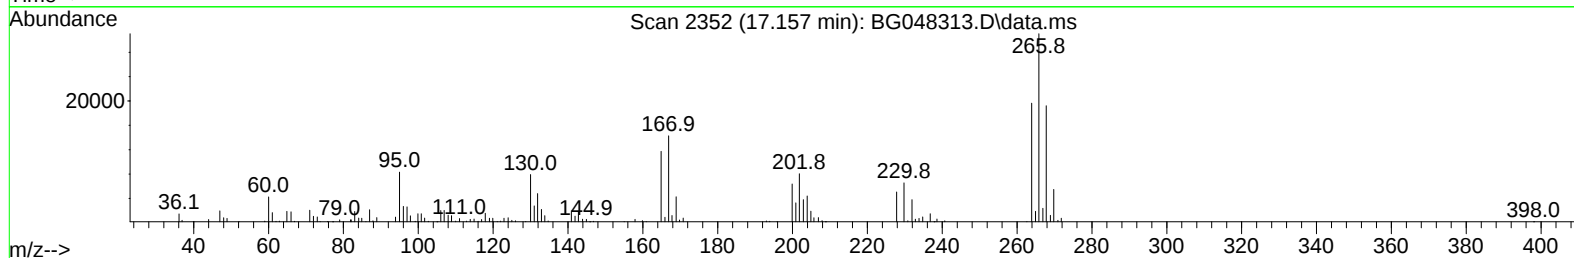


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030321\
Data File : BG048313.D
Acq On : 3 Mar 2021 14:38
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 03 17:30:44 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG021021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 03 16:40:27 2021
Response via : Initial Calibration

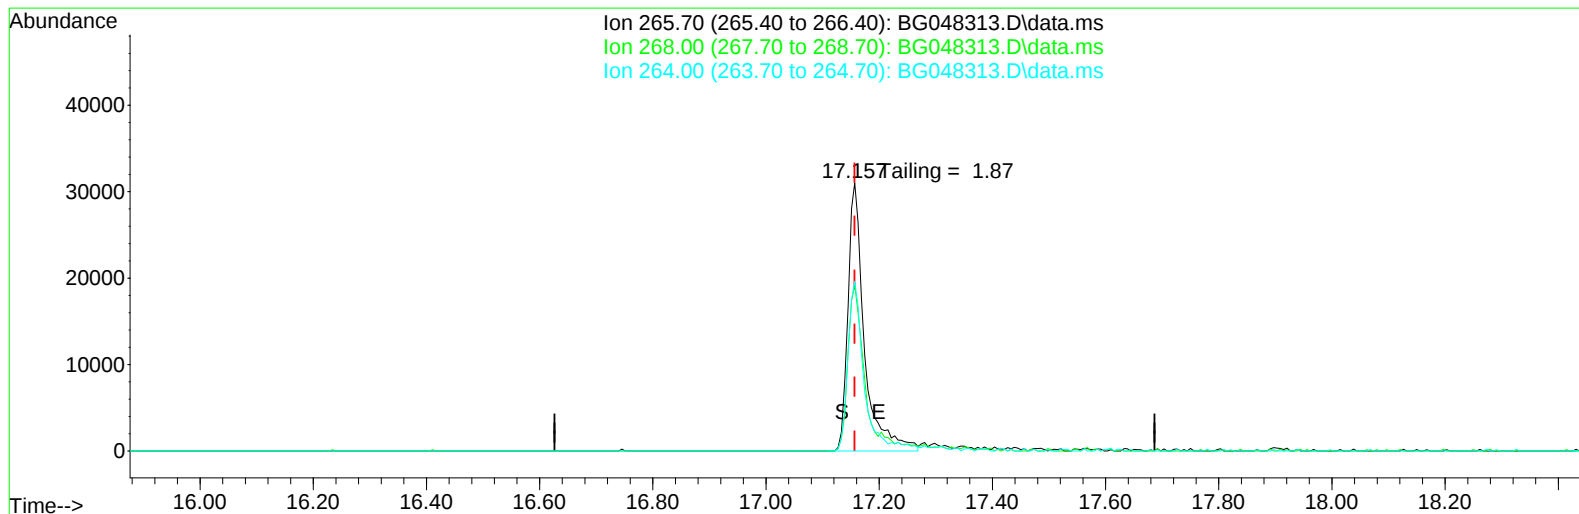

TIC: BG048313.D\data.ms

(70) Pentachlorophenol (C)




17.157min (+ 0.001) 21988.06 ng

response 62924

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.89
264.00	61.60	63.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030321\
 Data File : BG048313.D
 Acq On : 3 Mar 2021 14:38
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 03 17:30:44 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG021021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 03 16:40:27 2021
 Response via : Initial Calibration

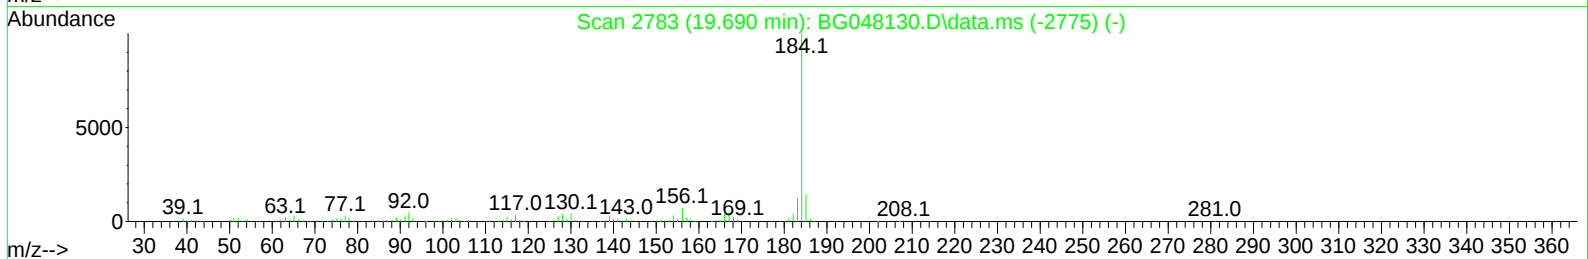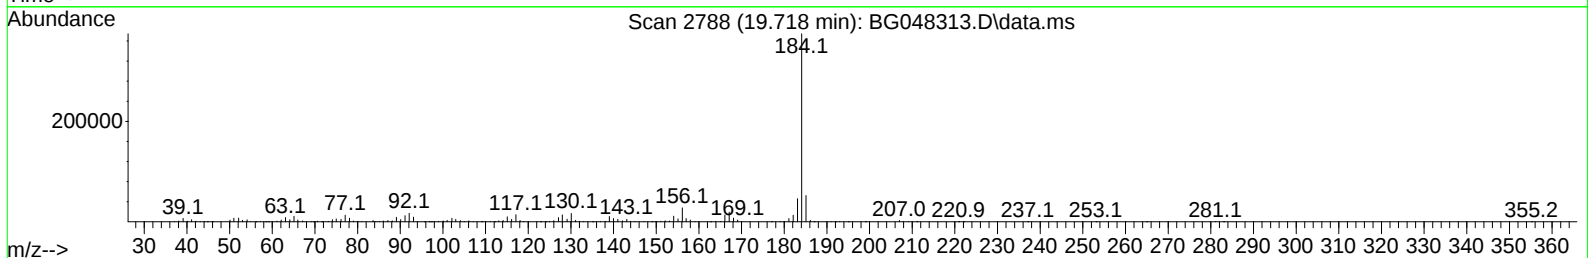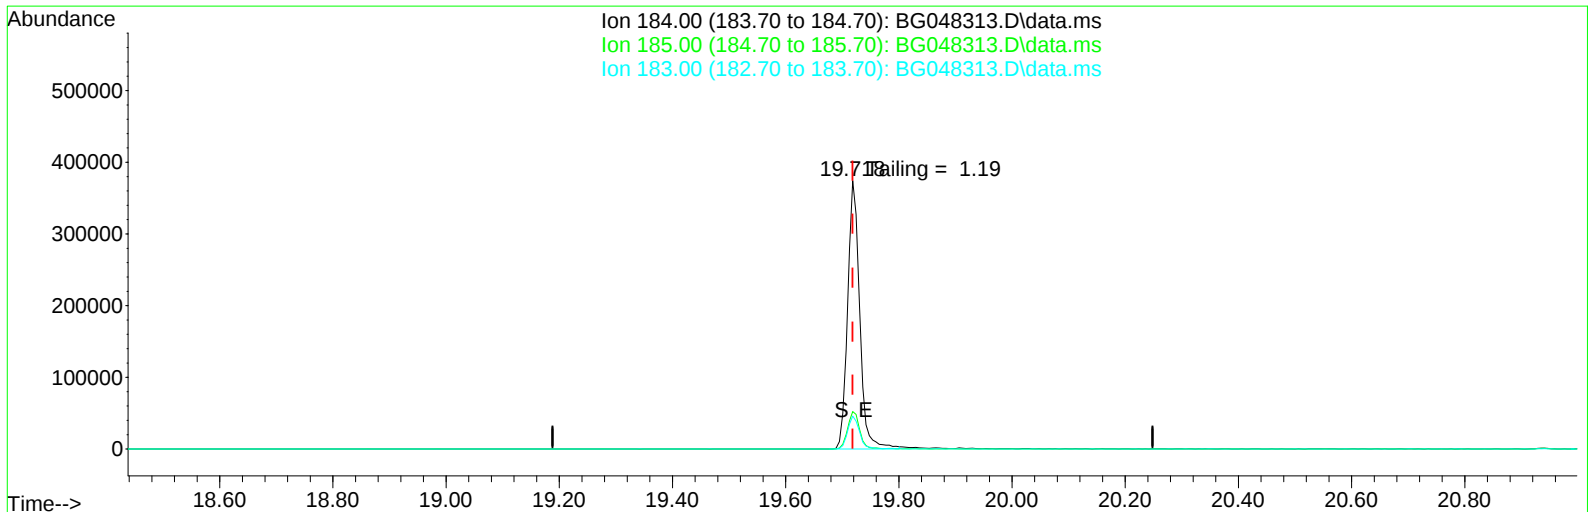

TIC: BG048313.D\data.ms

(77) Benzidine

19.718min (+ 0.001) 269155.73 ng

response 562847

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.97
183.00	13.20	12.33
0.00	0.00	0.00