

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030321\
 Data File : BG048315.D
 Acq On : 3 Mar 2021 16:10
 Operator : CG/JU
 Sample : PB134922BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB134922BL

Quant Time: Mar 03 18:18:44 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG021021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 03 16:40:27 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.105	152	33036	20.00	ng	# 0.00
21) Naphthalene-d8	10.925	136	128444	20.00	ng	0.00
39) Acenaphthene-d10	14.738	164	93367	20.00	ng	0.00
64) Phenanthrene-d10	17.488	188	235961	20.00	ng	# 0.00
76) Chrysene-d12	21.765	240	293088	20.00	ng	# 0.00
86) Perylene-d12	25.061	264	283263	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.690	112	293244	151.10	ng	0.00
7) Phenol-d6	7.312	99	389022	131.93	ng	0.00
23) Nitrobenzene-d5	9.280	82	287205	94.59	ng	0.00
42) 2,4,6-Tribromophenol	16.236	330	186293	124.74	ng	0.00
45) 2-Fluorobiphenyl	13.357	172	598166	89.82	ng	0.00
79) Terphenyl-d14	20.085	244	1216946	75.87	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030321\
Data File : BG048315.D
Acq On : 3 Mar 2021 16:10
Operator : CG/JU
Sample : PB134922BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB134922BL

Quant Time: Mar 03 18:18:44 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG021021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 03 16:40:27 2021
Response via : Initial Calibration




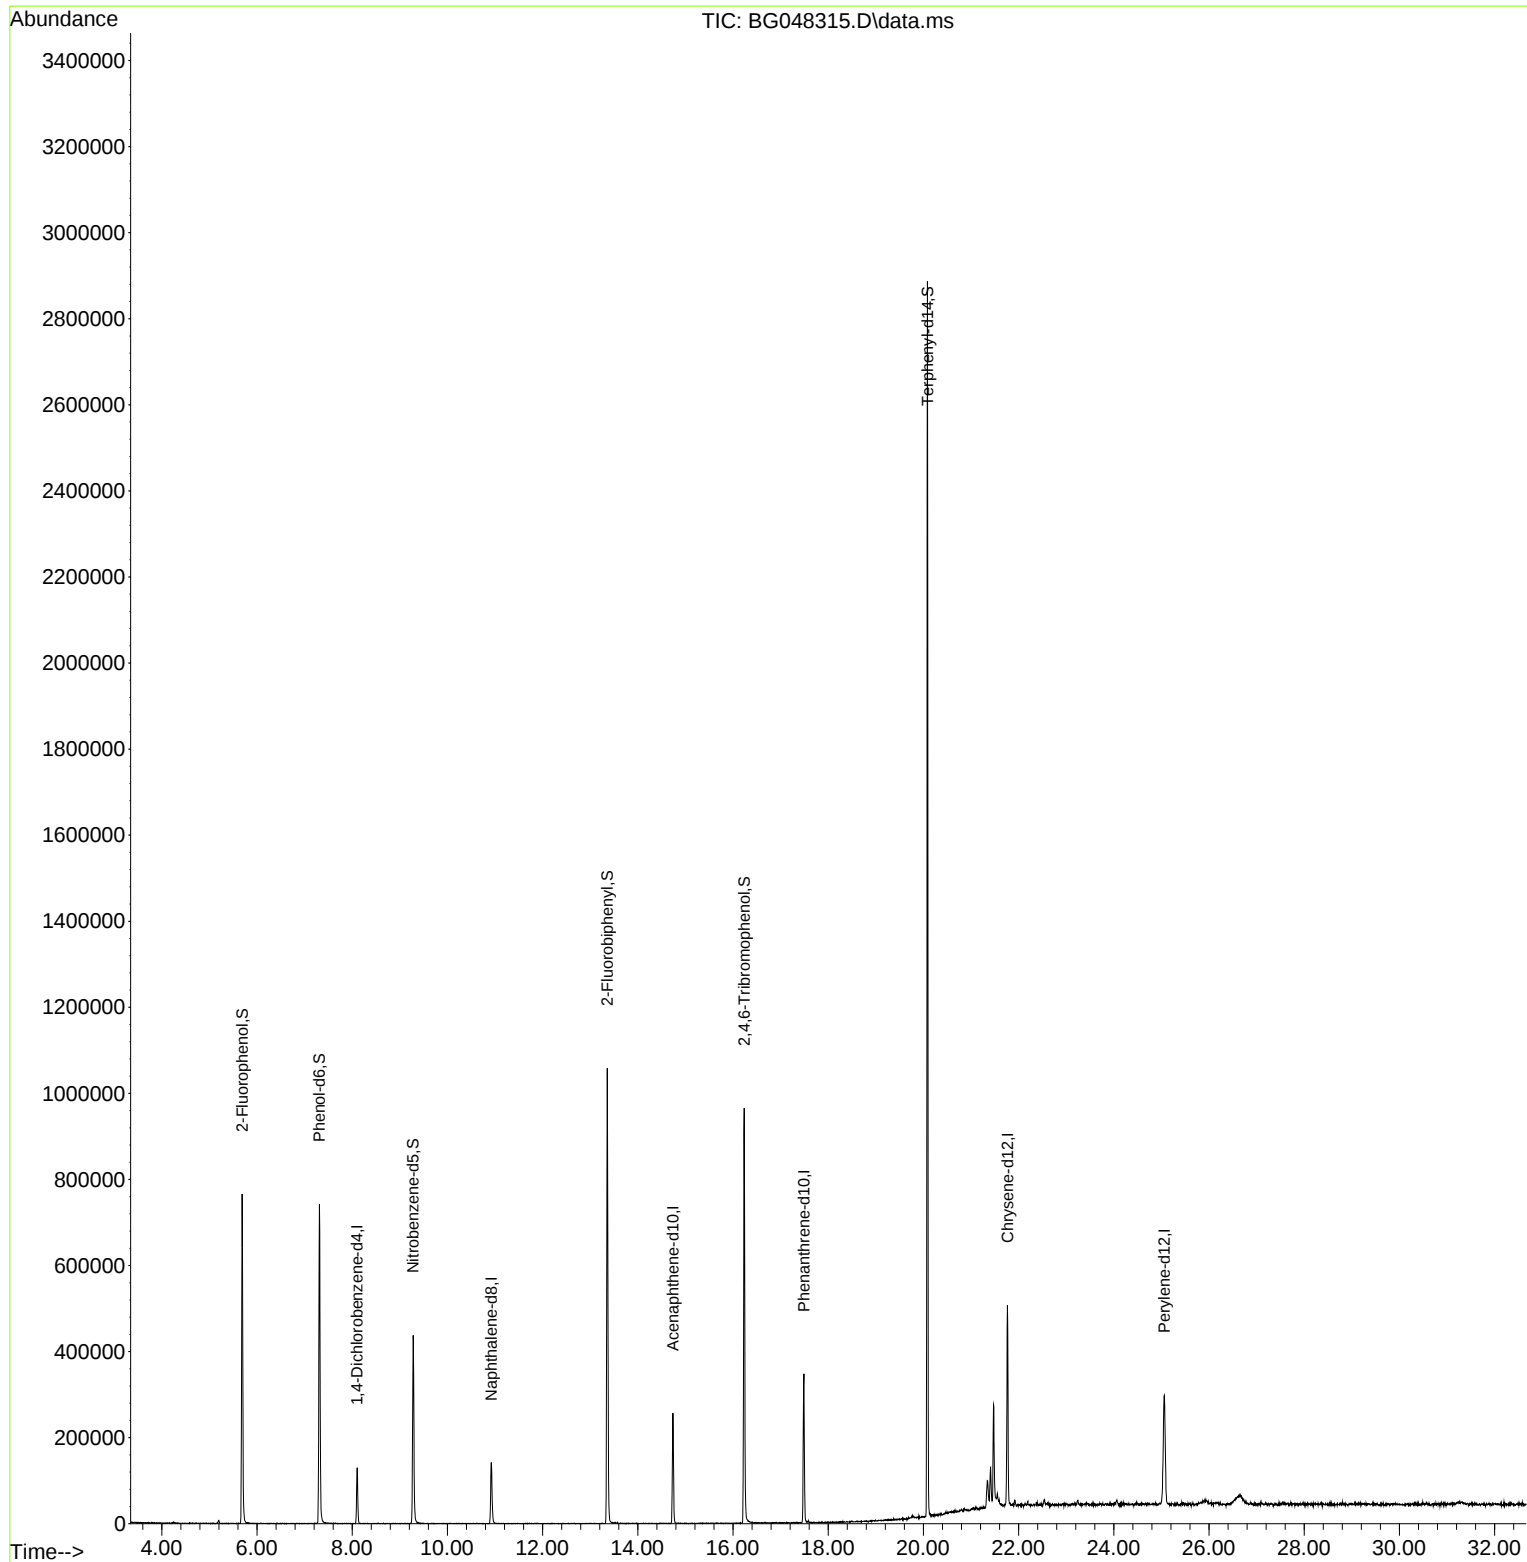




#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 8.105 min Scan# 811
Delta R.T. 0.003 min
Lab File: BG048315.D
Acq: 3 Mar 2021 16:10




Instrument :
BNA_G
ClientSampleId :
PB134922BL


Tgt Ion:152 Resp: 33036
Ion Ratio Lower Upper
152 100
150 156.4 125.0 187.6
115 63.3 41.8 62.6#

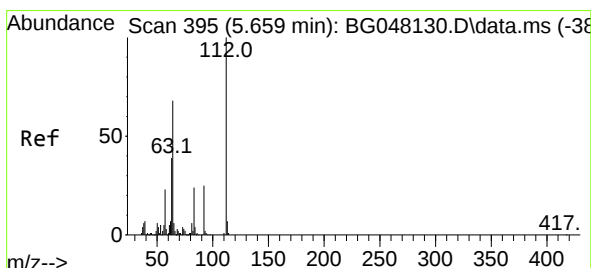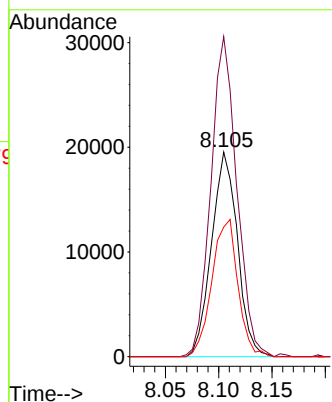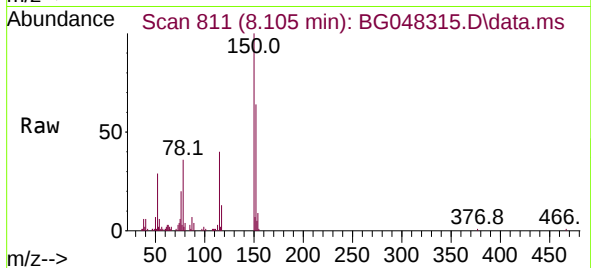

#5
2-Fluorophenol
Concen: 151.10 ng
RT: 5.690 min Scan# 400
Delta R.T. 0.003 min
Lab File: BG048315.D
Acq: 3 Mar 2021 16:10

Tgt Ion:112 Resp: 293244
Ion Ratio Lower Upper
112 100
64 71.3 46.7 70.1#
63 44.1 22.8 34.2#


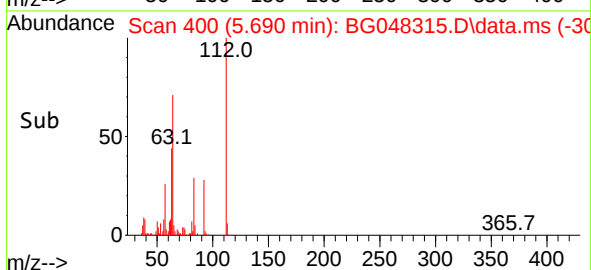
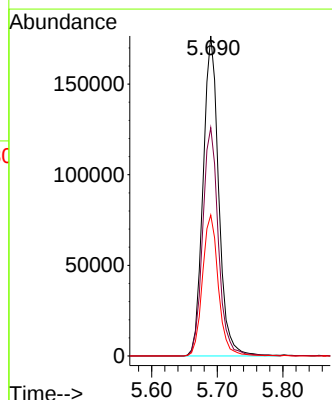





#7
Phenol-d6
Concen: 131.93 ng
RT: 7.312 min Scan# 676
Delta R.T. -0.003 min
Lab File: BG048315.D
Acq: 3 Mar 2021 16:10




Instrument :
BNA_G
ClientSampleId :
PB134922BL


Tgt Ion: 99 Resp: 389022
Ion Ratio Lower Upper
99 100
42 23.7 12.8 19.2#
71 51.3 24.6 36.8#

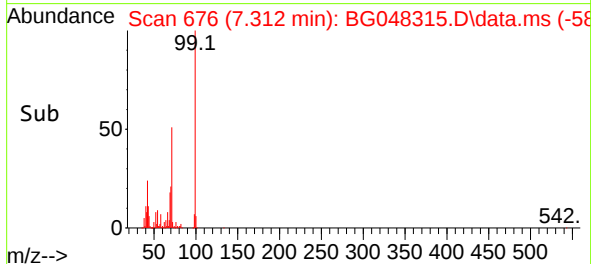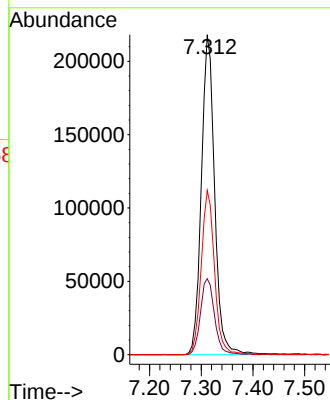

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 10.925 min Scan# 1291
Delta R.T. 0.003 min
Lab File: BG048315.D
Acq: 3 Mar 2021 16:10

Tgt Ion:136 Resp: 128444
Ion Ratio Lower Upper
136 100
137 10.8 9.1 13.7
54 7.8 6.2 9.4
68 5.5 5.0 7.4


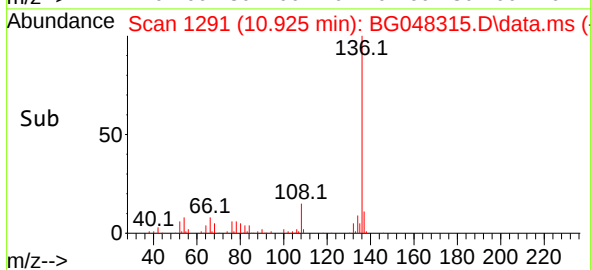
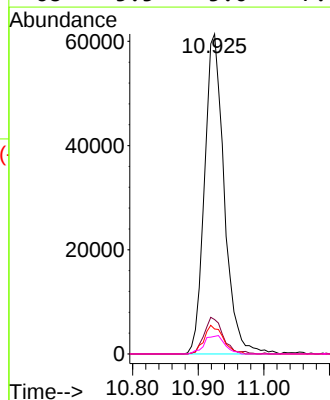
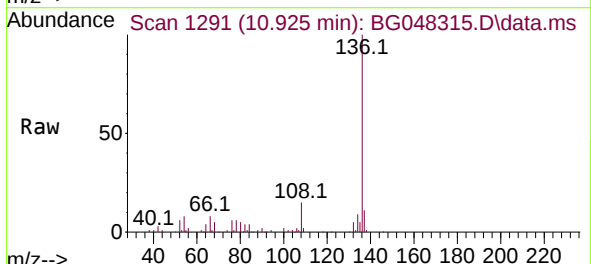


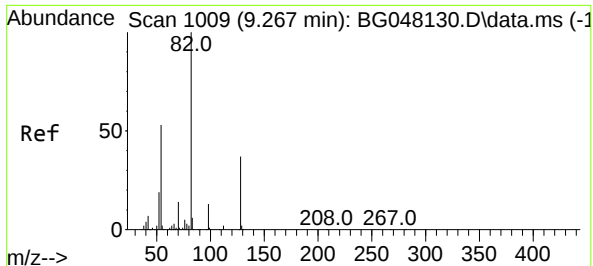

#23
Nitrobenzene-d5
Concen: 94.59 ng
RT: 9.280 min Scan# 1011
Delta R.T. -0.003 min
Lab File: BG048315.D
Acq: 3 Mar 2021 16:10




Instrument :
BNA_G
ClientSampleId :
PB134922BL


Tgt Ion: 82 Resp: 287205
Ion Ratio Lower Upper
82 100
128 33.1 37.0 55.6#
54 54.2 39.0 58.4

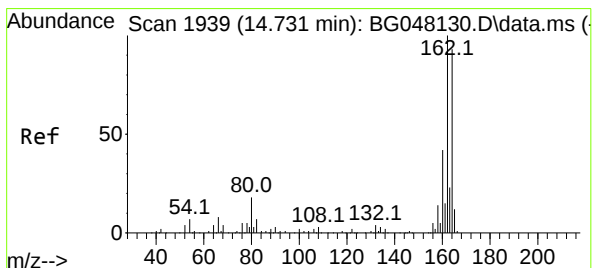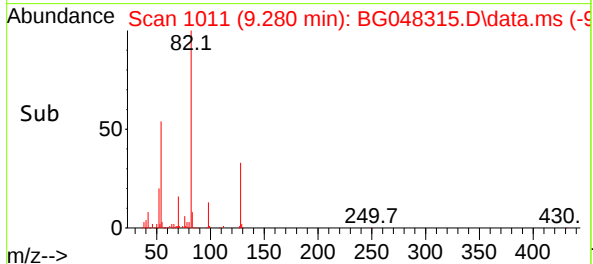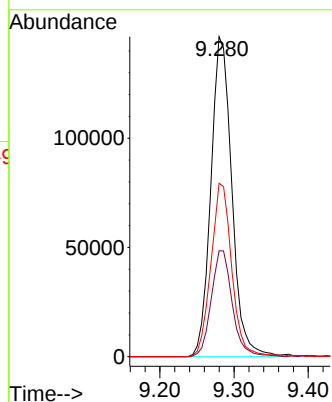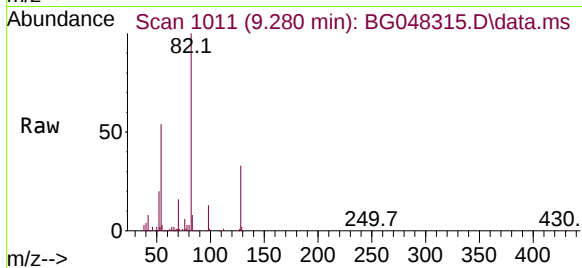

#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.738 min Scan# 1940
Delta R.T. 0.003 min
Lab File: BG048315.D
Acq: 3 Mar 2021 16:10


Tgt Ion: 164 Resp: 93367
Ion Ratio Lower Upper
164 100
162 104.8 82.3 123.5
160 42.9 35.3 52.9

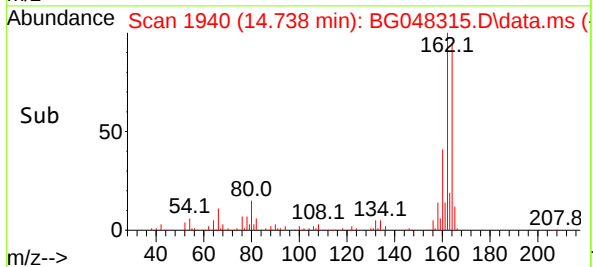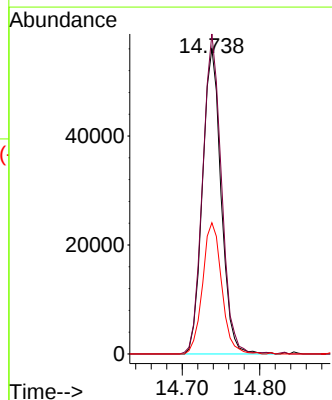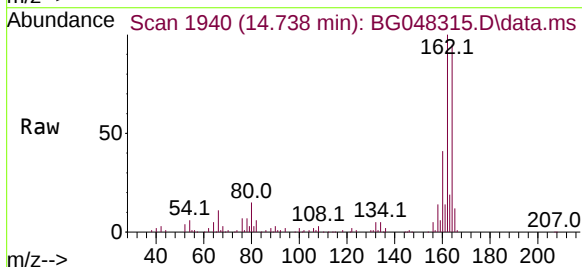






#42
2,4,6-Tribromophenol
Concen: 124.74 ng
RT: 16.236 min Scan# 2195
Delta R.T. -0.003 min
Lab File: BG048315.D
Acq: 3 Mar 2021 16:10


Instrument :
BNA_G
ClientSampleId :
PB134922BL

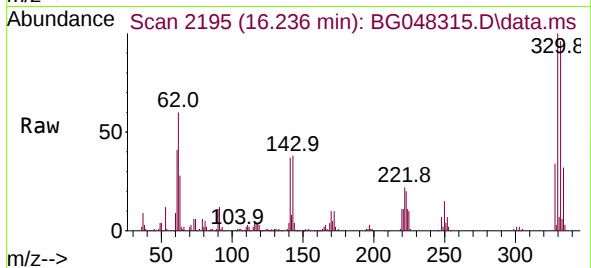



Tgt Ion:330 Resp: 186293
Ion Ratio Lower Upper
330 100
332 96.8 76.5 114.7
141 37.2 26.0 39.0

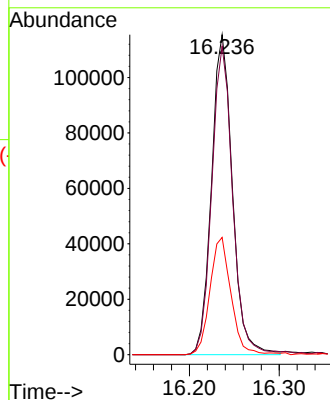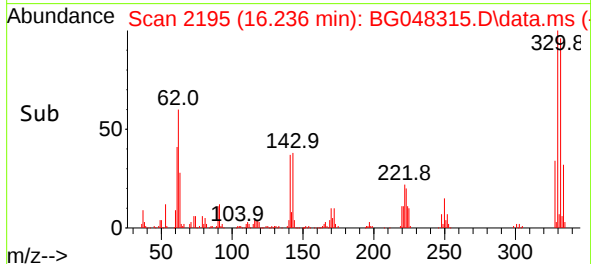


#45
2-Fluorobiphenyl
Concen: 89.82 ng
RT: 13.357 min Scan# 1705
Delta R.T. -0.003 min
Lab File: BG048315.D
Acq: 3 Mar 2021 16:10

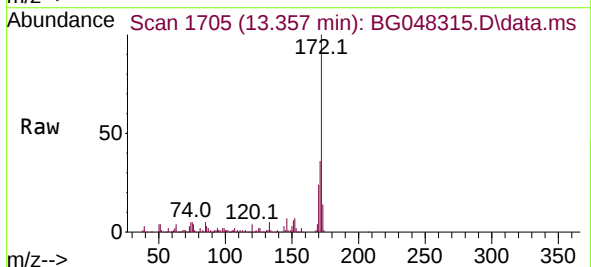

Tgt Ion:172 Resp: 598166
Ion Ratio Lower Upper
172 100
171 35.6 31.3 46.9
170 24.3 20.8 31.2



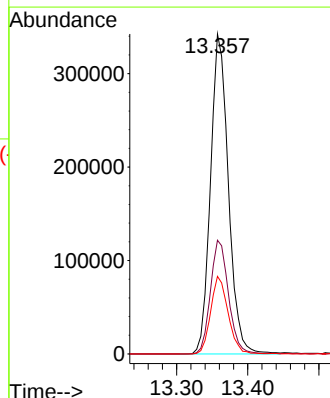
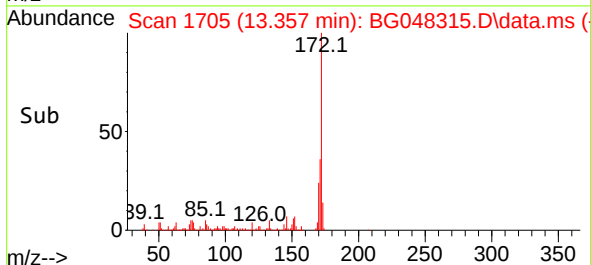




#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.488 min Scan# 2408
Delta R.T. 0.003 min
Lab File: BG048315.D
Acq: 3 Mar 2021 16:10




Instrument :
BNA_G
ClientSampleId :
PB134922BL


Tgt Ion:188 Resp: 235961
Ion Ratio Lower Upper
188 100
94 6.0 6.3 9.5#
80 7.4 7.0 10.6

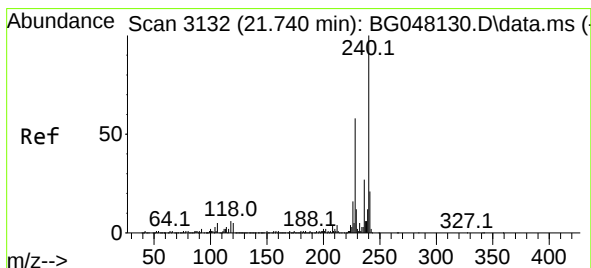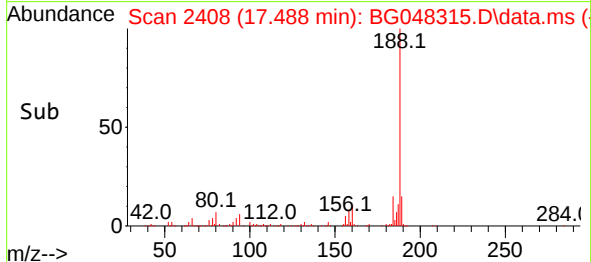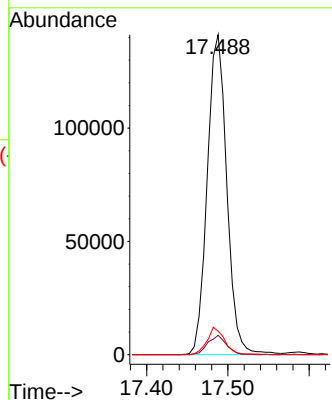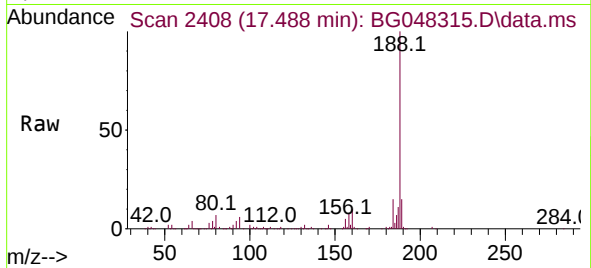

#76
Chrysene-d12
Concen: 20.00 ng
RT: 21.765 min Scan# 3136
Delta R.T. -0.003 min
Lab File: BG048315.D
Acq: 3 Mar 2021 16:10

Tgt Ion:240 Resp: 293088
Ion Ratio Lower Upper
240 100
120 4.6 6.2 9.4#
236 26.0 20.5 30.7


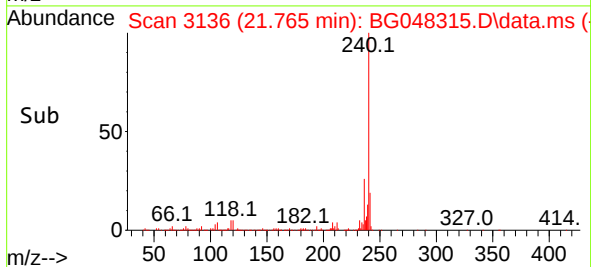
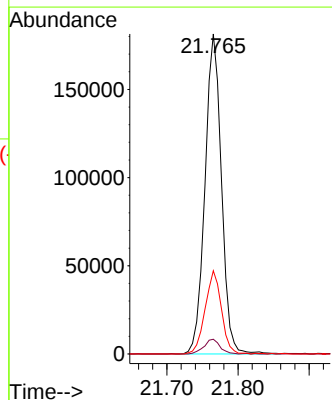
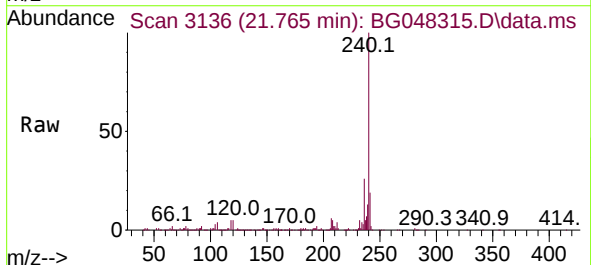




#79
 Terphenyl-d14
 Concen: 75.87 ng
 RT: 20.085 min Scan# 2850
 Delta R.T. 0.003 min
 Lab File: BG048315.D
 Acq: 3 Mar 2021 16:10

Instrument :
 BNA_G
 ClientSampleId :
 PB134922BL

Tgt Ion:244 Resp: 1216946
 Ion Ratio Lower Upper
 244 100
 212 8.8 6.7 10.1
 122 6.5 7.8 11.6#

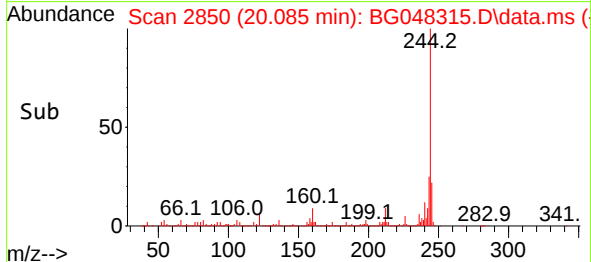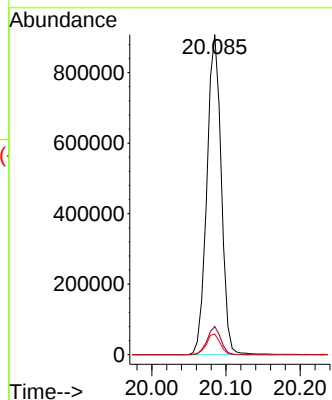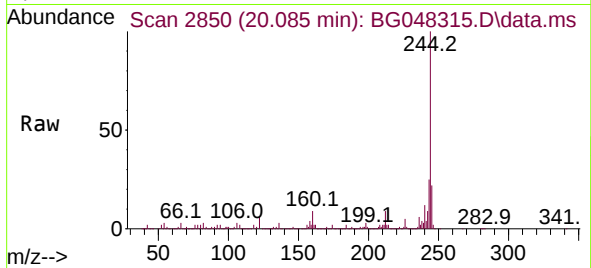

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 25.061 min Scan# 3697
 Delta R.T. -0.003 min
 Lab File: BG048315.D
 Acq: 3 Mar 2021 16:10

Tgt Ion:264 Resp: 283263
 Ion Ratio Lower Upper
 264 100
 260 23.1 18.8 28.2
 265 21.6 17.8 26.8

