
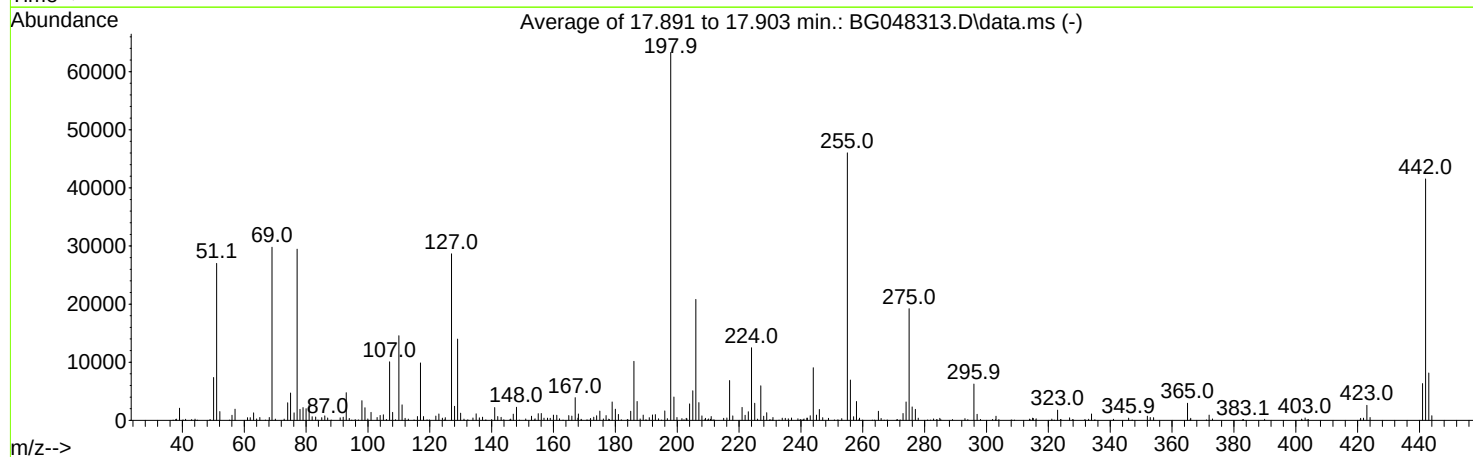


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030321\
 Data File : BG048313.D
 Acq On : 3 Mar 2021 14:38
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG021021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 03 16:40:27 2021

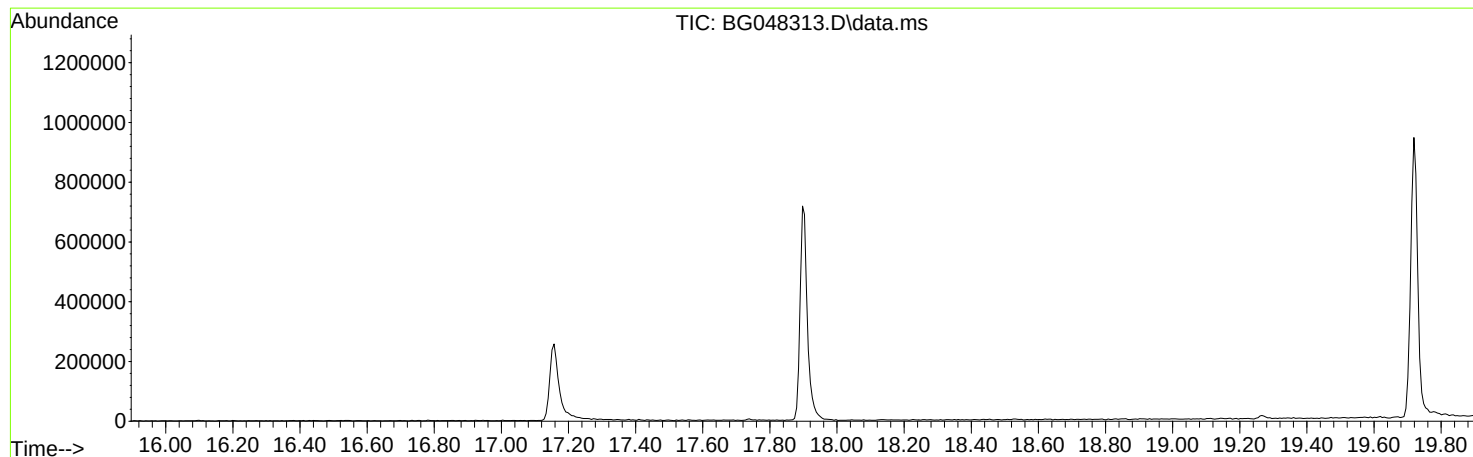

AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.7	27021	PASS
68	69	0.00	2	1.7	503	PASS
69	198	0.00	100	47.1	29797	PASS
70	69	0.00	2	0.7	211	PASS
127	198	10	80	45.3	28653	PASS
197	198	0.00	2	0.5	307	PASS
198	198	100	100	100.0	63291	PASS
199	198	5	9	6.4	4025	PASS
275	198	10	60	30.4	19214	PASS
365	198	1	100	4.7	2961	PASS
441	198	0.01	100	10.0	6326	PASS
442	198	50	100	65.6	41536	PASS
443	442	15	24	19.6	8151	PASS

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/3/2021	BNA_G	<u>BG048313.D</u>
Compound Name	Response	Retention Time
DDT	317538	20.94
DDD	740	20.5
DDE	595	19.99
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1335	318873	0.42

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030321\
Data File : BG048313.D
Acq On : 3 Mar 2021 14:38
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 03 17:30:44 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG021021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 03 16:40:27 2021
Response via : Initial Calibration

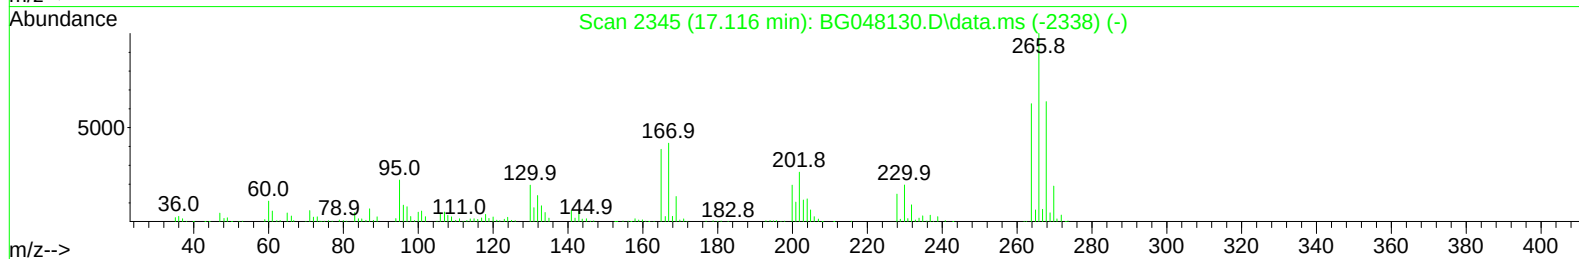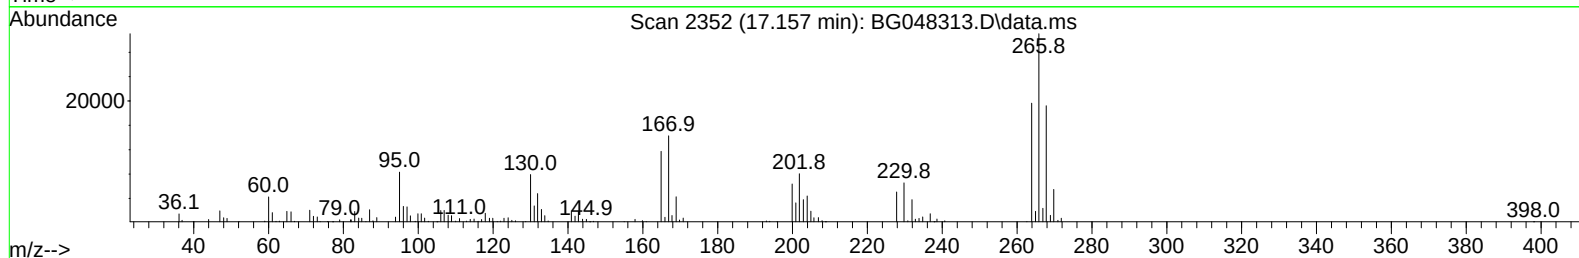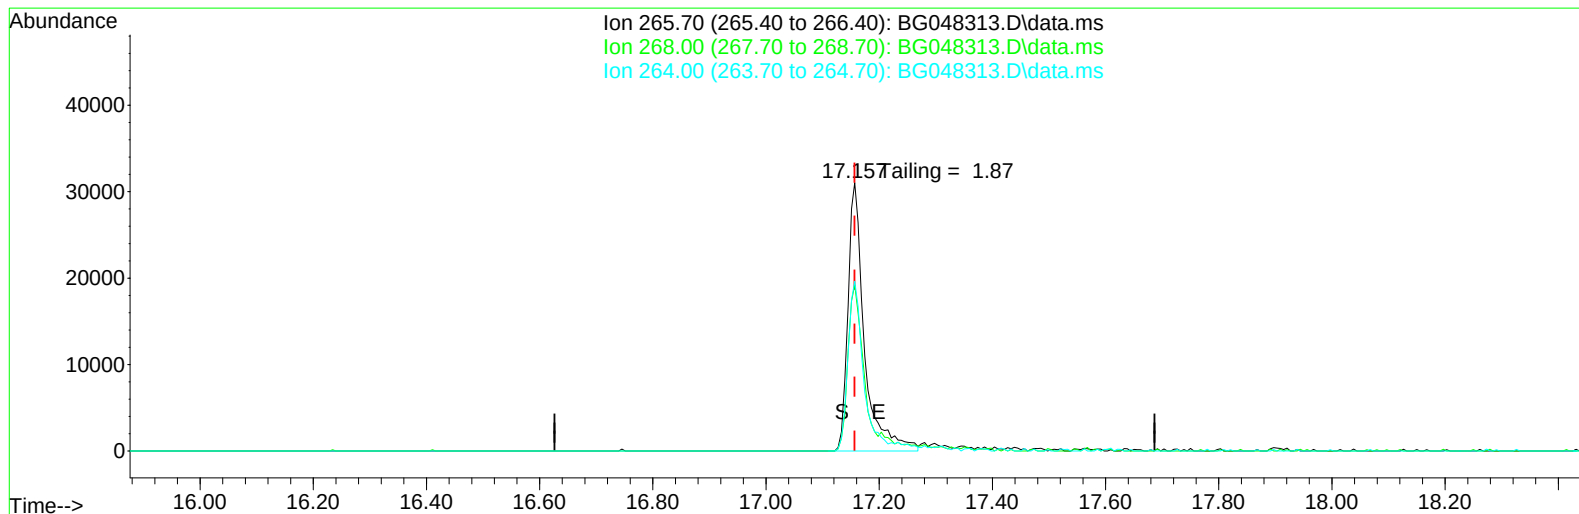

TIC: BG048313.D\data.ms

(70) Pentachlorophenol (C)

17.157min (+ 0.001) 21988.06 ng




response 62924

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.89
264.00	61.60	63.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030321\
 Data File : BG048313.D
 Acq On : 3 Mar 2021 14:38
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Mar 03 17:30:44 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG021021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 03 16:40:27 2021
 Response via : Initial Calibration

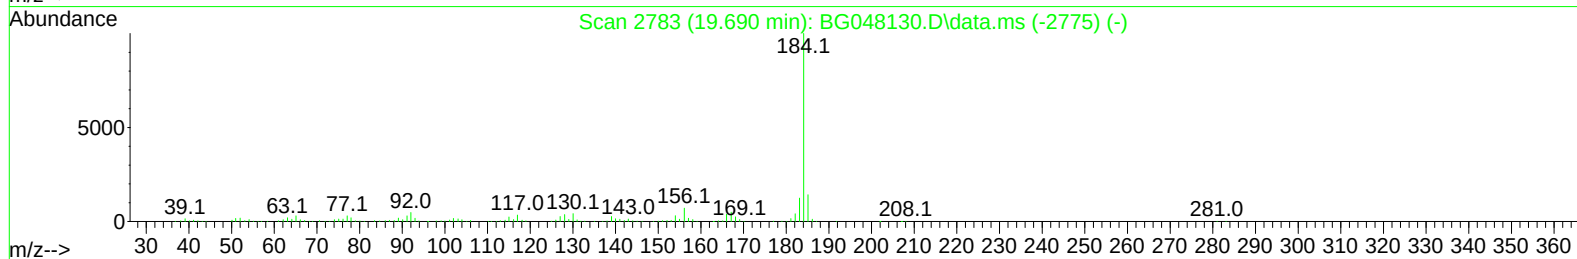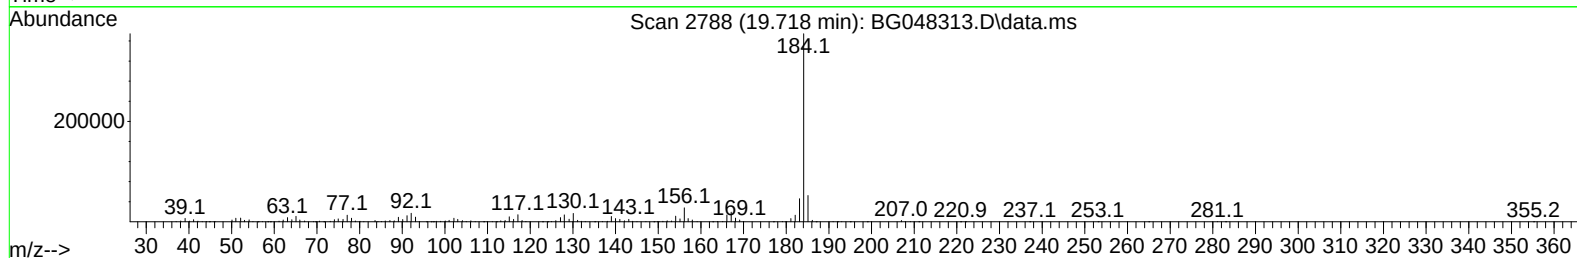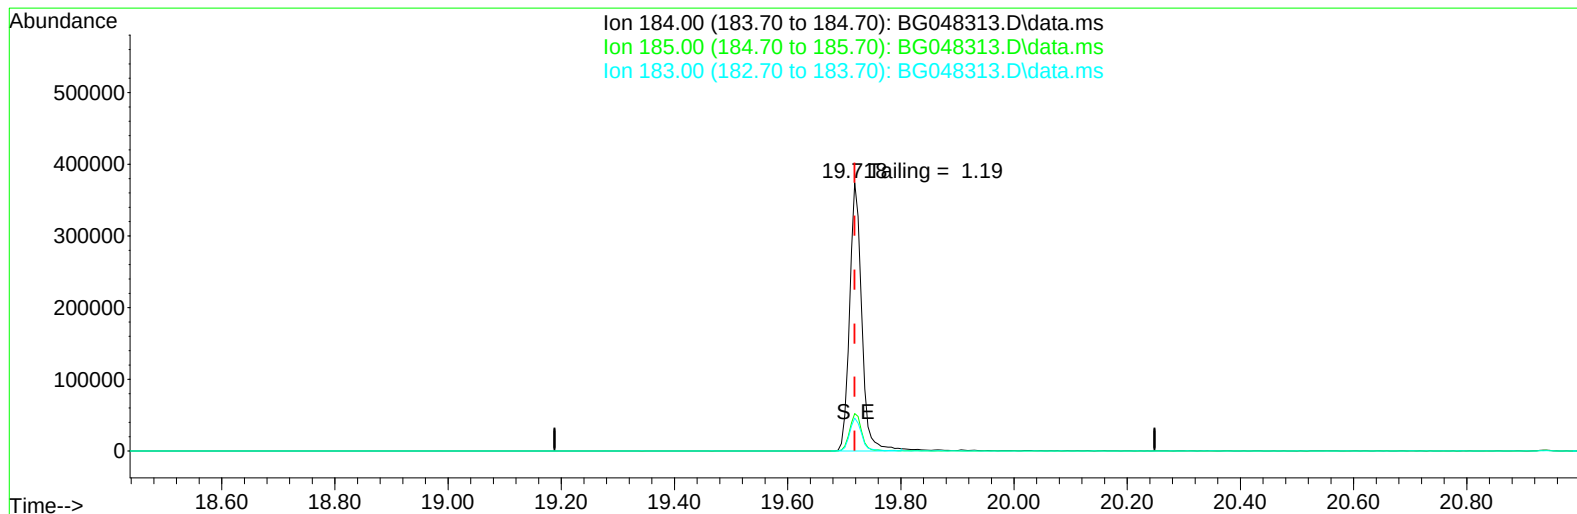

TIC: BG048313.D\data.ms

(77) Benzidine

19.718min (+ 0.001) 269155.73 ng

response 562847

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.97
183.00	13.20	12.33
0.00	0.00	0.00