




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030322\
Data File : BG052549.D
Acq On : 3 Mar 2022 11:35
Operator : CG/JU
Sample : PB143052BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK052

Manual IntegrationsAPPROVED

Quant Time: Mar 04 00:00:35 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 22 17:32:12 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/04/2022
Supervised By :Yogesh Patel 03/07/2022

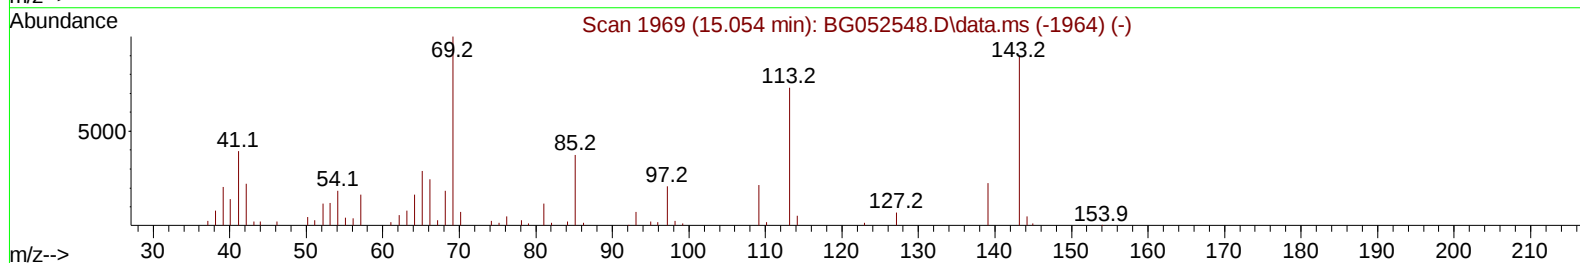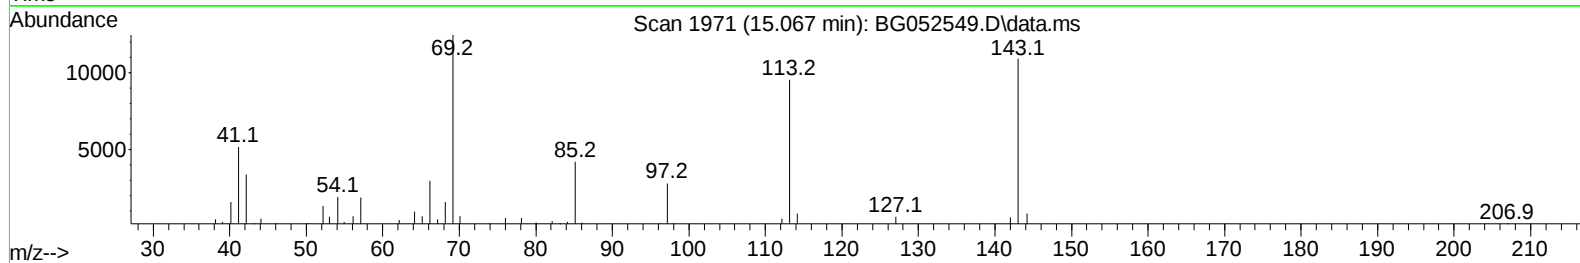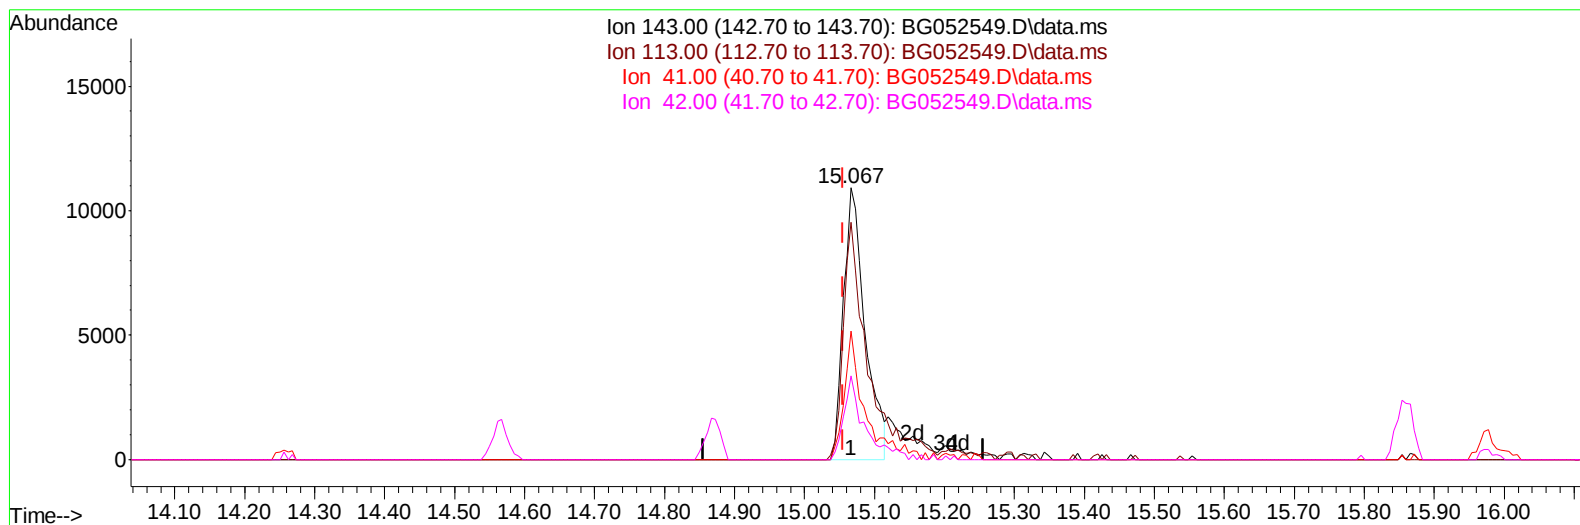

TIC: BG052549.D\data.ms

(54) 4-Nitrophenol-d4 (S)

15.067min (+ 0.012) 22.10 ng/u1

response 23385

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	80.30	87.41
41.00	44.40	47.34
42.00	29.70	30.88




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030322\
Data File : BG052549.D
Acq On : 3 Mar 2022 11:35
Operator : CG/JU
Sample : PB143052BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK052

Manual IntegrationsAPPROVED

Quant Time: Mar 04 00:15:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 22 17:32:12 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/04/2022
Supervised By :Yogesh Patel 03/07/2022

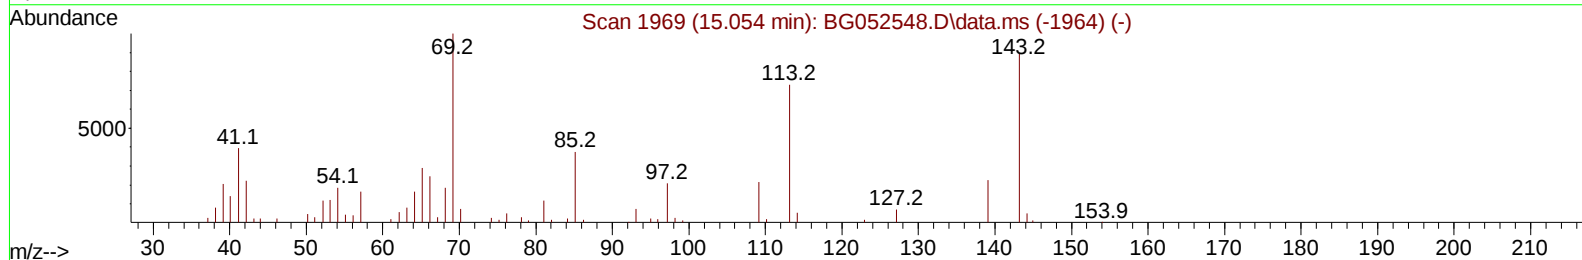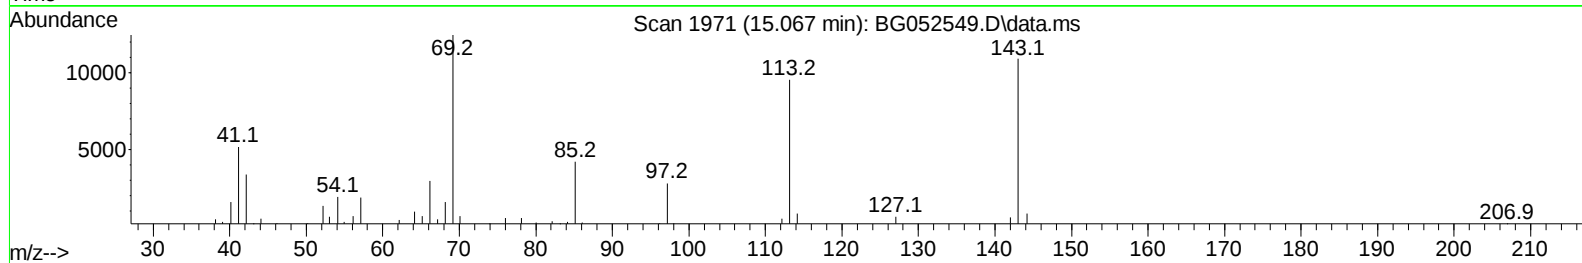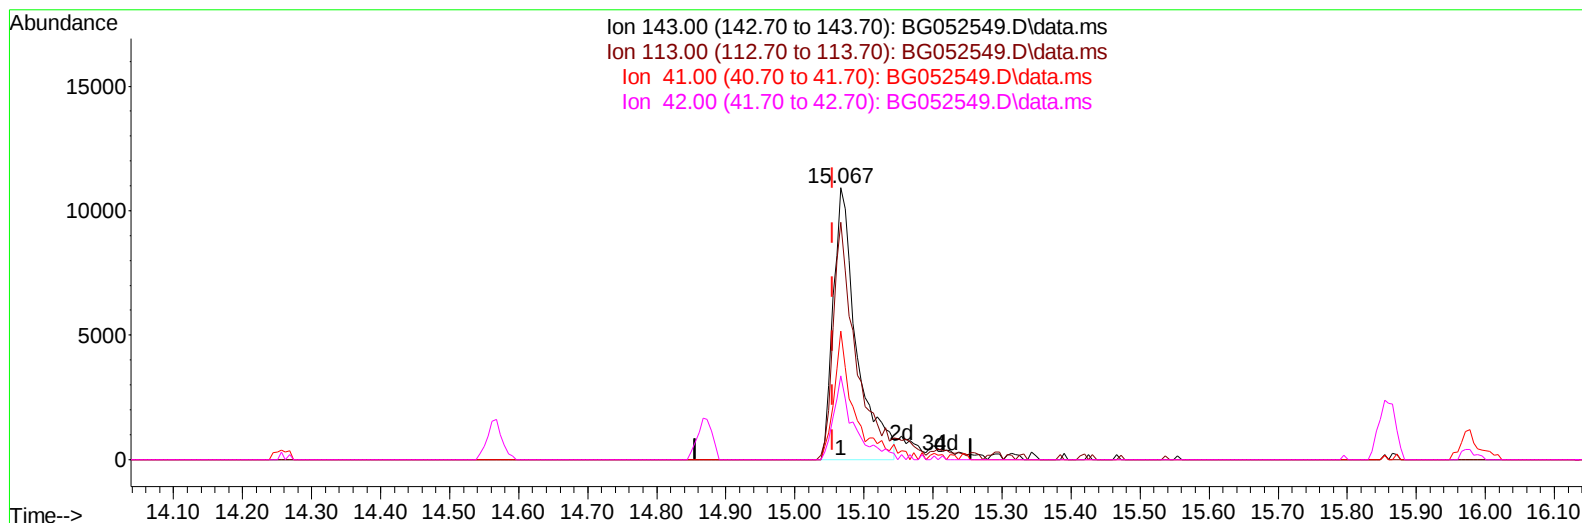

TIC: BG052549.D\data.ms

(54) 4-Nitrophenol-d4 (S)

15.067min (+ 0.012) 24.20 ng/ul m

response 25607

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	80.30	87.41
41.00	44.40	47.34
42.00	29.70	30.88

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030322\
 Data File : BG052549.D
 Acq On : 3 Mar 2022 11:35
 Operator : CG/JU
 Sample : PB143052BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK052

Manual IntegrationsAPPROVED

Quant Time: Mar 04 00:15:54 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 22 17:32:12 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/04/2022
 Supervised By :Yogesh Patel 03/07/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.229	152	26516	20.000	ng/ul	0.00
20) Naphthalene-d8	11.066	136	110480	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.873	164	81871	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.616	188	211401	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.934	240	215957	20.000	ng/ul	# 0.00
88) Perylene-d12	25.400	264	210804	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.547	96	3430	5.074	ng/uL	0.00
4) Pyridine-d5	3.976	84	50467	24.748	ng/ul	0.00
7) Phenol-d5	7.377	99	63309	25.179	ng/ul	0.01
9) Bis-(2-Chloroethyl)eth...	7.536	67	38610	26.276	ng/ul	0.00
11) 2-Chlorophenol-d4	7.759	132	44718	25.321	ng/ul	0.01
15) 4-Methylphenol-d8	8.934	113	50053	25.585	ng/ul	0.00
21) Nitrobenzene-d5	9.404	128	25321	26.885	ng/ul	0.00
24) 2-Nitrophenol-d4	10.132	143	27984	27.126	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.684	165	48184	25.046	ng/ul	0.01
31) 4-Chloroaniline-d4	11.190	131	69526	26.079	ng/ul	0.00
46) Dimethylphthalate-d6	14.262	166	203754	30.614	ng/ul	0.00
49) Acenaphthylene-d8	14.567	160	238762	29.060	ng/ul	0.00
54) 4-Nitrophenol-d4	15.067	143	25607m	24.203	ng/ul	0.01
60) Fluorene-d10	15.860	176	169073	28.917	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.977	200	28458	21.231	ng/ul	0.00
73) Anthracene-d10	17.716	188	311312	30.482	ng/ul	0.00
81) Pyrene-d10	19.995	212	389269	30.805	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.159	264	354875	31.379	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030322\
Data File : BG052549.D
Acq On : 3 Mar 2022 11:35
Operator : CG/JU
Sample : PB143052BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK052

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/04/2022
Supervised By :Yogesh Patel 03/07/2022

Quant Time: Mar 04 00:15:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 22 17:32:12 2022
Response via : Initial Calibration

