




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030322\
Data File : BG052555.D
Acq On : 3 Mar 2022 15:27
Operator : CG/JU
Sample : N1745-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
H0AA6

Manual IntegrationsAPPROVED

Quant Time: Mar 04 00:01:44 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 22 17:32:12 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/04/2022
Supervised By :Yogesh Patel 03/07/2022

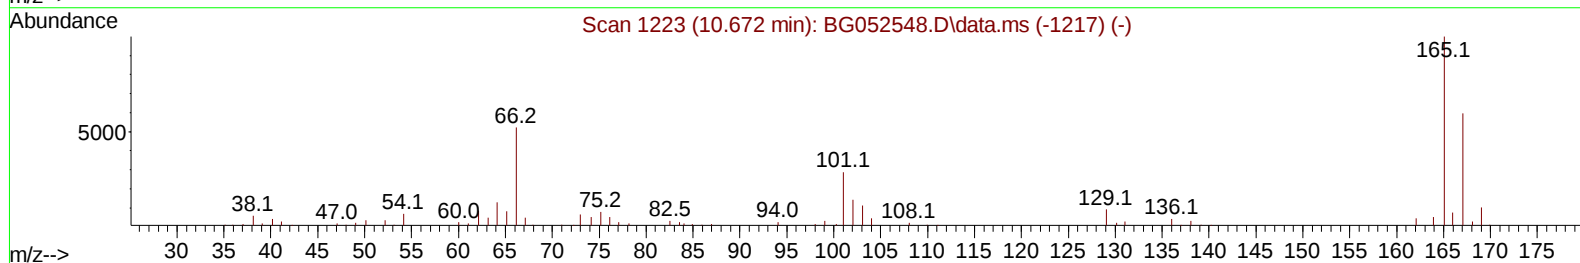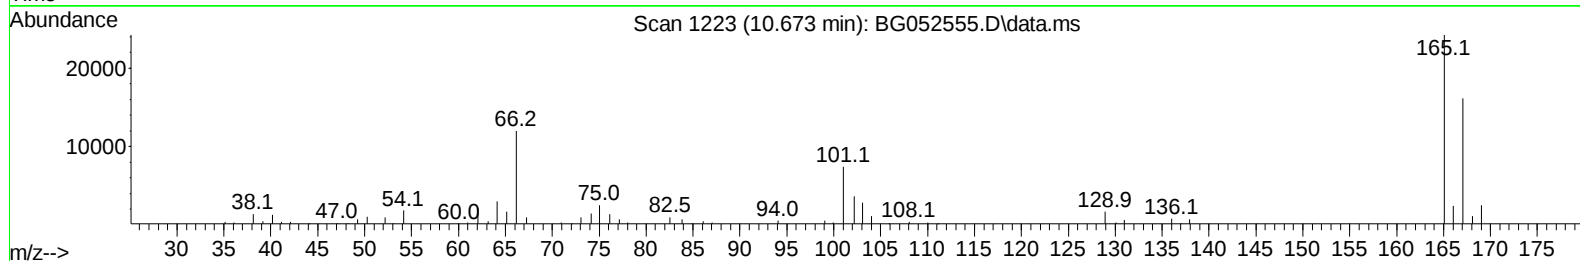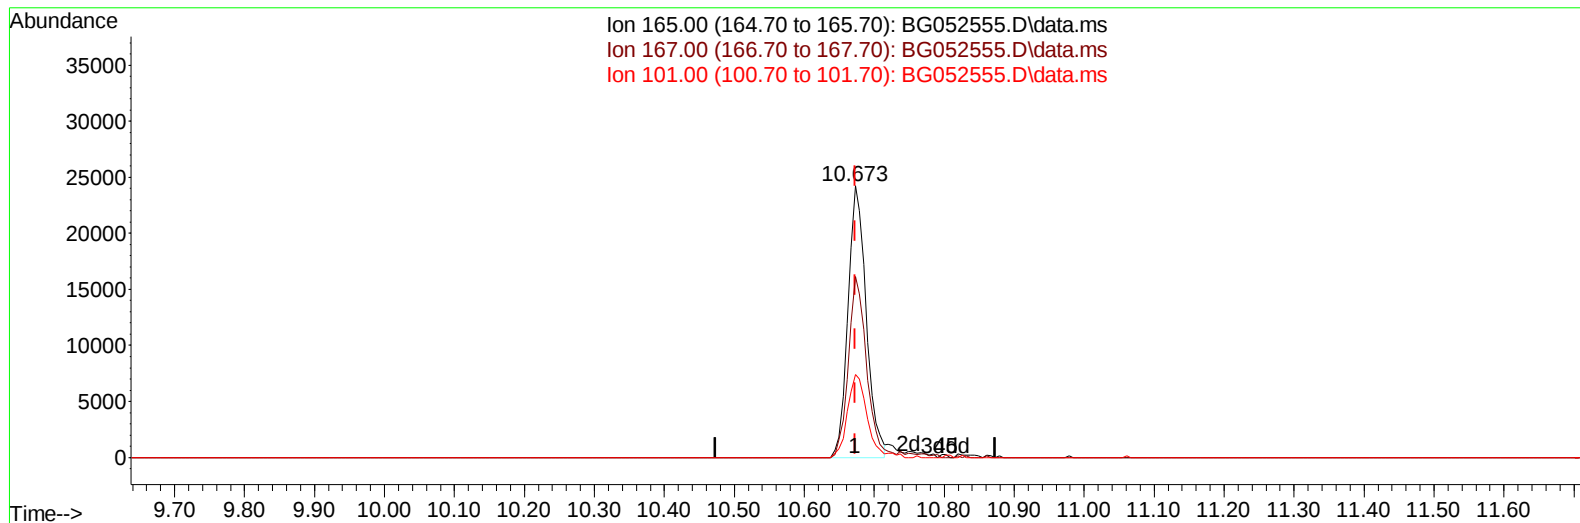

TIC: BG052555.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.673min (+ 0.000) 25.39 ng/u1

response 43726

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	64.30	66.62
101.00	34.40	30.66
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030322\
Data File : BG052555.D
Acq On : 3 Mar 2022 15:27
Operator : CG/JU
Sample : N1745-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
H0AA6

Manual IntegrationsAPPROVED

Quant Time: Mar 04 00:01:44 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 22 17:32:12 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/04/2022
Supervised By :Yogesh Patel 03/07/2022

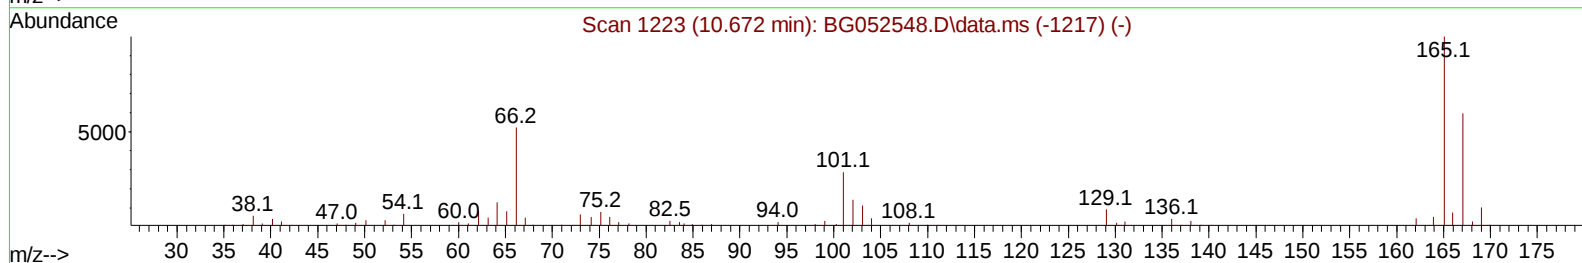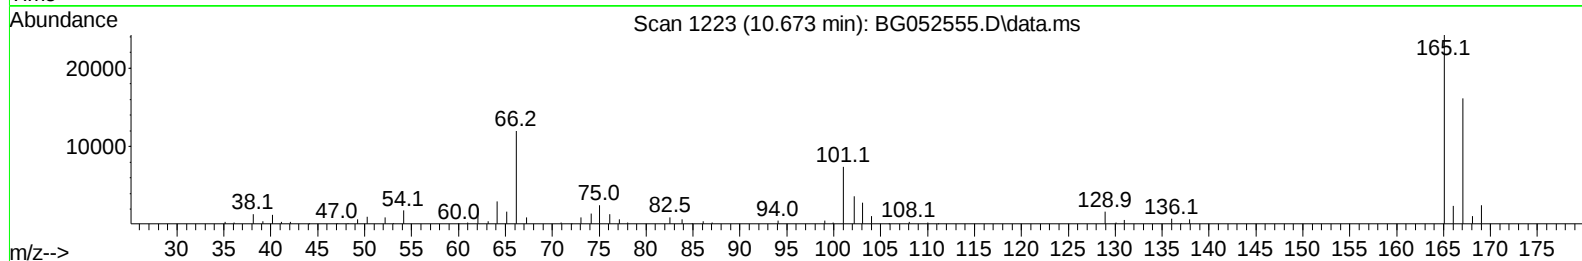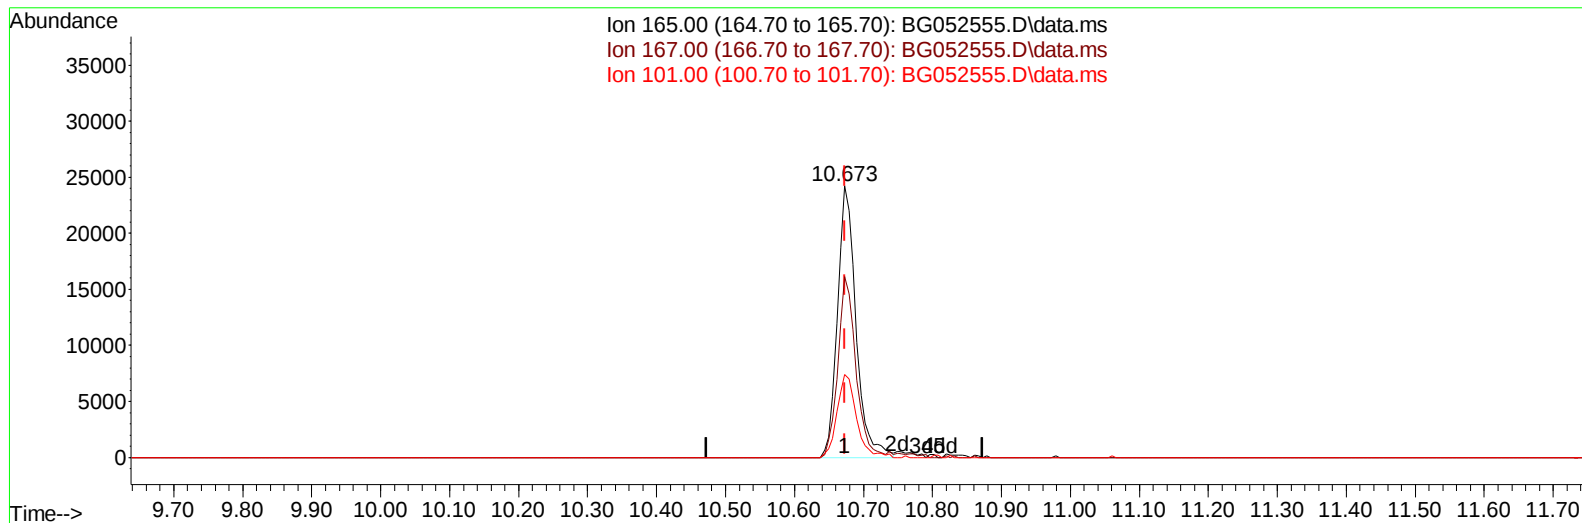

TIC: BG052555.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.673min (+ 0.000) 26.16 ng/ul m

response 45046

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	64.30	66.62
101.00	34.40	30.66
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030322\
Data File : BG052555.D
Acq On : 3 Mar 2022 15:27
Operator : CG/JU
Sample : N1745-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
H0AA6

Manual IntegrationsAPPROVED

Quant Time: Mar 04 00:01:44 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 22 17:32:12 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/04/2022
Supervised By :Yogesh Patel 03/07/2022

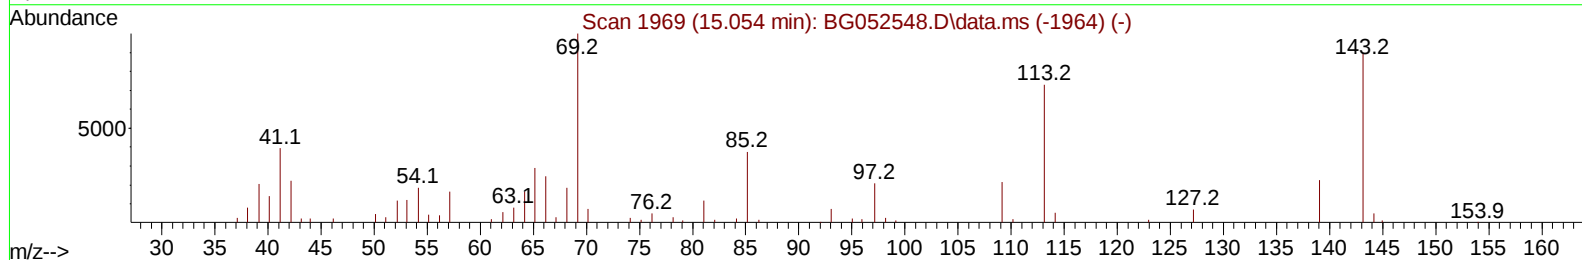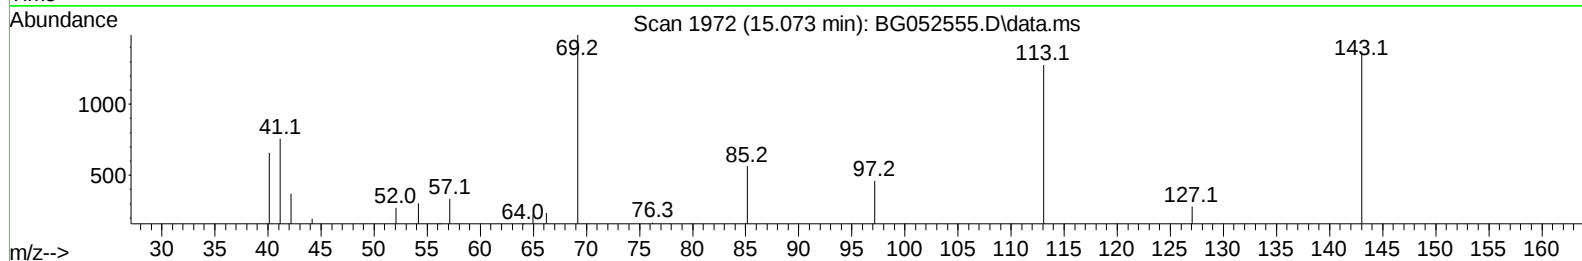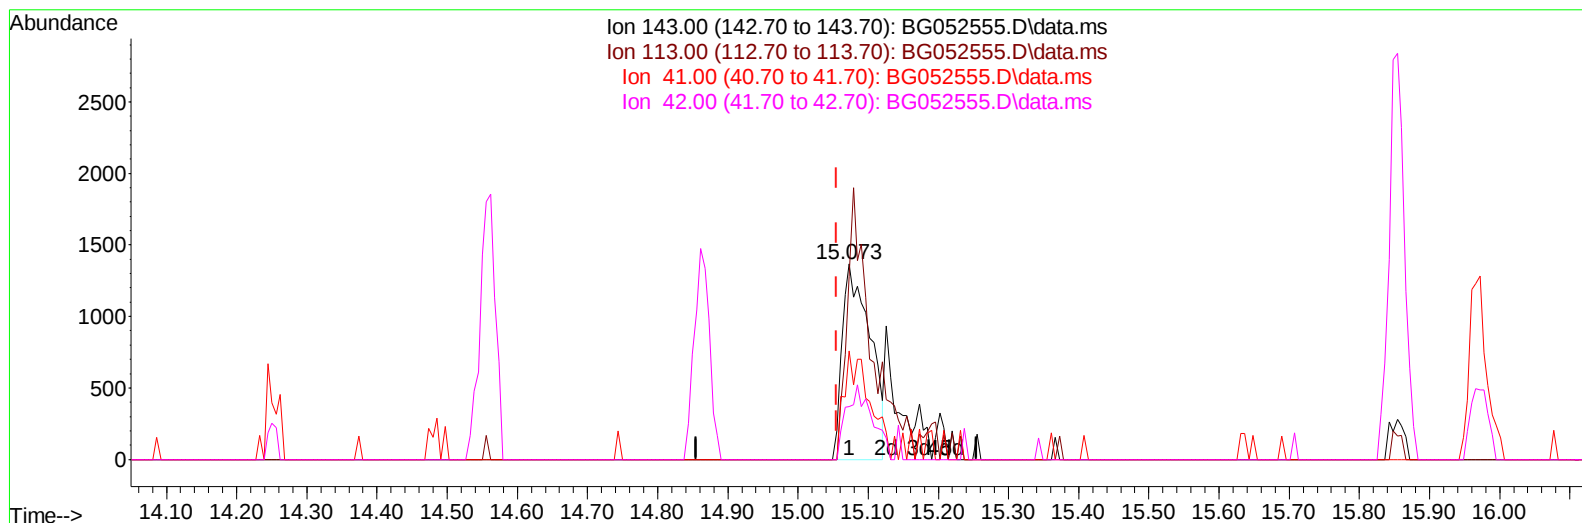

TIC: BG052555.D\data.ms

(54) 4-Nitrophenol-d4 (S)

15.073min (+ 0.018) 3.91 ng/u1

response 3754

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	80.30	93.41
41.00	44.40	55.42#
42.00	29.70	26.94




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030322\
Data File : BG052555.D
Acq On : 3 Mar 2022 15:27
Operator : CG/JU
Sample : N1745-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
H0AA6

Manual IntegrationsAPPROVED

Quant Time: Mar 04 00:01:44 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 22 17:32:12 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/04/2022
Supervised By :Yogesh Patel 03/07/2022

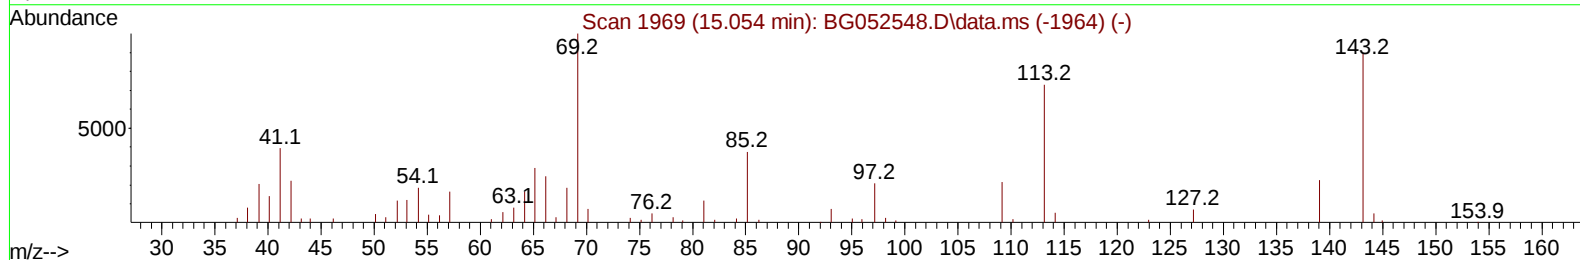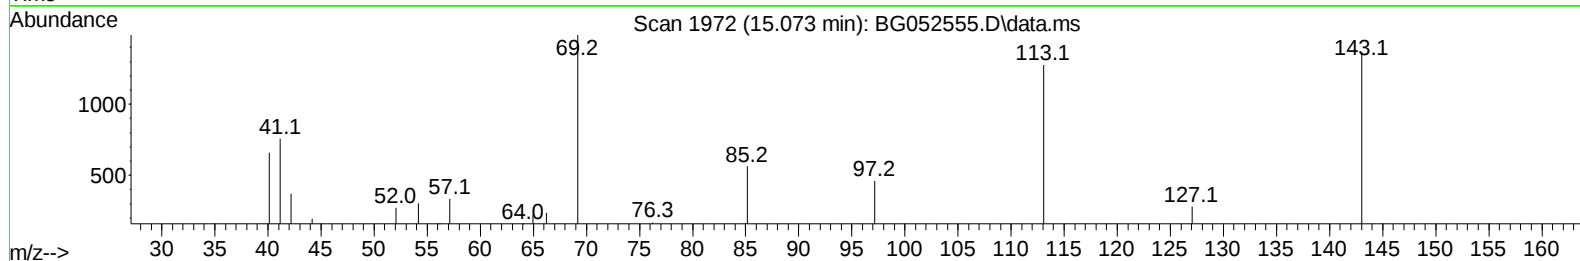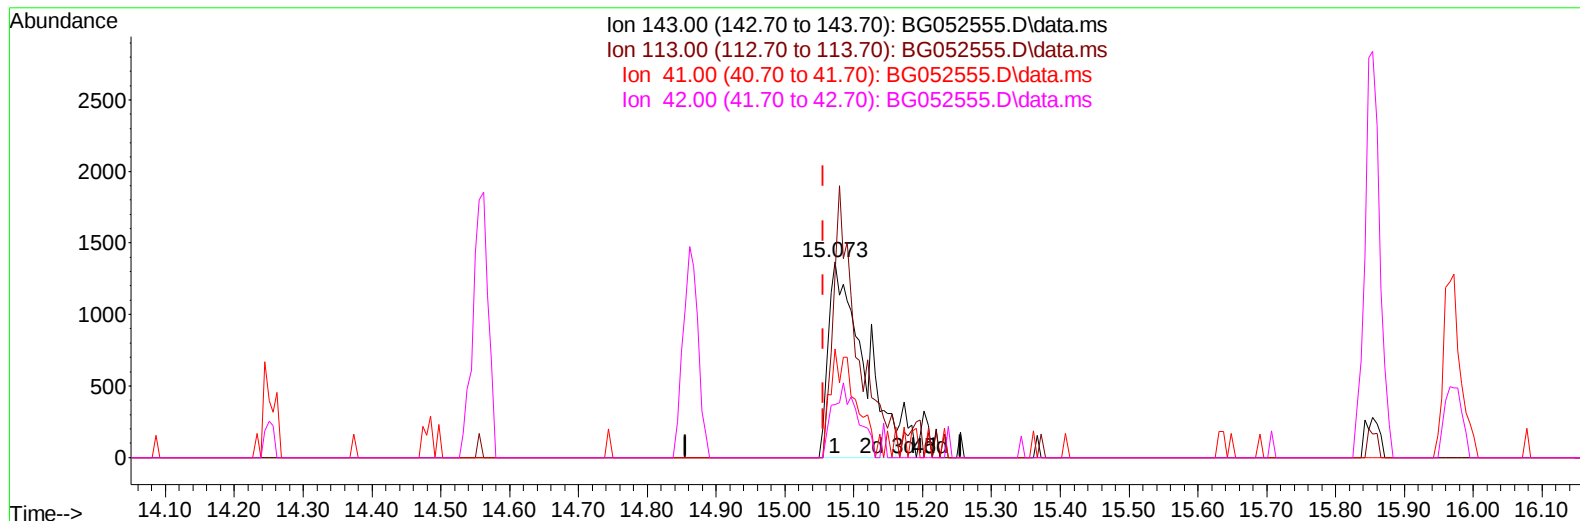

TIC: BG052555.D\data.ms

(54) 4-Nitrophenol-d4 (S)

15.073min (+ 0.018) 4.99 ng/ul m

response 4790

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	80.30	93.41
41.00	44.40	55.42#
42.00	29.70	26.94

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030322\
 Data File : BG052555.D
 Acq On : 3 Mar 2022 15:27
 Operator : CG/JU
 Sample : N1745-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 H0AA6

Manual IntegrationsAPPROVED

Quant Time: Mar 04 00:01:44 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 22 17:32:12 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/04/2022
 Supervised By :Yogesh Patel 03/07/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.217	152	22317	20.000	ng/ul	0.00
20) Naphthalene-d8	11.055	136	98894	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.861	164	74322	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.611	188	191003	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.928	240	200142	20.000	ng/ul	# 0.00
88) Perylene-d12	25.394	264	199555	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.547	96	2138	3.758	ng/uL	0.00
4) Pyridine-d5	3.982	84	10569	6.158	ng/ul	0.00
7) Phenol-d5	7.366	99	14890	7.036	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.524	67	40101	32.426	ng/ul	0.00
11) 2-Chlorophenol-d4	7.747	132	36413	24.498	ng/ul	0.00
15) 4-Methylphenol-d8	8.928	113	25327	15.382	ng/ul	0.00
21) Nitrobenzene-d5	9.392	128	26072	30.925	ng/ul	0.00
24) 2-Nitrophenol-d4	10.127	143	27437	29.712	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.673	165	45046m	26.158	ng/ul	0.00
31) 4-Chloroaniline-d4	11.184	131	56664	23.744	ng/ul	0.00
46) Dimethylphthalate-d6	14.250	166	216935	35.905	ng/ul	0.00
49) Acenaphthylene-d8	14.556	160	250559	33.593	ng/ul	0.00
54) 4-Nitrophenol-d4	15.073	143	4790m	4.987	ng/ul	0.02
60) Fluorene-d10	15.854	176	194300	36.607	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.966	200	30507	25.190	ng/ul	0.00
73) Anthracene-d10	17.710	188	363028	39.342	ng/ul	0.00
81) Pyrene-d10	19.996	212	449878	38.414	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.153	264	419474	39.181	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030322\
Data File : BG052555.D
Acq On : 3 Mar 2022 15:27
Operator : CG/JU
Sample : N1745-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
H0AA6

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/04/2022
Supervised By :Yogesh Patel 03/07/2022

Quant Time: Mar 04 00:01:44 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 22 17:32:12 2022
Response via : Initial Calibration

