




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030322\
Data File : BG052571.D
Acq On : 4 Mar 2022 8:55
Operator : CG/JU
Sample : PB143070BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK070

Manual IntegrationsAPPROVED

Quant Time: Mar 04 09:32:06 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 22 17:32:12 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/04/2022
Supervised By :Yogesh Patel 03/07/2022

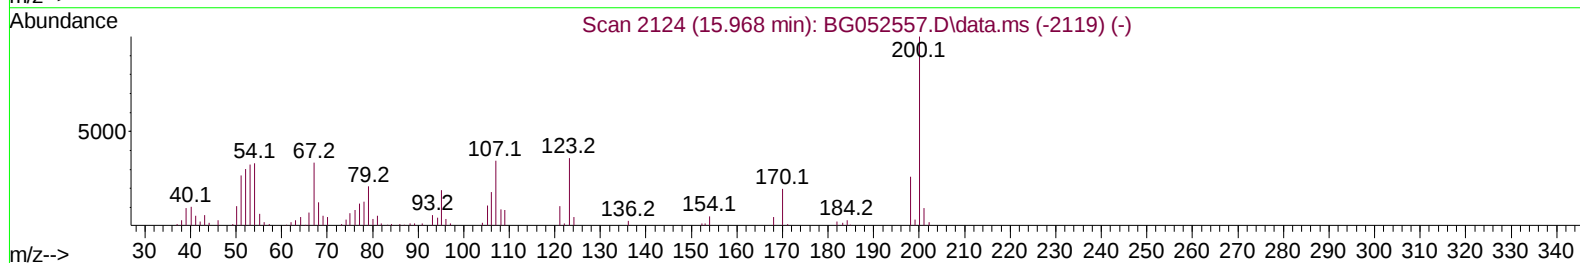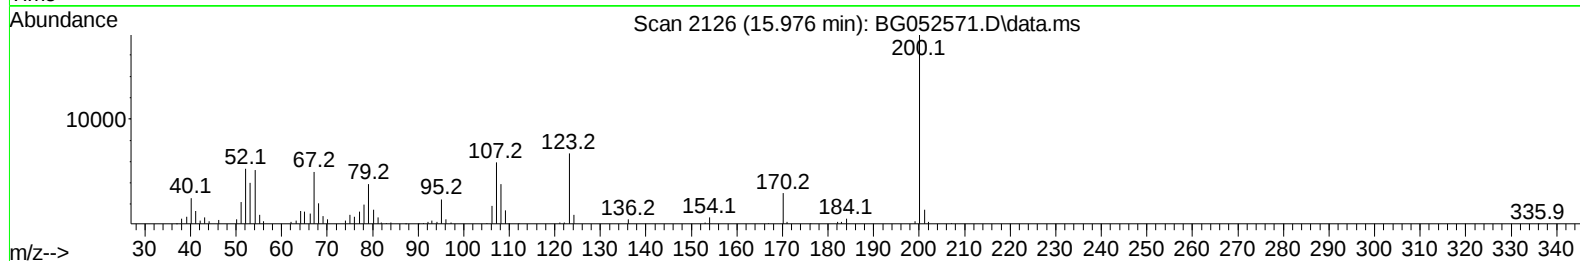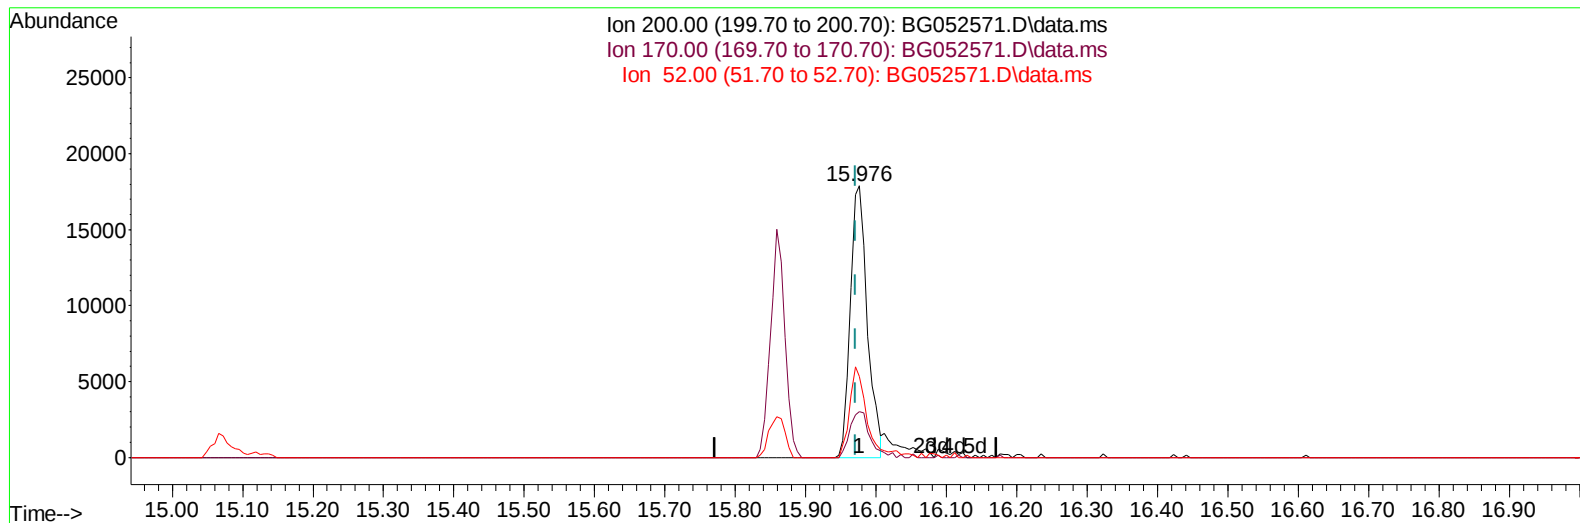

TIC: BG052571.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.976min (+ 0.005) 20.40 ng/u1

response 29788

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	19.80	16.92
52.00	47.40	29.73#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030322\
 Data File : BG052571.D
 Acq On : 4 Mar 2022 8:55
 Operator : CG/JU
 Sample : PB143070BL
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK070

Manual IntegrationsAPPROVED

Quant Time: Mar 04 09:32:06 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 22 17:32:12 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/04/2022
 Supervised By :Yogesh Patel 03/07/2022

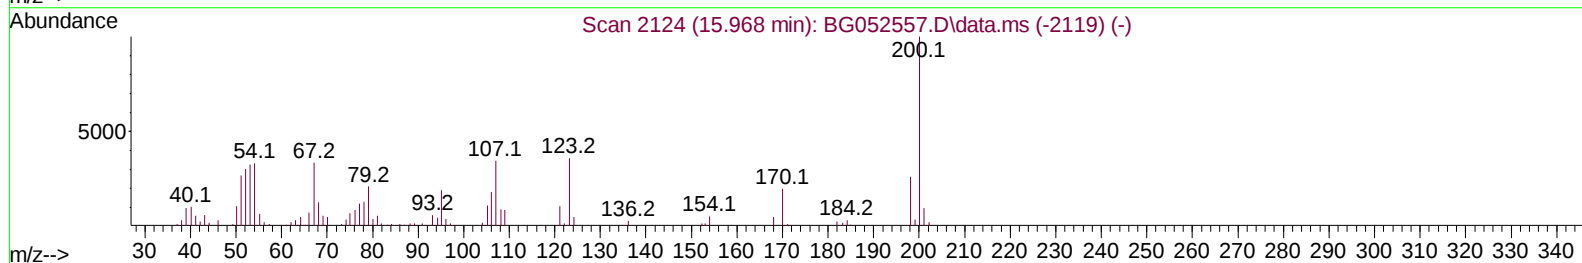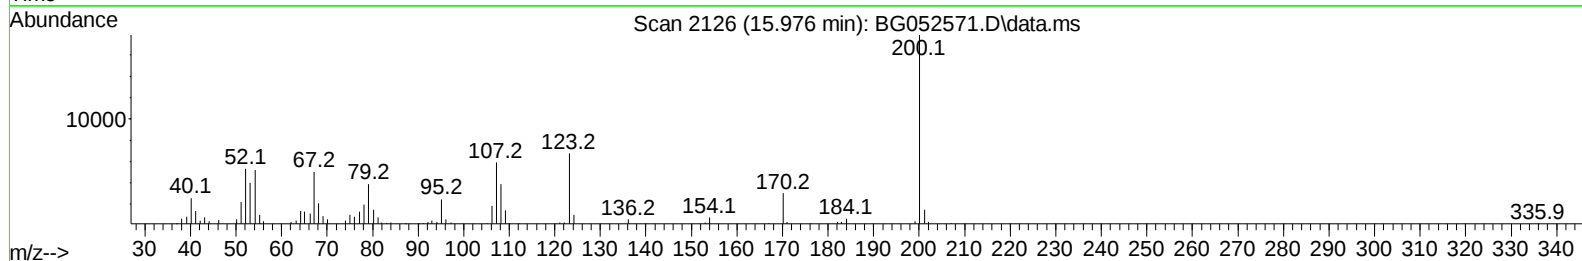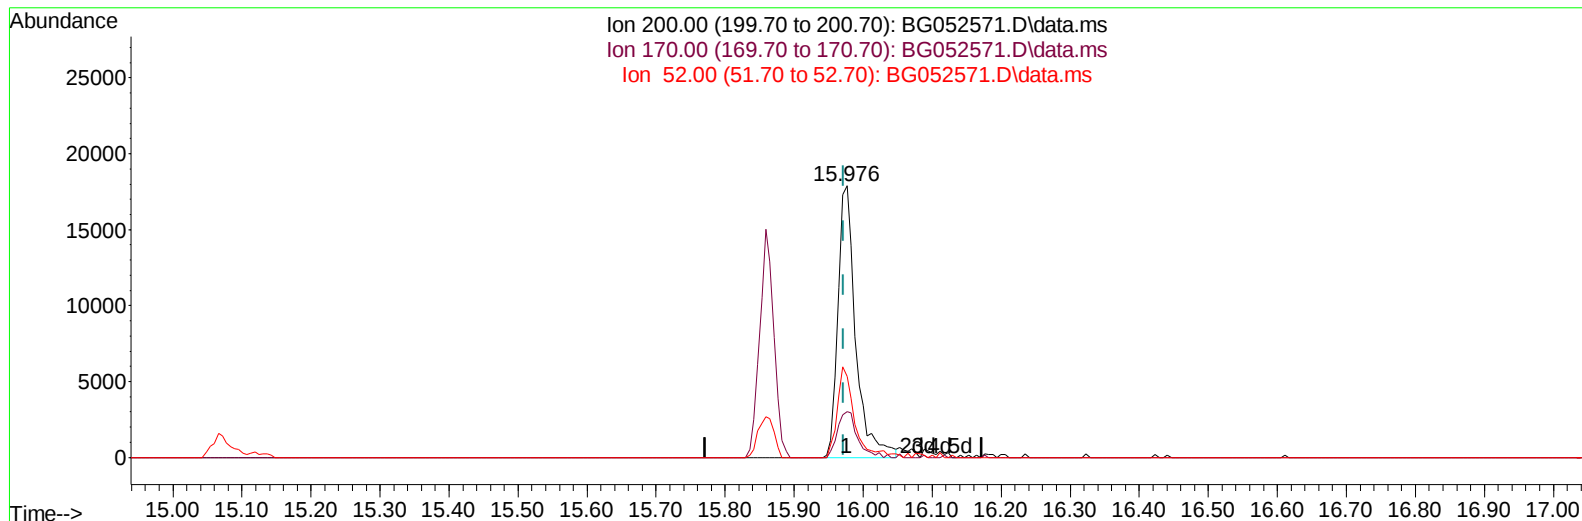

TIC: BG052571.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.976min (+ 0.005) 21.92 ng/ul m

response 32008

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	19.80	16.92
52.00	47.40	29.73#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030322\
 Data File : BG052571.D
 Acq On : 4 Mar 2022 8:55
 Operator : CG/JU
 Sample : PB143070BL
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK070

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/04/2022
 Supervised By :Yogesh Patel 03/07/2022

Quant Time: Mar 04 09:32:06 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 22 17:32:12 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.228	152	26765	20.000	ng/ul	0.00
20) Naphthalene-d8	11.065	136	117050	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.872	164	91795	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.615	188	230260	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.933	240	231864	20.000	ng/ul	# 0.00
88) Perylene-d12	25.399	264	225023	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.546	96	3664	5.370	ng/uL	0.00
4) Pyridine-d5	3.975	84	53967	26.218	ng/ul	0.00
7) Phenol-d5	7.376	99	69384	27.339	ng/ul	0.01
9) Bis-(2-Chloroethyl)eth...	7.541	67	43593	29.391	ng/ul	0.01
11) 2-Chlorophenol-d4	7.764	132	49196	27.598	ng/ul	0.02
15) 4-Methylphenol-d8	8.939	113	55311	28.010	ng/ul	0.00
21) Nitrobenzene-d5	9.403	128	27885	27.945	ng/ul	0.00
24) 2-Nitrophenol-d4	10.137	143	31708	29.011	ng/ul	0.01
28) 2,4-Dichlorophenol-d3	10.690	165	54417	26.698	ng/ul	0.02
31) 4-Chloroaniline-d4	11.195	131	75711	26.805	ng/ul	0.00
46) Dimethylphthalate-d6	14.261	166	221139	29.634	ng/ul	0.00
49) Acenaphthylene-d8	14.567	160	259889	28.212	ng/ul	0.00
54) 4-Nitrophenol-d4	15.066	143	27281	22.997	ng/ul	0.01
60) Fluorene-d10	15.859	176	187895	28.662	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.976	200	32008m	21.923	ng/ul	0.00
73) Anthracene-d10	17.715	188	328210	29.505	ng/ul	0.00
81) Pyrene-d10	19.995	212	413931	30.509	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.152	264	372436	30.851	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030322\
Data File : BG052571.D
Acq On : 4 Mar 2022 8:55
Operator : CG/JU
Sample : PB143070BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK070

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/04/2022
Supervised By :Yogesh Patel 03/07/2022

Quant Time: Mar 04 09:32:06 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 22 17:32:12 2022
Response via : Initial Calibration

