

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030322\
 Data File : BG052550.D
 Acq On : 3 Mar 2022 12:13
 Operator : CG/JU
 Sample : PB143054BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK054

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052550.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.541	3	9	13	rBV3	7872	11424	1.20%	0.134%
2	3.970	79	82	98	rBV	69853	128496	13.44%	1.503%
3	4.322	139	142	146	rBV4	1974	2696	0.28%	0.032%
4	4.598	188	189	194	rBV2	1024	1630	0.17%	0.019%
5	4.745	211	214	217	rVB2	989	1293	0.14%	0.015%
6	5.380	321	322	327	rVB3	1167	1217	0.13%	0.014%
7	5.468	332	337	340	rBV3	814	1727	0.18%	0.020%
8	7.365	651	660	670	rBV	102430	171870	17.98%	2.011%
9	7.524	677	687	696	rBV	76369	128147	13.41%	1.499%
10	7.665	708	711	716	rBV3	923	1466	0.15%	0.017%
11	7.747	718	725	733	rVV	92109	159044	16.64%	1.861%
12	8.217	799	805	815	rBV	81603	138604	14.50%	1.622%
13	8.716	886	890	893	rBV	979	1703	0.18%	0.020%
14	8.928	919	926	936	rBV	117554	209510	21.92%	2.451%
15	9.392	997	1005	1013	rBV	98122	178532	18.68%	2.089%
16	9.480	1017	1020	1023	rVB2	721	1134	0.12%	0.013%
17	10.120	1121	1129	1139	rBV	81960	150231	15.72%	1.758%
18	10.672	1217	1223	1239	rBV	107470	211295	22.11%	2.472%
19	11.054	1280	1288	1297	rVB	123709	217428	22.75%	2.544%
20	11.184	1303	1310	1320	rBV2	117346	223440	23.38%	2.614%
21	12.634	1553	1557	1562	rVB3	1835	2823	0.30%	0.033%
22	14.250	1826	1832	1840	rBV	289830	426236	44.59%	4.987%
23	14.561	1878	1885	1894	rBV	294240	478882	50.10%	5.602%
24	14.867	1930	1937	1945	rBV	218951	349873	36.60%	4.093%
25	15.061	1964	1970	1984	rBV2	71505	166466	17.42%	1.947%
26	15.854	2098	2105	2114	rBV	415414	615057	64.35%	7.196%
27	15.971	2119	2125	2138	rBV	96925	168267	17.60%	1.969%
28	16.095	2143	2146	2151	rVB3	2167	2834	0.30%	0.033%
29	17.399	2363	2368	2373	rBV4	1451	2083	0.22%	0.024%
30	17.610	2398	2404	2414	rBV	311490	488743	51.13%	5.718%
31	17.716	2414	2422	2433	rBV	472269	755191	79.01%	8.835%
32	17.957	2457	2463	2465	rBV2	1228	1831	0.19%	0.021%
33	19.372	2702	2704	2708	rVB2	1052	1357	0.14%	0.016%
34	19.490	2722	2724	2726	rVB2	1455	1388	0.15%	0.016%
35	19.519	2726	2729	2730	rBV	1355	1343	0.14%	0.016%
36	19.560	2732	2736	2742	rVB4	7861	12015	1.26%	0.141%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030322\
 Data File : BG052550.D
 Acq On : 3 Mar 2022 12:13
 Operator : CG/JU
 Sample : PB143054BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK054

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
 Title : SVOA CALIBRATION

37	19.631	2745	2748	2752	rVV2	5016	7393	0.77%	0.086%
38	19.995	2802	2810	2817	rVV	667821	955866	100.00%	11.183%
39	20.271	2852	2857	2859	rBV5	1382	1834	0.19%	0.021%
40	20.371	2870	2874	2876	rBV3	1732	2336	0.24%	0.027%

41	20.559	2905	2906	2909	rBV3	1357	1427	0.15%	0.017%
42	21.035	2986	2987	2989	rBV2	2108	1241	0.13%	0.015%
43	21.193	3012	3014	3018	rBV5	1803	1813	0.19%	0.021%
44	21.270	3025	3027	3028	rBV2	1360	1126	0.12%	0.013%
45	21.287	3028	3030	3033	rVB4	2515	2387	0.25%	0.028%

46	21.317	3033	3035	3036	rBV2	1709	1478	0.15%	0.017%
47	21.381	3045	3046	3048	rBV2	2427	2009	0.21%	0.024%
48	21.446	3055	3057	3059	rBV3	2345	2524	0.26%	0.030%
49	21.628	3085	3088	3092	rBV3	2897	5027	0.53%	0.059%
50	21.928	3133	3139	3149	rVB	306408	532706	55.73%	6.232%

51	22.028	3154	3156	3158	rBV3	1940	2207	0.23%	0.026%
52	22.210	3185	3187	3188	rBV2	1984	1419	0.15%	0.017%
53	22.474	3230	3232	3233	rBV3	2266	1397	0.15%	0.016%
54	22.603	3252	3254	3256	rBV3	2260	1974	0.21%	0.023%
55	22.750	3277	3279	3284	rVB5	3698	4540	0.47%	0.053%

56	23.197	3353	3355	3358	rVB3	2900	2138	0.22%	0.025%
57	23.467	3400	3401	3402	rBV2	2416	1224	0.13%	0.014%
58	23.496	3404	3406	3407	rBV2	4952	3553	0.37%	0.042%
59	24.090	3505	3507	3509	rBV3	3164	3245	0.34%	0.038%
60	24.372	3550	3555	3561	rVB7	8710	19309	2.02%	0.226%

61	24.818	3629	3631	3635	rVB4	2286	2269	0.24%	0.027%
62	25.153	3678	3688	3704	rVB	294976	871332	91.16%	10.194%
63	25.394	3718	3729	3742	rBV2	188021	562737	58.87%	6.583%
64	25.570	3757	3759	3760	rBV2	1980	1444	0.15%	0.017%
65	25.746	3787	3789	3790	rBV	2399	1704	0.18%	0.020%

66	26.063	3841	3843	3844	rBV2	2362	1984	0.21%	0.023%
67	26.140	3855	3856	3859	rBV3	2745	2566	0.27%	0.030%
68	26.198	3864	3866	3867	rBV2	2531	1302	0.14%	0.015%
69	26.592	3930	3933	3934	rBV3	3941	3757	0.39%	0.044%
70	26.633	3934	3940	3952	rVB8	12873	40932	4.28%	0.479%

71	27.127	4022	4024	4026	rBV3	2414	2236	0.23%	0.026%
72	27.397	4068	4070	4072	rBV3	2768	2201	0.23%	0.026%
73	27.573	4098	4100	4102	rBV3	2892	2375	0.25%	0.028%
74	27.608	4104	4106	4110	rVB5	3299	3844	0.40%	0.045%
75	27.773	4132	4134	4137	rBV3	2355	2460	0.26%	0.029%

76	27.802	4137	4139	4140	rBV2	2791	1651	0.17%	0.019%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030322\
 Data File : BG052550.D
 Acq On : 3 Mar 2022 12:13
 Operator : CG/JU
 Sample : PB143054BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK054

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
 Title : SVOA CALIBRATION

77	28.090	4185	4188	4189	rBV3	3734	4414	0.46%	0.052%
78	28.108	4189	4191	4192	rBV2	5312	4663	0.49%	0.055%
79	28.184	4202	4204	4206	rBV3	2225	1781	0.19%	0.021%
80	28.501	4256	4258	4259	rBV	2833	1397	0.15%	0.016%
81	28.560	4266	4268	4269	rBV2	2219	1568	0.16%	0.018%
82	28.771	4302	4304	4307	rVB4	2598	1710	0.18%	0.020%
83	29.265	4386	4388	4391	rBV2	3050	3476	0.36%	0.041%
84	29.670	4455	4457	4460	rVB2	2591	1754	0.18%	0.021%
85	29.882	4488	4493	4494	rBV3	6447	8157	0.85%	0.095%
86	30.023	4515	4517	4518	rBV2	2526	1382	0.14%	0.016%
87	30.099	4528	4530	4531	rBV2	2330	1465	0.15%	0.017%
88	30.246	4554	4555	4557	rBV2	2530	1596	0.17%	0.019%
89	30.346	4570	4572	4573	rBV2	2381	1823	0.19%	0.021%
90	30.434	4585	4587	4590	rBV2	2469	2709	0.28%	0.032%
91	31.121	4702	4704	4707	rVB4	2934	2459	0.26%	0.029%
92	31.151	4707	4709	4710	rVB2	3476	1614	0.17%	0.019%
93	31.192	4714	4716	4721	rVB6	3849	4366	0.46%	0.051%
94	31.233	4721	4723	4724	rBV2	2314	1404	0.15%	0.016%
95	31.386	4745	4749	4753	rBV6	2206	3454	0.36%	0.040%
96	31.480	4763	4765	4771	rVB5	2985	4160	0.44%	0.049%
97	31.914	4835	4839	4841	rBV3	2444	3627	0.38%	0.042%
98	32.002	4851	4854	4855	rBV3	3838	4120	0.43%	0.048%
99	32.126	4873	4875	4876	rVB2	3826	2282	0.24%	0.027%
100	32.484	4932	4936	4937	rBV4	2127	2170	0.23%	0.025%




Sum of corrected areas: 8547794

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030322\
Data File : BG052550.D
Acq On : 3 Mar 2022 12:13
Operator : CG/JU
Sample : PB143054BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK054

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

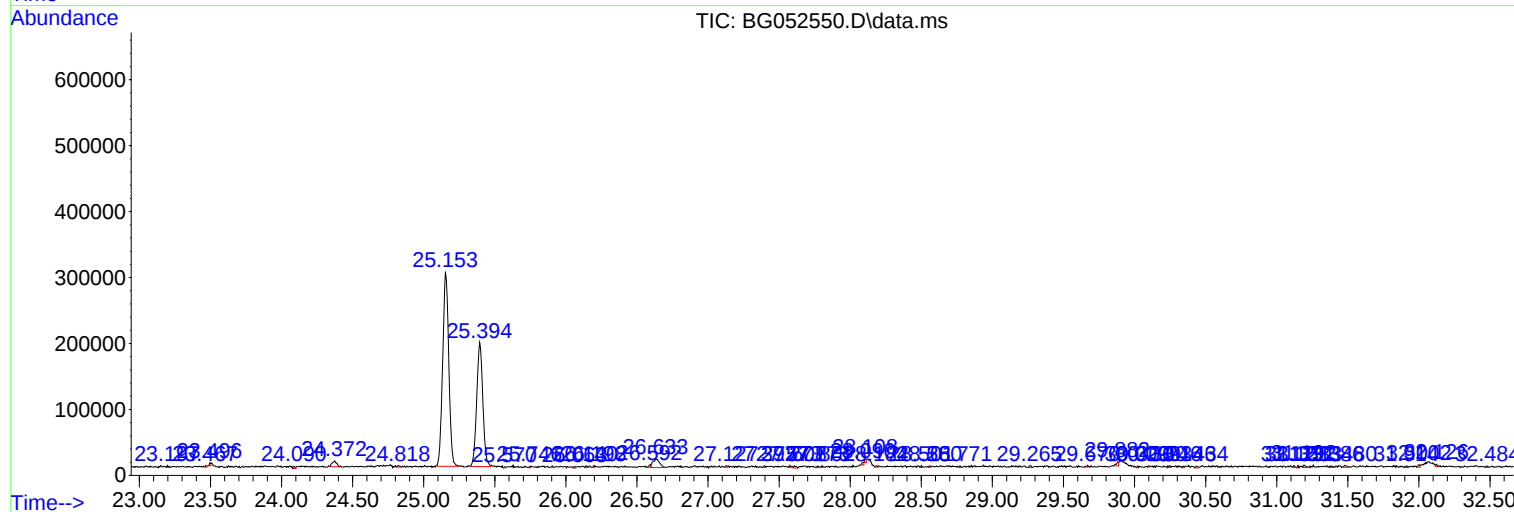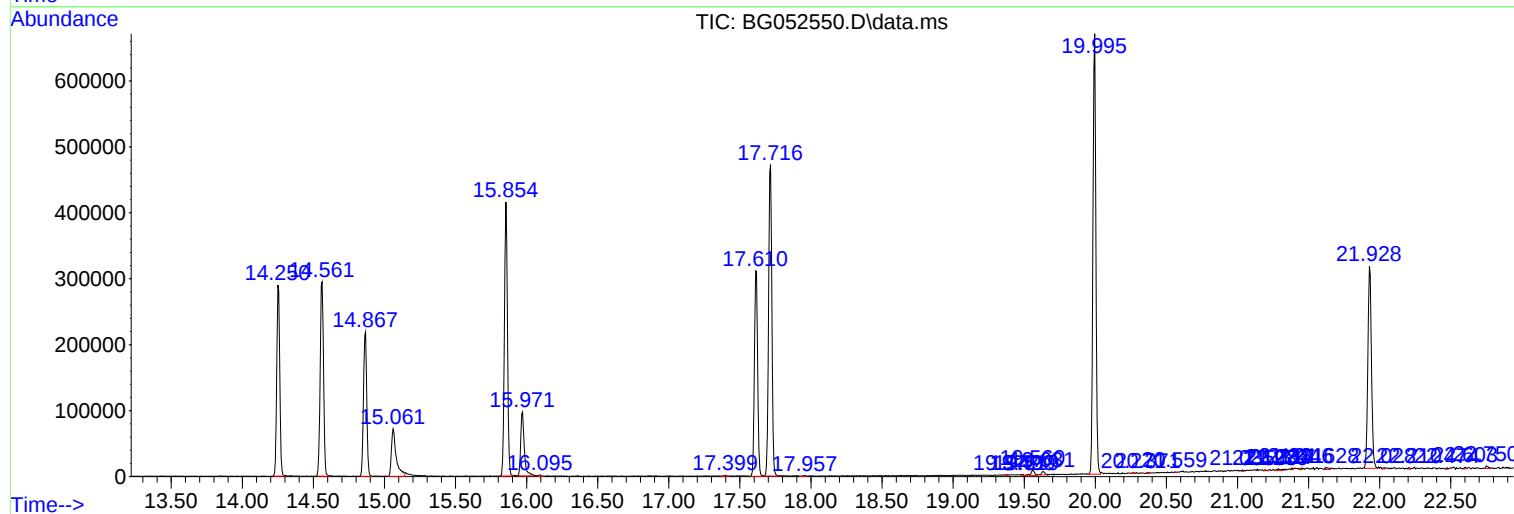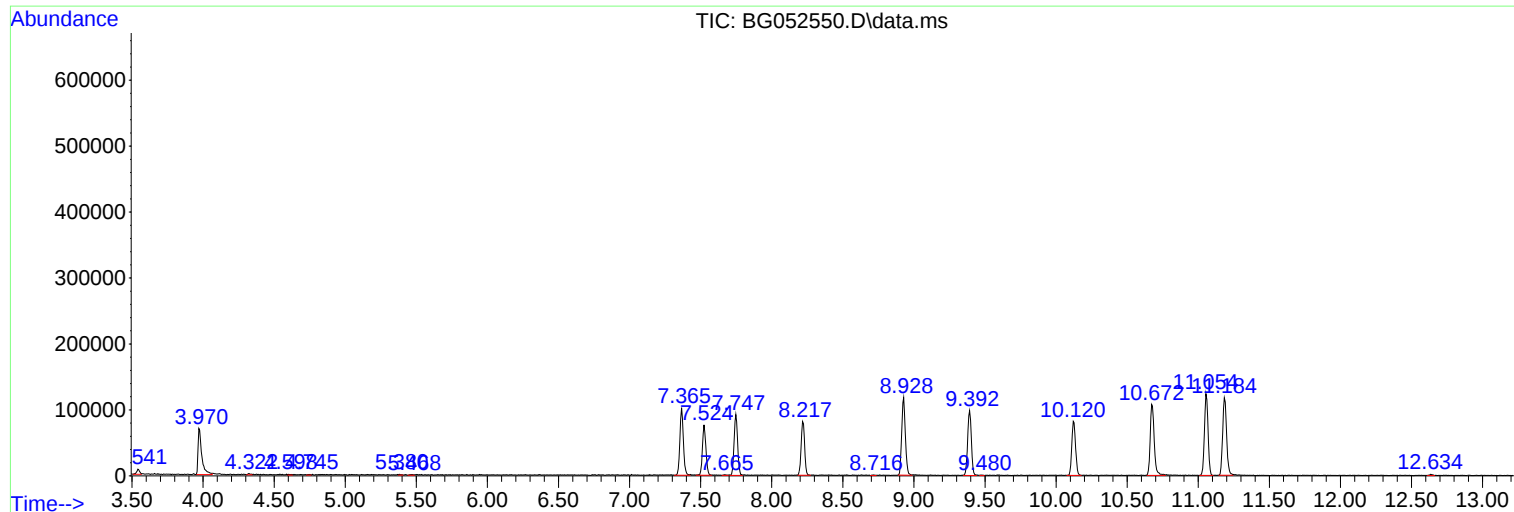

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030322\
Data File : BG052550.D
Acq On : 3 Mar 2022 12:13
Operator : CG/JU
Sample : PB143054BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK054

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030322\
Data File : BG052550.D
Acq On : 3 Mar 2022 12:13
Operator : CG/JU
Sample : PB143054BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK054

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc