

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030322\
 Data File : BG052553.D
 Acq On : 3 Mar 2022 14:09
 Operator : CG/JU
 Sample : N1745-07
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 H0AA7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052553.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.541	6	9	15	rVV2	5250	6557	0.62%	0.078%
2	3.981	81	84	95	rBV	16650	30454	2.86%	0.364%
3	4.322	140	142	146	rVB	1483	1888	0.18%	0.023%
4	4.921	241	244	247	rBV3	963	1202	0.11%	0.014%
5	6.513	512	515	518	rBV2	1047	1598	0.15%	0.019%
6	7.371	655	661	668	rBV2	24273	43364	4.07%	0.518%
7	7.524	681	687	696	rVB	83048	141116	13.24%	1.685%
8	7.747	718	725	733	rVV	80659	140063	13.14%	1.672%
9	7.823	737	738	743	rVB2	1239	1297	0.12%	0.015%
10	8.217	798	805	815	rVB	79466	138854	13.02%	1.658%
11	8.928	919	926	936	rBV	69445	121129	11.36%	1.446%
12	9.392	997	1005	1014	rBV	107751	194260	18.22%	2.320%
13	9.797	1072	1074	1078	rBV	980	1356	0.13%	0.016%
14	10.126	1122	1130	1140	rVB	87599	157772	14.80%	1.884%
15	10.672	1216	1223	1236	rBV	113465	213159	19.99%	2.545%
16	11.054	1281	1288	1295	rBV	116403	212044	19.89%	2.532%
17	11.183	1304	1310	1321	rBV	103975	197027	18.48%	2.353%
18	12.634	1553	1557	1561	rVB4	2001	3127	0.29%	0.037%
19	14.256	1826	1833	1846	rBV	295096	449021	42.12%	5.361%
20	14.561	1877	1885	1892	rBV	326599	507206	47.57%	6.056%
21	14.861	1929	1936	1945	rBV	213244	339812	31.87%	4.057%
22	15.072	1967	1972	1980	rBV4	11765	27859	2.61%	0.333%
23	15.642	2063	2069	2075	rBV3	2124	3692	0.35%	0.044%
24	15.854	2098	2105	2112	rBV	430620	673598	63.18%	8.043%
25	15.971	2119	2125	2134	rBV	109651	189252	17.75%	2.260%
26	16.100	2144	2147	2150	rVB2	2659	2868	0.27%	0.034%
27	16.194	2159	2163	2167	rBV3	1215	1950	0.18%	0.023%
28	17.340	2356	2358	2363	rVB5	1401	1732	0.16%	0.021%
29	17.393	2365	2367	2370	rBV2	961	1136	0.11%	0.014%
30	17.498	2382	2385	2392	rVB4	3226	3955	0.37%	0.047%
31	17.616	2396	2405	2413	rVV	294129	463286	43.45%	5.532%
32	17.710	2415	2421	2432	rVV	554457	868900	81.50%	10.375%
33	17.810	2435	2438	2441	rVB3	1417	1947	0.18%	0.023%
34	17.868	2444	2448	2452	rVV3	2273	3190	0.30%	0.038%
35	17.992	2467	2469	2475	rVB	1113	1664	0.16%	0.020%
36	18.256	2510	2514	2518	rVB	7531	8521	0.80%	0.102%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030322\
 Data File : BG052553.D
 Acq On : 3 Mar 2022 14:09
 Operator : CG/JU
 Sample : N1745-07
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 H0AA7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
 Title : SVOA CALIBRATION

37	18.550	2559	2564	2568	rBV2	2624	4597	0.43%	0.055%
38	19.249	2678	2683	2684	rBV2	1314	1680	0.16%	0.020%
39	19.325	2695	2696	2700	rBV4	1565	1651	0.15%	0.020%
40	19.390	2704	2707	2708	rBV	1866	1475	0.14%	0.018%

41	19.408	2708	2710	2714	rVB3	2995	3833	0.36%	0.046%
42	19.560	2732	2736	2741	rVB3	8262	12351	1.16%	0.147%
43	19.631	2744	2748	2752	rBV2	7447	11033	1.03%	0.132%
44	19.719	2762	2763	2766	rBV2	1273	1275	0.12%	0.015%
45	19.754	2766	2769	2772	rVV5	826	1175	0.11%	0.014%

46	19.878	2786	2790	2793	rBV6	2753	4528	0.42%	0.054%
47	19.930	2797	2799	2803	rBV3	1707	2222	0.21%	0.027%
48	19.995	2803	2810	2818	rBV	743377	1066173	100.00%	12.730%
49	20.441	2883	2886	2888	rVB3	1361	1479	0.14%	0.018%
50	20.471	2888	2891	2893	rBV3	1604	2066	0.19%	0.025%

51	20.541	2901	2903	2906	rVV2	1251	1453	0.14%	0.017%
52	20.641	2918	2920	2924	rVV3	1956	1768	0.17%	0.021%
53	20.712	2929	2932	2933	rBV2	1167	1241	0.12%	0.015%
54	20.812	2948	2949	2951	rBV2	1337	1238	0.12%	0.015%
55	20.876	2958	2960	2965	rBV4	1713	2281	0.21%	0.027%

56	21.111	2996	3000	3003	rBV6	1745	2409	0.23%	0.029%
57	21.928	3133	3139	3149	rVB2	296914	499671	46.87%	5.966%
58	22.104	3167	3169	3171	rBV2	1898	1402	0.13%	0.017%
59	22.374	3214	3215	3217	rVB2	3063	1309	0.12%	0.016%
60	22.468	3229	3231	3233	rVB3	3259	2276	0.21%	0.027%

61	22.492	3233	3235	3236	rBV2	2453	1941	0.18%	0.023%
62	22.750	3277	3279	3282	rBV4	2618	1947	0.18%	0.023%
63	22.879	3299	3301	3302	rBV2	2753	2051	0.19%	0.024%
64	22.950	3311	3313	3314	rBV	2148	1521	0.14%	0.018%
65	23.073	3333	3334	3335	rBV	2962	1413	0.13%	0.017%

66	23.796	3455	3457	3459	rBV3	2011	1354	0.13%	0.016%
67	23.978	3487	3488	3491	rBV3	2477	1588	0.15%	0.019%
68	24.289	3539	3541	3544	rVB4	2294	2388	0.22%	0.029%
69	24.366	3551	3554	3556	rBV3	3462	4870	0.46%	0.058%
70	24.448	3566	3568	3570	rVB2	2254	2107	0.20%	0.025%

71	24.589	3590	3592	3593	rBV2	2282	2013	0.19%	0.024%
72	24.659	3602	3604	3605	rBV2	2561	1620	0.15%	0.019%
73	24.724	3613	3615	3618	rVB3	2447	1929	0.18%	0.023%
74	24.877	3639	3641	3642	rBV2	1875	1170	0.11%	0.014%
75	25.153	3676	3688	3704	rBV2	329659	997307	93.54%	11.908%

76	25.388	3718	3728	3741	rBV3	162879	510239	47.86%	6.092%
----	--------	------	------	------	------	--------	--------	--------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030322\
 Data File : BG052553.D
 Acq On : 3 Mar 2022 14:09
 Operator : CG/JU
 Sample : N1745-07
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 H0AA7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
 Title : SVOA CALIBRATION

77	25.629	3767	3769	3770	rVB2	2802	1559	0.15%	0.019%
78	25.658	3772	3774	3775	rVV2	2641	1594	0.15%	0.019%
79	26.016	3831	3835	3836	rBV3	2756	4213	0.40%	0.050%
80	26.604	3932	3935	3936	rBV3	2611	3065	0.29%	0.037%
81	26.798	3966	3968	3971	rBV4	1916	2329	0.22%	0.028%
82	26.862	3978	3979	3981	rBV2	3046	1908	0.18%	0.023%
83	26.991	3999	4001	4002	rBV2	2280	1765	0.17%	0.021%
84	27.279	4049	4050	4051	rBV	3239	1669	0.16%	0.020%
85	27.550	4094	4096	4097	rBV2	2563	2038	0.19%	0.024%
86	28.272	4215	4219	4221	rBV5	2726	3971	0.37%	0.047%
87	29.512	4428	4430	4431	rBV2	2378	2127	0.20%	0.025%
88	29.788	4474	4477	4478	rBV2	2447	2298	0.22%	0.027%
89	30.075	4524	4526	4528	rBV	1888	1588	0.15%	0.019%
90	30.440	4586	4588	4591	rVB4	2402	2079	0.19%	0.025%
91	30.534	4602	4604	4605	rBV2	1823	1484	0.14%	0.018%
92	30.733	4636	4638	4640	rBV3	2441	2587	0.24%	0.031%
93	31.315	4736	4737	4738	rBV	2712	1214	0.11%	0.014%
94	31.509	4768	4770	4771	rBV	1933	1234	0.12%	0.015%
95	31.585	4781	4783	4784	rBV2	2683	1836	0.17%	0.022%
96	31.615	4787	4788	4790	rVB2	2914	1694	0.16%	0.020%
97	31.720	4804	4806	4808	rVV3	2066	1614	0.15%	0.019%
98	31.744	4808	4810	4812	rVB3	2180	1566	0.15%	0.019%
99	31.902	4835	4837	4840	rVB3	2756	1398	0.13%	0.017%
100	32.020	4854	4857	4860	rBV4	3898	6310	0.59%	0.075%




Sum of corrected areas: 8375040

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030322\
Data File : BG052553.D
Acq On : 3 Mar 2022 14:09
Operator : CG/JU
Sample : N1745-07
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
H0AA7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

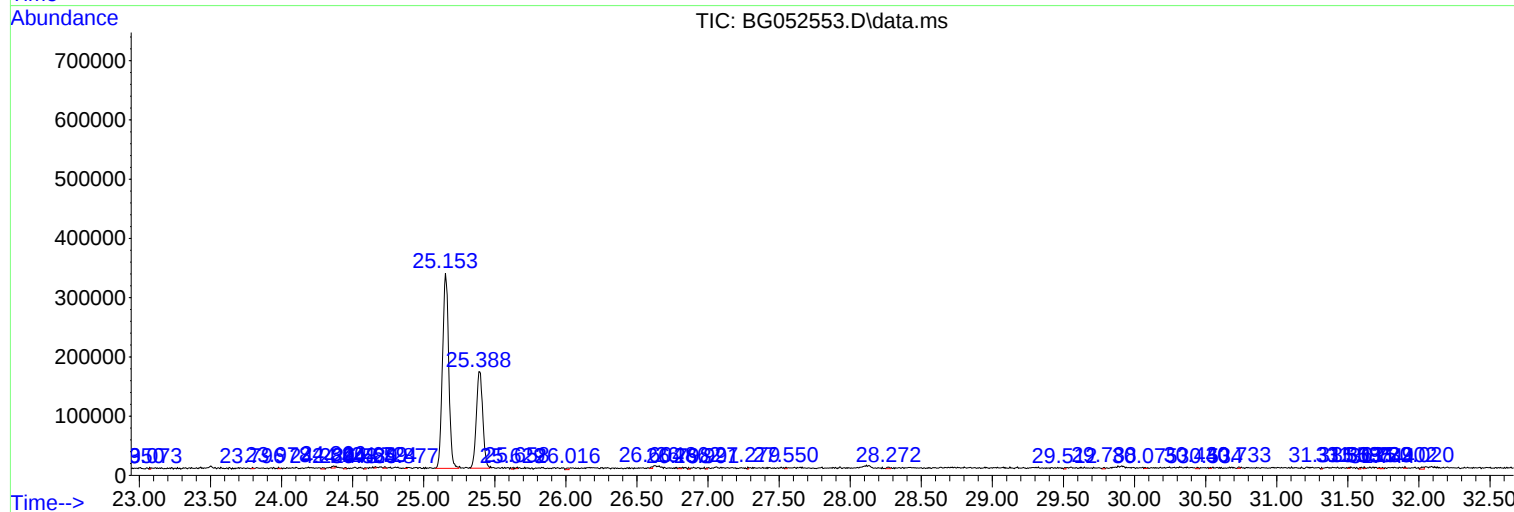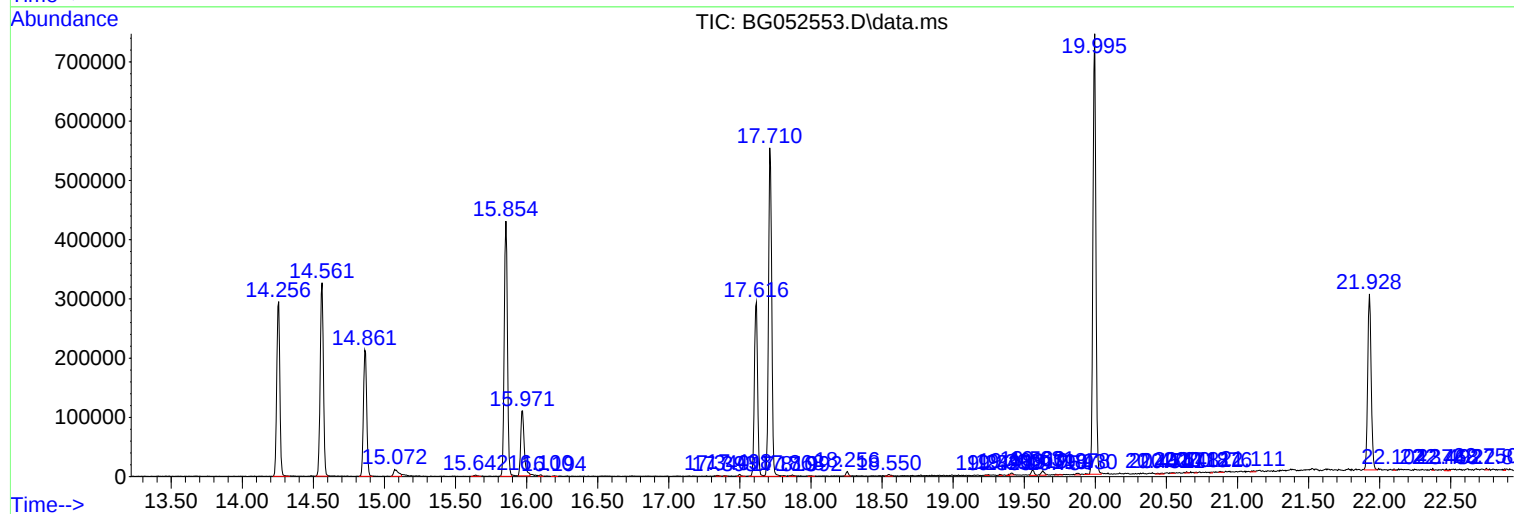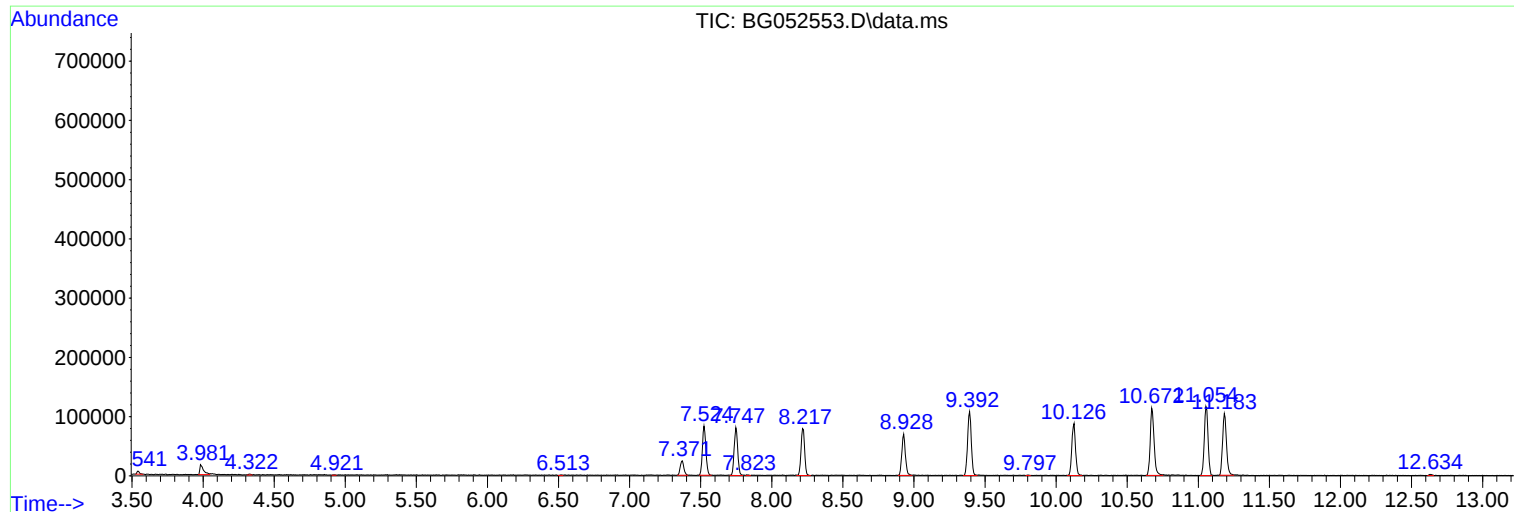

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030322\
Data File : BG052553.D
Acq On : 3 Mar 2022 14:09
Operator : CG/JU
Sample : N1745-07
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
H0AA7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030322\
Data File : BG052553.D
Acq On : 3 Mar 2022 14:09
Operator : CG/JU
Sample : N1745-07
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
H0AA7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc