

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030322\
 Data File : BG052559.D
 Acq On : 3 Mar 2022 18:01
 Operator : CG/JU
 Sample : PB143070BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK070

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052559.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.546	6	10	15	rVB3	6452	9738	1.02%	0.113%
2	3.628	19	24	27	rBV3	1839	2965	0.31%	0.034%
3	3.916	71	73	79	rVB4	1176	1743	0.18%	0.020%
4	3.975	79	83	99	rBV	73105	135935	14.27%	1.579%
5	4.098	103	104	107	rVB3	1917	1392	0.15%	0.016%
6	4.269	130	133	137	rVB4	1036	1360	0.14%	0.016%
7	4.327	139	143	147	rBV3	2172	3168	0.33%	0.037%
8	4.938	245	247	249	rBV	1551	1410	0.15%	0.016%
9	6.348	484	487	492	rBV5	1059	1591	0.17%	0.018%
10	6.759	555	557	560	rBV3	1140	1392	0.15%	0.016%
11	7.364	654	660	670	rBV2	100723	177806	18.66%	2.066%
12	7.523	679	687	697	rBV	78047	134835	14.15%	1.567%
13	7.746	717	725	733	rBV	97625	164024	17.21%	1.906%
14	7.899	746	751	755	rBV3	728	1444	0.15%	0.017%
15	8.216	798	805	813	rBV2	83123	140725	14.77%	1.635%
16	8.610	869	872	877	rBV	814	1463	0.15%	0.017%
17	8.727	889	892	895	rVB2	1075	1361	0.14%	0.016%
18	8.927	917	926	935	rBV	119555	215945	22.66%	2.509%
19	9.391	997	1005	1013	rVV	101882	184206	19.33%	2.140%
20	10.120	1120	1129	1140	rBV	88818	158145	16.60%	1.838%
21	10.672	1216	1223	1234	rBV	112987	215007	22.57%	2.498%
22	11.054	1281	1288	1296	rBV	123261	219281	23.01%	2.548%
23	11.183	1302	1310	1325	rBV	120369	230401	24.18%	2.677%
24	12.640	1556	1558	1562	rVB3	1782	1643	0.17%	0.019%
25	14.255	1825	1833	1841	rBV	296820	433127	45.46%	5.033%
26	14.561	1878	1885	1893	rBV	311546	495925	52.05%	5.762%
27	14.866	1929	1937	1943	rBV	222890	355095	37.27%	4.126%
28	15.060	1964	1970	1987	rBV2	70398	168909	17.73%	1.963%
29	15.853	2098	2105	2117	rVV	419292	640079	67.18%	7.437%
30	15.965	2119	2124	2133	rVV	102531	171297	17.98%	1.990%
31	16.059	2137	2140	2142	rVV3	2342	3312	0.35%	0.038%
32	16.100	2142	2147	2150	rVV3	2289	4192	0.44%	0.049%
33	17.398	2364	2368	2369	rVV3	1377	1385	0.15%	0.016%
34	17.615	2398	2405	2412	rBV	322340	495617	52.02%	5.759%
35	17.709	2414	2421	2434	rVV	487474	757356	79.49%	8.800%
36	19.466	2716	2720	2722	rBV3	1193	1400	0.15%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030322\
 Data File : BG052559.D
 Acq On : 3 Mar 2022 18:01
 Operator : CG/JU
 Sample : PB143070BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK070

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
 Title : SVOA CALIBRATION

37	19.560	2730	2736	2741	rBV5	7059	10831	1.14%	0.126%
38	19.636	2743	2749	2752	rVV2	5926	8599	0.90%	0.100%
39	19.947	2800	2802	2803	rBV2	1981	1343	0.14%	0.016%
40	19.994	2803	2810	2823	rVV	657332	952825	100.00%	11.071%

41	20.118	2829	2831	2834	rVB3	1797	1682	0.18%	0.020%
42	20.159	2836	2838	2839	rBV2	2075	1557	0.16%	0.018%
43	20.188	2841	2843	2844	rVV2	1705	1440	0.15%	0.017%
44	20.218	2846	2848	2851	rVV4	1228	1442	0.15%	0.017%
45	20.259	2853	2855	2858	rVB3	1590	1824	0.19%	0.021%

46	20.294	2858	2861	2863	rBV3	1420	1893	0.20%	0.022%
47	20.547	2901	2904	2908	rBV4	2640	3053	0.32%	0.035%
48	20.582	2908	2910	2912	rBV3	2190	2368	0.25%	0.028%
49	20.652	2920	2922	2924	rBV3	2077	1788	0.19%	0.021%
50	21.287	3027	3030	3032	rBV4	2041	2231	0.23%	0.026%

51	21.310	3032	3034	3035	rBV2	2214	1506	0.16%	0.017%
52	21.357	3039	3042	3043	rBV3	2950	3585	0.38%	0.042%
53	21.627	3086	3088	3091	rBV3	3006	3766	0.40%	0.044%
54	21.927	3132	3139	3149	rVV	310547	537016	56.36%	6.240%
55	22.015	3152	3154	3156	rVB3	2577	1362	0.14%	0.016%

56	22.191	3181	3184	3185	rBV3	2459	2659	0.28%	0.031%
57	22.385	3215	3217	3219	rVB2	3674	2762	0.29%	0.032%
58	22.409	3219	3221	3222	rBV2	2215	1885	0.20%	0.022%
59	23.261	3364	3366	3367	rBV2	2183	1633	0.17%	0.019%
60	23.496	3402	3406	3409	rBV6	3268	3847	0.40%	0.045%

61	23.707	3440	3442	3444	rBV3	2033	1809	0.19%	0.021%
62	24.018	3493	3495	3496	rBV2	1760	1298	0.14%	0.015%
63	24.271	3536	3538	3540	rBV3	1950	2086	0.22%	0.024%
64	24.447	3566	3568	3570	rBV3	2049	1677	0.18%	0.019%
65	24.494	3574	3576	3577	rBV2	1924	1355	0.14%	0.016%

66	24.559	3585	3587	3588	rVB2	3129	1814	0.19%	0.021%
67	25.152	3675	3688	3707	rBV2	296827	894833	93.91%	10.397%
68	25.387	3717	3728	3739	rBV2	174323	542704	56.96%	6.306%
69	25.610	3763	3766	3769	rBV5	2419	3116	0.33%	0.036%
70	25.681	3777	3778	3779	rBV	3982	2003	0.21%	0.023%

71	25.728	3785	3786	3788	rBV2	1591	1276	0.13%	0.015%
72	25.939	3821	3822	3824	rVB2	3076	1527	0.16%	0.018%
73	25.957	3824	3825	3827	rBV2	2597	2031	0.21%	0.024%
74	26.192	3861	3865	3866	rBV3	3171	3262	0.34%	0.038%
75	26.527	3920	3922	3924	rBV3	3252	2643	0.28%	0.031%

76	27.584	4100	4102	4104	rBV3	2264	2025	0.21%	0.024%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030322\
 Data File : BG052559.D
 Acq On : 3 Mar 2022 18:01
 Operator : CG/JU
 Sample : PB143070BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK070

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
 Title : SVOA CALIBRATION

77	27.825	4141	4143	4147	rBV5	2045	2892	0.30%	0.034%
78	27.913	4156	4158	4159	rBV2	2062	1359	0.14%	0.016%
79	28.019	4174	4176	4177	rBV2	1910	1461	0.15%	0.017%
80	28.089	4186	4188	4190	rBV2	2449	2536	0.27%	0.029%
81	28.506	4257	4259	4261	rBV3	2599	2573	0.27%	0.030%
82	28.630	4278	4280	4283	rVB4	2450	2207	0.23%	0.026%
83	28.765	4301	4303	4304	rBV2	2037	1709	0.18%	0.020%
84	29.006	4340	4344	4345	rBV4	2340	3089	0.32%	0.036%
85	29.041	4348	4350	4351	rVB2	2235	1278	0.13%	0.015%
86	29.288	4390	4392	4397	rBV5	1899	2739	0.29%	0.032%
87	29.382	4405	4408	4409	rBV3	2698	2483	0.26%	0.029%
88	29.887	4488	4494	4496	rBV6	2518	5255	0.55%	0.061%
89	30.850	4656	4658	4661	rBV4	2028	2051	0.22%	0.024%
90	31.068	4693	4695	4698	rBV4	1678	1367	0.14%	0.016%
91	31.120	4702	4704	4705	rBV2	2690	1679	0.18%	0.020%
92	31.185	4713	4715	4716	rBV2	2095	1361	0.14%	0.016%
93	31.297	4732	4734	4736	rBV3	2310	1663	0.17%	0.019%
94	31.637	4790	4792	4794	rVB3	2642	1848	0.19%	0.021%
95	31.802	4818	4820	4821	rBV2	2671	1379	0.14%	0.016%
96	31.966	4846	4848	4852	rBV4	2264	2063	0.22%	0.024%
97	32.008	4852	4855	4857	rBV3	2199	3248	0.34%	0.038%
98	32.102	4869	4871	4873	rVB2	2449	1858	0.19%	0.022%
99	32.401	4920	4922	4928	rBV8	2544	3815	0.40%	0.044%
100	32.460	4930	4932	4933	rVB2	2601	1301	0.14%	0.015%




Sum of corrected areas: 8606244

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030322\
Data File : BG052559.D
Acq On : 3 Mar 2022 18:01
Operator : CG/JU
Sample : PB143070BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK070

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

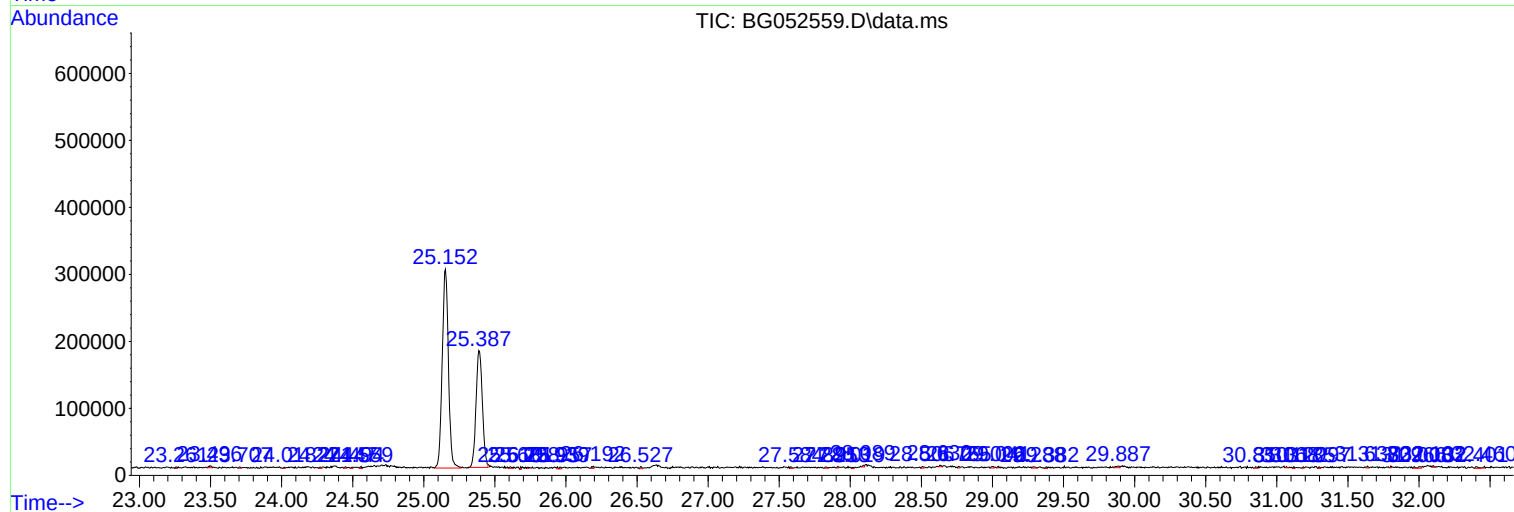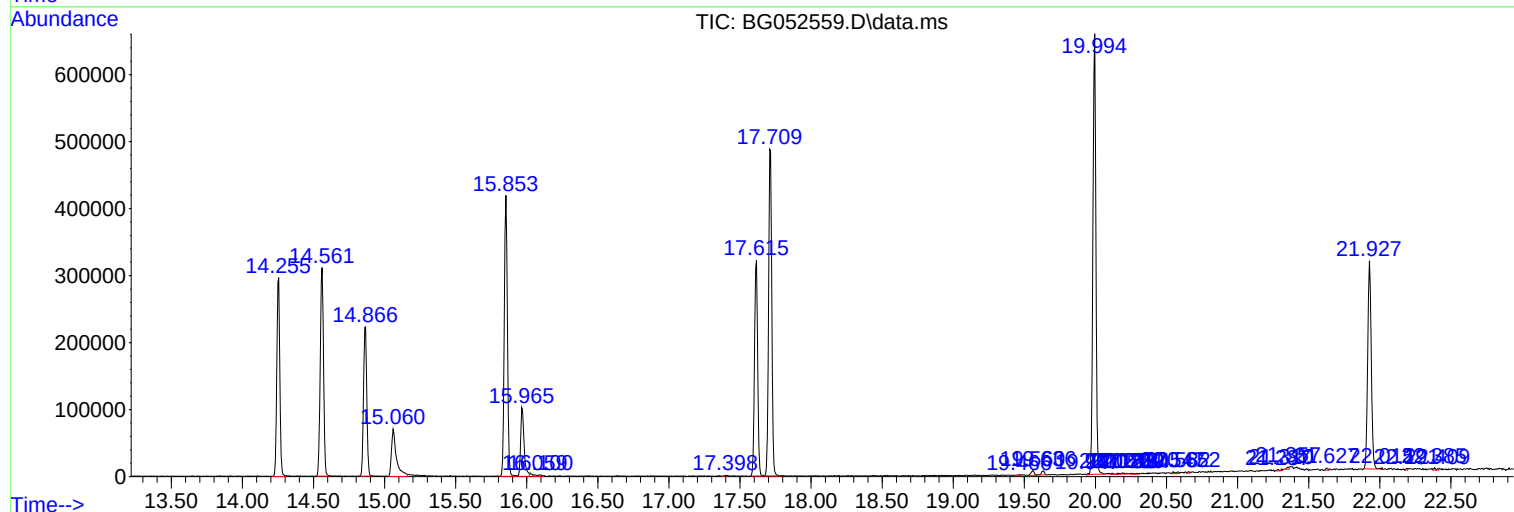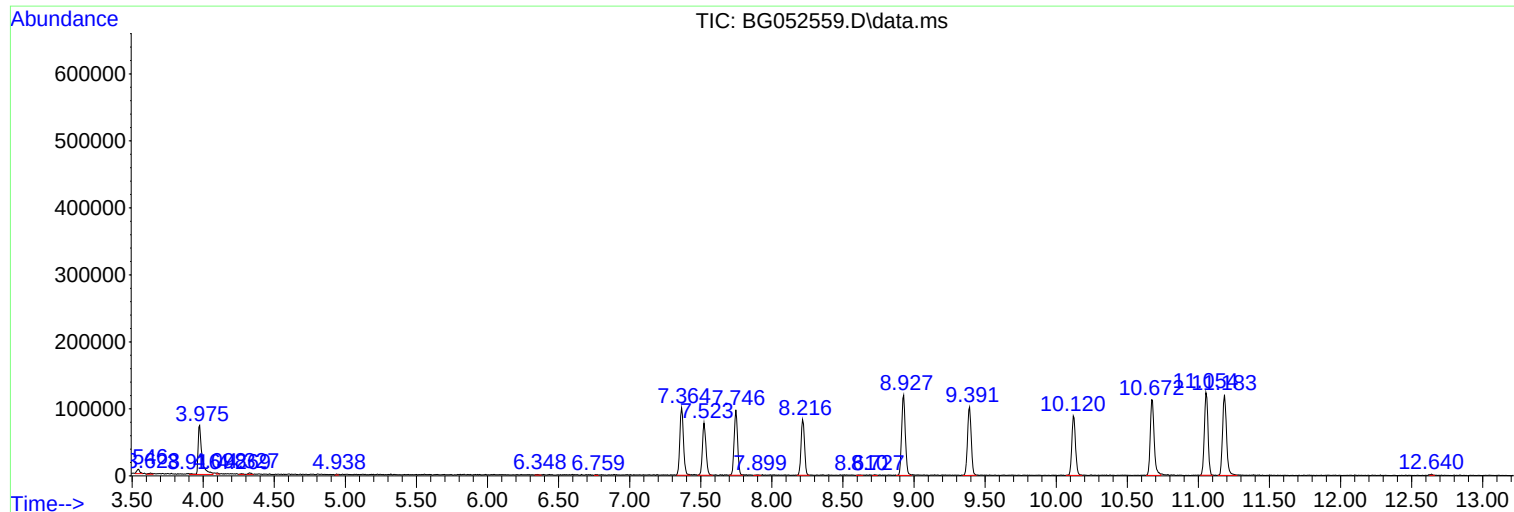

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030322\
Data File : BG052559.D
Acq On : 3 Mar 2022 18:01
Operator : CG/JU
Sample : PB143070BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK070

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030322\
Data File : BG052559.D
Acq On : 3 Mar 2022 18:01
Operator : CG/JU
Sample : PB143070BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK070

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------