

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030322\
 Data File : BG052561.D
 Acq On : 3 Mar 2022 19:18
 Operator : CG/JU
 Sample : N1745-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 H0AA3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052561.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.547	5	10	14	rVB2	5422	8167	0.78%	0.099%
2	3.987	82	85	96	rBV	12492	23700	2.25%	0.288%
3	4.322	139	142	146	rBV3	1388	1719	0.16%	0.021%
4	7.365	654	660	668	rBV2	26229	48264	4.59%	0.586%
5	7.524	680	687	696	rVB	78160	131549	12.51%	1.596%
6	7.747	717	725	735	rBV	78653	134866	12.83%	1.636%
7	8.217	797	805	817	rBV	77978	132789	12.63%	1.611%
8	8.928	919	926	938	rVB2	69515	123785	11.77%	1.502%
9	9.392	996	1005	1011	rBV	102080	182914	17.40%	2.219%
10	9.809	1074	1076	1080	rVB3	1484	1433	0.14%	0.017%
11	10.120	1123	1129	1138	rVB2	79344	146058	13.89%	1.772%
12	10.672	1217	1223	1238	rBV	106268	202014	19.21%	2.451%
13	10.819	1243	1248	1249	rBV4	1360	1855	0.18%	0.023%
14	11.054	1281	1288	1297	rVB	119404	207244	19.71%	2.514%
15	11.183	1304	1310	1321	rBV	106490	191724	18.23%	2.326%
16	12.634	1551	1557	1560	rBV2	1747	2652	0.25%	0.032%
17	12.840	1587	1592	1596	rBV3	1929	2514	0.24%	0.030%
18	13.463	1695	1698	1702	rVB2	1675	1894	0.18%	0.023%
19	13.668	1731	1733	1737	rBV3	1624	1807	0.17%	0.022%
20	14.250	1826	1832	1840	rBV	292725	423481	40.28%	5.138%
21	14.379	1852	1854	1861	rVB2	641	1379	0.13%	0.017%
22	14.485	1868	1872	1876	rVB4	2391	3311	0.31%	0.040%
23	14.555	1878	1884	1895	rVB	305312	492427	46.83%	5.974%
24	14.861	1929	1936	1944	rBV	203908	332596	31.63%	4.035%
25	15.078	1967	1973	1982	rBV4	15155	40113	3.82%	0.487%
26	15.172	1987	1989	1994	rVB4	1571	2237	0.21%	0.027%
27	15.489	2040	2043	2047	rVB	1457	1823	0.17%	0.022%
28	15.636	2064	2068	2071	rBV2	3704	6007	0.57%	0.073%
29	15.683	2074	2076	2080	rVB4	1216	1463	0.14%	0.018%
30	15.854	2098	2105	2118	rBV	432084	650765	61.89%	7.895%
31	15.965	2119	2124	2136	rBV	129014	202171	19.23%	2.453%
32	16.088	2142	2145	2151	rVB5	2750	4049	0.39%	0.049%
33	16.188	2156	2162	2167	rBV3	2331	3773	0.36%	0.046%
34	16.517	2216	2218	2221	rBV2	1767	2090	0.20%	0.025%
35	16.547	2221	2223	2227	rVB4	1494	2067	0.20%	0.025%
36	16.729	2251	2254	2259	rVB4	1391	1744	0.17%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030322\
 Data File : BG052561.D
 Acq On : 3 Mar 2022 19:18
 Operator : CG/JU
 Sample : N1745-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 H0AA3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
 Title : SVOA CALIBRATION

37	17.070	2307	2312	2315	rBV2	1416	2079	0.20%	0.025%
38	17.228	2337	2339	2343	rVB2	1194	1629	0.15%	0.020%
39	17.334	2353	2357	2362	rBV3	3672	5929	0.56%	0.072%
40	17.393	2362	2367	2372	rVB4	3638	6095	0.58%	0.074%
41	17.492	2381	2384	2389	rVB4	9149	11032	1.05%	0.134%
42	17.610	2398	2404	2411	rBV	303512	459346	43.69%	5.573%
43	17.710	2415	2421	2429	rVV	543713	844453	80.31%	10.245%
44	17.868	2444	2448	2453	rBV	12104	16695	1.59%	0.203%
45	17.998	2468	2470	2473	rVB3	1822	1700	0.16%	0.021%
46	18.086	2481	2485	2491	rVB3	3745	5205	0.50%	0.063%
47	18.203	2500	2505	2508	rBV6	1103	1769	0.17%	0.021%
48	18.250	2510	2513	2518	rVB4	3540	5184	0.49%	0.063%
49	18.362	2530	2532	2533	rBV	1964	1650	0.16%	0.020%
50	18.426	2540	2543	2544	rBV3	1372	1378	0.13%	0.017%
51	18.550	2561	2564	2568	rVB	10438	11487	1.09%	0.139%
52	18.767	2598	2601	2605	rBV4	3261	5162	0.49%	0.063%
53	18.849	2613	2615	2618	rBV3	1284	1547	0.15%	0.019%
54	18.891	2620	2622	2627	rVB5	4842	5748	0.55%	0.070%
55	19.126	2660	2662	2664	rVB3	3076	2087	0.20%	0.025%
56	19.337	2693	2698	2704	rBV7	6014	10365	0.99%	0.126%
57	19.554	2732	2735	2741	rBV6	10052	17325	1.65%	0.210%
58	19.936	2798	2800	2802	rBV2	3035	2513	0.24%	0.030%
59	19.989	2803	2809	2818	rVB	705896	1051442	100.00%	12.756%
60	20.306	2861	2863	2865	rBV3	2428	3155	0.30%	0.038%
61	21.105	2997	2999	3003	rBV5	3568	3214	0.31%	0.039%
62	21.928	3132	3139	3146	rBV	282021	494832	47.06%	6.003%
63	25.153	3676	3688	3701	rVB2	357771	1034278	98.37%	12.548%
64	25.388	3718	3728	3739	rBV2	176323	517074	49.18%	6.273%




Sum of corrected areas: 8242817

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030322\
Data File : BG052561.D
Acq On : 3 Mar 2022 19:18
Operator : CG/JU
Sample : N1745-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
H0AA3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

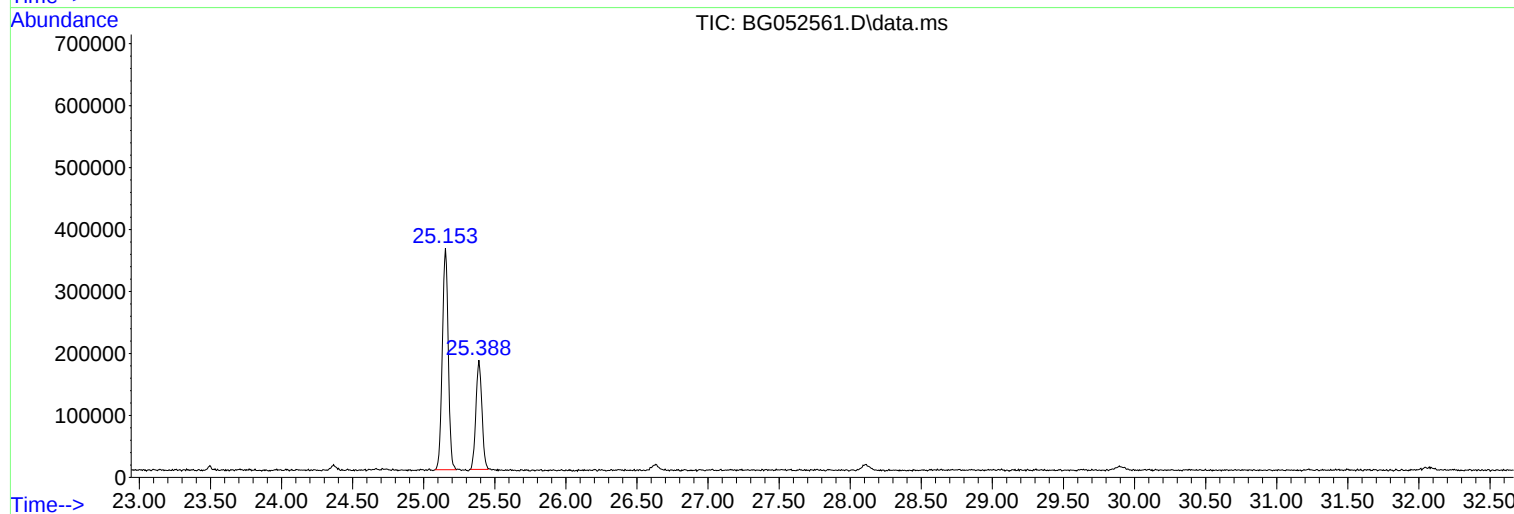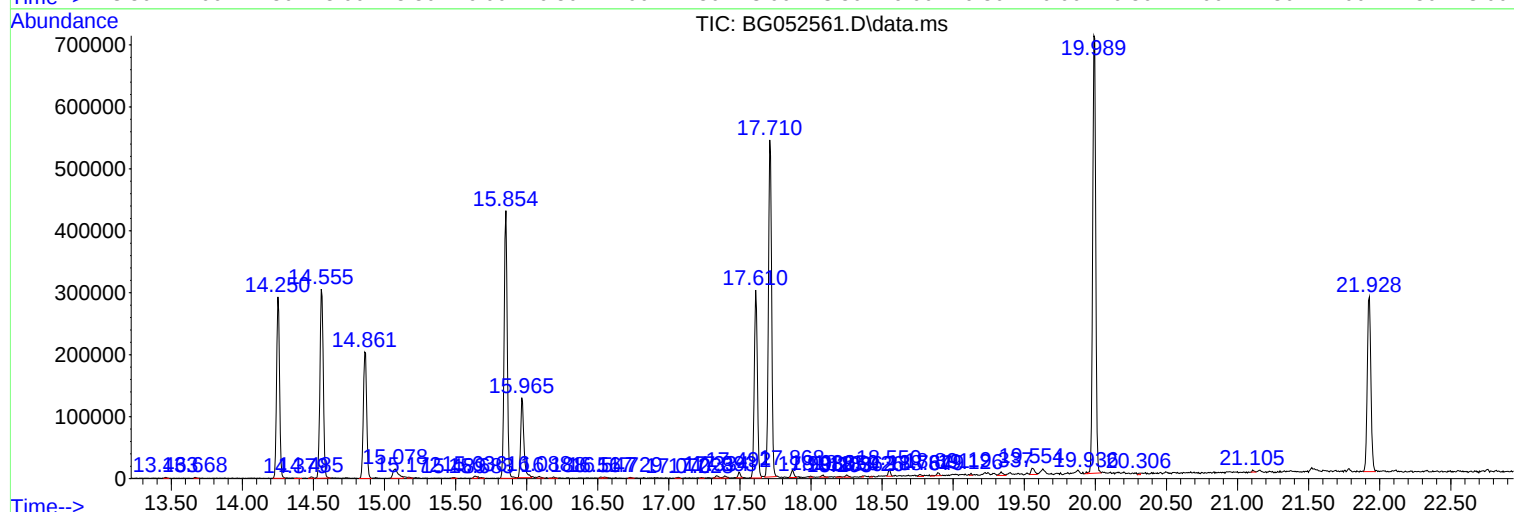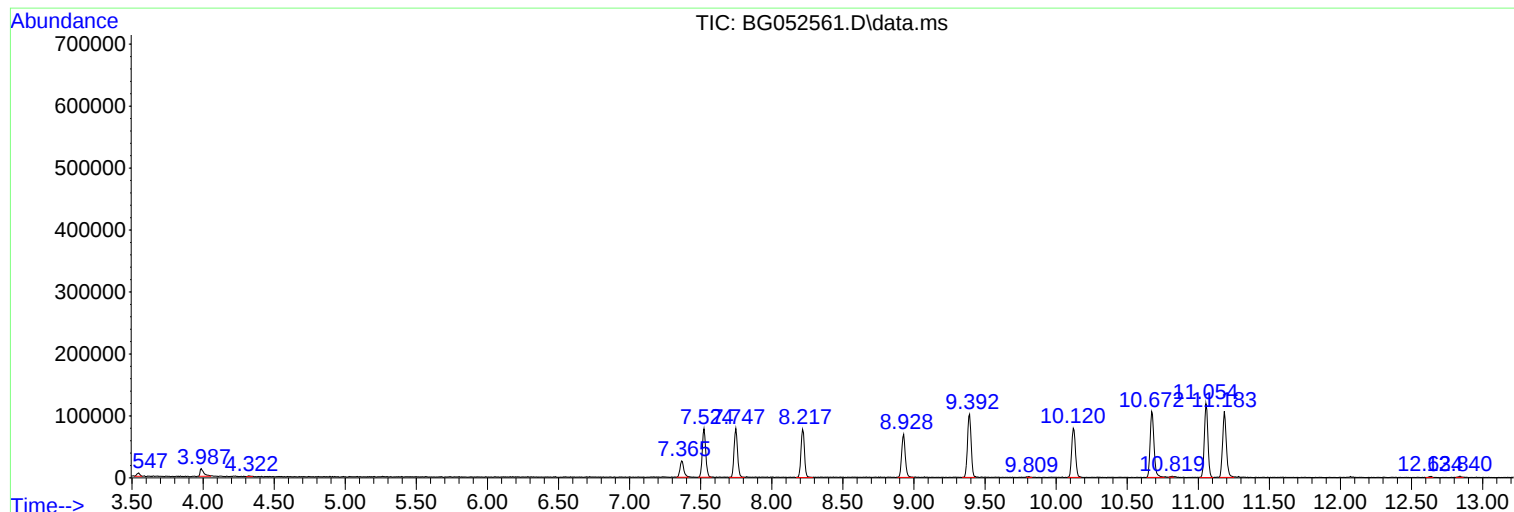

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030322\
Data File : BG052561.D
Acq On : 3 Mar 2022 19:18
Operator : CG/JU
Sample : N1745-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
H0AA3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030322\
Data File : BG052561.D
Acq On : 3 Mar 2022 19:18
Operator : CG/JU
Sample : N1745-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
H0AA3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc