

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030322\
 Data File : BG052571.D
 Acq On : 4 Mar 2022 8:55
 Operator : CG/JU
 Sample : PB143070BL
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK070

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052571.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.546	3	10	16	rBV5	7146	12808	1.29%	0.139%
2	3.975	79	83	103	rBV	82916	150383	15.15%	1.636%
3	4.104	103	105	108	rVV2	1342	1217	0.12%	0.013%
4	4.333	140	144	150	rVV2	2185	3422	0.34%	0.037%
5	4.704	201	207	210	rVB2	833	1591	0.16%	0.017%
6	5.232	293	297	300	rVB3	833	1197	0.12%	0.013%
7	5.367	317	320	323	rBV2	975	1328	0.13%	0.014%
8	5.467	332	337	339	rVB2	983	1368	0.14%	0.015%
9	6.096	436	444	447	rBV2	804	2073	0.21%	0.023%
10	6.137	447	451	453	rBV2	969	1098	0.11%	0.012%
11	6.225	464	466	470	rVB2	807	1089	0.11%	0.012%
12	7.376	656	662	673	rBV	110277	197605	19.91%	2.150%
13	7.541	683	690	699	rVB	87503	146835	14.79%	1.598%
14	7.758	721	727	736	rVV	100252	179725	18.11%	1.956%
15	8.234	801	808	815	rBV	94766	157936	15.91%	1.719%
16	8.939	921	928	940	rBV2	134913	237578	23.94%	2.585%
17	9.321	991	993	999	rBV2	596	1106	0.11%	0.012%
18	9.403	999	1007	1017	rVB	115434	202337	20.39%	2.202%
19	10.137	1125	1132	1141	rBV	92462	165386	16.66%	1.800%
20	10.690	1219	1226	1237	rVV	122851	239605	24.14%	2.607%
21	10.772	1239	1240	1242	rVV	1634	1173	0.12%	0.013%
22	11.065	1282	1290	1299	rVB	138253	244297	24.61%	2.658%
23	11.195	1305	1312	1326	rBV	133258	252582	25.45%	2.749%
24	12.652	1554	1560	1564	rBV3	1645	3342	0.34%	0.036%
25	14.261	1828	1834	1841	rBV	325881	455097	45.85%	4.952%
26	14.567	1879	1886	1896	rBV	344604	534116	53.82%	5.812%
27	14.872	1930	1938	1946	rBV	239060	392771	39.57%	4.274%
28	15.066	1965	1971	1989	rBV2	74469	177289	17.86%	1.929%
29	15.225	1995	1998	2003	rVB3	1111	1812	0.18%	0.020%
30	15.859	2100	2106	2113	rBV	458210	672695	67.78%	7.320%
31	15.976	2120	2126	2138	rBV2	105450	186335	18.77%	2.028%
32	16.100	2144	2147	2150	rVB2	1423	1701	0.17%	0.019%
33	16.323	2179	2185	2186	rBV2	773	1144	0.12%	0.012%
34	17.210	2334	2336	2340	rVB3	925	1089	0.11%	0.012%
35	17.398	2365	2368	2371	rBV3	1165	1452	0.15%	0.016%
36	17.615	2399	2405	2413	rBV	339254	530622	53.46%	5.774%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030322\
 Data File : BG052571.D
 Acq On : 4 Mar 2022 8:55
 Operator : CG/JU
 Sample : PB143070BL
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK070

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
 Title : SVOA CALIBRATION

37	17.715	2415	2422	2431	rBV	512342	801178	80.72%	8.718%
38	19.019	2642	2644	2648	rVB2	961	1273	0.13%	0.014%
39	19.566	2732	2737	2740	rVV4	7569	11053	1.11%	0.120%
40	19.636	2744	2749	2753	rBV	7603	10247	1.03%	0.112%
41	19.695	2758	2759	2764	rVB3	1467	1580	0.16%	0.017%
42	19.730	2764	2765	2768	rBV2	1103	1293	0.13%	0.014%
43	19.995	2804	2810	2821	rVV	702131	992486	100.00%	10.800%
44	20.183	2840	2842	2843	rBV2	1498	1098	0.11%	0.012%
45	20.282	2855	2859	2861	rBV5	1270	1718	0.17%	0.019%
46	20.423	2882	2883	2886	rBV2	1171	1117	0.11%	0.012%
47	20.670	2923	2925	2927	rBV3	1866	1354	0.14%	0.015%
48	20.846	2953	2955	2958	rVB3	2109	1964	0.20%	0.021%
49	20.882	2958	2961	2963	rBV4	2459	3516	0.35%	0.038%
50	20.952	2972	2973	2975	rBV2	1987	1492	0.15%	0.016%
51	20.970	2975	2976	2979	rVV3	2248	2287	0.23%	0.025%
52	21.046	2987	2989	2992	rBV4	2437	2453	0.25%	0.027%
53	21.070	2992	2993	2995	rBV2	2349	1332	0.13%	0.014%
54	21.310	3032	3034	3036	rBV	1717	1510	0.15%	0.016%
55	21.334	3036	3038	3039	rBV	2406	2196	0.22%	0.024%
56	21.363	3039	3043	3044	rBV4	3064	3677	0.37%	0.040%
57	21.475	3060	3062	3064	rBV3	1709	2025	0.20%	0.022%
58	21.628	3084	3088	3092	rBV2	8793	12857	1.30%	0.140%
59	21.698	3098	3100	3102	rBV3	1968	2008	0.20%	0.022%
60	21.933	3132	3140	3151	rBV	329259	580660	58.51%	6.319%
61	22.820	3289	3291	3292	rVB2	2591	1433	0.14%	0.016%
62	22.838	3292	3294	3295	rBV	2044	1218	0.12%	0.013%
63	23.026	3324	3326	3329	rVB3	2062	1743	0.18%	0.019%
64	23.137	3343	3345	3347	rVB3	2732	1629	0.16%	0.018%
65	23.161	3347	3349	3350	rBV2	1872	1591	0.16%	0.017%
66	23.995	3489	3491	3493	rBV3	2136	1916	0.19%	0.021%
67	24.201	3524	3526	3528	rBV3	1688	2158	0.22%	0.023%
68	24.265	3535	3537	3538	rBV2	2407	1365	0.14%	0.015%
69	24.459	3568	3570	3572	rBV2	1824	1587	0.16%	0.017%
70	24.541	3582	3584	3587	rBV4	2322	2181	0.22%	0.024%
71	24.894	3642	3644	3645	rBV	1955	1211	0.12%	0.013%
72	25.088	3675	3677	3678	rBV2	2331	1748	0.18%	0.019%
73	25.164	3678	3690	3705	rVV3	300195	913721	92.06%	9.943%
74	25.399	3719	3730	3743	rBV	183597	573189	57.75%	6.237%
75	25.487	3743	3745	3747	rVB2	3641	2591	0.26%	0.028%
76	25.892	3812	3814	3817	rVB3	2364	2099	0.21%	0.023%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030322\
 Data File : BG052571.D
 Acq On : 4 Mar 2022 8:55
 Operator : CG/JU
 Sample : PB143070BL
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK070

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
 Title : SVOA CALIBRATION

77	26.192	3863	3865	3868	rVB4	2413	2527	0.25%	0.027%
78	26.615	3933	3937	3938	rBV4	4851	5833	0.59%	0.063%
79	26.644	3940	3942	3949	rVB6	8137	12567	1.27%	0.137%
80	27.226	4039	4041	4043	rBV3	1843	1640	0.17%	0.018%
81	28.084	4184	4187	4188	rBV3	3551	4204	0.42%	0.046%
82	28.113	4188	4192	4196	rVV6	5631	10901	1.10%	0.119%
83	28.266	4216	4218	4219	rVB2	2119	1157	0.12%	0.013%
84	28.442	4246	4248	4251	rBV3	2292	2419	0.24%	0.026%
85	28.589	4272	4273	4275	rBV2	2126	1718	0.17%	0.019%
86	28.771	4303	4304	4307	rBV3	1888	1590	0.16%	0.017%
87	28.935	4331	4332	4334	rBV2	2117	1511	0.15%	0.016%
88	29.740	4467	4469	4470	rBV2	1900	1683	0.17%	0.018%
89	29.869	4490	4491	4492	rBV	2738	1673	0.17%	0.018%
90	30.433	4586	4587	4588	rBV	3417	1944	0.20%	0.021%
91	30.903	4665	4667	4670	rVB4	2836	2896	0.29%	0.032%
92	31.579	4780	4782	4785	rVB4	1963	1253	0.13%	0.014%
93	31.820	4821	4823	4825	rBV3	2151	1604	0.16%	0.017%
94	31.961	4845	4847	4849	rVB2	2425	1680	0.17%	0.018%
95	31.984	4849	4851	4854	rBV5	1957	2593	0.26%	0.028%
96	32.025	4856	4858	4860	rVB3	2552	1537	0.15%	0.017%
97	32.049	4860	4862	4863	rBV2	3530	2511	0.25%	0.027%
98	32.090	4868	4869	4875	rVV5	3011	3859	0.39%	0.042%
99	32.554	4946	4948	4949	rBV	1739	1527	0.15%	0.017%
100	32.583	4952	4953	4955	rVB2	2497	1757	0.18%	0.019%




Sum of corrected areas: 9189542

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030322\
Data File : BG052571.D
Acq On : 4 Mar 2022 8:55
Operator : CG/JU
Sample : PB143070BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK070

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

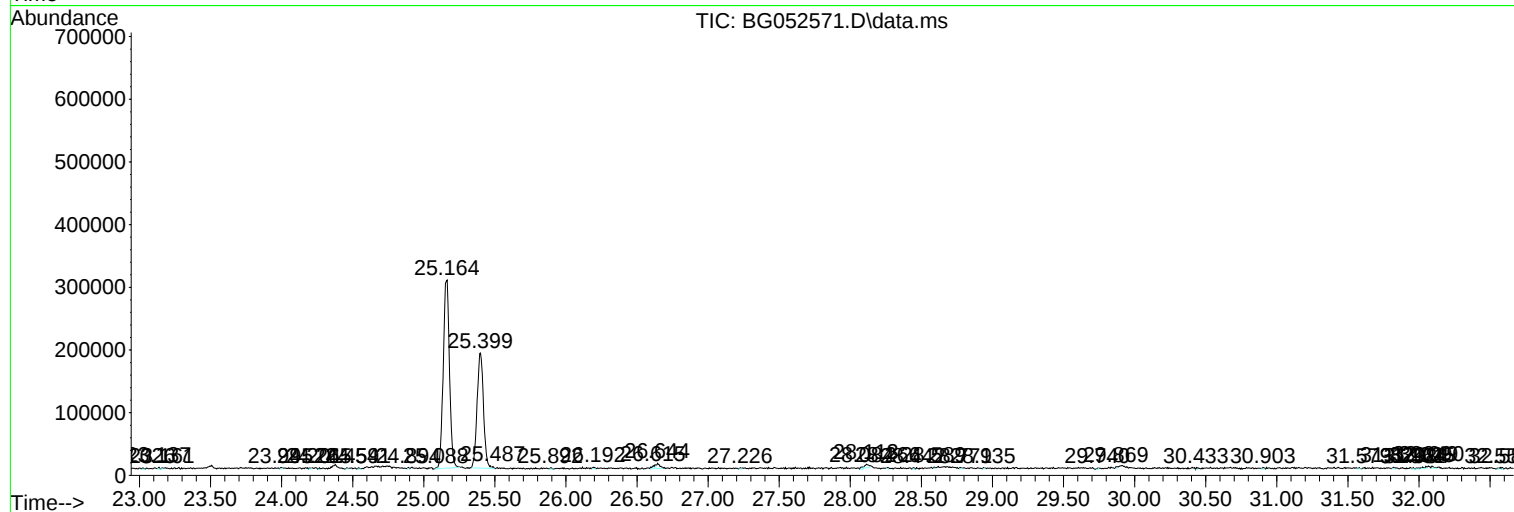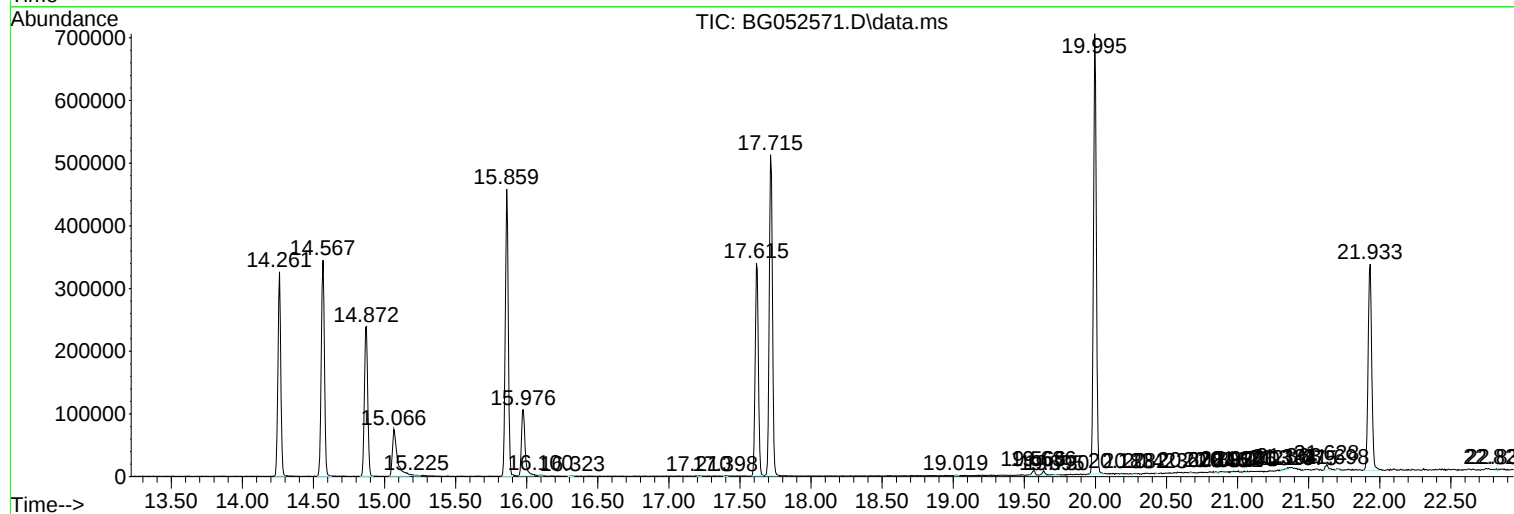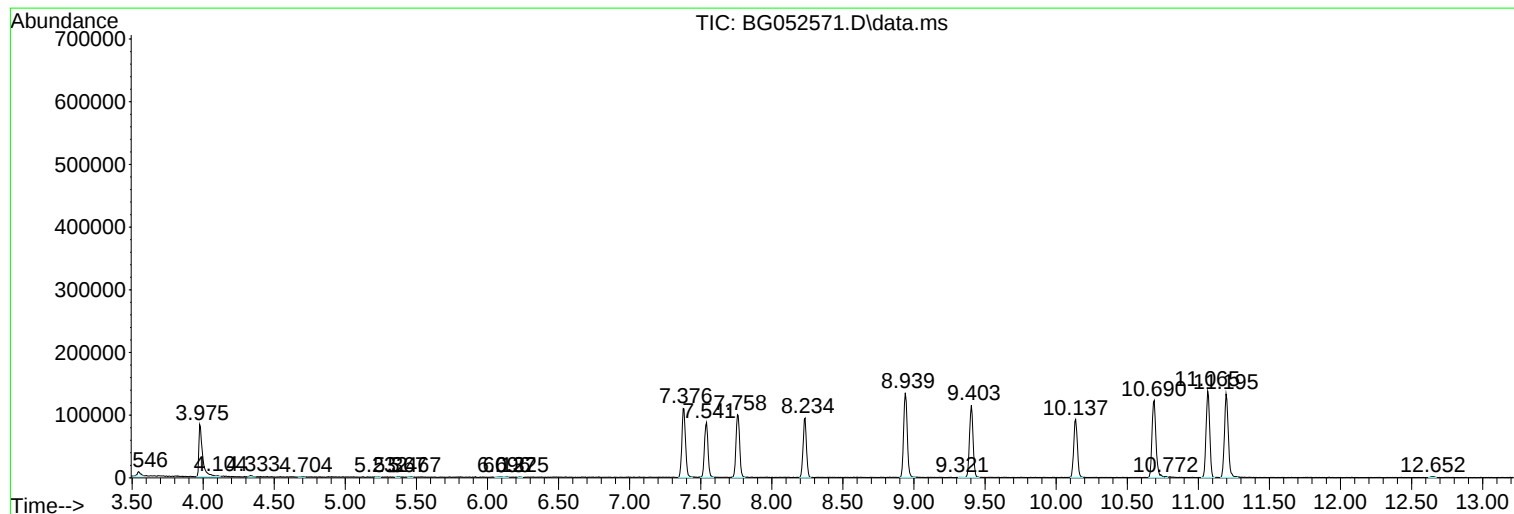

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030322\
Data File : BG052571.D
Acq On : 4 Mar 2022 8:55
Operator : CG/JU
Sample : PB143070BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK070

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030322\
Data File : BG052571.D
Acq On : 4 Mar 2022 8:55
Operator : CG/JU
Sample : PB143070BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK070

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc