

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030322\
 Data File : BG052577.D
 Acq On : 4 Mar 2022 13:53
 Operator : CG/JU
 Sample : PB143006BL
 Misc : GCMS CONFIRMATION
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK006

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052577.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.799	51	53	54	rBV	897	859	0.16%	0.039%
2	3.817	54	56	61	rVV2	4486	5517	1.01%	0.250%
3	4.316	138	141	148	rVB3	1831	2351	0.43%	0.107%
4	4.445	160	163	166	rBV2	1100	1166	0.21%	0.053%
5	4.710	206	208	210	rVB	829	676	0.12%	0.031%
6	4.810	222	225	228	rVB3	943	1080	0.20%	0.049%
7	5.009	257	259	261	rVB	742	640	0.12%	0.029%
8	5.133	278	280	282	rBV2	728	578	0.11%	0.026%
9	5.244	297	299	302	rBV3	609	843	0.15%	0.038%
10	5.667	369	371	378	rVB	857	1563	0.29%	0.071%
11	5.720	378	380	382	rBV	561	605	0.11%	0.027%
12	5.979	423	424	428	rBV2	464	636	0.12%	0.029%
13	6.102	443	445	448	rVB2	609	663	0.12%	0.030%
14	6.513	513	515	520	rVB	545	722	0.13%	0.033%
15	6.607	529	531	535	rVB2	588	685	0.12%	0.031%
16	6.642	535	537	542	rVB	590	797	0.15%	0.036%
17	6.707	545	548	550	rBV	715	733	0.13%	0.033%
18	7.142	617	622	623	rBV2	765	1208	0.22%	0.055%
19	7.253	640	641	645	rBV2	628	606	0.11%	0.027%
20	7.488	678	681	683	rBV	584	775	0.14%	0.035%
21	7.970	759	763	764	rBV	839	874	0.16%	0.040%
22	8.005	767	769	774	rVB2	668	773	0.14%	0.035%
23	8.217	798	805	814	rVB	91559	154092	28.11%	6.988%
24	8.328	821	824	828	rBV2	379	628	0.11%	0.028%
25	8.540	856	860	863	rBV	766	1105	0.20%	0.050%
26	9.415	1005	1009	1010	rBV	591	660	0.12%	0.030%
27	9.462	1015	1017	1019	rBV2	587	768	0.14%	0.035%
28	9.539	1026	1030	1032	rBV2	840	810	0.15%	0.037%
29	9.697	1055	1057	1059	rBV2	562	631	0.12%	0.029%
30	10.537	1196	1200	1201	rBV2	805	817	0.15%	0.037%
31	10.790	1240	1243	1245	rBV2	529	609	0.11%	0.028%
32	11.054	1280	1288	1295	rBV	108190	197900	36.10%	8.974%
33	11.142	1301	1303	1306	rVB2	688	630	0.11%	0.029%
34	11.501	1361	1364	1366	rVB2	578	662	0.12%	0.030%
35	11.524	1366	1368	1370	rBV	687	669	0.12%	0.030%
36	11.841	1419	1422	1425	rVB	547	684	0.12%	0.031%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030322\
 Data File : BG052577.D
 Acq On : 4 Mar 2022 13:53
 Operator : CG/JU
 Sample : PB143006BL
 Misc : GCMS CONFIRMATION
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK006

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
 Title : SVOA CALIBRATION

37	13.298	1665	1670	1672	rBV	485	807	0.15%	0.037%
38	13.480	1697	1701	1705	rBV	524	813	0.15%	0.037%
39	13.557	1712	1714	1719	rVB2	590	762	0.14%	0.035%
40	14.297	1837	1840	1842	rBV	689	781	0.14%	0.035%
41	14.543	1879	1882	1884	rBV	917	1151	0.21%	0.052%
42	14.861	1930	1936	1948	rBV	178543	285384	52.06%	12.942%
43	15.178	1986	1990	1992	rVB2	551	634	0.12%	0.029%
44	15.936	2118	2119	2123	rBV2	594	609	0.11%	0.028%
45	16.394	2194	2197	2199	rBV	509	691	0.13%	0.031%
46	16.594	2228	2231	2234	rVB2	676	803	0.15%	0.036%
47	16.676	2243	2245	2247	rBV2	666	618	0.11%	0.028%
48	16.976	2293	2296	2299	rBV2	669	1058	0.19%	0.048%
49	17.116	2318	2320	2325	rVB	625	598	0.11%	0.027%
50	17.516	2385	2388	2390	rBV	782	725	0.13%	0.033%
51	17.610	2396	2404	2419	rBV	247366	420081	76.64%	19.050%
52	17.816	2436	2439	2444	rVB3	727	915	0.17%	0.041%
53	18.009	2469	2472	2474	rBV	775	790	0.14%	0.036%
54	18.661	2580	2583	2586	rBV3	667	787	0.14%	0.036%
55	18.738	2594	2596	2599	rBV2	1090	1279	0.23%	0.058%
56	18.849	2614	2615	2618	rVB2	907	717	0.13%	0.033%
57	18.990	2638	2639	2642	rVB	1036	885	0.16%	0.040%
58	19.026	2642	2645	2648	rBV	599	776	0.14%	0.035%
59	19.190	2672	2673	2675	rBV	797	638	0.12%	0.029%
60	19.243	2681	2682	2685	rBV2	822	770	0.14%	0.035%
61	19.296	2689	2691	2694	rBV2	804	654	0.12%	0.030%
62	19.343	2696	2699	2703	rBV4	865	1355	0.25%	0.061%
63	19.413	2709	2711	2715	rBV3	562	791	0.14%	0.036%
64	19.513	2724	2728	2732	rBV3	1157	2346	0.43%	0.106%
65	19.689	2756	2758	2760	rBV	1173	761	0.14%	0.035%
66	19.866	2786	2788	2790	rBV2	903	760	0.14%	0.034%
67	19.913	2794	2796	2799	rBV3	1109	1331	0.24%	0.060%
68	20.065	2820	2822	2824	rBV3	1113	839	0.15%	0.038%
69	20.154	2836	2837	2838	rVB	1677	591	0.11%	0.027%
70	20.271	2854	2857	2858	rBV	1294	1338	0.24%	0.061%
71	20.988	2977	2979	2980	rBV2	1991	1176	0.21%	0.053%
72	21.928	3131	3139	3148	rBV	293793	548152	100.00%	24.858%
73	25.382	3717	3727	3745	rVB2	165429	533626	97.35%	24.199%
74	30.305	4563	4565	4569	rBV5	2903	3358	0.61%	0.152%

Sum of corrected areas: 2205165




Instrument :
BNA_G
ClientSampleId :
SBLK006

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030322\
Data File : BG052577.D
Acq On : 4 Mar 2022 13:53
Operator : CG/JU
Sample : PB143006BL
Misc : GCMS CONFIRMATION
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK006

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

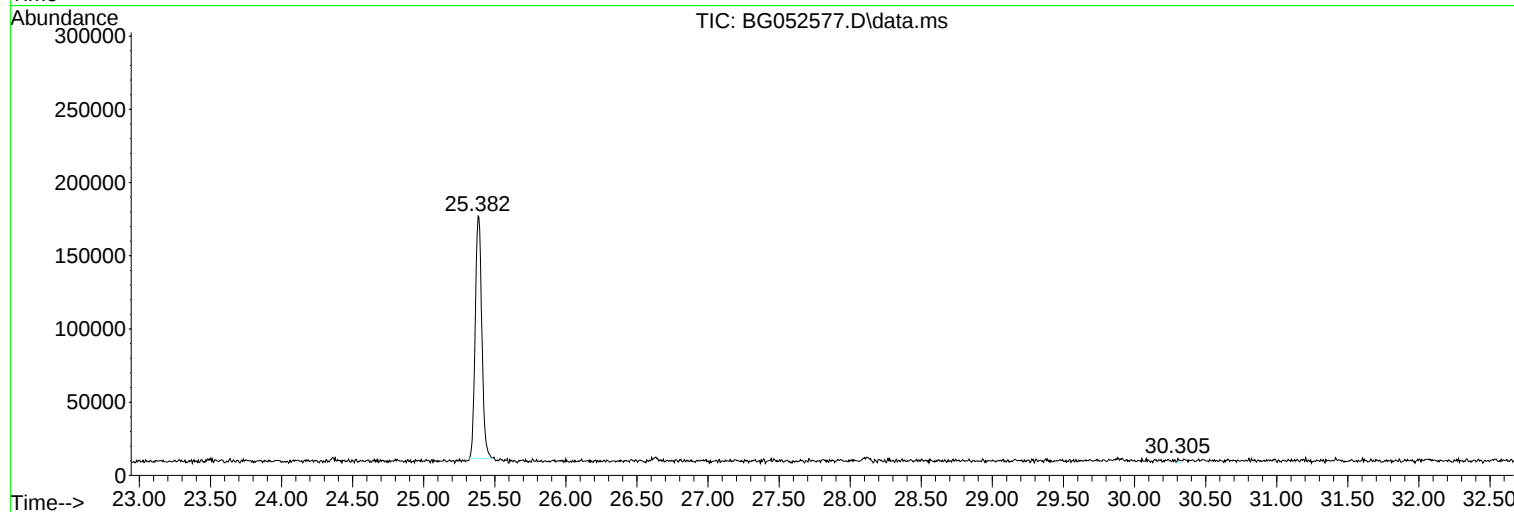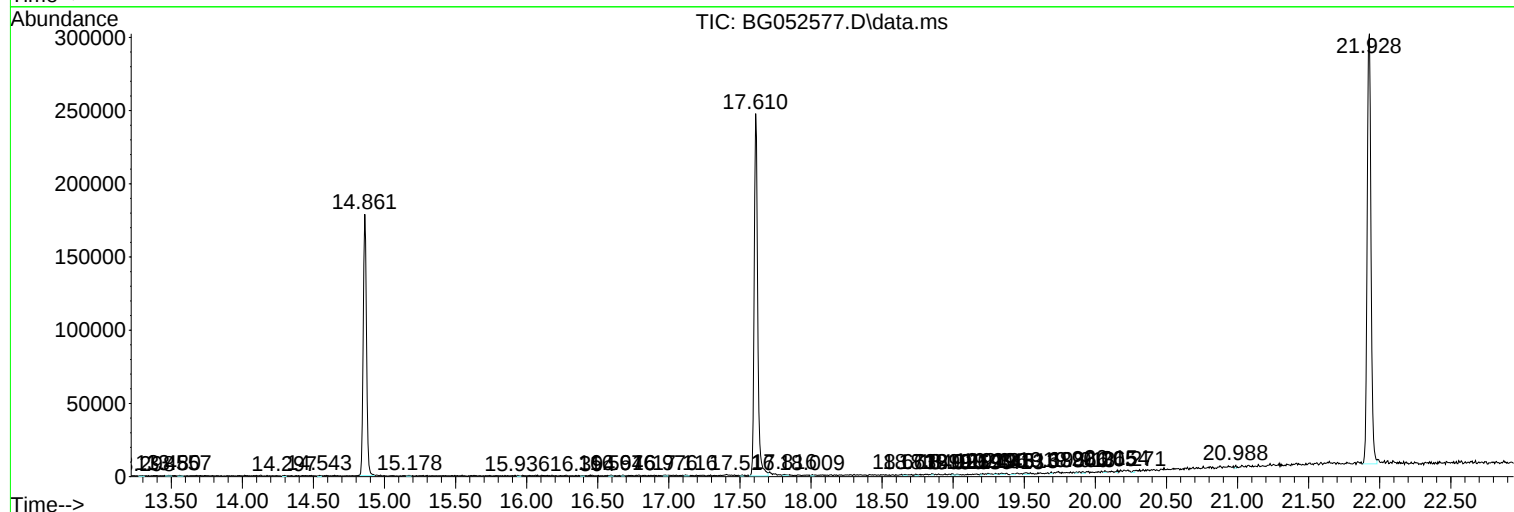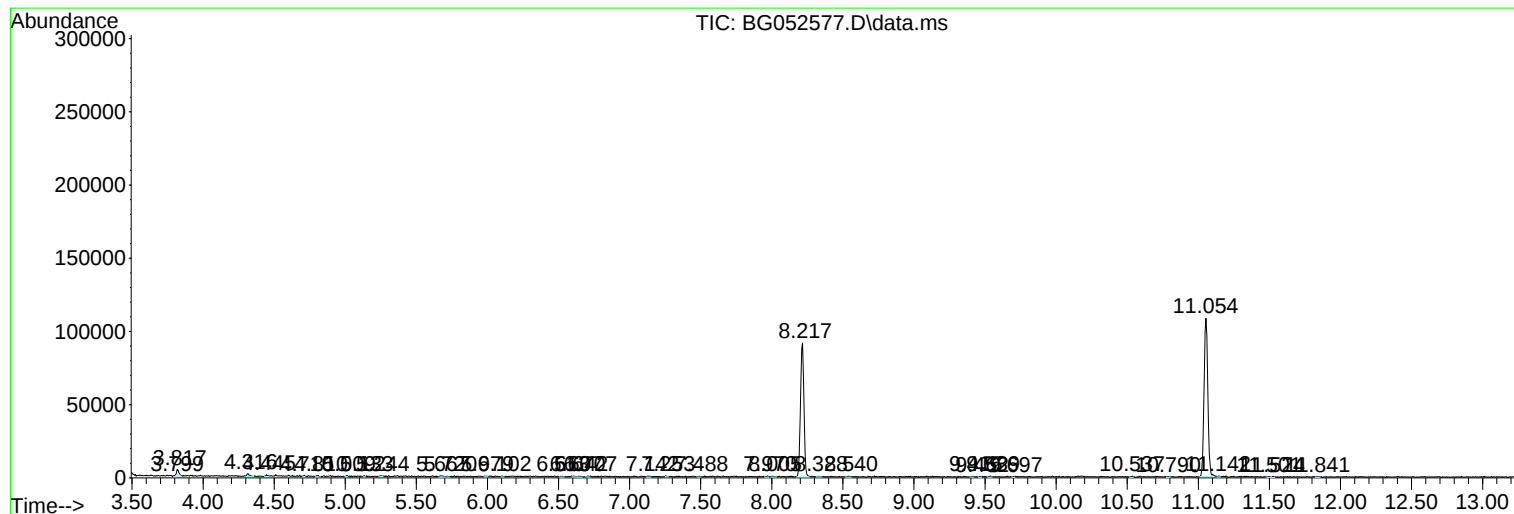

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030322\
Data File : BG052577.D
Acq On : 4 Mar 2022 13:53
Operator : CG/JU
Sample : PB143006BL
Misc : GCMS CONFIRMATION
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK006

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030322\
Data File : BG052577.D
Acq On : 4 Mar 2022 13:53
Operator : CG/JU
Sample : PB143006BL
Misc : GCMS CONFIRMATION
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK006

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc