

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030322\
 Data File : BG052579.D
 Acq On : 4 Mar 2022 15:11
 Operator : CG/JU
 Sample : N1697-03
 Misc : GCMS CONFIRMATION
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGZJ8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052579.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.632	22	24	27	rVB	731	614	0.12%	0.027%
2	3.790	46	51	53	rBV2	3092	3792	0.74%	0.164%
3	3.826	53	57	61	rVB3	12711	15682	3.05%	0.678%
4	4.160	112	114	117	rBV	621	613	0.12%	0.027%
5	4.207	119	122	125	rVV2	839	1085	0.21%	0.047%
6	4.313	136	140	148	rVB4	3174	5158	1.00%	0.223%
7	4.372	148	150	153	rBV	832	897	0.17%	0.039%
8	4.425	156	159	164	rBV2	1304	1787	0.35%	0.077%
9	4.689	201	204	207	rBV	643	667	0.13%	0.029%
10	4.765	213	217	218	rBV2	620	895	0.17%	0.039%
11	5.188	285	289	291	rBV2	731	700	0.14%	0.030%
12	5.247	295	299	300	rBV	633	669	0.13%	0.029%
13	5.370	317	320	321	rBV	631	728	0.14%	0.031%
14	5.600	358	359	363	rBV2	467	573	0.11%	0.025%
15	6.117	446	447	451	rBV2	681	941	0.18%	0.041%
16	6.263	469	472	475	rBV2	532	755	0.15%	0.033%
17	6.780	557	560	564	rBV2	456	797	0.15%	0.034%
18	6.898	577	580	582	rBV2	648	912	0.18%	0.039%
19	7.009	596	599	601	rBV	638	847	0.16%	0.037%
20	7.468	674	677	679	rVB2	597	602	0.12%	0.026%
21	8.084	779	782	785	rBV2	447	631	0.12%	0.027%
22	8.143	789	792	796	rBV2	530	814	0.16%	0.035%
23	8.214	798	804	812	rVB	93103	157512	30.63%	6.814%
24	9.500	1021	1023	1025	rVB	815	622	0.12%	0.027%
25	9.530	1025	1028	1031	rBV	591	1017	0.20%	0.044%
26	10.734	1231	1233	1237	rVB2	703	1025	0.20%	0.044%
27	10.851	1249	1253	1256	rBV2	460	651	0.13%	0.028%
28	11.051	1280	1287	1300	rBV	109791	211056	41.04%	9.130%
29	11.145	1300	1303	1305	rVB2	759	714	0.14%	0.031%
30	12.790	1579	1583	1584	rBV2	486	611	0.12%	0.026%
31	13.119	1635	1639	1642	rVB2	539	829	0.16%	0.036%
32	13.847	1760	1763	1766	rBV2	486	773	0.15%	0.033%
33	14.053	1796	1798	1799	rBV	706	643	0.13%	0.028%
34	14.529	1875	1879	1882	rBV2	524	701	0.14%	0.030%
35	14.858	1929	1935	1952	rBV	181871	304591	59.22%	13.177%
36	14.975	1952	1955	1956	rVV	1421	1209	0.24%	0.052%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030322\
 Data File : BG052579.D
 Acq On : 4 Mar 2022 15:11
 Operator : CG/JU
 Sample : N1697-03
 Misc : GCMS CONFIRMATION
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGZJ8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
 Title : SVOA CALIBRATION

37	14.999	1956	1959	1961	rVB	673	707	0.14%	0.031%
38	15.580	2057	2058	2063	rVB	570	725	0.14%	0.031%
39	16.320	2183	2184	2187	rVB	756	628	0.12%	0.027%
40	16.350	2187	2189	2192	rBV	865	1050	0.20%	0.045%

41	16.520	2215	2218	2222	rVB	575	769	0.15%	0.033%
42	16.579	2227	2228	2230	rBV	859	597	0.12%	0.026%
43	16.820	2268	2269	2272	rBV2	684	559	0.11%	0.024%
44	16.896	2280	2282	2284	rBV2	627	604	0.12%	0.026%
45	17.049	2307	2308	2313	rBV2	842	665	0.13%	0.029%

46	17.184	2328	2331	2333	rBV2	511	604	0.12%	0.026%
47	17.219	2333	2337	2340	rVV3	454	846	0.16%	0.037%
48	17.290	2345	2349	2350	rBV2	719	609	0.12%	0.026%
49	17.307	2350	2352	2355	rBV	447	592	0.12%	0.026%
50	17.401	2365	2368	2369	rBV	788	648	0.13%	0.028%

51	17.495	2381	2384	2387	rBV3	548	741	0.14%	0.032%
52	17.566	2394	2396	2397	rBV2	601	611	0.12%	0.026%
53	17.613	2397	2404	2416	rVV	249671	409182	79.56%	17.702%
54	17.812	2436	2438	2442	rVB	611	640	0.12%	0.028%
55	17.936	2458	2459	2462	rBV	563	565	0.11%	0.024%

56	18.083	2482	2484	2488	rVB2	682	609	0.12%	0.026%
57	18.212	2504	2506	2509	rVB2	972	740	0.14%	0.032%
58	18.235	2509	2510	2512	rVB	1116	600	0.12%	0.026%
59	18.259	2512	2514	2517	rBV2	1031	1203	0.23%	0.052%
60	18.318	2520	2524	2528	rVV3	2102	2606	0.51%	0.113%

61	18.376	2531	2534	2536	rVV3	1335	1669	0.32%	0.072%
62	18.400	2536	2538	2542	rVV2	3909	3402	0.66%	0.147%
63	18.429	2542	2543	2546	rVB	1383	791	0.15%	0.034%
64	18.541	2560	2562	2564	rBV2	1393	1004	0.20%	0.043%
65	18.564	2564	2566	2568	rVB3	1053	792	0.15%	0.034%

66	18.670	2581	2584	2588	rBV3	2942	3957	0.77%	0.171%
67	18.729	2591	2594	2598	rVV3	4063	5344	1.04%	0.231%
68	18.776	2598	2602	2608	rVB4	5242	7664	1.49%	0.332%
69	18.917	2625	2626	2629	rVB	802	783	0.15%	0.034%
70	18.958	2631	2633	2634	rBV	1512	825	0.16%	0.036%

71	18.981	2634	2637	2638	rBV	889	919	0.18%	0.040%
72	18.999	2638	2640	2642	rVB2	1349	859	0.17%	0.037%
73	19.017	2642	2643	2644	rBV	1200	583	0.11%	0.025%
74	19.075	2649	2653	2654	rVV	1205	1225	0.24%	0.053%
75	19.093	2654	2656	2658	rVV2	1547	1361	0.26%	0.059%

76	19.128	2660	2662	2667	rBV	822	1037	0.20%	0.045%
----	--------	------	------	------	-----	-----	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030322\
 Data File : BG052579.D
 Acq On : 4 Mar 2022 15:11
 Operator : CG/JU
 Sample : N1697-03
 Misc : GCMS CONFIRMATION
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGZJ8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
 Title : SVOA CALIBRATION

77	19.211	2674	2676	2677	rBV	732	729	0.14%	0.032%
78	19.269	2685	2686	2688	rBV	1708	1243	0.24%	0.054%
79	19.328	2692	2696	2699	rVB4	965	1673	0.33%	0.072%
80	19.387	2705	2706	2711	rBV3	2354	2626	0.51%	0.114%
81	19.440	2713	2715	2716	rBV2	1075	800	0.16%	0.035%
82	19.510	2724	2727	2729	rBV3	3295	3486	0.68%	0.151%
83	19.575	2736	2738	2739	rBV2	924	824	0.16%	0.036%
84	19.610	2743	2744	2748	rVB2	1684	1604	0.31%	0.069%
85	19.663	2748	2753	2758	rBV2	10548	17096	3.32%	0.740%
86	19.698	2758	2759	2760	rBV	1648	716	0.14%	0.031%
87	19.780	2771	2773	2778	rVB2	5892	6995	1.36%	0.303%
88	19.845	2782	2784	2785	rBV2	2233	1700	0.33%	0.074%
89	19.927	2796	2798	2799	rBV2	1285	661	0.13%	0.029%
90	20.021	2811	2814	2817	rBV3	4513	5841	1.14%	0.253%
91	20.192	2842	2843	2844	rBV	2591	1368	0.27%	0.059%
92	20.227	2847	2849	2853	rVB4	4583	5604	1.09%	0.242%
93	20.291	2859	2860	2861	rBV	1897	860	0.17%	0.037%
94	20.491	2889	2894	2897	rBV5	11729	14971	2.91%	0.648%
95	20.615	2913	2915	2917	rBV3	2576	1981	0.39%	0.086%
96	20.761	2937	2940	2944	rVB5	8240	9821	1.91%	0.425%
97	21.719	3101	3103	3107	rVB5	4376	4879	0.95%	0.211%
98	21.925	3131	3138	3146	rBV2	283351	514324	100.00%	22.250%
99	24.357	3548	3552	3560	rVB5	16281	36063	7.01%	1.560%
100	25.390	3717	3728	3739	rVB2	158641	494261	96.10%	21.382%




Sum of corrected areas: 2311554

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030322\
Data File : BG052579.D
Acq On : 4 Mar 2022 15:11
Operator : CG/JU
Sample : N1697-03
Misc : GCMS CONFIRMATION
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGZJ8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

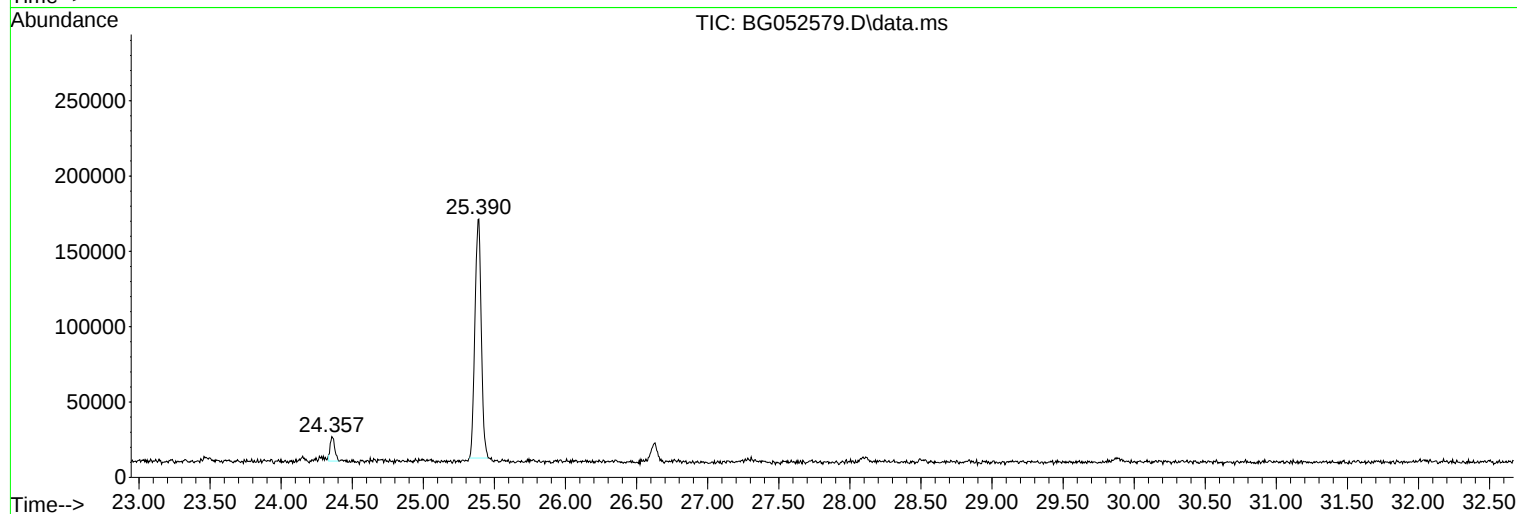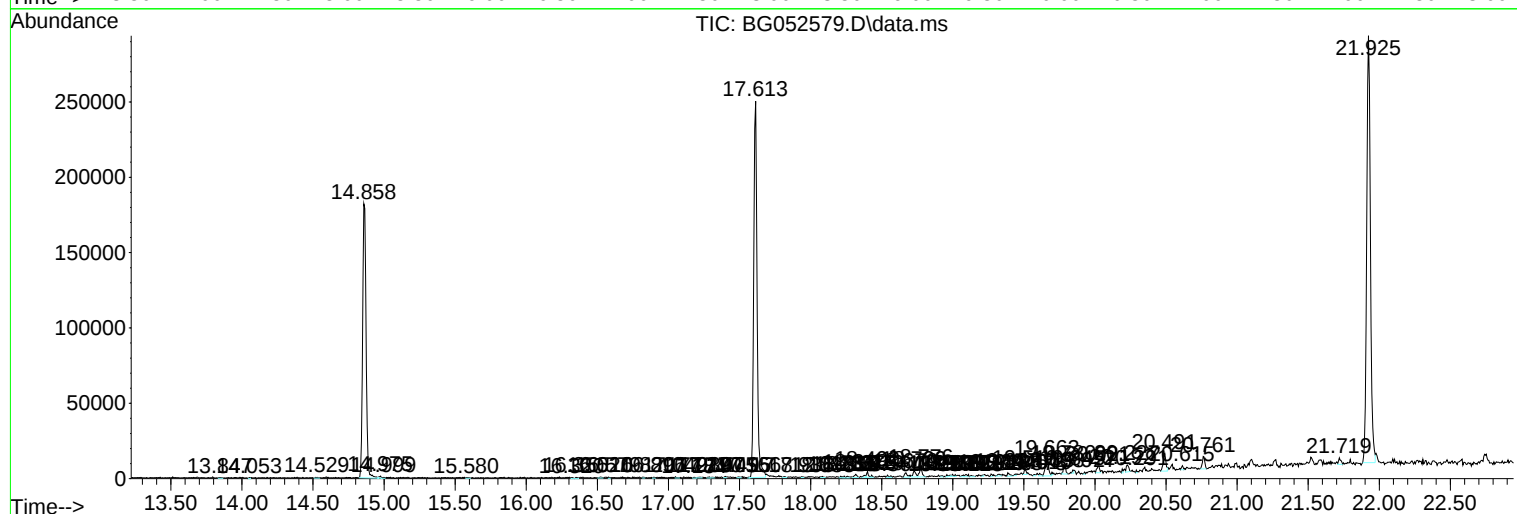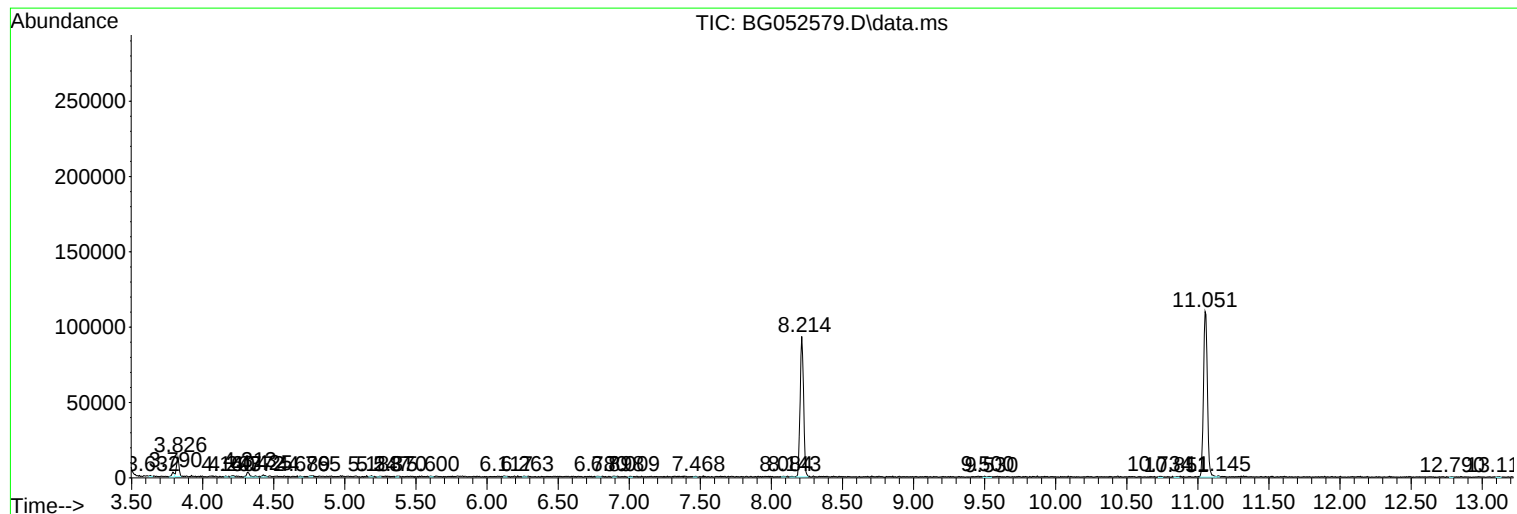

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030322\
Data File : BG052579.D
Acq On : 4 Mar 2022 15:11
Operator : CG/JU
Sample : N1697-03
Misc : GCMS CONFIRMATION
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGZJ8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030322\
Data File : BG052579.D
Acq On : 4 Mar 2022 15:11
Operator : CG/JU
Sample : N1697-03
Misc : GCMS CONFIRMATION
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGZJ8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc