
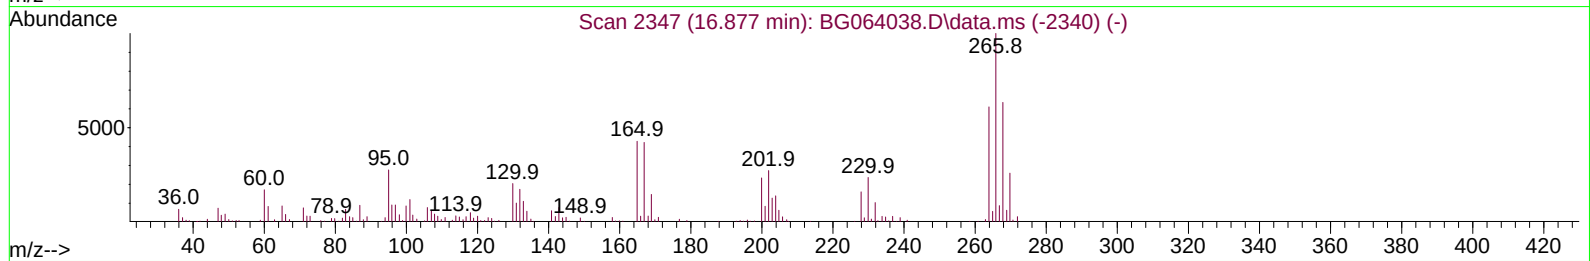
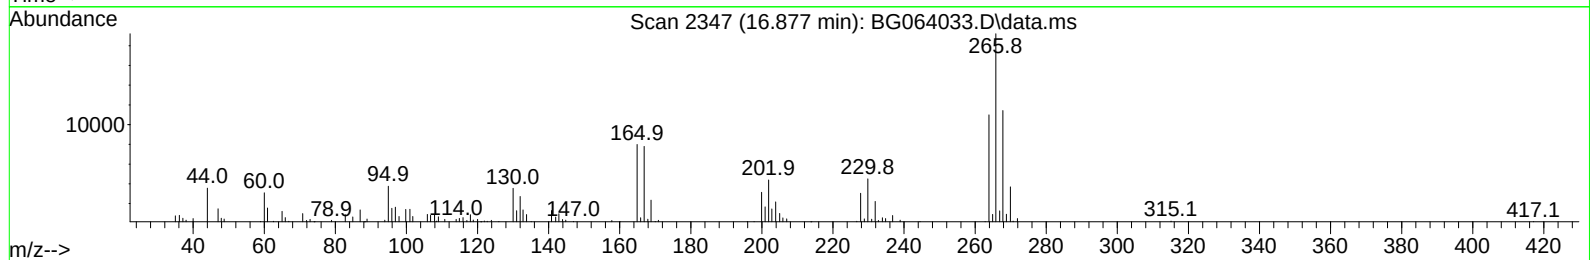


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030325\
Data File : BG064033.D
Acq On : 3 Mar 2025 10:35
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 04 08:37:18 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 04 08:17:09 2025
Response via : Initial Calibration

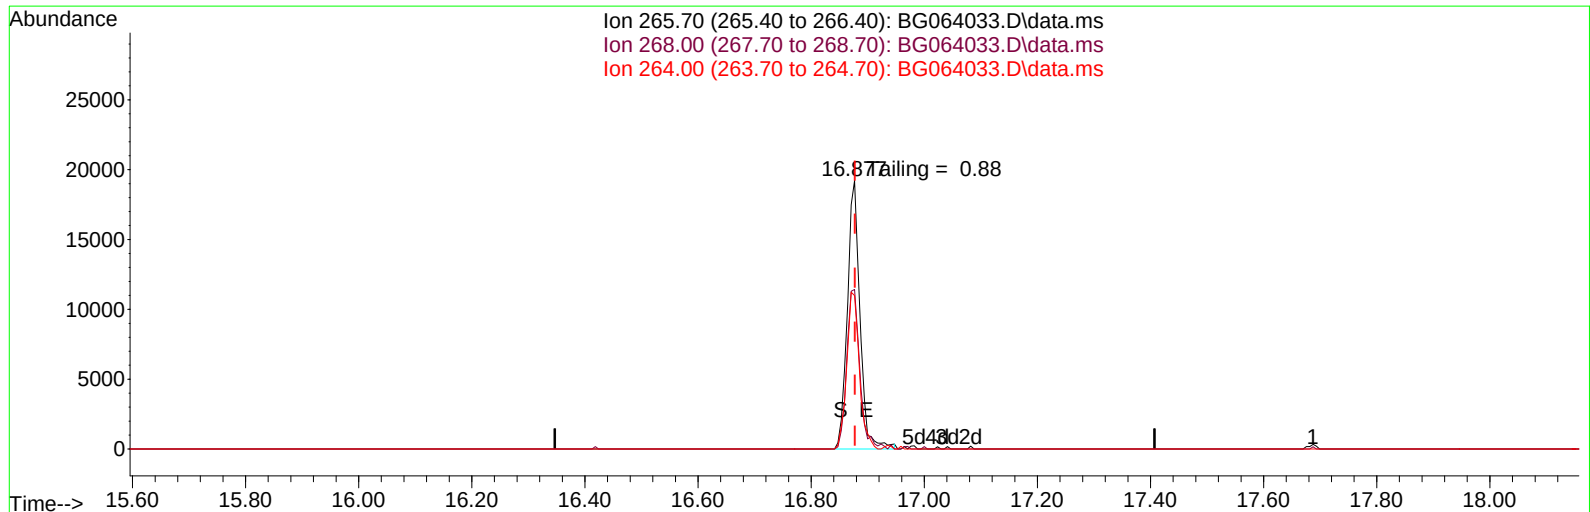

TIC: BG064033.D\data.ms

(70) Pentachlorophenol (C)




16.877min (-0.000) 68188.31 ng m

response 29855

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.40	59.47
264.00	61.00	57.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030325\
Data File : BG064033.D
Acq On : 3 Mar 2025 10:35
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 04 08:37:18 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 04 08:17:09 2025
Response via : Initial Calibration

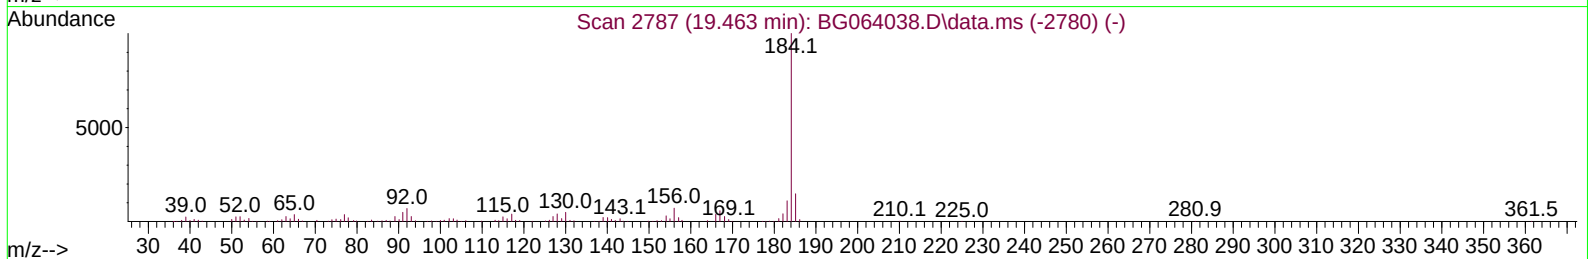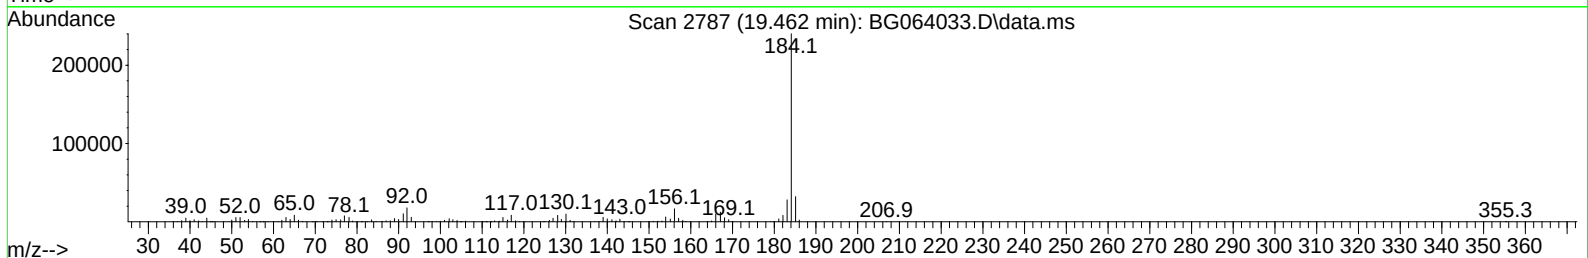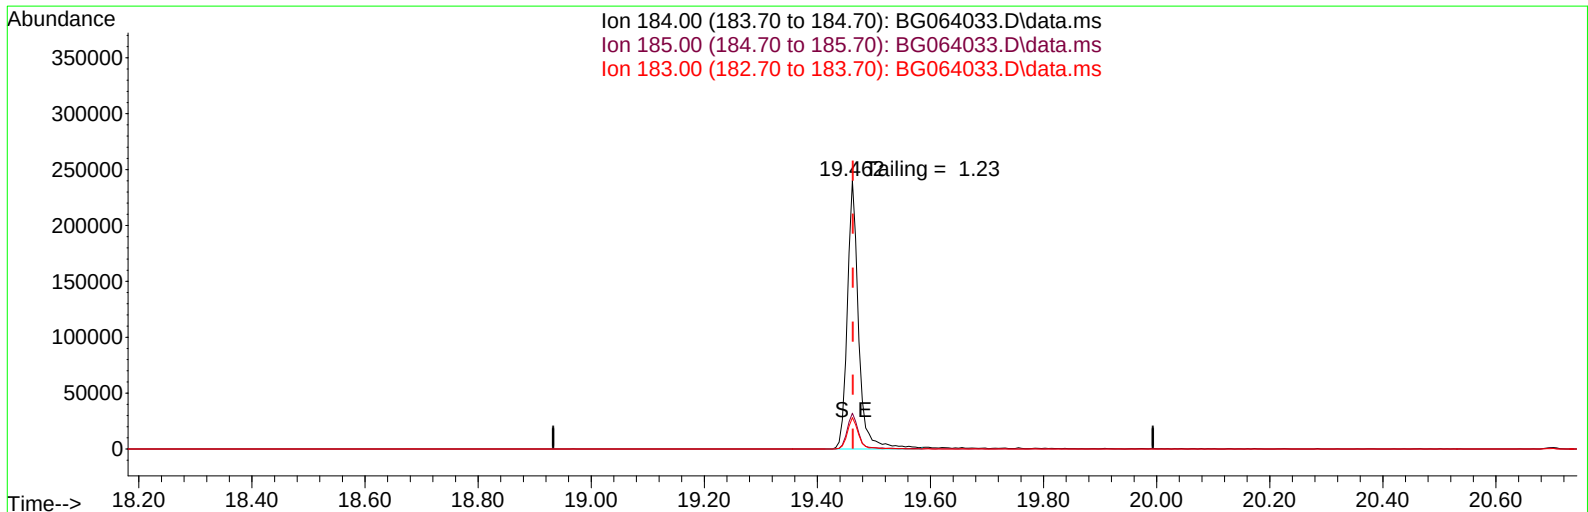

TIC: BG064033.D\data.ms

(77) Benzidine

19.462min (-0.001) 0.00 ng

response 332587

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	13.39
183.00	11.00	11.72
0.00	0.00	0.00