
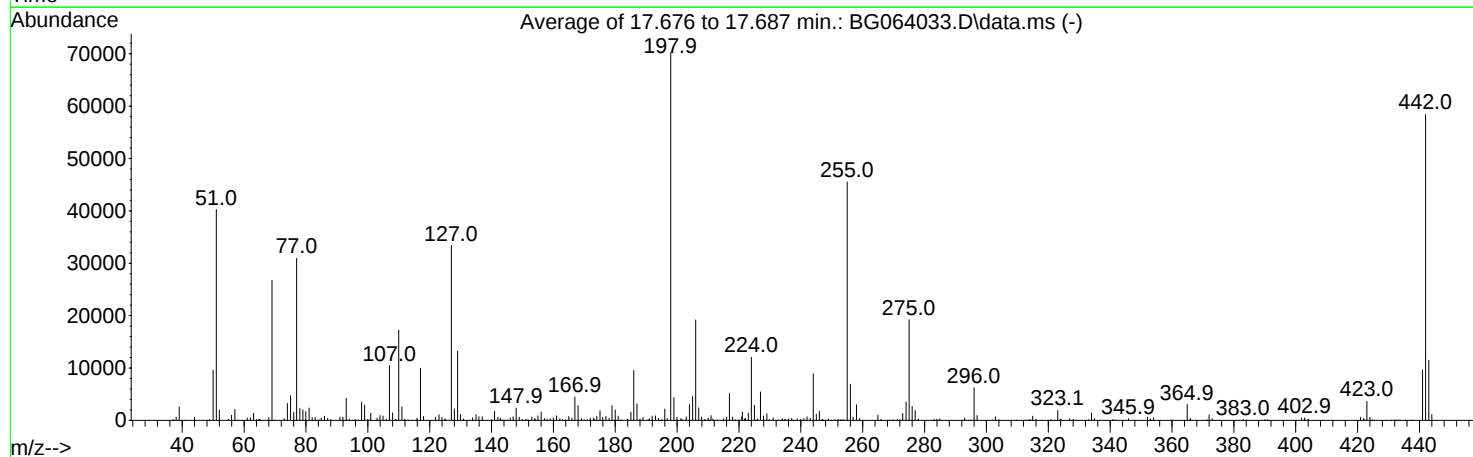


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030325\
Data File : BG064033.D
Acq On : 3 Mar 2025 10:35
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030325.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Mar 04 08:17:09 2025

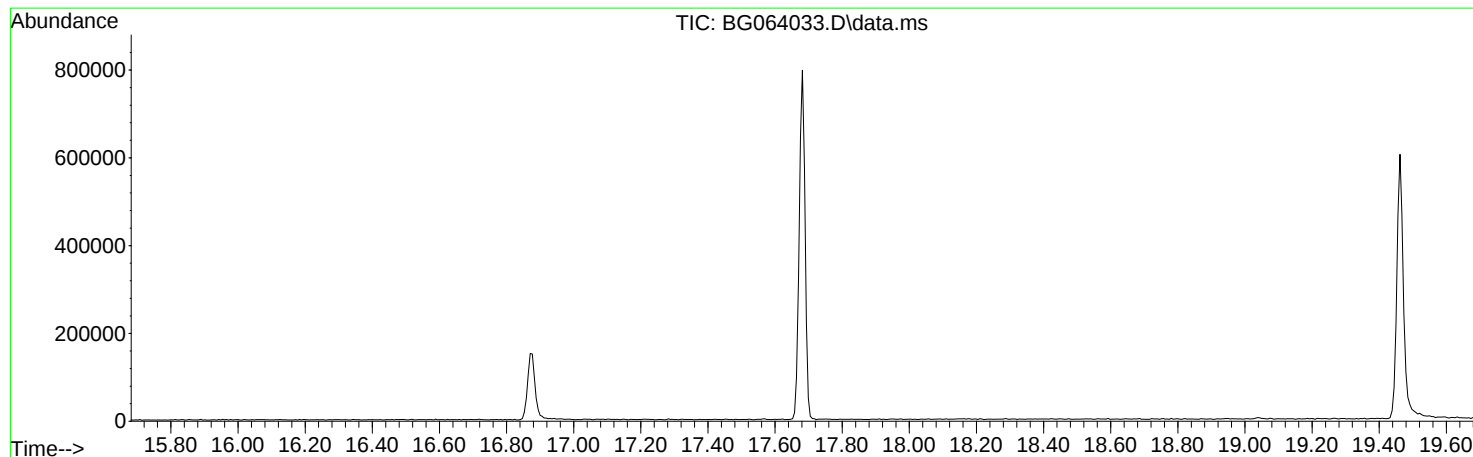




AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.3	40272	PASS
68	69	0.00	2	1.9	521	PASS
69	198	0.00	100	38.1	26765	PASS
70	69	0.00	2	0.2	64	PASS
127	198	10	80	47.5	33397	PASS
197	198	0.00	2	0.5	337	PASS
198	198	100	100	100.0	70240	PASS
199	198	5	9	6.2	4376	PASS
275	198	10	60	27.4	19229	PASS
365	198	1	100	4.3	3048	PASS
441	198	0.01	100	13.7	9631	PASS
442	442	50	100	100.0	58427	PASS
443	442	15	24	19.6	11479	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030325\
Data File : BG064033.D
Acq On : 3 Mar 2025 10:35
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 04 08:37:18 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 04 08:17:09 2025
Response via : Initial Calibration

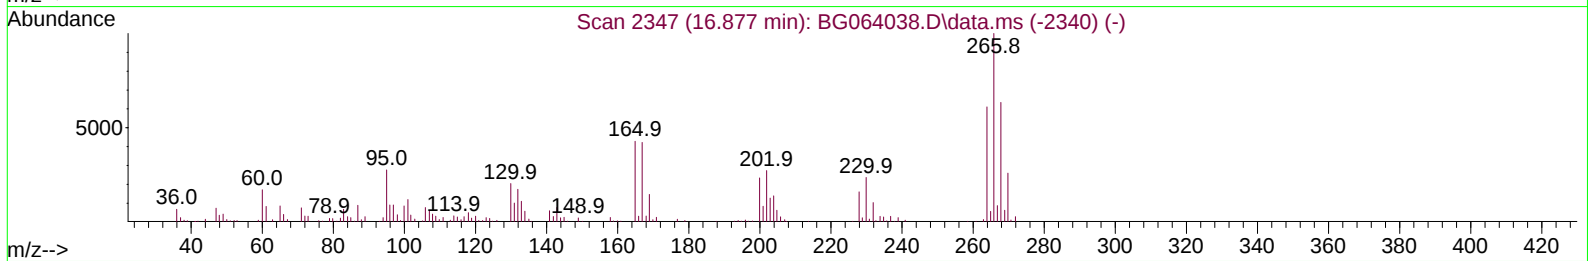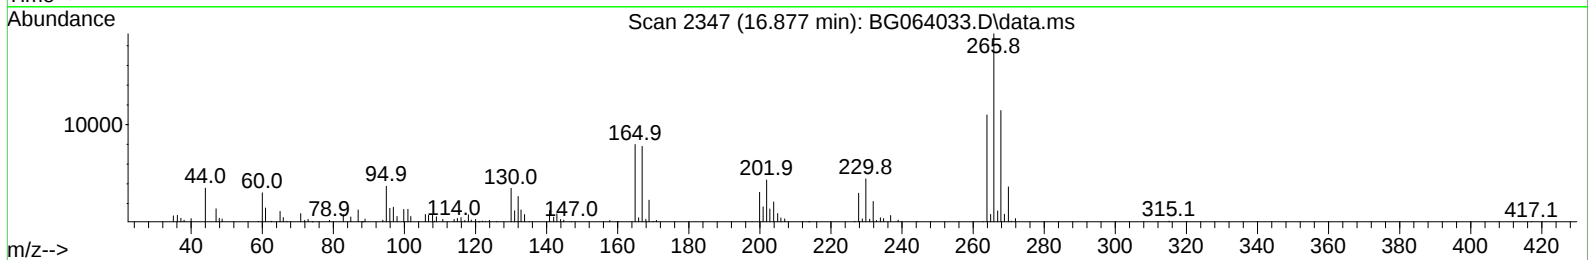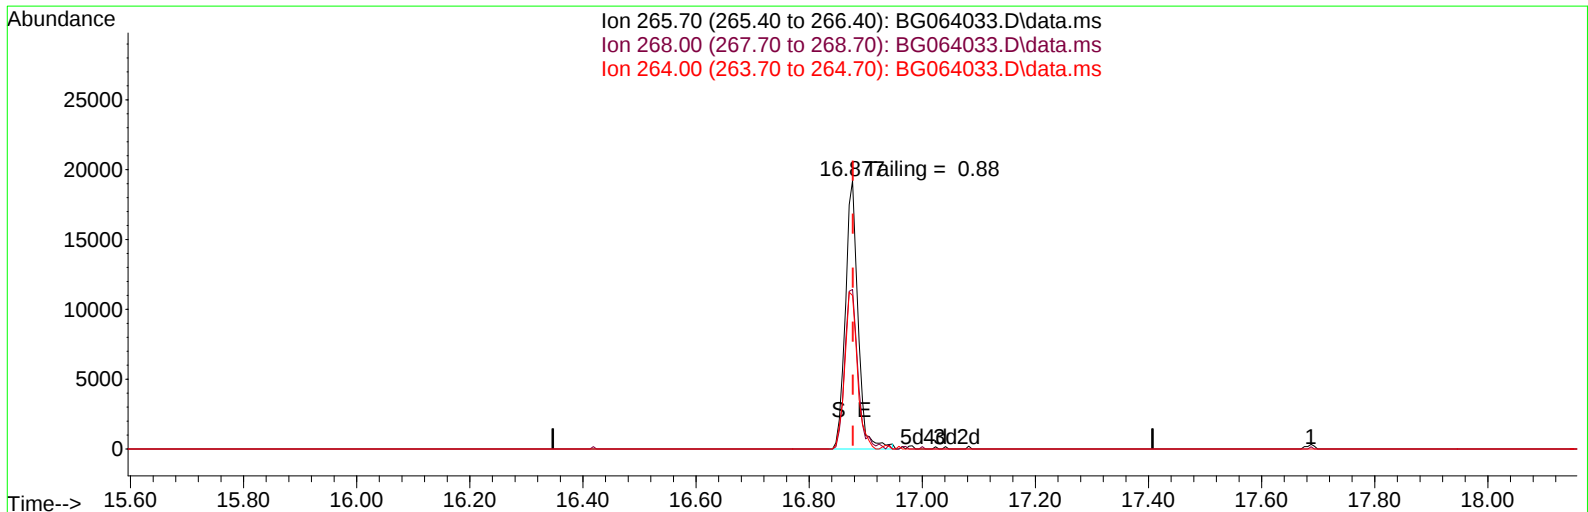

TIC: BG064033.D\data.ms

(70) Pentachlorophenol (C)

16.877min (-0.000) 68188.31 ng m




response 29855

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.40	59.47
264.00	61.00	57.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030325\
Data File : BG064033.D
Acq On : 3 Mar 2025 10:35
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 04 08:37:18 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 04 08:17:09 2025
Response via : Initial Calibration

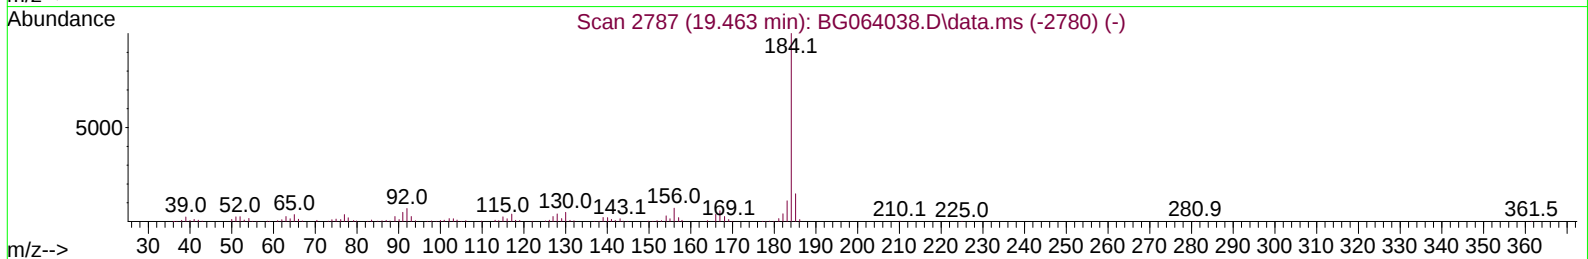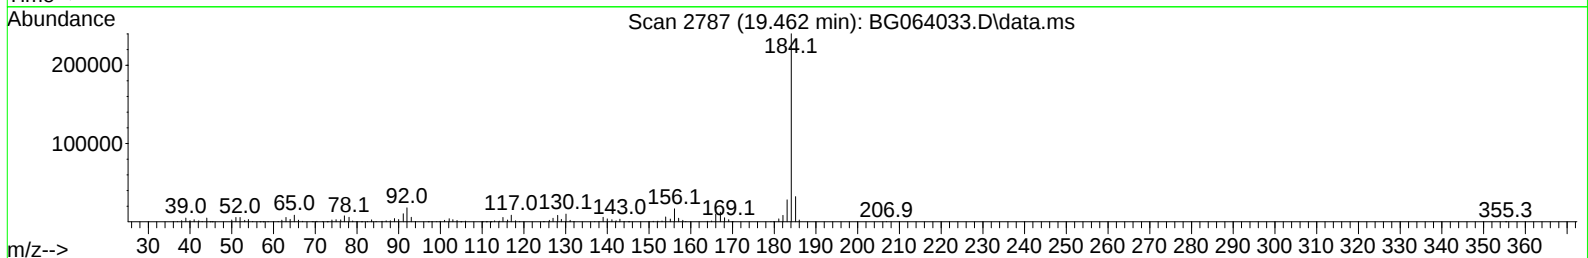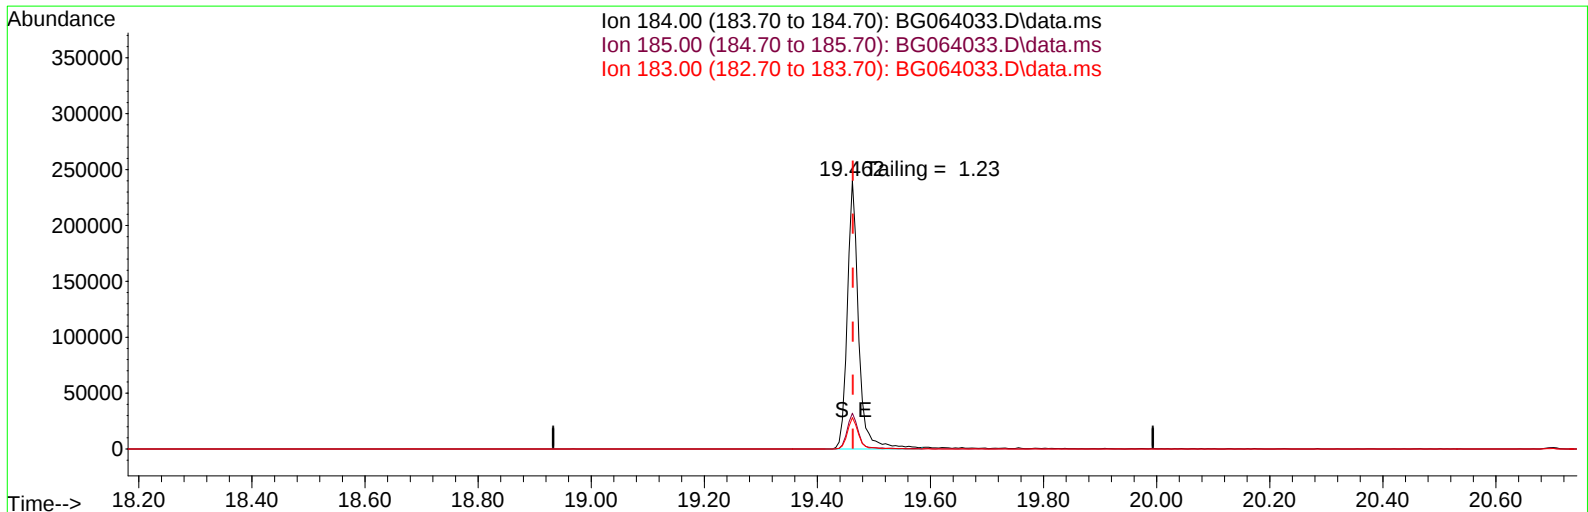

TIC: BG064033.D\data.ms

(77) Benzidine

19.462min (-0.001) 0.00 ng

response 332587

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	13.39
183.00	11.00	11.72
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/3/2025	BNA_G	<u>BG064033.D</u>
Compound Name	Response	Retention Time
DDT	117779	20.701
DDD	1502	20.314
DDE	0	19.786
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1502	119281	1.26

Instrument :
BNA_G
ClientSampleId :
DFTPP