

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030416\
 Data File : BG021275.D
 Acq On : 4 Mar 2016 18:14
 Operator : UM/SJ
 Sample : PB88618TB
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SLEB15

Quant Time: Mar 05 00:58:17 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Mar 05 00:52:50 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.13	152	8574	20.00	ng/ul	0.00
18) Naphthalene-d8	10.94	136	41222	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.74	164	24719	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.47	188	57069	20.00	ng/ul	0.00
78) Chrysene-d12	21.74	240	63792	20.00	ng/ul	0.00
86) Perylene-d12	24.99	264	59488	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.54	96	1650	7.82	ng/uL	0.00
5) Phenol-d5	7.27	99	34991	38.53	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.45	67	25614	42.30	ng/ul	0.00
9) 2-Chlorophenol-d4	7.66	132	25588	40.39	ng/ul	0.00
13) 4-Methylphenol-d8	8.82	113	28029	39.09	ng/ul	0.00
19) Nitrobenzene-d5	9.29	128	13801	41.33	ng/ul	0.00
22) 2-Nitrophenol-d4	10.02	143	14576	40.94	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.55	165	23135	36.37	ng/ul	0.00
29) 4-Chloroaniline-d4	11.07	131	38743	48.03	ng/ul	0.00
44) Dimethylphthalate-d6	14.14	166	88862	42.90	ng/ul	0.00
47) Acenaphthylene-d8	14.44	160	108115	41.94	ng/ul	0.00
52) 4-Nitrophenol-d4	14.92	143	15749	39.01	ng/ul	0.00
58) Fluorene-d10	15.73	176	76028	41.79	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.83	200	14436	35.25	ng/ul	0.00
71) Anthracene-d10	17.57	188	123682	43.58	ng/ul	0.00
79) Pyrene-d10	19.85	212	143544	44.45	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.78	264	137376	42.78	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
15) N-Nitroso-di-n-propylamine	8.82	70	942	1.25	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030416\
Data File : BG021275.D
Acq On : 4 Mar 2016 18:14
Operator : UM/SJ
Sample : PB88618TB
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SLEB15

Quant Time: Mar 05 00:58:17 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Mar 05 00:52:50 2016
Response via : Initial Calibration

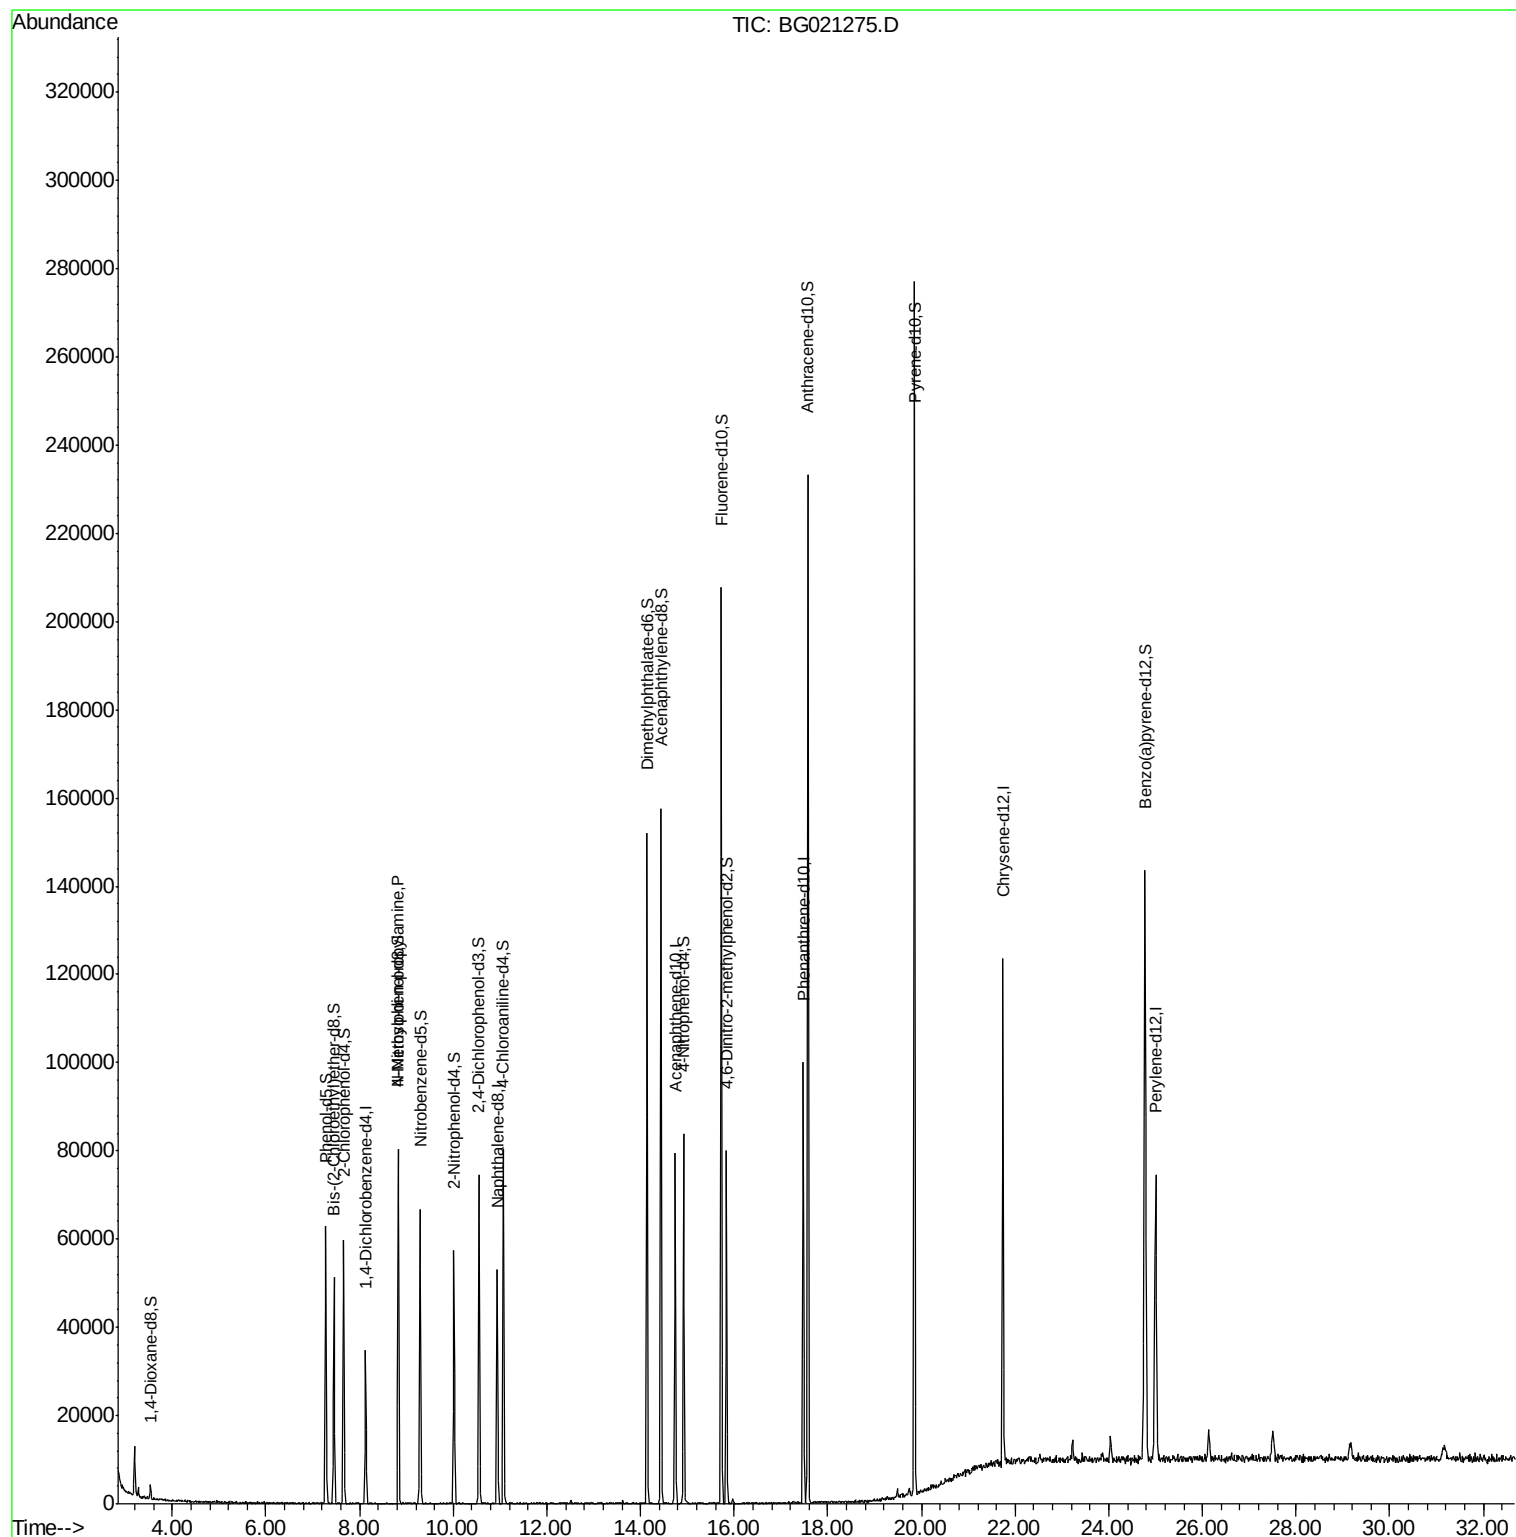

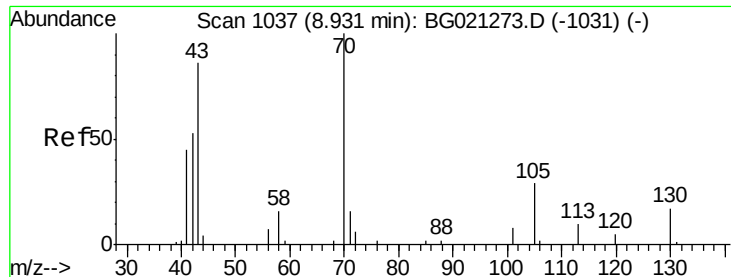

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.25 ng/ul
 RT: 8.82 min Scan# 1019
 Delta R.T. -0.11 min
 Lab File: BG021275.D
 Acq: 4 Mar 2016 18:14

Instrument :
 BNA_G
 ClientSampleId :
 SLEB15

Tgt Ion: 70 Resp: 942
 Ion Ratio Lower Upper
 70 100
 42 303.8 45.7 68.5#
 101 0.0 5.7 8.5#
 130 0.0 15.7 23.5#

