

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030416\
 Data File : BG021278.D
 Acq On : 4 Mar 2016 20:12
 Operator : UM/SJ
 Sample : H1626-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JHFH8

Quant Time: Mar 05 00:58:41 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Mar 05 00:52:50 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.13	152	10672	20.00	ng/ul	0.00
18) Naphthalene-d8	10.94	136	51872	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.74	164	31270	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.48	188	75900	20.00	ng/ul	0.00
78) Chrysene-d12	21.73	240	83930	20.00	ng/ul	0.00
86) Perylene-d12	25.00	264	75998	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.53	96	352	1.34	ng/uL	0.00
5) Phenol-d5	7.28	99	12685	11.22	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.45	67	9356	12.41	ng/ul	0.00
9) 2-Chlorophenol-d4	7.66	132	9069	11.50	ng/ul	0.00
13) 4-Methylphenol-d8	8.82	113	11040	12.37	ng/ul	0.00
19) Nitrobenzene-d5	9.29	128	5102	12.14	ng/ul	0.00
22) 2-Nitrophenol-d4	10.01	143	5119	11.43	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.55	165	9223	11.52	ng/ul	0.00
29) 4-Chloroaniline-d4	11.07	131	13983	13.77	ng/ul	0.00
44) Dimethylphthalate-d6	14.14	166	38648	14.75	ng/ul	0.00
47) Acenaphthylene-d8	14.43	160	46160	14.16	ng/ul	0.00
52) 4-Nitrophenol-d4	14.91	143	7128	13.96	ng/ul	0.00
58) Fluorene-d10	15.72	176	34229	14.87	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.83	200	6298	11.56	ng/ul	0.00
71) Anthracene-d10	17.58	188	59593	15.79	ng/ul	0.00
79) Pyrene-d10	19.85	212	75272	17.72	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.77	264	74359	18.12	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.19	163	14353	5.09	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030416\
Data File : BG021278.D
Acq On : 4 Mar 2016 20:12
Operator : UM/SJ
Sample : H1626-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JHFH8

Quant Time: Mar 05 00:58:41 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Mar 05 00:52:50 2016
Response via : Initial Calibration

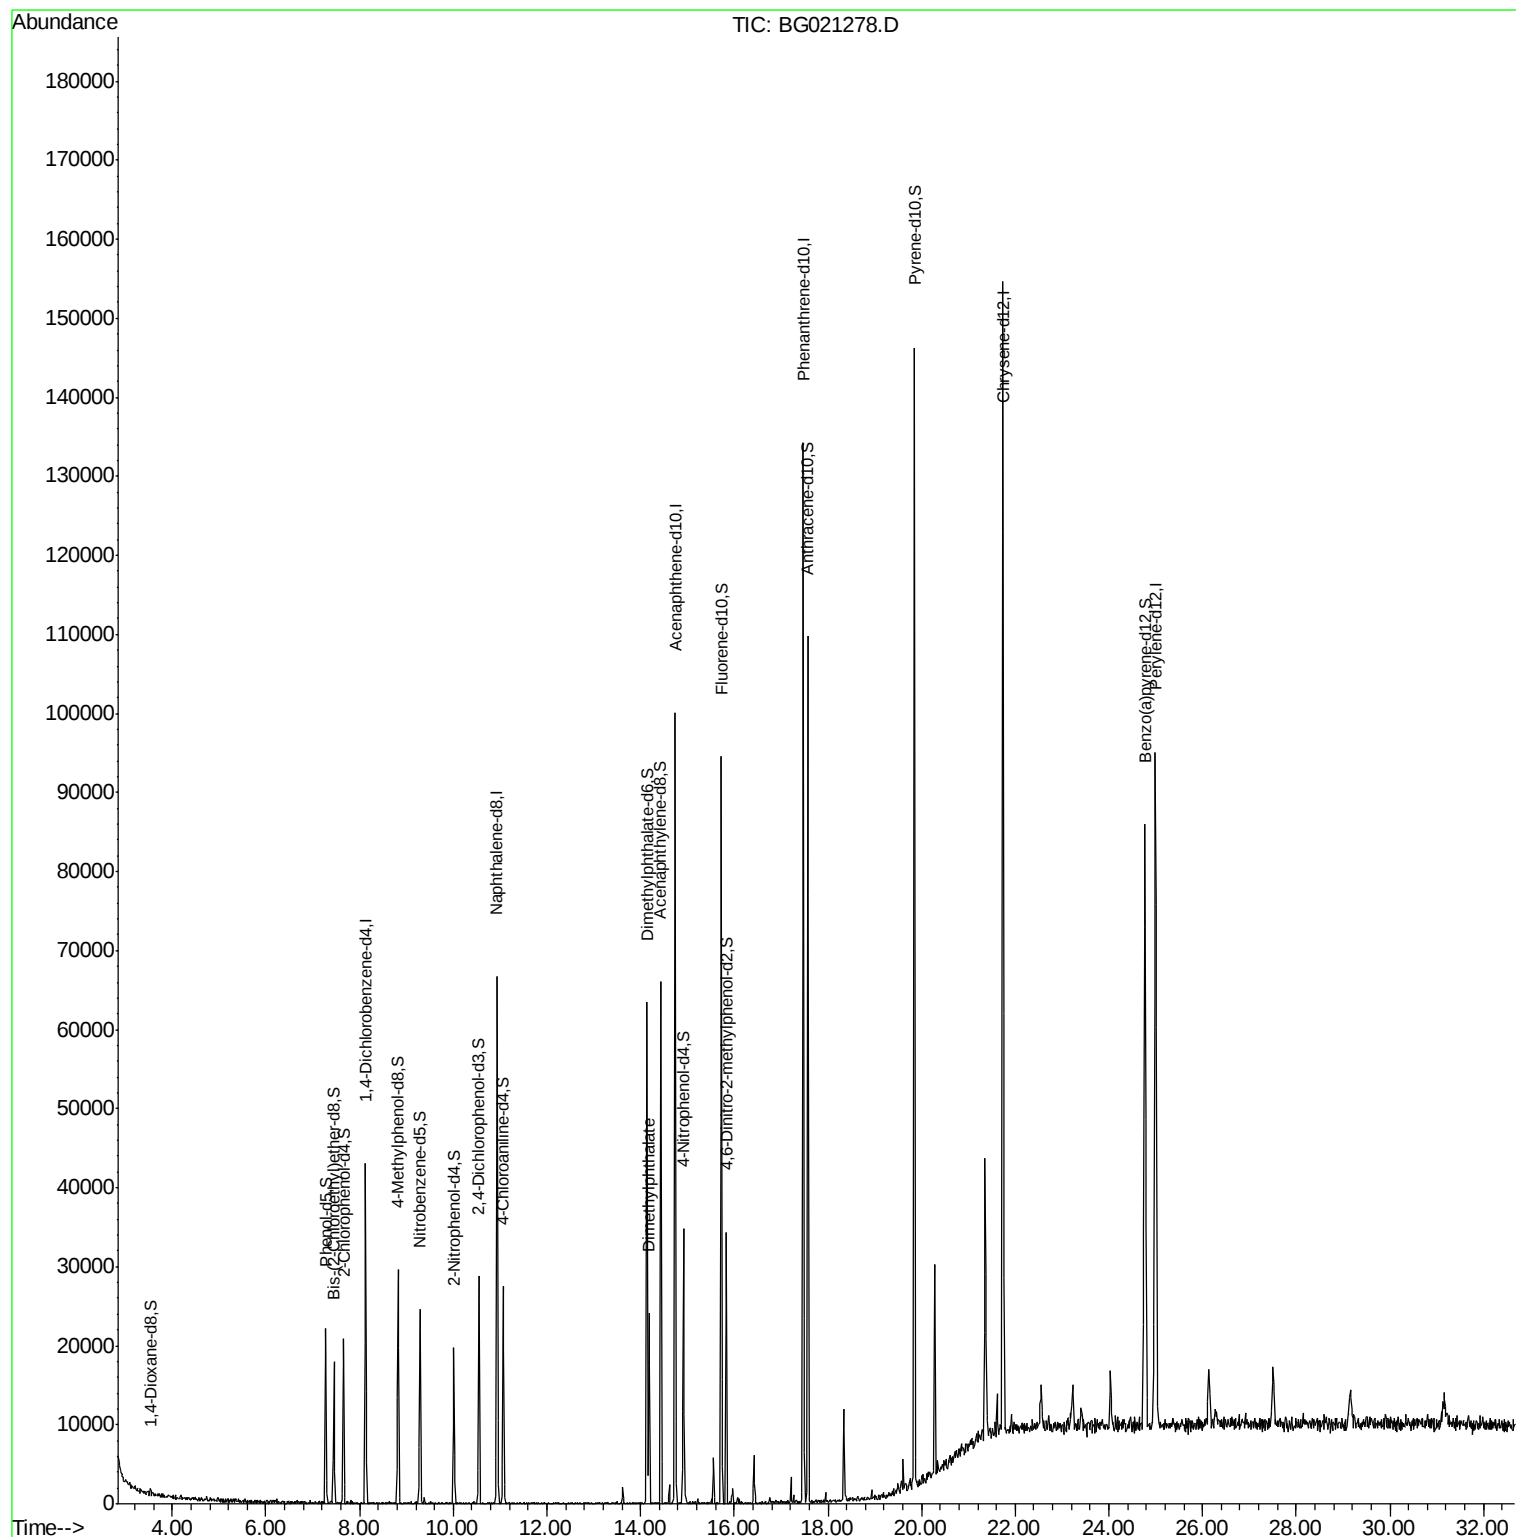

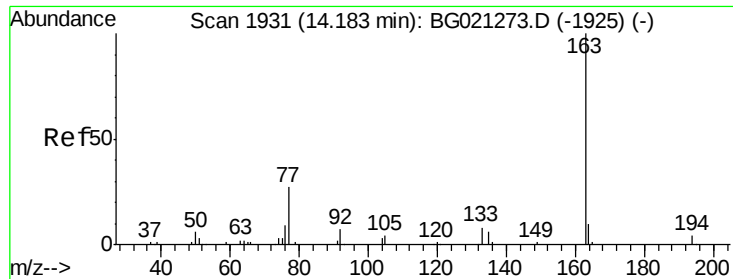

#45

Dimethylphthalate

Concen: 5.09 ng/ul

RT: 14.19 min Scan# 1931

Delta R.T. 0.00 min

Lab File: BG021278.D


Acq: 4 Mar 2016 20:12

Instrument :

BNA_G

ClientSampleId :

JH8

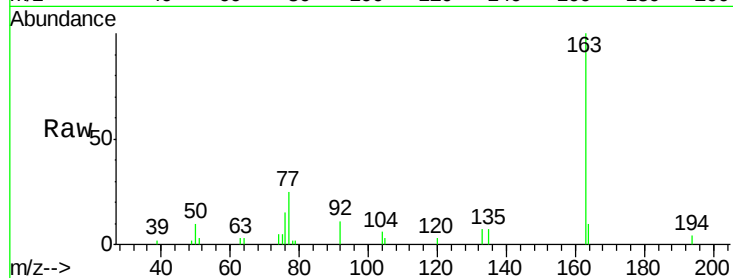


Tgt Ion:163 Resp: 14353

Ion Ratio Lower Upper

163 100

194 4.1 2.8 4.2

164 9.8 8.2 12.2

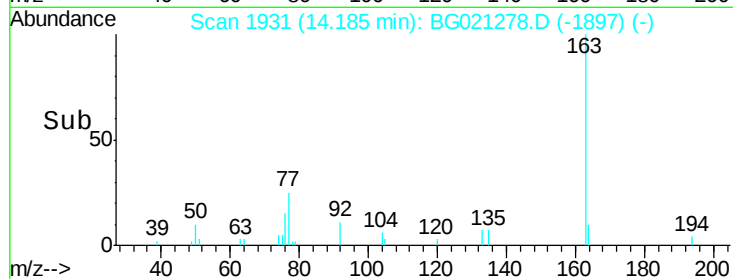

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

