

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030416\
 Data File : BG021279.D
 Acq On : 4 Mar 2016 20:51
 Operator : UM/SJ
 Sample : H1626-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JHFH9

Quant Time: Mar 05 00:58:48 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Mar 05 00:52:50 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.13	152	9342	20.00	ng/ul	0.00
18) Naphthalene-d8	10.94	136	44709	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.74	164	26359	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.47	188	61236	20.00	ng/ul	0.00
78) Chrysene-d12	21.74	240	67026	20.00	ng/ul	0.00
86) Perylene-d12	25.00	264	62555	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.53	96	1109	4.82	ng/uL	0.00
5) Phenol-d5	7.27	99	28007	28.31	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.45	67	22720	34.44	ng/ul	0.00
9) 2-Chlorophenol-d4	7.66	132	22478	32.56	ng/ul	0.00
13) 4-Methylphenol-d8	8.83	113	18462	23.63	ng/ul	0.00
19) Nitrobenzene-d5	9.29	128	12198	33.68	ng/ul	0.00
22) 2-Nitrophenol-d4	10.01	143	12629	32.71	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.55	165	21942	31.80	ng/ul	0.00
29) 4-Chloroaniline-d4	11.06	131	24086	27.53	ng/ul	0.00
44) Dimethylphthalate-d6	14.14	166	78633	35.60	ng/ul	0.00
47) Acenaphthylene-d8	14.44	160	99864	36.33	ng/ul	0.00
52) 4-Nitrophenol-d4	14.92	143	11664	27.09	ng/ul	0.00
58) Fluorene-d10	15.73	176	72025	37.13	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.84	200	13168	29.96	ng/ul	0.00
71) Anthracene-d10	17.57	188	113778	37.36	ng/ul	0.00
79) Pyrene-d10	19.85	212	130685	38.52	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.77	264	129271	38.28	ng/ul	0.00


Target Compounds					Qvalue
45) Dimethylphthalate	14.18	163	31742	13.36 ng/ul#	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030416\
Data File : BG021279.D
Acq On : 4 Mar 2016 20:51
Operator : UM/SJ
Sample : H1626-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JHFH9

Quant Time: Mar 05 00:58:48 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Mar 05 00:52:50 2016
Response via : Initial Calibration

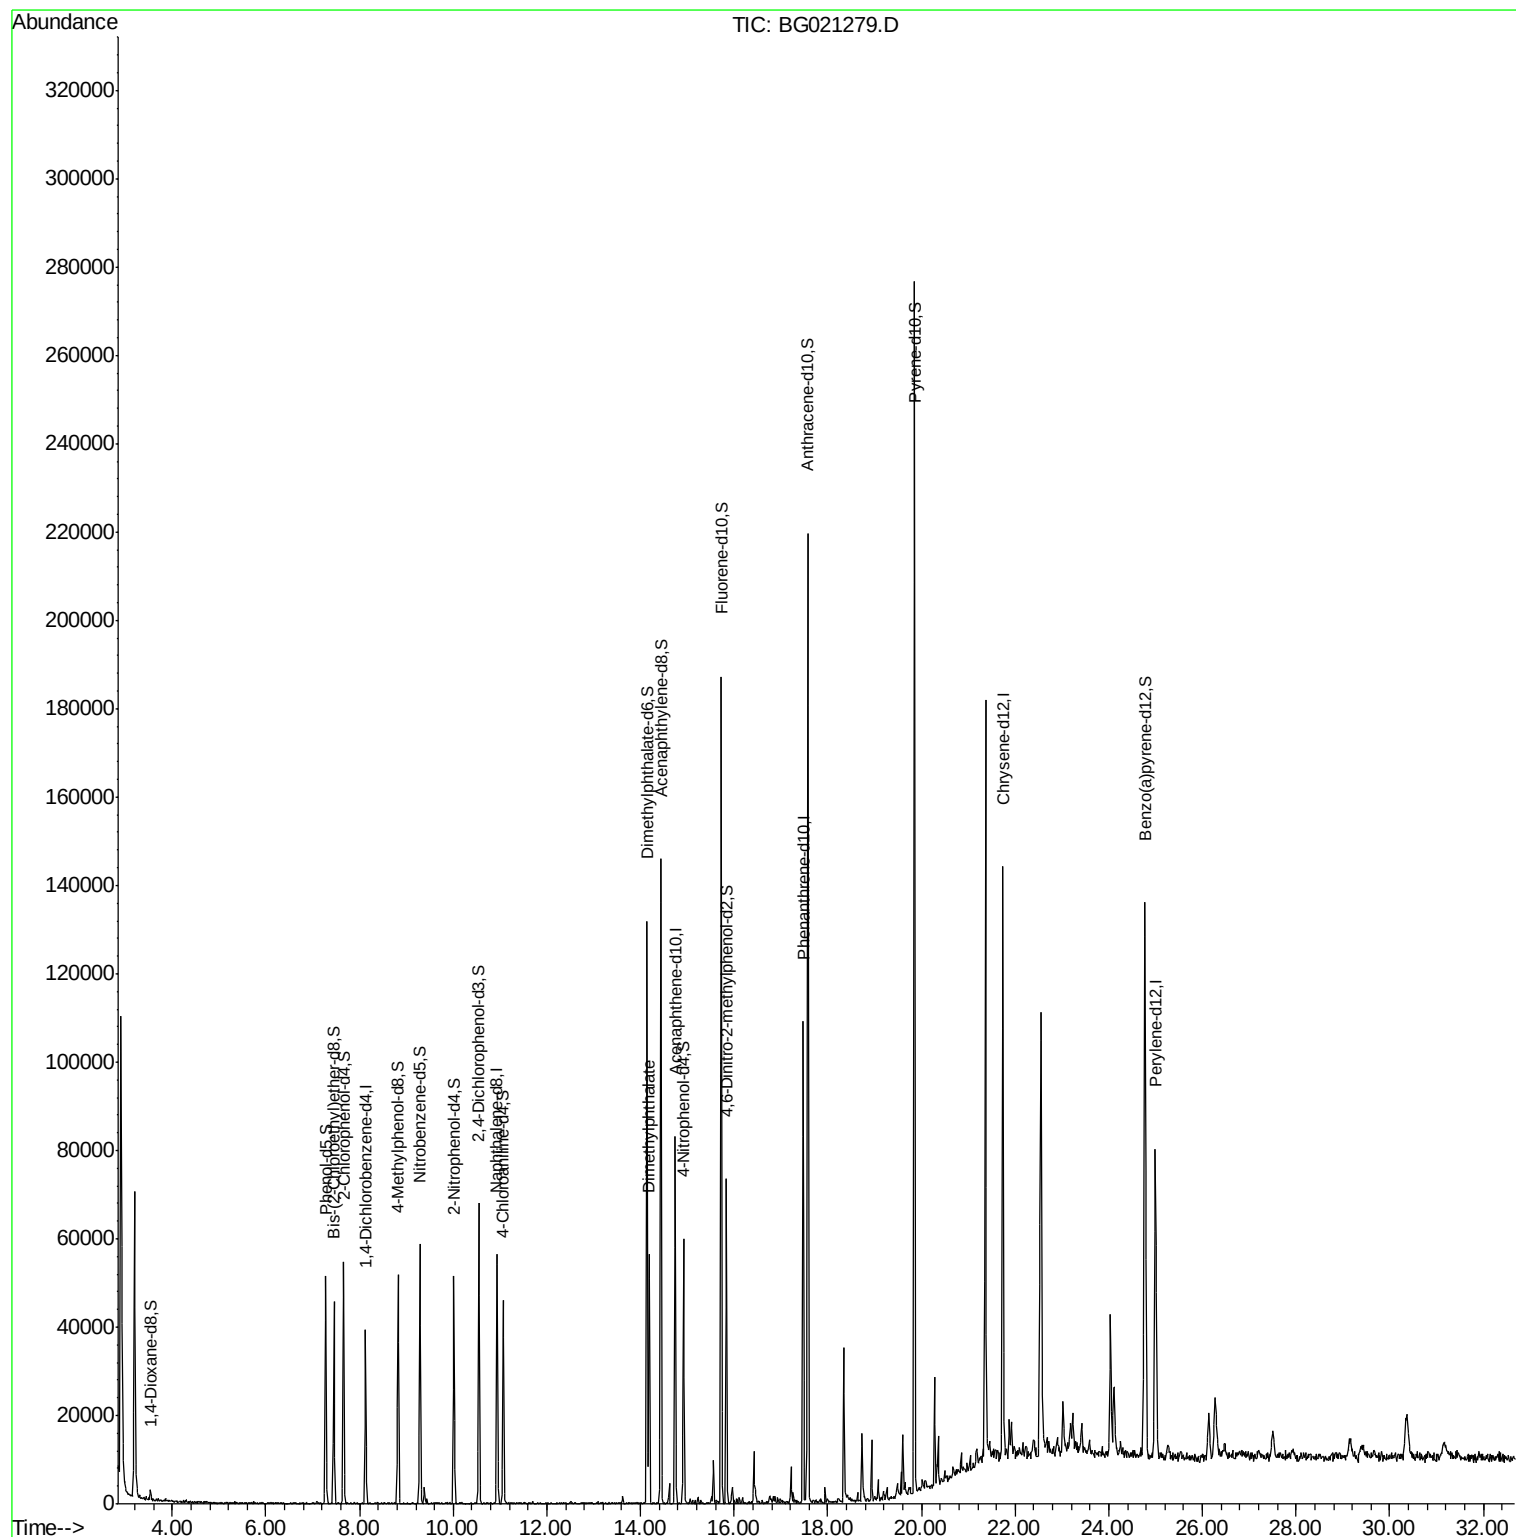

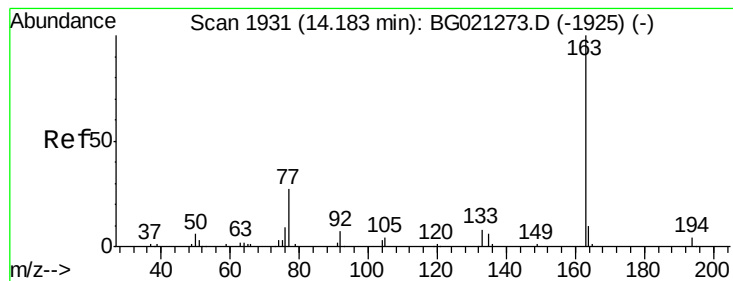

#45

Dimethylphthalate

Concen: 13.36 ng/ul

RT: 14.18 min Scan# 1931

Delta R.T. 0.00 min

Lab File: BG021279.D


Acq: 4 Mar 2016 20:51

Instrument :

BNA_G

ClientSampleId :

JH9H9

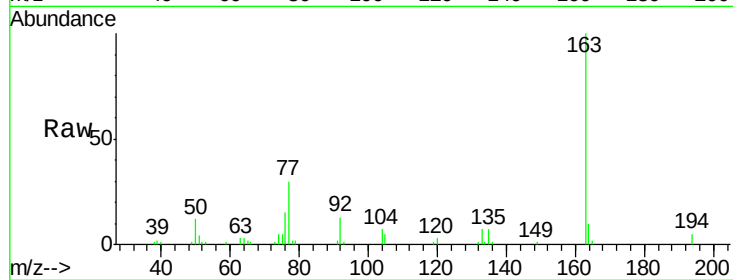

Tgt Ion:	163	Resp:	31742
Ion	Ratio	Lower	Upper
163	100		
194	4.6	2.8	4.2#
164	9.6	8.2	12.2

