

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030416\
 Data File : BG021280.D
 Acq On : 4 Mar 2016 21:31
 Operator : UM/SJ
 Sample : H1626-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JHFJ0

Quant Time: Mar 05 00:58:55 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Mar 05 00:52:50 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.13	152	10567	20.00	ng/ul	0.00
18) Naphthalene-d8	10.94	136	49139	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.74	164	29458	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.47	188	72104	20.00	ng/ul	0.00
78) Chrysene-d12	21.74	240	78541	20.00	ng/ul	0.00
86) Perylene-d12	24.99	264	72246	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.53	96	1073	4.12	ng/uL	0.00
5) Phenol-d5	7.27	99	27367	24.45	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.45	67	19113	25.61	ng/ul	0.00
9) 2-Chlorophenol-d4	7.66	132	19716	25.25	ng/ul	0.00
13) 4-Methylphenol-d8	8.82	113	22506	25.47	ng/ul	0.00
19) Nitrobenzene-d5	9.29	128	10459	26.27	ng/ul	0.00
22) 2-Nitrophenol-d4	10.02	143	10910	25.71	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.55	165	19502	25.72	ng/ul	0.00
29) 4-Chloroaniline-d4	11.07	131	29686	30.87	ng/ul	0.00
44) Dimethylphthalate-d6	14.14	166	75724	30.67	ng/ul	0.00
47) Acenaphthylene-d8	14.44	160	91319	29.73	ng/ul	0.00
52) 4-Nitrophenol-d4	14.92	143	14200	29.51	ng/ul	0.00
58) Fluorene-d10	15.72	176	66954	30.88	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.83	200	13154	25.42	ng/ul	0.00
71) Anthracene-d10	17.57	188	112477	31.37	ng/ul	0.00
79) Pyrene-d10	19.85	212	128804	32.40	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.78	264	122723	31.47	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.18	163	33008	12.43	ng/ul#	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030416\
Data File : BG021280.D
Acq On : 4 Mar 2016 21:31
Operator : UM/SJ
Sample : H1626-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JHFJ0

Quant Time: Mar 05 00:58:55 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Mar 05 00:52:50 2016
Response via : Initial Calibration

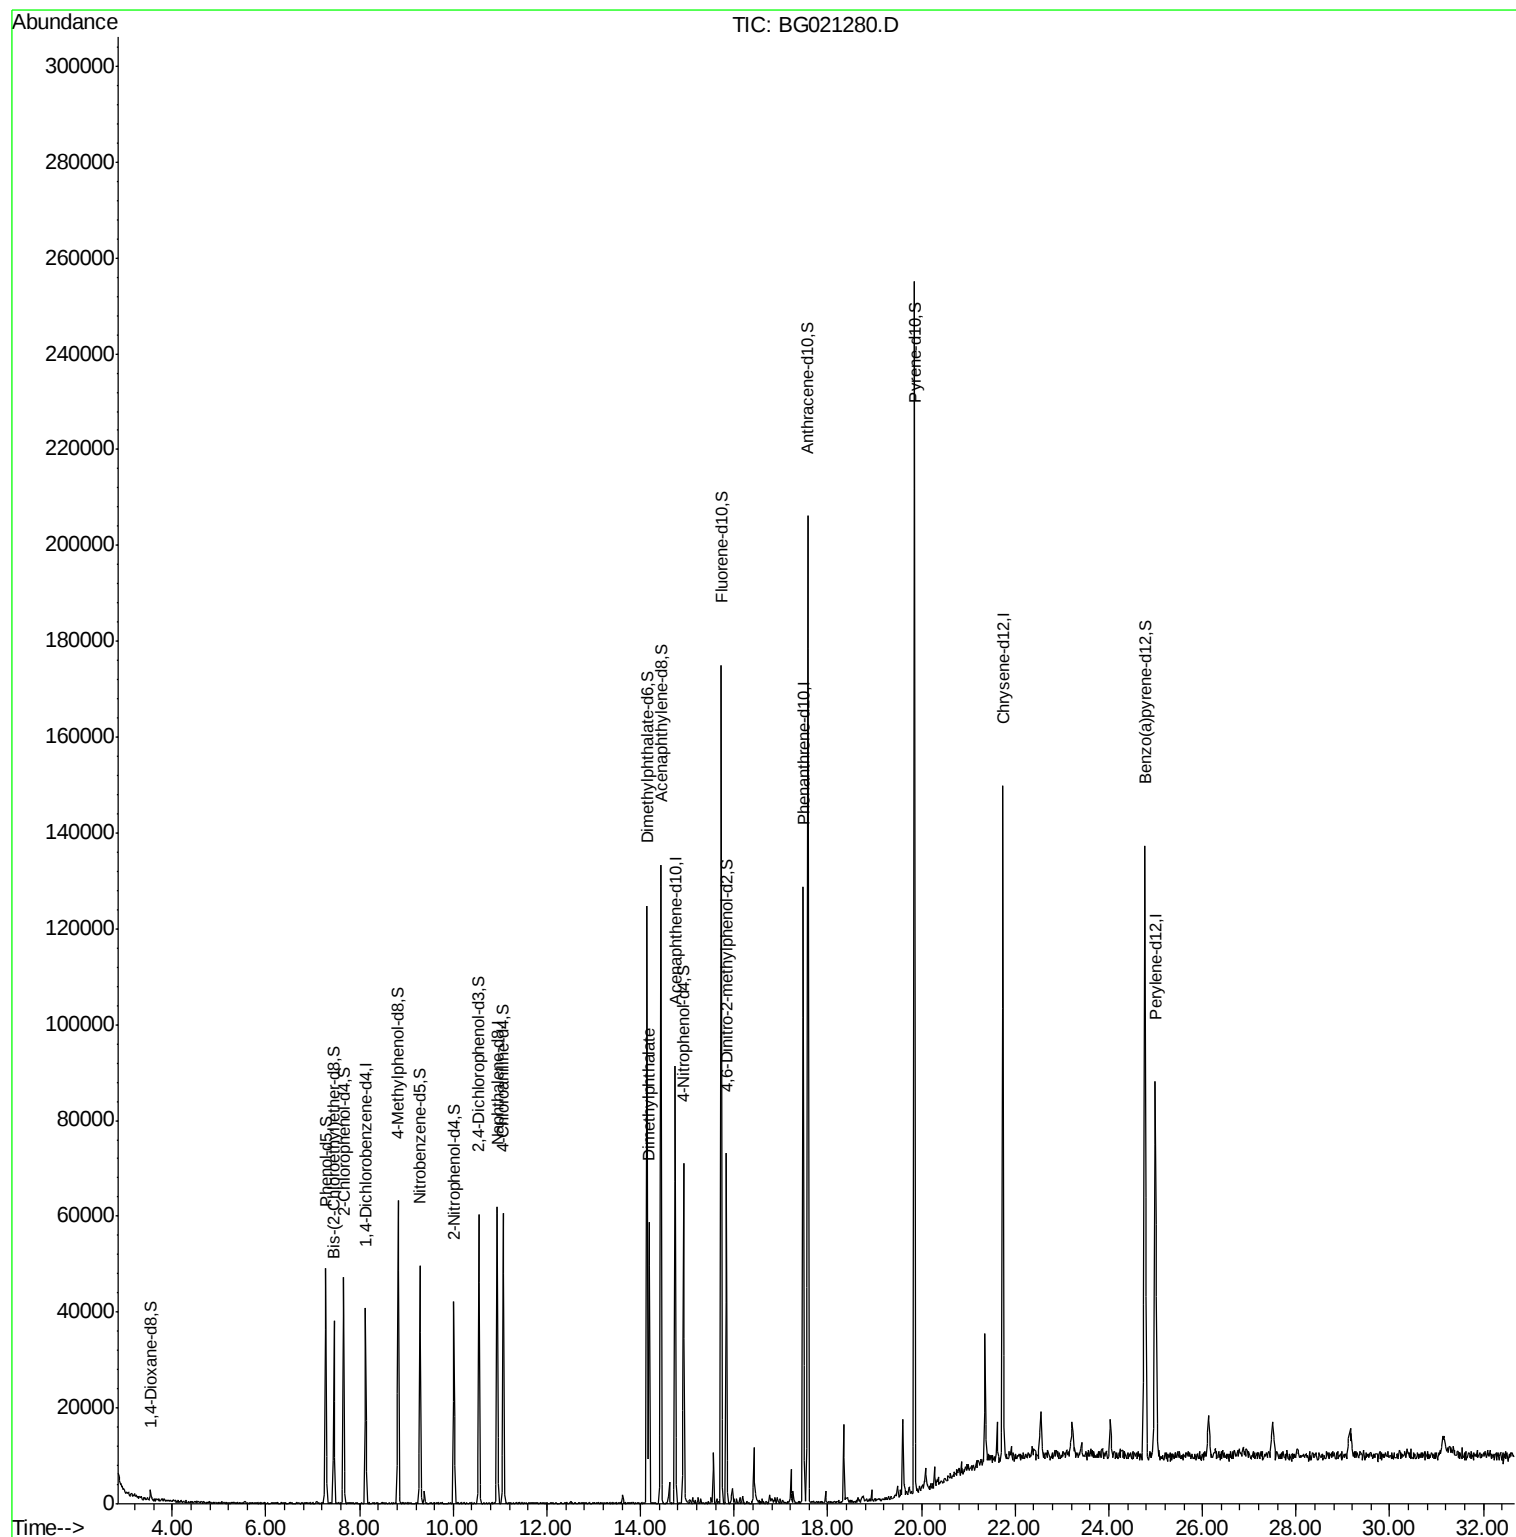

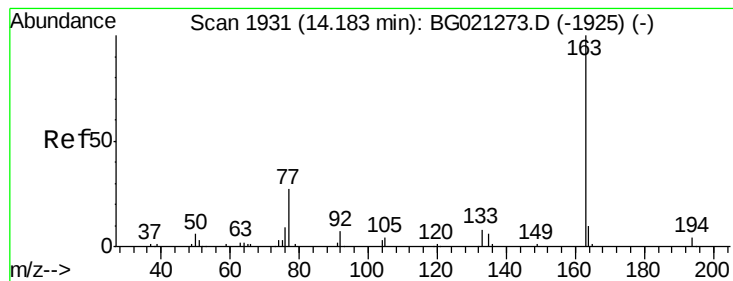

#45

Dimethylphthalate

Concen: 12.43 ng/ul

RT: 14.18 min Scan# 1931

Delta R.T. -0.00 min

Lab File: BG021280.D


Acq: 4 Mar 2016 21:31

Instrument :

BNA_G

ClientSampleId :

JHFJ0

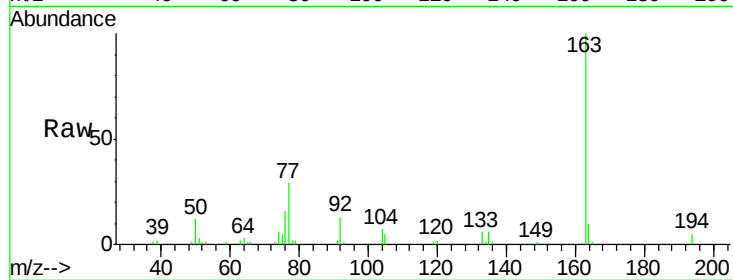

Tgt Ion:	163	Resp:	33008
Ion	Ratio	Lower	Upper
163	100		
194	4.9	2.8	4.2#
164	10.0	8.2	12.2

