

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030416\
 Data File : BG021281.D
 Acq On : 4 Mar 2016 22:10
 Operator : UM/SJ
 Sample : H1626-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JHFJ1

Quant Time: Mar 05 00:59:02 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Mar 05 00:52:50 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.13	152	11397	20.00	ng/ul	0.00
18) Naphthalene-d8	10.94	136	52870	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.74	164	31079	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.48	188	72161	20.00	ng/ul	0.00
78) Chrysene-d12	21.74	240	80810	20.00	ng/ul	0.00
86) Perylene-d12	25.00	264	74290	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.54	96	168	0.60	ng/uL	0.00
5) Phenol-d5	7.28	99	6756	5.60	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.45	67	4677	5.81	ng/ul	0.00
9) 2-Chlorophenol-d4	7.66	132	5183	6.15	ng/ul	0.00
13) 4-Methylphenol-d8	8.82	113	5397	5.66	ng/ul	0.00
19) Nitrobenzene-d5	9.29	128	2673	6.24	ng/ul	0.00
22) 2-Nitrophenol-d4	10.01	143	3012	6.60	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.55	165	6837	8.38	ng/ul	0.00
29) 4-Chloroaniline-d4	11.07	131	9914	9.58	ng/ul	0.00
44) Dimethylphthalate-d6	14.14	166	50267	19.30	ng/ul	0.00
47) Acenaphthylene-d8	14.43	160	46213	14.26	ng/ul	0.00
52) 4-Nitrophenol-d4	14.91	143	11451	22.56	ng/ul	0.00
58) Fluorene-d10	15.73	176	46467	20.32	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.83	200	11393	22.00	ng/ul	0.00
71) Anthracene-d10	17.58	188	102805	28.65	ng/ul	0.00
79) Pyrene-d10	19.85	212	132931	32.50	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.77	264	132097	32.94	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.18	163	15480	5.52	ng/ul#	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030416\
Data File : BG021281.D
Acq On : 4 Mar 2016 22:10
Operator : UM/SJ
Sample : H1626-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JHFJ1

Quant Time: Mar 05 00:59:02 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Mar 05 00:52:50 2016
Response via : Initial Calibration

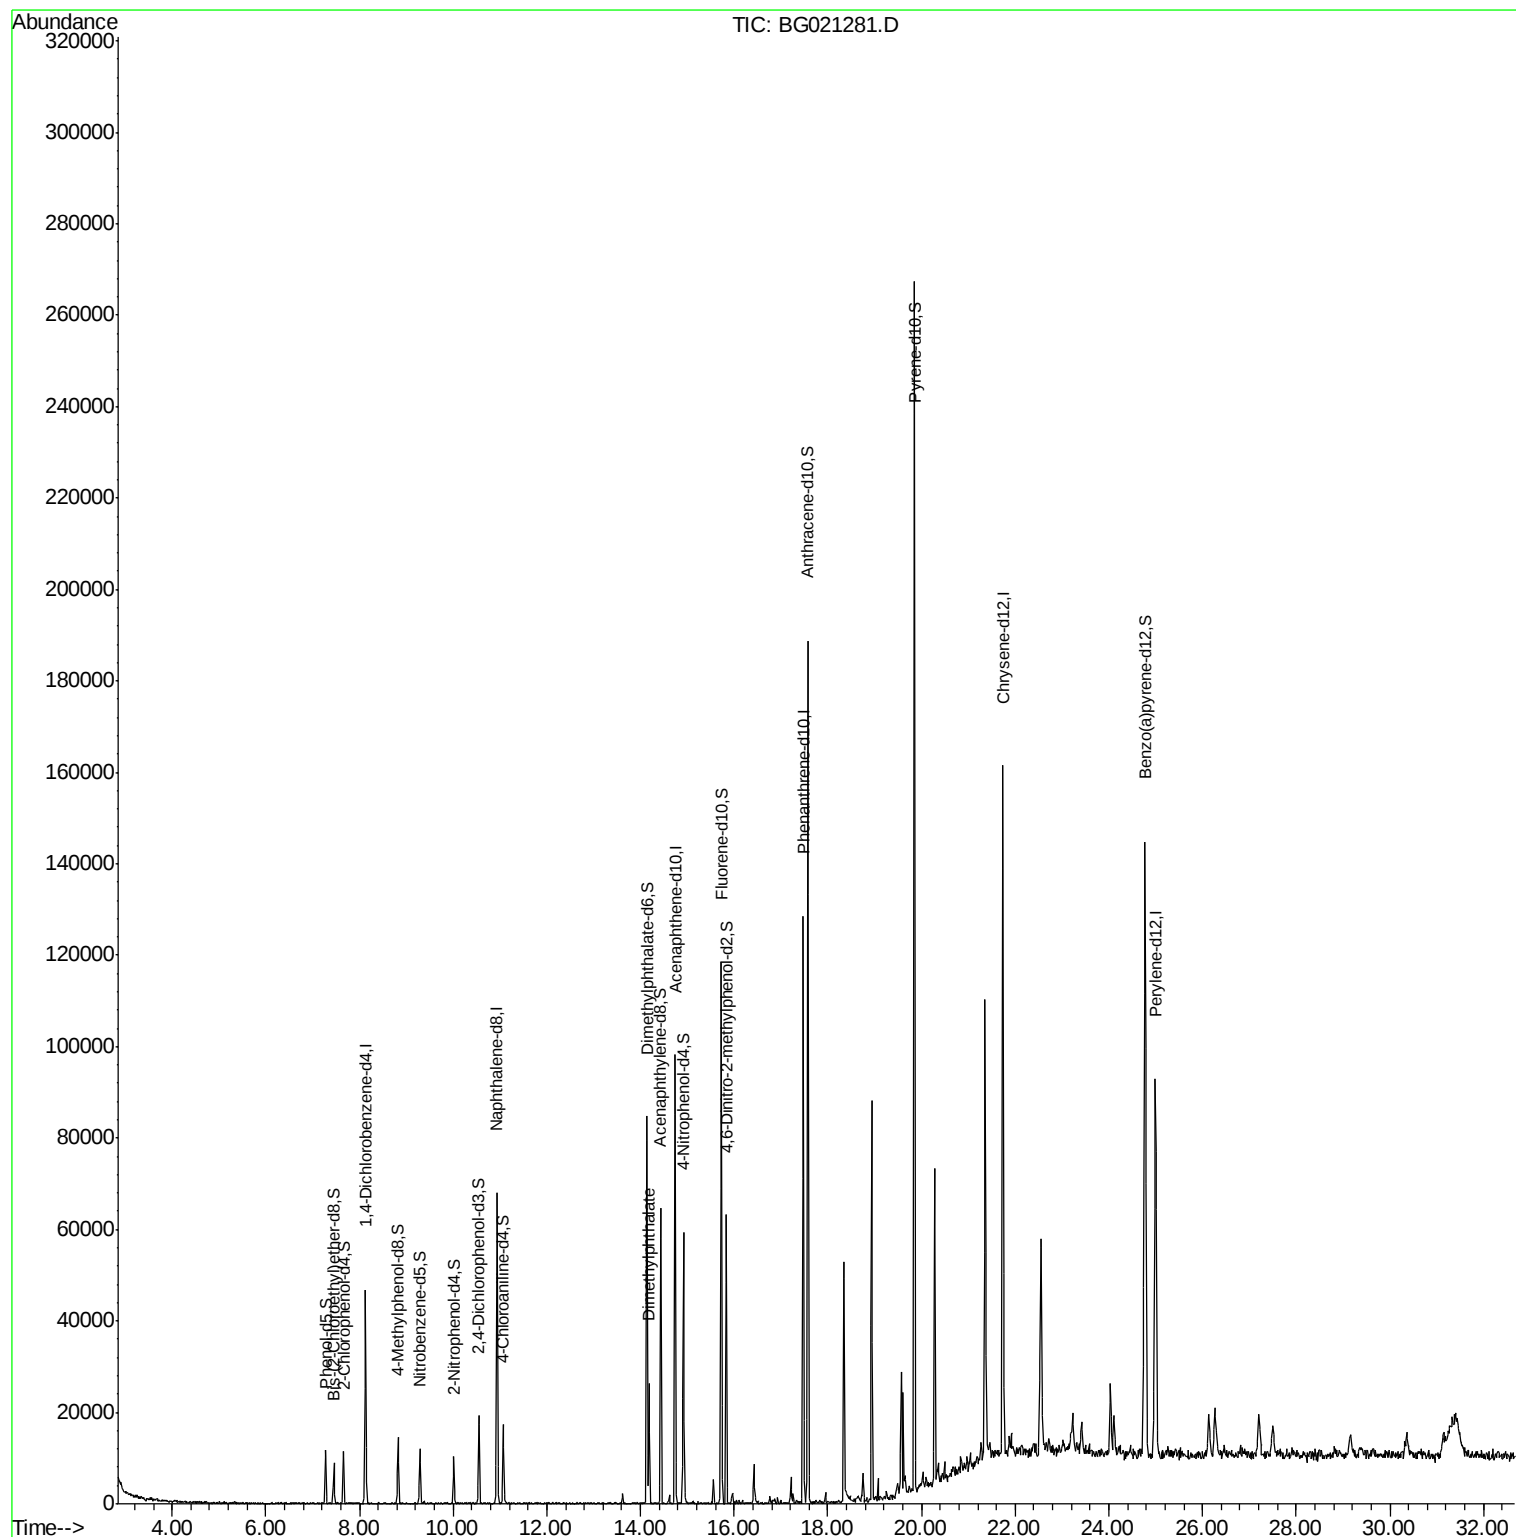

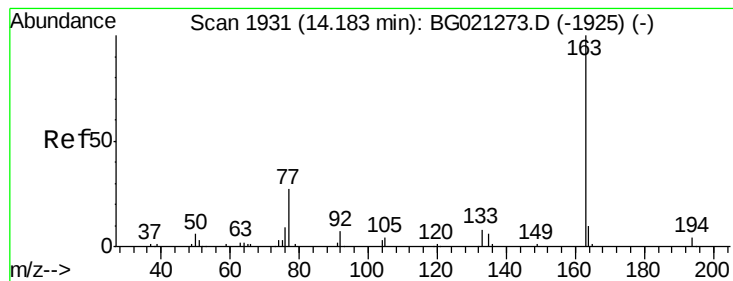

#45

Dimethylphthalate

Concen: 5.52 ng/ul

RT: 14.18 min Scan# 1930

Delta R.T. -0.00 min

Lab File: BG021281.D


Acq: 4 Mar 2016 22:10

Instrument :

BNA_G

ClientSampleId :

JHFJ1

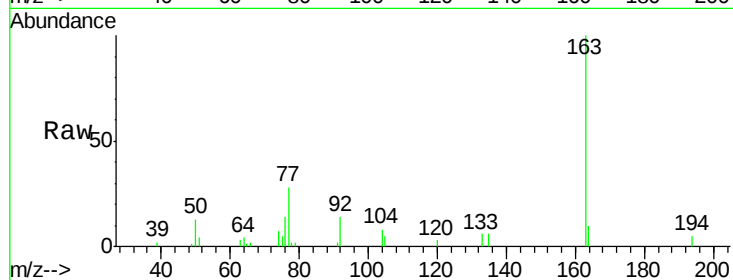

Tgt Ion:	163	Resp:	15480
Ion	Ratio	Lower	Upper
163	100		
194	4.9	2.8	4.2#
164	9.9	8.2	12.2

