

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030416\
 Data File : BG021289.D
 Acq On : 5 Mar 2016 3:31
 Operator : UM/SJ
 Sample : H1626-18
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JHFK3

Quant Time: Mar 05 05:58:22 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Mar 05 05:52:35 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.13	152	11345	20.00	ng/ul	0.00
18) Naphthalene-d8	10.94	136	55605	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.73	164	32577	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.47	188	72770	20.00	ng/ul	0.00
78) Chrysene-d12	21.74	240	78457	20.00	ng/ul	0.00
86) Perylene-d12	25.00	264	74364	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.54	96	1227	4.39	ng/uL	0.00
5) Phenol-d5	7.28	99	33719	28.06	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.45	67	25145	31.38	ng/ul	0.00
9) 2-Chlorophenol-d4	7.66	132	25432	30.34	ng/ul	0.00
13) 4-Methylphenol-d8	8.82	113	27635	29.13	ng/ul	0.00
19) Nitrobenzene-d5	9.29	128	13347	29.63	ng/ul	0.00
22) 2-Nitrophenol-d4	10.02	143	14386	29.96	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.55	165	25315	29.50	ng/ul	0.00
29) 4-Chloroaniline-d4	11.07	131	35433	32.56	ng/ul	0.00
44) Dimethylphthalate-d6	14.14	166	88029	32.24	ng/ul	0.00
47) Acenaphthylene-d8	14.44	160	111820	32.91	ng/ul	0.00
52) 4-Nitrophenol-d4	14.92	143	14227	26.74	ng/ul	0.00
58) Fluorene-d10	15.73	176	78589	32.78	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.83	200	14244	27.27	ng/ul	0.00
71) Anthracene-d10	17.57	188	119526	33.03	ng/ul	0.00
79) Pyrene-d10	19.85	212	135562	34.13	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.78	264	133685	33.30	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.19	163	55632	18.94	ng/ul#	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030416\
Data File : BG021289.D
Acq On : 5 Mar 2016 3:31
Operator : UM/SJ
Sample : H1626-18
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JHFK3

Quant Time: Mar 05 05:58:22 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Mar 05 05:52:35 2016
Response via : Initial Calibration

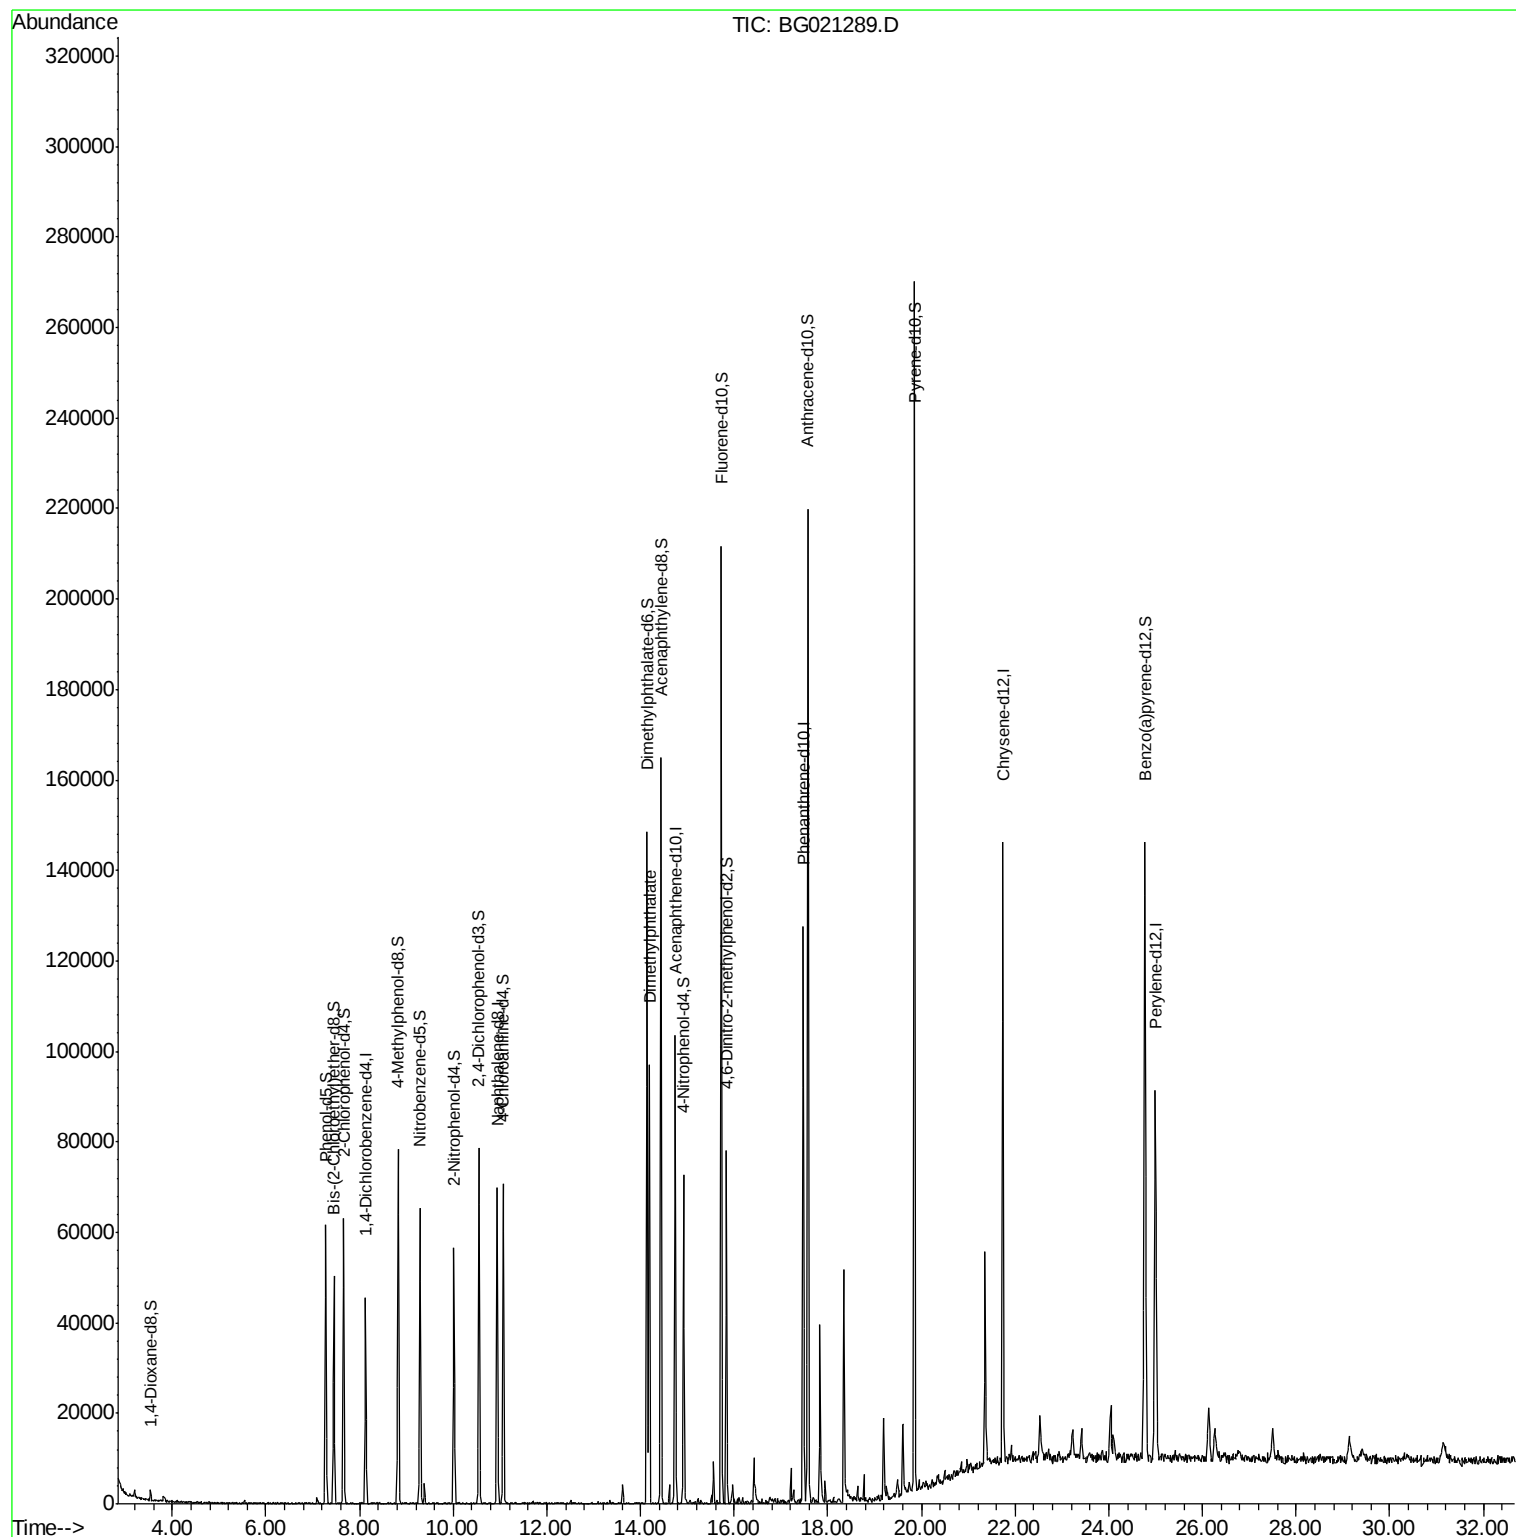

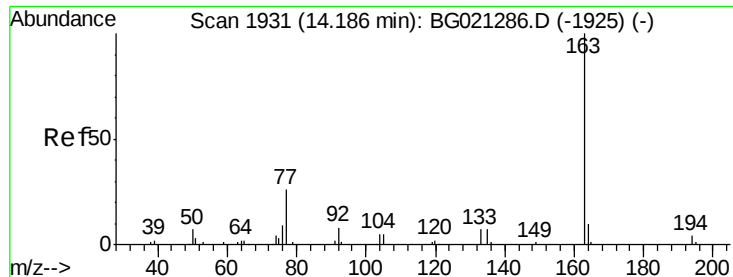

#45

Dimethylphthalate

Concen: 18.94 ng/ul

RT: 14.19 min Scan# 1932

Delta R.T. 0.00 min

Lab File: BG021289.D

Acq: 5 Mar 2016 3:31

Instrument :

BNA_G

ClientSampleId :

JHFK3


Tgt Ion:163 Resp: 55632

Ion Ratio Lower Upper

163 100

194 4.4 2.8 4.2#

164 10.0 8.2 12.2

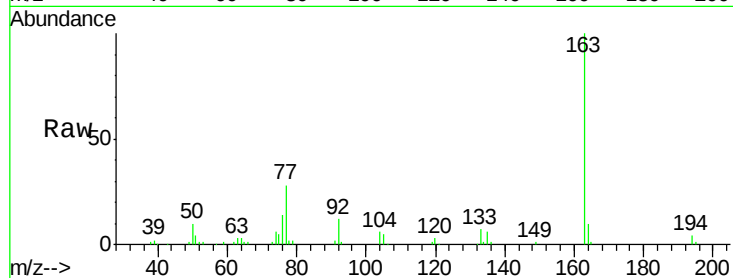

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

