

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030416\
 Data File : BG021293.D
 Acq On : 5 Mar 2016 6:08
 Operator : UM/SJ
 Sample : PB88690BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK90

Quant Time: Mar 07 00:51:02 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Mar 05 05:52:35 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.13	152	10969	20.00	ng/ul	0.00
18) Naphthalene-d8	10.94	136	50509	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.74	164	30464	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.58	188	142320	20.00	ng/ul	0.10
78) Chrysene-d12	21.74	240	78629	20.00	ng/ul	0.00
86) Perylene-d12	24.99	264	72470	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.53	96	2008	7.43	ng/uL	0.00
5) Phenol-d5	7.28	99	39901	34.35	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.45	67	28646	36.98	ng/ul	0.00
9) 2-Chlorophenol-d4	7.66	132	29357	36.22	ng/ul	0.00
13) 4-Methylphenol-d8	8.82	113	32200	35.10	ng/ul	0.00
19) Nitrobenzene-d5	9.29	128	15474	37.82	ng/ul	0.00
22) 2-Nitrophenol-d4	10.02	143	16589	38.03	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.55	165	27570	35.37	ng/ul	0.00
29) 4-Chloroaniline-d4	11.07	131	42906	43.41	ng/ul	0.00
44) Dimethylphthalate-d6	14.14	166	96576	37.83	ng/ul	0.00
47) Acenaphthylene-d8	14.43	160	122533	38.57	ng/ul	0.00
52) 4-Nitrophenol-d4	14.92	143	18184	36.54	ng/ul	0.00
58) Fluorene-d10	15.73	176	85584	38.17	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.83	200	15967	15.63	ng/ul	0.00
71) Anthracene-d10	17.58	188	142320	20.11	ng/ul	0.00
79) Pyrene-d10	19.84	212	157789	39.64	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.77	264	151914	38.83	ng/ul	0.00


Target Compounds					Qvalue
15) N-Nitroso-di-n-propylamine	8.82	70	1005	1.05 ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030416\
Data File : BG021293.D
Acq On : 5 Mar 2016 6:08
Operator : UM/SJ
Sample : PB88690BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK90

Quant Time: Mar 07 00:51:02 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Mar 05 05:52:35 2016
Response via : Initial Calibration

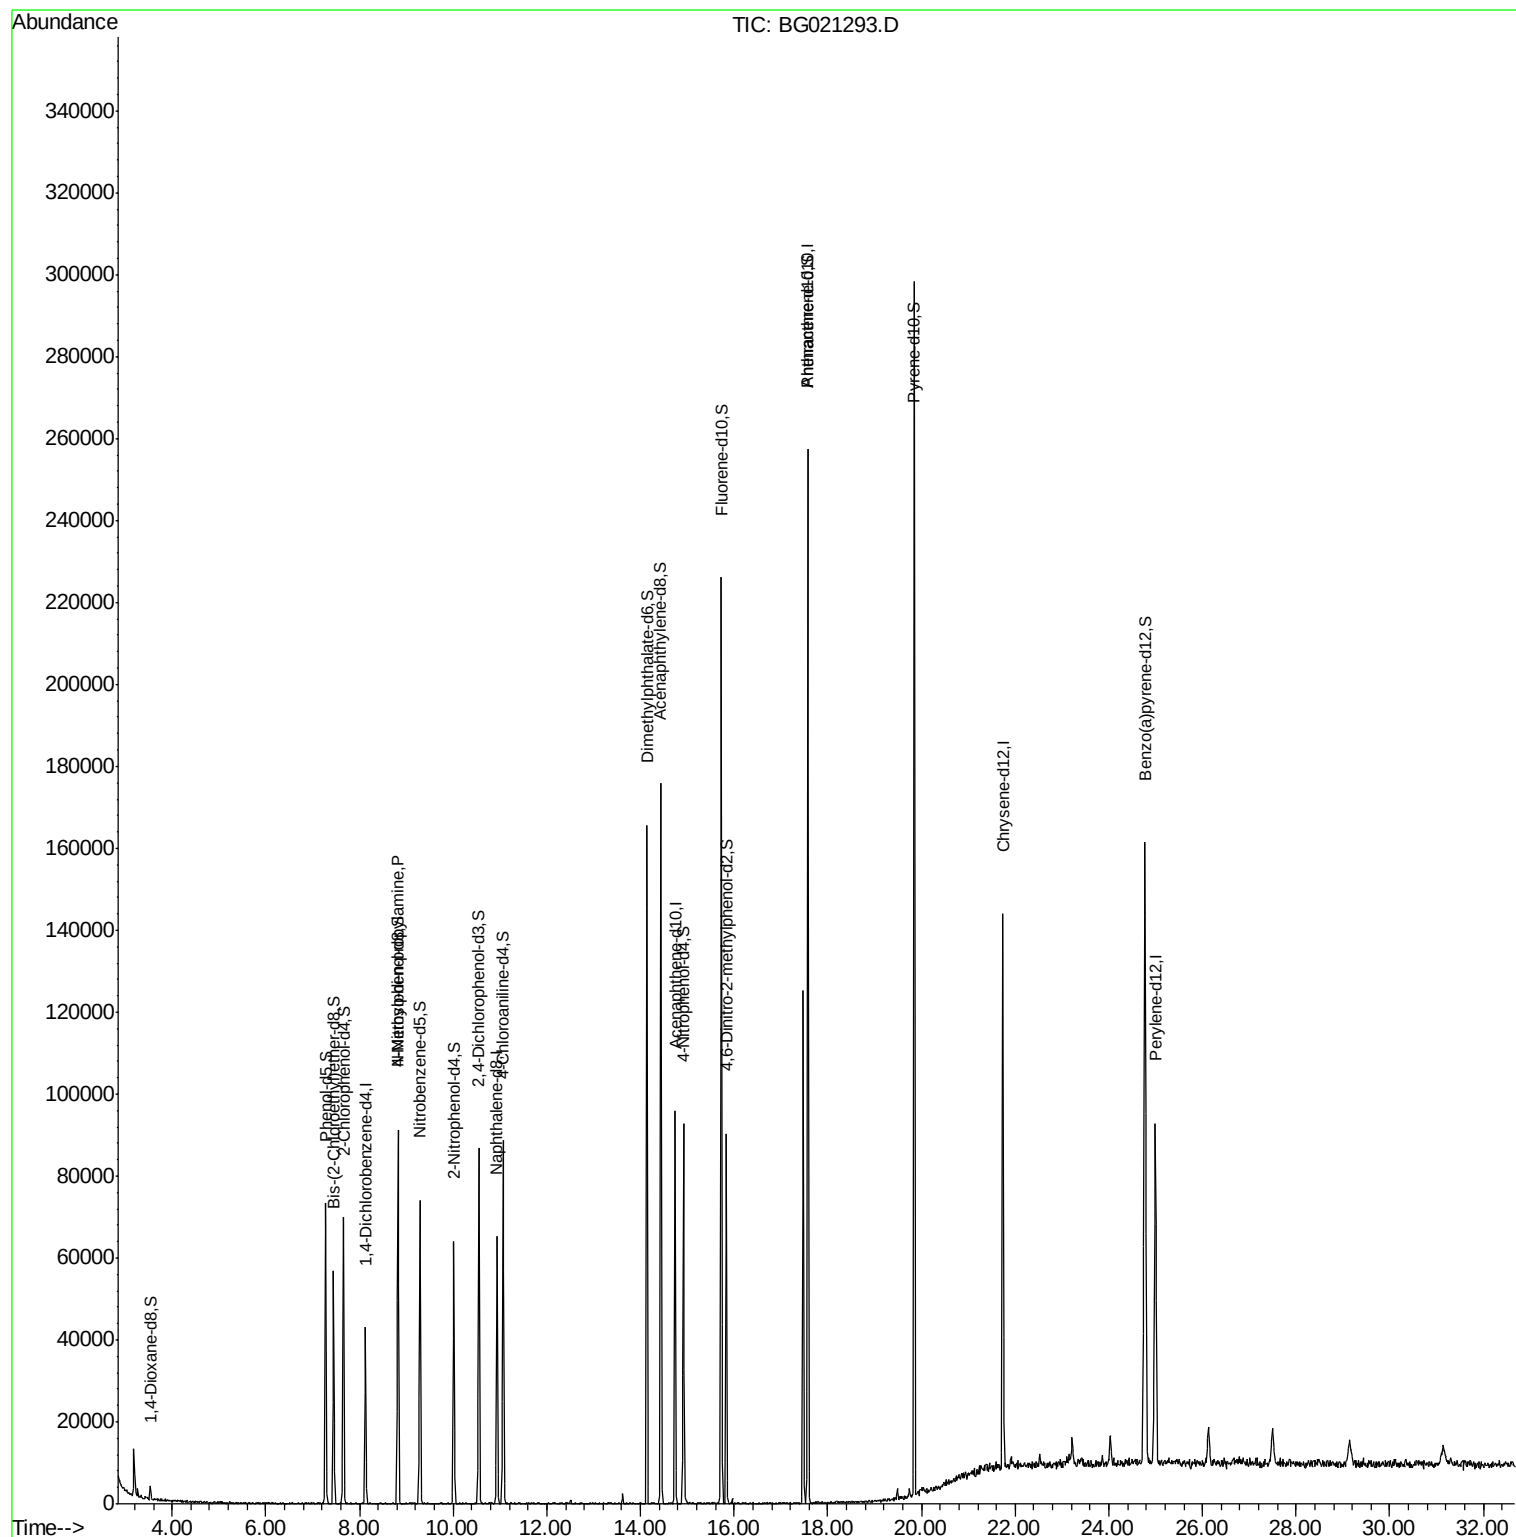

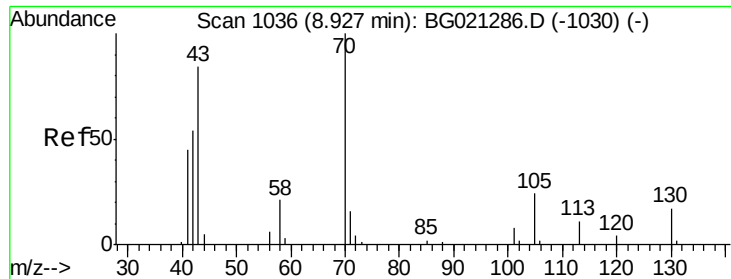

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.05 ng/ul
 RT: 8.82 min Scan# 1017
 Delta R.T. -0.11 min
 Lab File: BG021293.D
 Acq: 5 Mar 2016 6:08

Instrument :
 BNA_G
 ClientSampleId :
 SBLK90

Tgt Ion: 70 Resp: 1005
 Ion Ratio Lower Upper
 70 100
 42 311.7 45.7 68.5#
 101 0.0 5.7 8.5#
 130 0.0 15.7 23.5#

