

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030416\
 Data File : BG021296.D
 Acq On : 5 Mar 2016 8:06
 Operator : UM/SJ
 Sample : PB88673BL
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK73

Quant Time: Mar 07 00:51:23 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Mar 05 05:52:35 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.13	152	9423	20.00	ng/ul	0.00
18) Naphthalene-d8	10.93	136	46472	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.74	164	27020	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.57	188	131498	20.00	ng/ul	0.10
78) Chrysene-d12	21.73	240	69442	20.00	ng/ul	0.00
86) Perylene-d12	24.99	264	64845	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.54	96	1694	7.30	ng/uL	0.00
5) Phenol-d5	7.27	99	38119	38.19	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.45	67	27004	40.58	ng/ul	0.00
9) 2-Chlorophenol-d4	7.66	132	27781	39.90	ng/ul	0.00
13) 4-Methylphenol-d8	8.82	113	30933	39.26	ng/ul	0.00
19) Nitrobenzene-d5	9.29	128	14857	39.47	ng/ul	0.00
22) 2-Nitrophenol-d4	10.01	143	15882	39.57	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.55	165	26330	36.72	ng/ul	0.00
29) 4-Chloroaniline-d4	11.07	131	41050	45.14	ng/ul	0.00
44) Dimethylphthalate-d6	14.14	166	94145	41.58	ng/ul	0.00
47) Acenaphthylene-d8	14.44	160	117196	41.59	ng/ul	0.00
52) 4-Nitrophenol-d4	14.92	143	17591	39.86	ng/ul	0.00
58) Fluorene-d10	15.73	176	81510	40.99	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.83	200	15044	15.94	ng/ul	0.00
71) Anthracene-d10	17.57	188	131498	20.11	ng/ul	0.00
79) Pyrene-d10	19.85	212	149873	42.63	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.77	264	145136	41.46	ng/ul	0.00


Target Compounds					Qvalue
15) N-Nitroso-di-n-propylamine	8.82	70	942	1.14 ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030416\
Data File : BG021296.D
Acq On : 5 Mar 2016 8:06
Operator : UM/SJ
Sample : PB88673BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK73

Quant Time: Mar 07 00:51:23 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Mar 05 05:52:35 2016
Response via : Initial Calibration

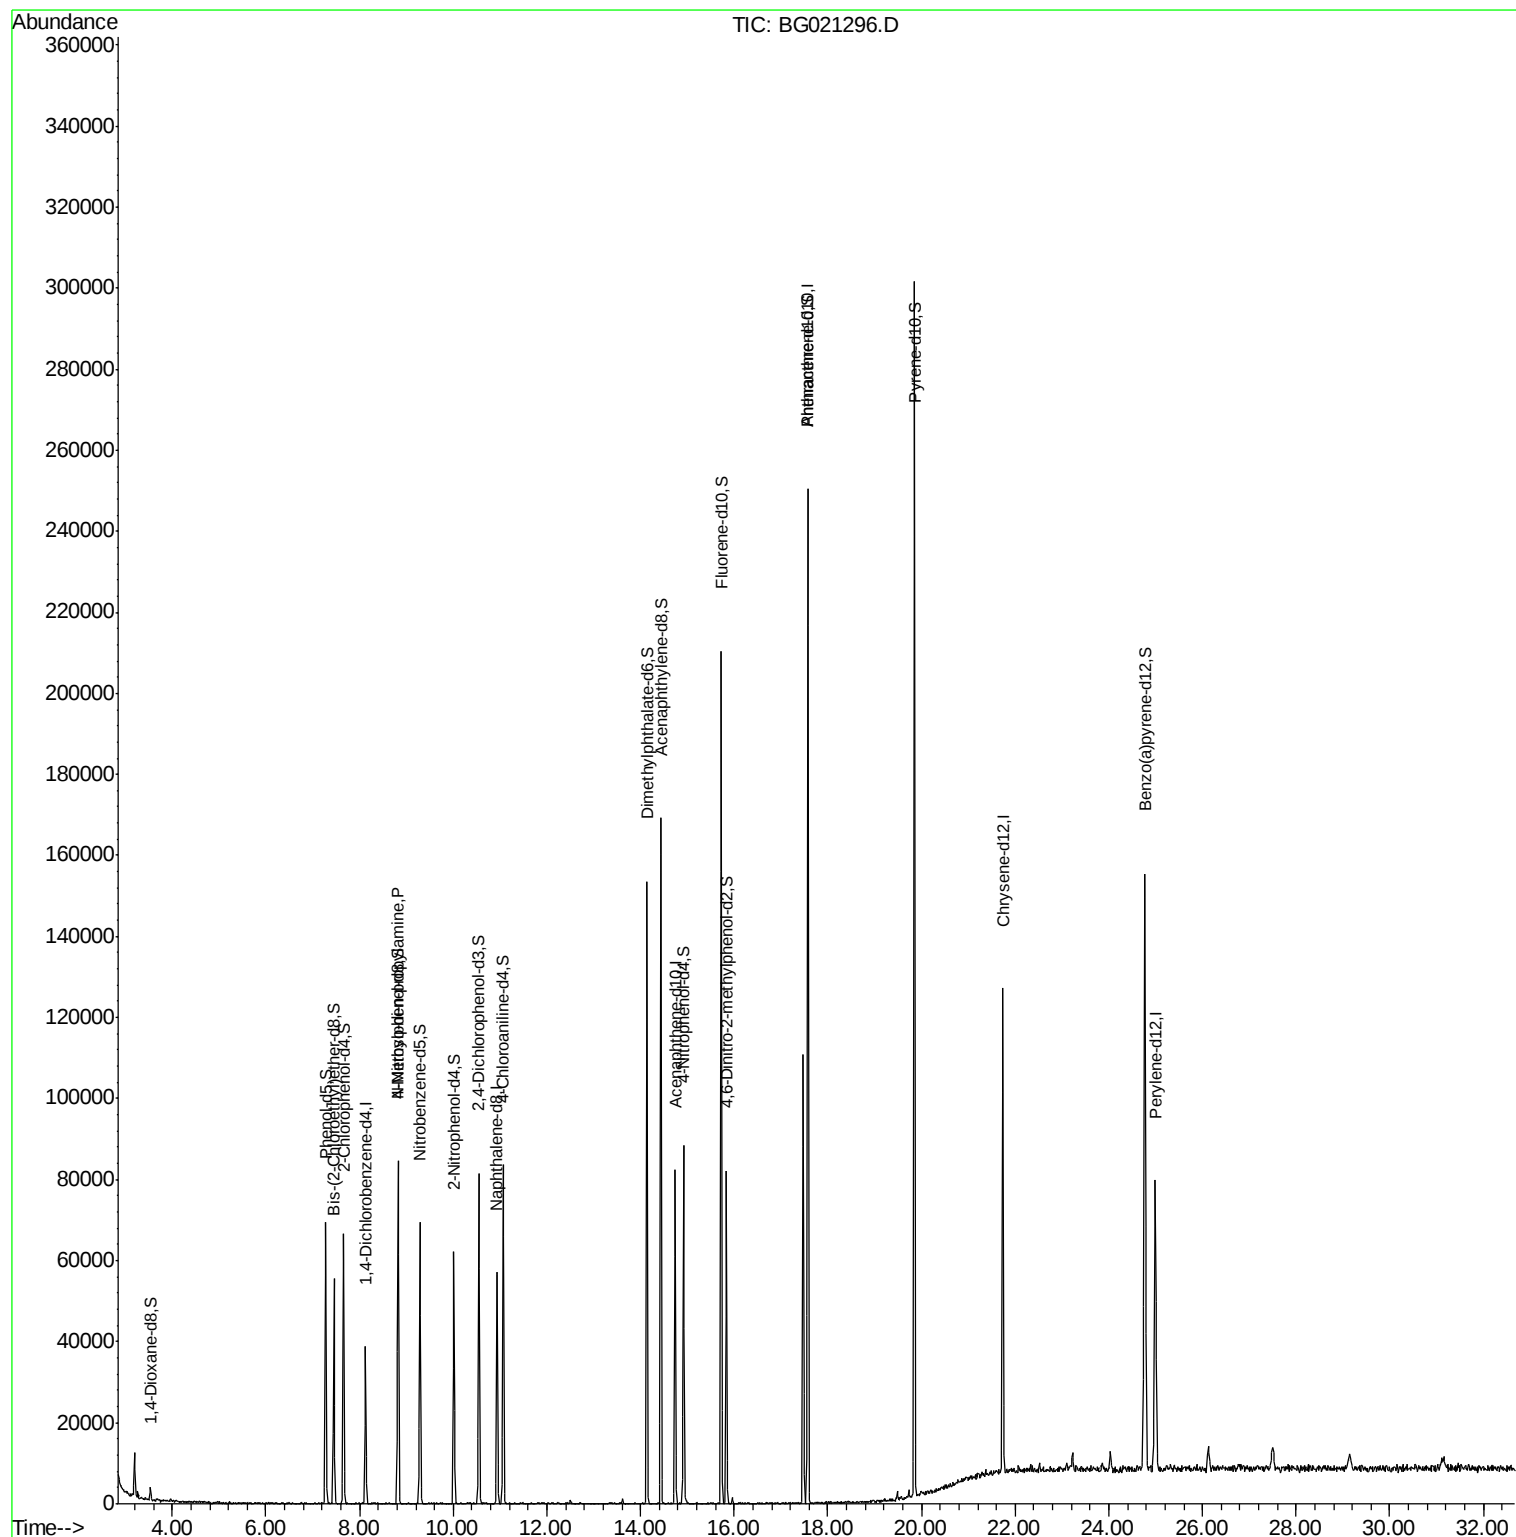

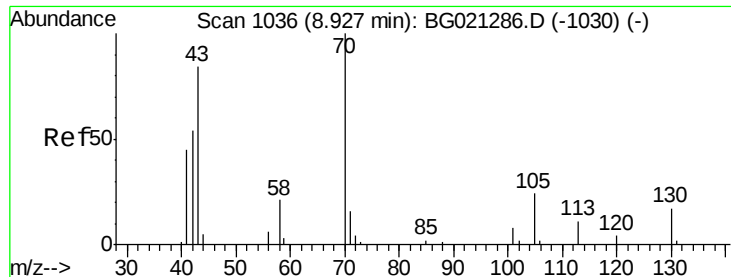

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.14 ng/ul
 RT: 8.82 min Scan# 1018
 Delta R.T. -0.11 min
 Lab File: BG021296.D
 Acq: 5 Mar 2016 8:06

Instrument :
 BNA_G
 ClientSampleId :
 SBLK73

Tgt Ion: 70 Resp: 942
 Ion Ratio Lower Upper
 70 100
 42 315.4 45.7 68.5#
 101 0.0 5.7 8.5#
 130 0.0 15.7 23.5#

