

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030416\
 Data File : BG021302.D
 Acq On : 5 Mar 2016 12:39
 Operator : UM/SJ
 Sample : H1665-06
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 H0099

Quant Time: Mar 07 03:14:46 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Mar 07 03:13:46 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.13	152	9060	20.00	ng/ul	0.00
18) Naphthalene-d8	10.93	136	42985	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.74	164	25626	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.47	188	60624	20.00	ng/ul	0.00
78) Chrysene-d12	21.73	240	68539	20.00	ng/ul	0.00
86) Perylene-d12	24.98	264	63342	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.53	96	115	0.52	ng/uL	0.00
5) Phenol-d5	7.28	99	5648	5.89	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.44	67	19539	30.54	ng/ul	0.00
9) 2-Chlorophenol-d4	7.65	132	16785	25.07	ng/ul	0.00
13) 4-Methylphenol-d8	8.82	113	11086	14.63	ng/ul	0.00
19) Nitrobenzene-d5	9.29	128	10729	30.81	ng/ul	0.00
22) 2-Nitrophenol-d4	10.01	143	11324	30.51	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.55	165	19503	29.40	ng/ul	0.00
29) 4-Chloroaniline-d4	11.06	131	1095	1.30	ng/ul	0.00
44) Dimethylphthalate-d6	14.14	166	72285	33.66	ng/ul	0.00
47) Acenaphthylene-d8	14.43	160	90237	33.77	ng/ul	0.00
52) 4-Nitrophenol-d4	14.91	143	2292	5.48	ng/ul	0.00
58) Fluorene-d10	15.72	176	64501	34.20	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.83	200	11962	27.49	ng/ul	0.00
71) Anthracene-d10	17.57	188	103469	34.32	ng/ul	0.00
79) Pyrene-d10	19.84	212	116303	33.52	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.77	264	112831	33.00	ng/ul	0.00


Target Compounds					Qvalue
45) Dimethylphthalate	14.18	163	44285	19.17 ng/ul#	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030416\
Data File : BG021302.D
Acq On : 5 Mar 2016 12:39
Operator : UM/SJ
Sample : H1665-06
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
H0099

Quant Time: Mar 07 03:14:46 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Mar 07 03:13:46 2016
Response via : Initial Calibration

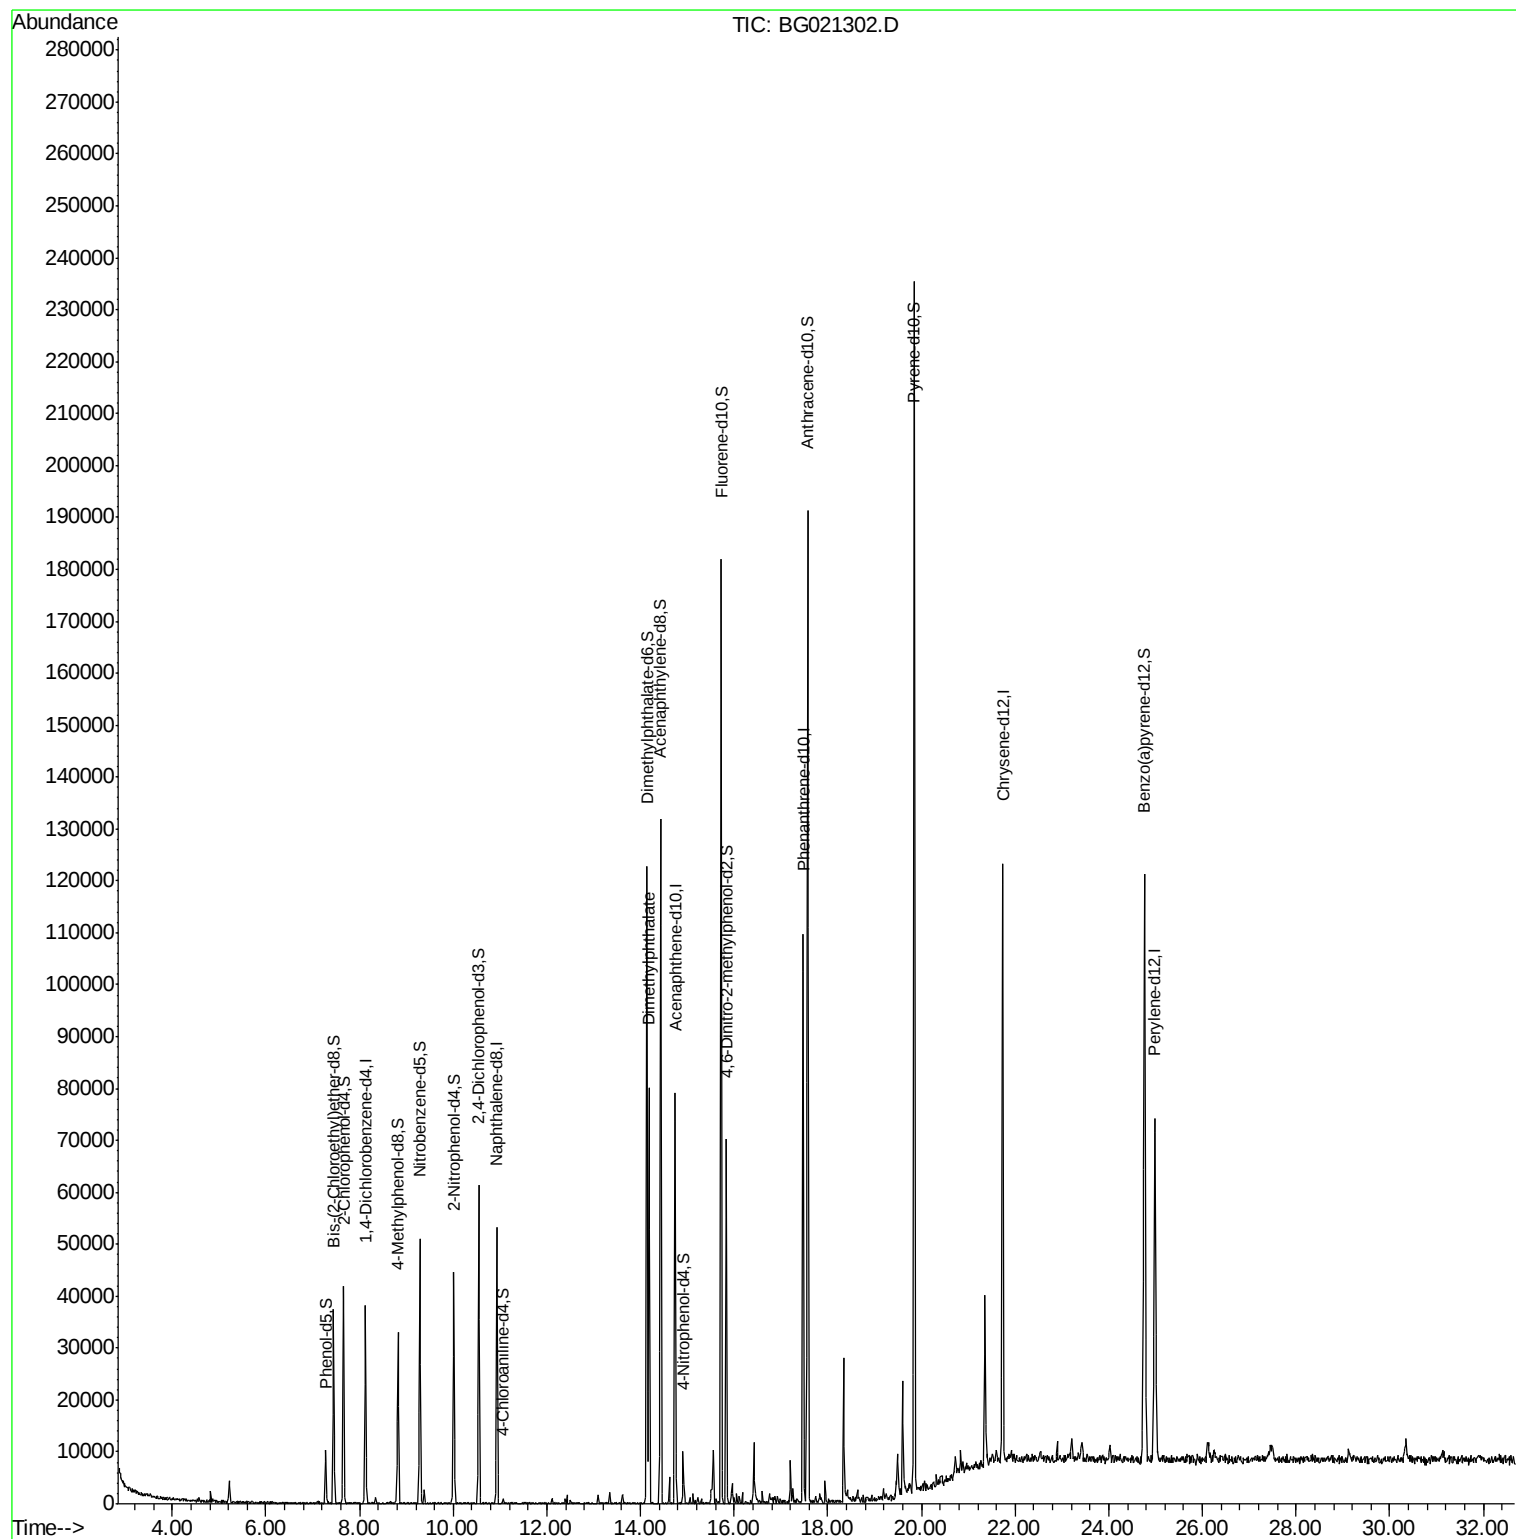

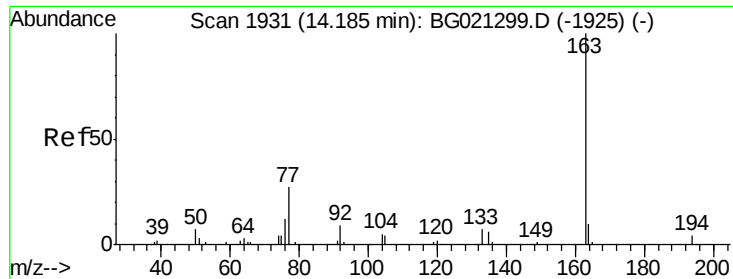

#45

Dimethylphthalate

Concen: 19.17 ng/ul

RT: 14.18 min Scan# 1931

Delta R.T. -0.00 min

Lab File: BG021302.D


Acq: 5 Mar 2016 12:39

Instrument :

BNA_G

ClientSampleId :

H0099

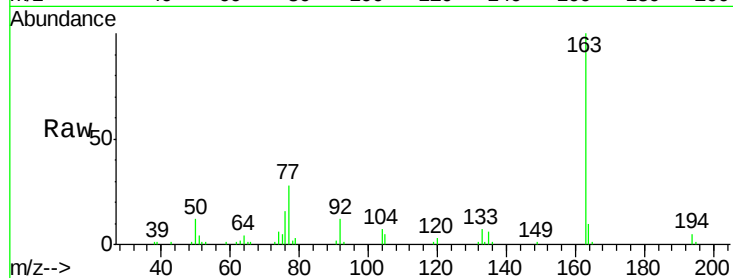

Tgt Ion:	163	Resp:	44285
Ion	Ratio	Lower	Upper
163	100		
194	4.5	2.8	4.2#
164	10.3	8.2	12.2

