

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030416\
 Data File : BG021283.D
 Acq On : 4 Mar 2016 23:28
 Operator : UM/SJ
 Sample : H1626-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JHFJ3

Quant Time: Mar 05 00:59:16 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Mar 05 00:52:50 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.13	152	11822	20.00	ng/ul	0.00
18) Naphthalene-d8	10.94	136	59806	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.74	164	35089	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.48	188	76127	20.00	ng/ul	0.00
78) Chrysene-d12	21.74	240	84030	20.00	ng/ul	0.00
86) Perylene-d12	25.00	264	78601	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.54	96	1335	4.59	ng/uL	0.00
5) Phenol-d5	7.28	99	35227	28.13	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.45	67	24180	28.96	ng/ul	0.00
9) 2-Chlorophenol-d4	7.65	132	24841	28.43	ng/ul	0.00
13) 4-Methylphenol-d8	8.82	113	29701	30.04	ng/ul	0.00
19) Nitrobenzene-d5	9.29	128	13242	27.33	ng/ul	0.00
22) 2-Nitrophenol-d4	10.01	143	14404	27.89	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.55	165	25607	27.75	ng/ul	0.00
29) 4-Chloroaniline-d4	11.07	131	33540	28.66	ng/ul	0.00
44) Dimethylphthalate-d6	14.14	166	88474	30.09	ng/ul	0.00
47) Acenaphthylene-d8	14.44	160	111472	30.46	ng/ul	0.00
52) 4-Nitrophenol-d4	14.92	143	14700	25.65	ng/ul	0.00
58) Fluorene-d10	15.73	176	78336	30.34	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.83	200	14549	26.63	ng/ul	0.00
71) Anthracene-d10	17.57	188	120724	31.89	ng/ul	0.00
79) Pyrene-d10	19.85	212	138540	32.57	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.78	264	135222	31.87	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.18	163	37702	11.92	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030416\
Data File : BG021283.D
Acq On : 4 Mar 2016 23:28
Operator : UM/SJ
Sample : H1626-06
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JHFJ3

Quant Time: Mar 05 00:59:16 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Mar 05 00:52:50 2016
Response via : Initial Calibration

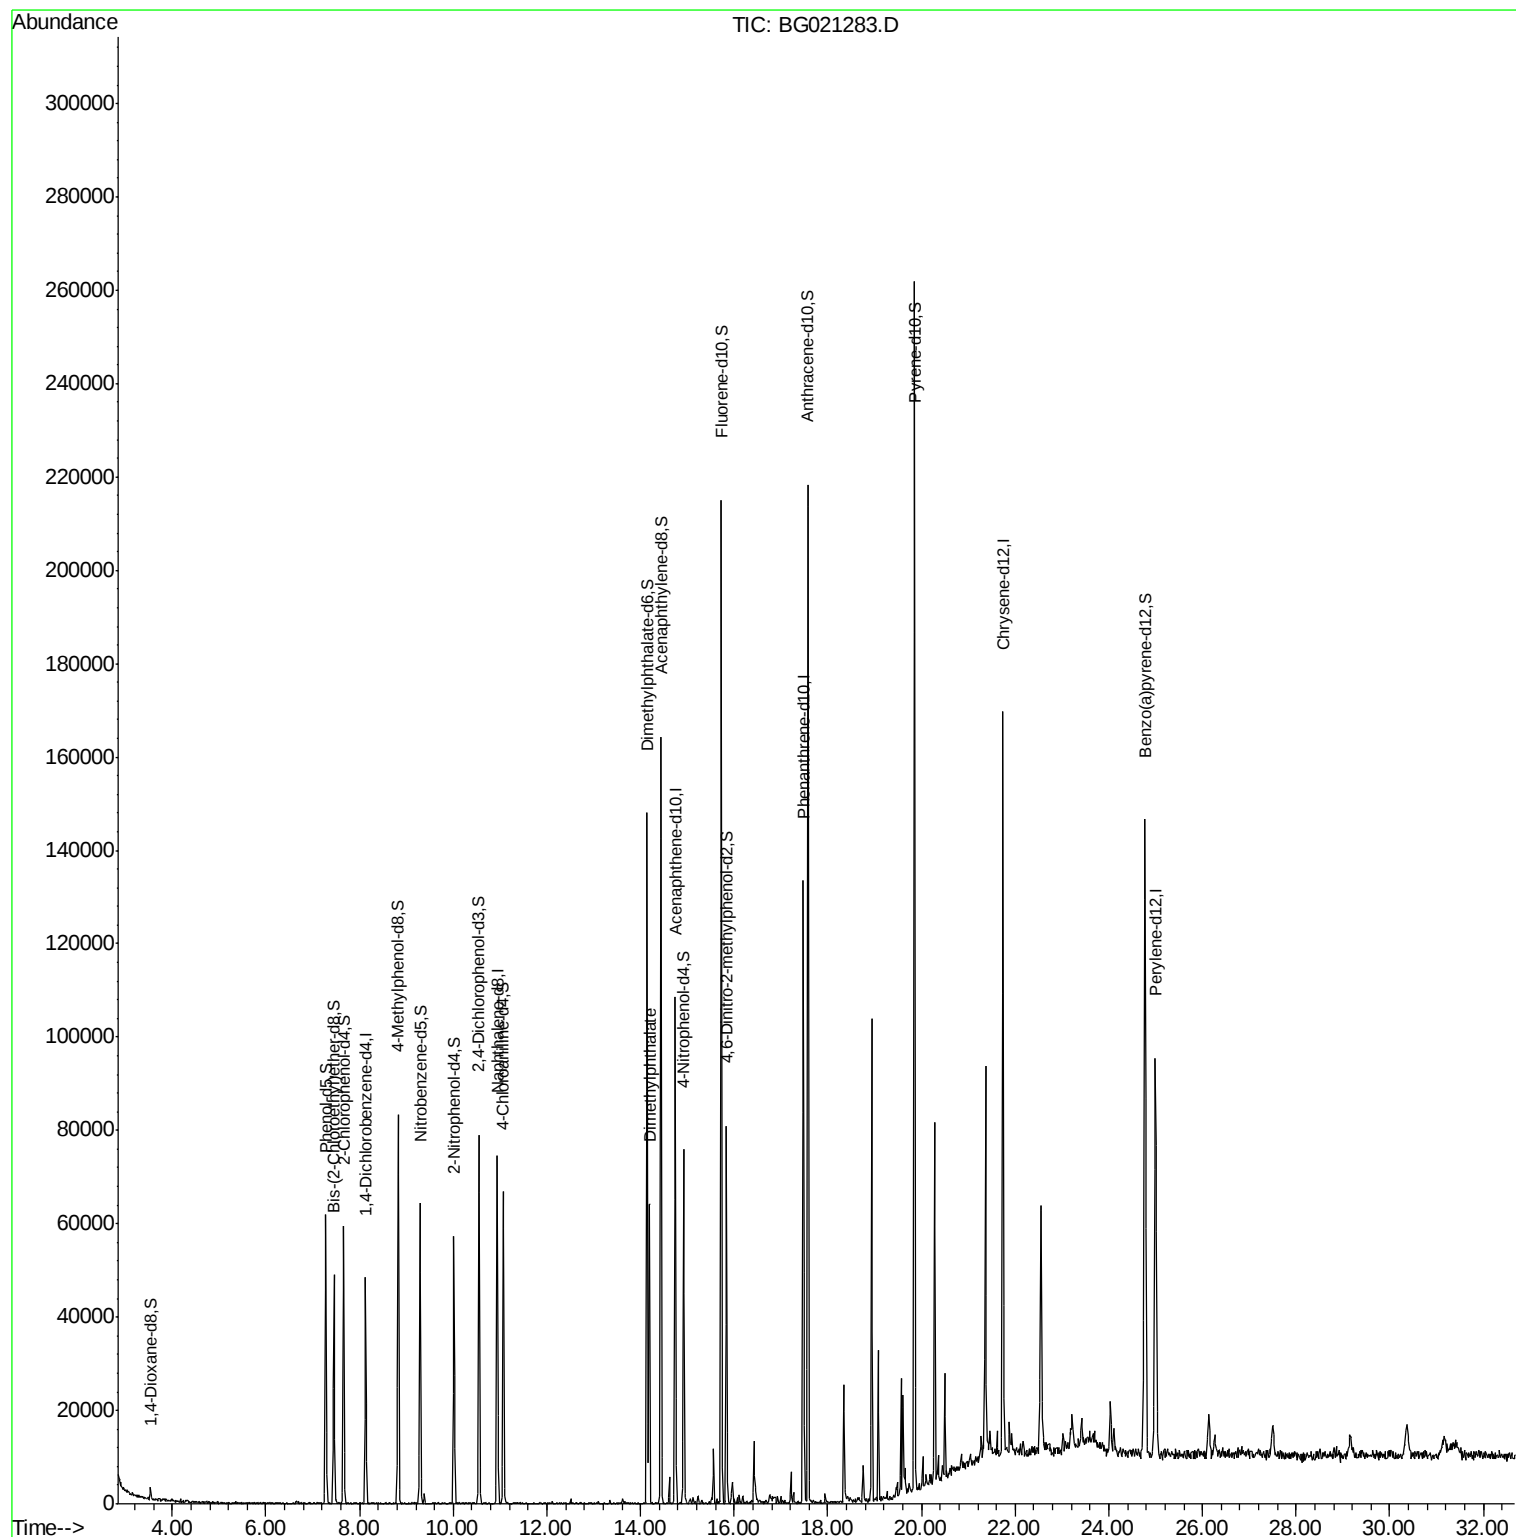

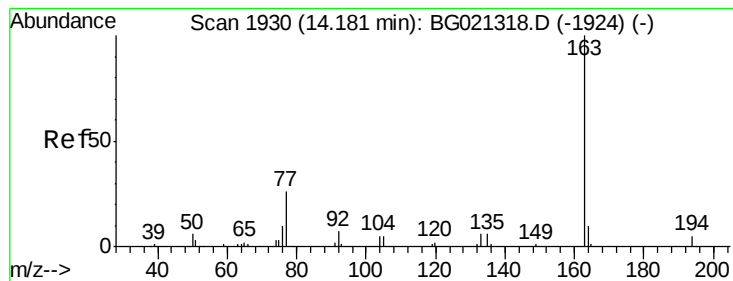

#45

Dimethylphthalate

Concen: 11.92 ng/ul

RT: 14.18 min Scan# 1931

Delta R.T. -0.00 min

Lab File: BG021283.D


Acq: 4 Mar 2016 23:28

Instrument :

BNA_G

ClientSampleId :

JHFJ3

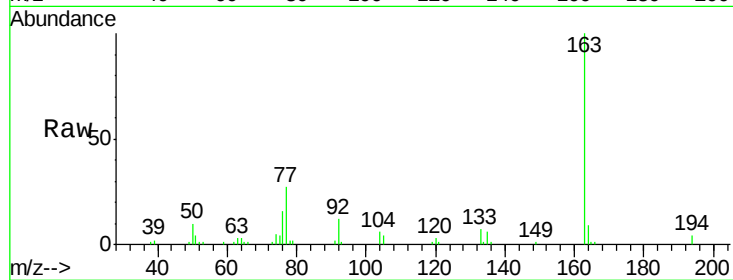


Tgt Ion:163 Resp: 37702

Ion Ratio Lower Upper

163 100

194 3.7 2.8 4.2

164 9.5 8.2 12.2

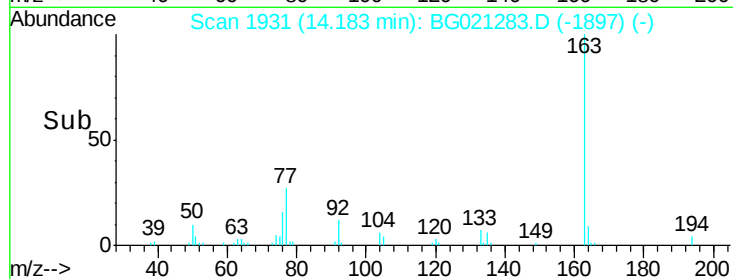

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

