

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030416\
 Data File : BG021285.D
 Acq On : 5 Mar 2016 00:47
 Operator : UM/SJ
 Sample : H1626-15
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JHFK0

Quant Time: Mar 05 02:17:39 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Mar 05 00:52:50 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.13	152	13111	20.00	ng/ul	0.00
18) Naphthalene-d8	10.94	136	62308	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.74	164	36705	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.47	188	79984	20.00	ng/ul	0.00
78) Chrysene-d12	21.74	240	85443	20.00	ng/ul	0.00
86) Perylene-d12	25.00	264	80076	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.54	96	1608	4.98	ng/uL	0.00
5) Phenol-d5	7.27	99	35772	25.76	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.45	67	25282	27.30	ng/ul	0.00
9) 2-Chlorophenol-d4	7.66	132	25540	26.36	ng/ul	0.00
13) 4-Methylphenol-d8	8.82	113	29415	26.83	ng/ul	0.00
19) Nitrobenzene-d5	9.29	128	14616	28.96	ng/ul	0.00
22) 2-Nitrophenol-d4	10.02	143	15533	28.87	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.55	165	26093	27.14	ng/ul	0.00
29) 4-Chloroaniline-d4	11.07	131	39821	32.66	ng/ul	0.00
44) Dimethylphthalate-d6	14.14	166	94663	30.78	ng/ul	0.00
47) Acenaphthylene-d8	14.44	160	117168	30.61	ng/ul	0.00
52) 4-Nitrophenol-d4	14.92	143	15978	26.65	ng/ul	0.00
58) Fluorene-d10	15.72	176	81372	30.12	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.83	200	14851	25.87	ng/ul	0.00
71) Anthracene-d10	17.57	188	124949	31.41	ng/ul	0.00
79) Pyrene-d10	19.85	212	140964	32.59	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.78	264	138585	32.06	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.18	163	37766	11.41	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030416\
Data File : BG021285.D
Acq On : 5 Mar 2016 00:47
Operator : UM/SJ
Sample : H1626-15
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JHFK0

Quant Time: Mar 05 02:17:39 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Mar 05 00:52:50 2016
Response via : Initial Calibration

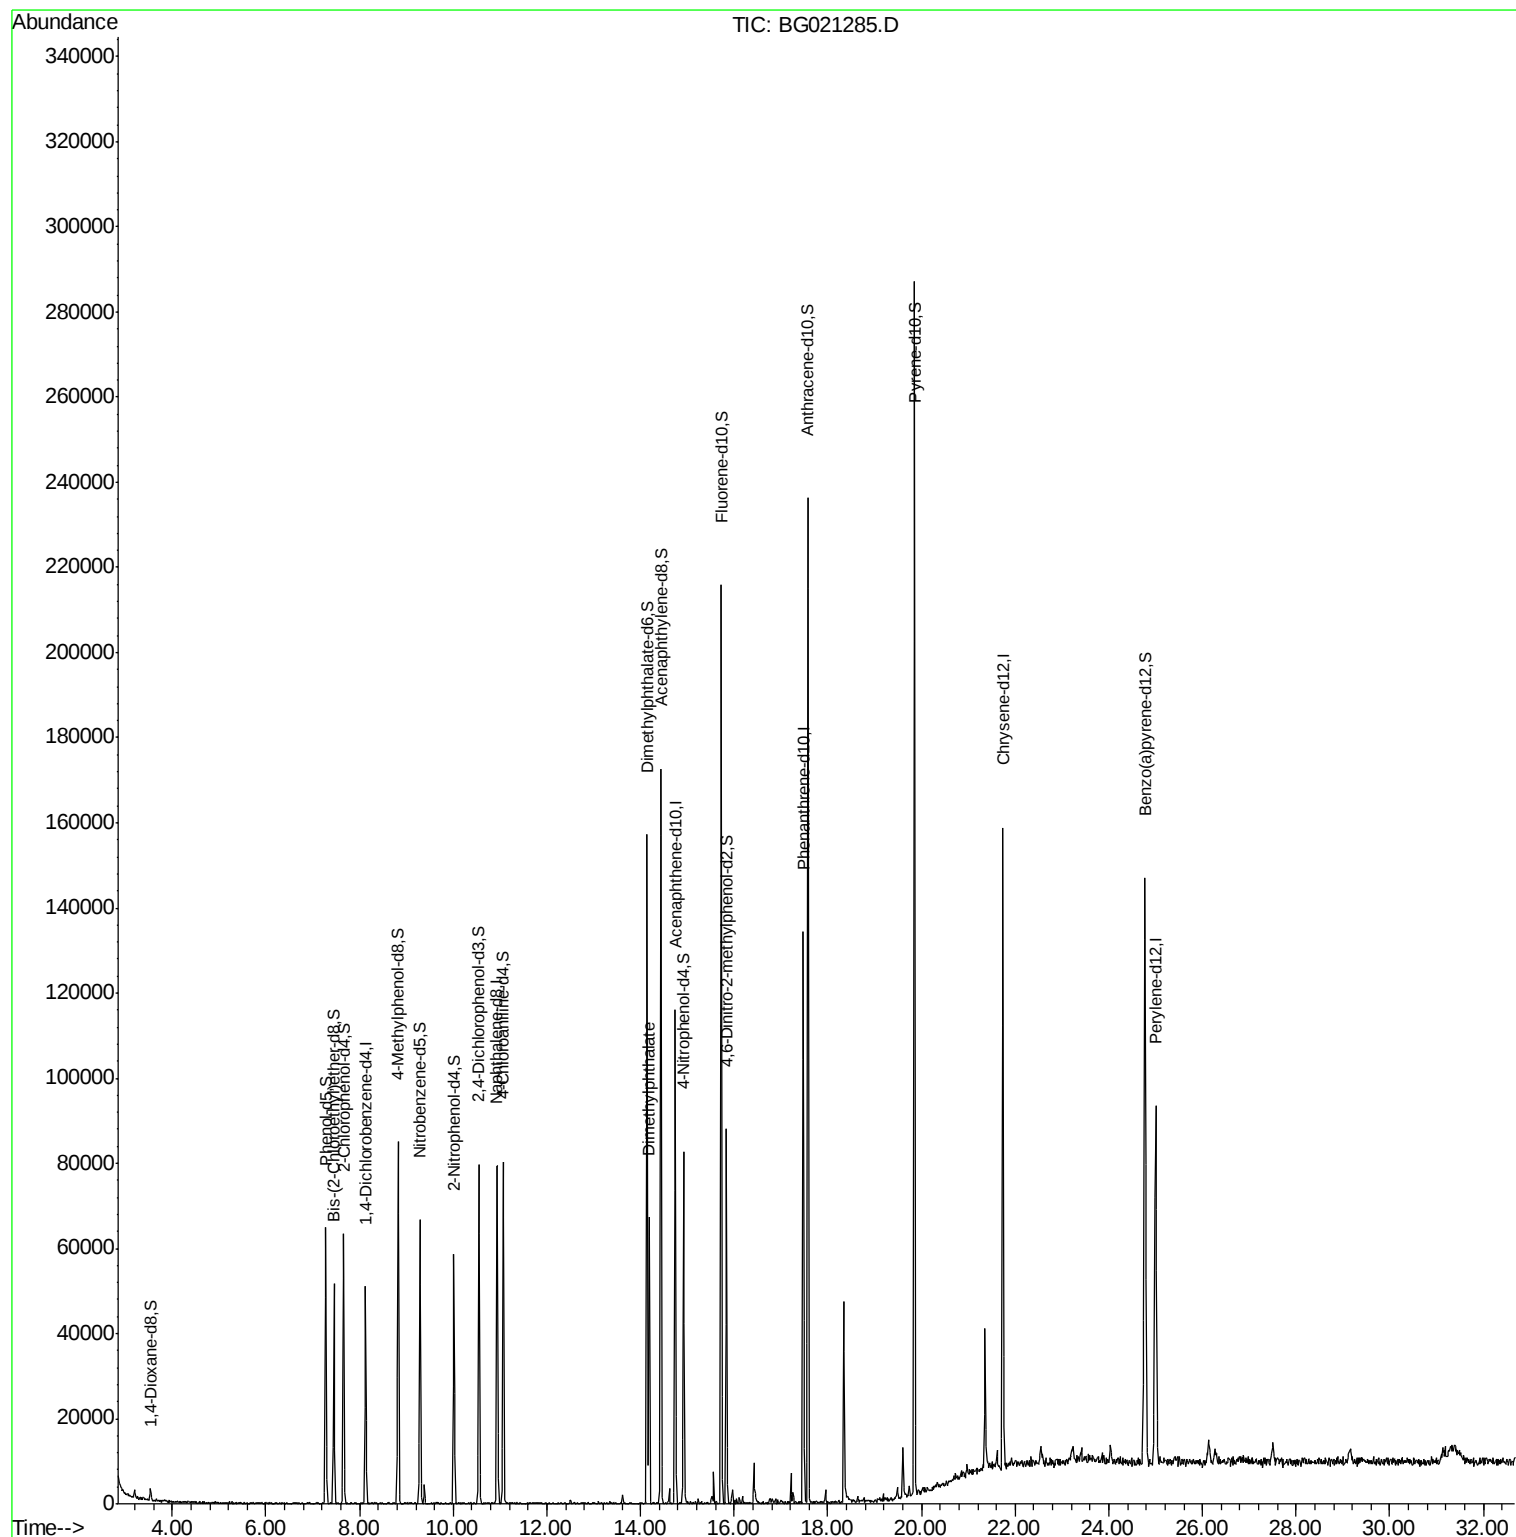


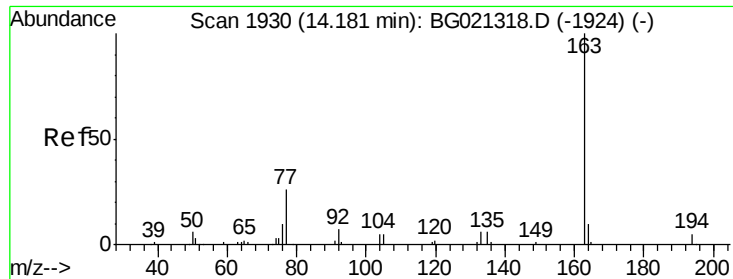

#45
 Dimethylphthalate
 Concen: 11.41 ng/ul
 RT: 14.18 min Scan# 1931
 Delta R.T. 0.00 min
 Lab File: BG021285.D
 Acq: 5 Mar 2016 00:47

Instrument :
 BNA_G
 ClientSampleId :
 JHFK0

Tgt Ion:163 Resp: 37766
 Ion Ratio Lower Upper
 163 100
 194 3.8 2.8 4.2
 164 9.6 8.2 12.2

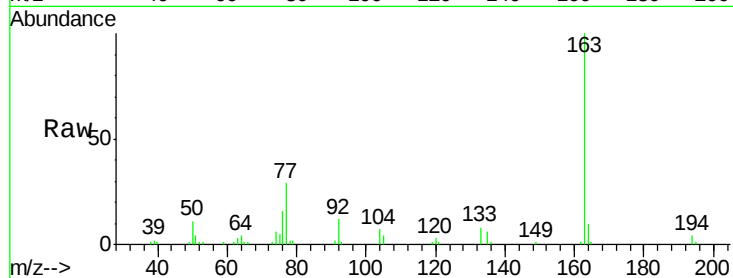

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

