

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030416\
 Data File : BG021287.D
 Acq On : 5 Mar 2016 2:13
 Operator : UM/SJ
 Sample : H1626-16
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JHFK1

Quant Time: Mar 05 05:58:09 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Mar 05 05:52:35 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.13	152	10374	20.00	ng/ul	0.00
18) Naphthalene-d8	10.94	136	48870	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.74	164	29337	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.47	188	68915	20.00	ng/ul	0.00
78) Chrysene-d12	21.74	240	75390	20.00	ng/ul	0.00
86) Perylene-d12	25.00	264	69457	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.53	96	1357	5.31	ng/uL	0.00
5) Phenol-d5	7.27	99	33930	30.88	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.45	67	23326	31.84	ng/ul	0.00
9) 2-Chlorophenol-d4	7.66	132	24357	31.77	ng/ul	0.00
13) 4-Methylphenol-d8	8.82	113	27374	31.55	ng/ul	0.00
19) Nitrobenzene-d5	9.29	128	12991	32.82	ng/ul	0.00
22) 2-Nitrophenol-d4	10.01	143	13918	32.98	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.55	165	23668	31.38	ng/ul	0.00
29) 4-Chloroaniline-d4	11.06	131	36428	38.09	ng/ul	0.00
44) Dimethylphthalate-d6	14.14	166	84518	34.38	ng/ul	0.00
47) Acenaphthylene-d8	14.44	160	105571	34.51	ng/ul	0.00
52) 4-Nitrophenol-d4	14.92	143	15861	33.10	ng/ul	0.00
58) Fluorene-d10	15.72	176	75433	34.94	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.84	200	14215	28.74	ng/ul	0.00
71) Anthracene-d10	17.57	188	120815	35.25	ng/ul	0.00
79) Pyrene-d10	19.85	212	140137	36.72	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.77	264	135194	36.06	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.18	163	31371	11.86	ng/ul#	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030416\
Data File : BG021287.D
Acq On : 5 Mar 2016 2:13
Operator : UM/SJ
Sample : H1626-16
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JHFK1

Quant Time: Mar 05 05:58:09 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Mar 05 05:52:35 2016
Response via : Initial Calibration

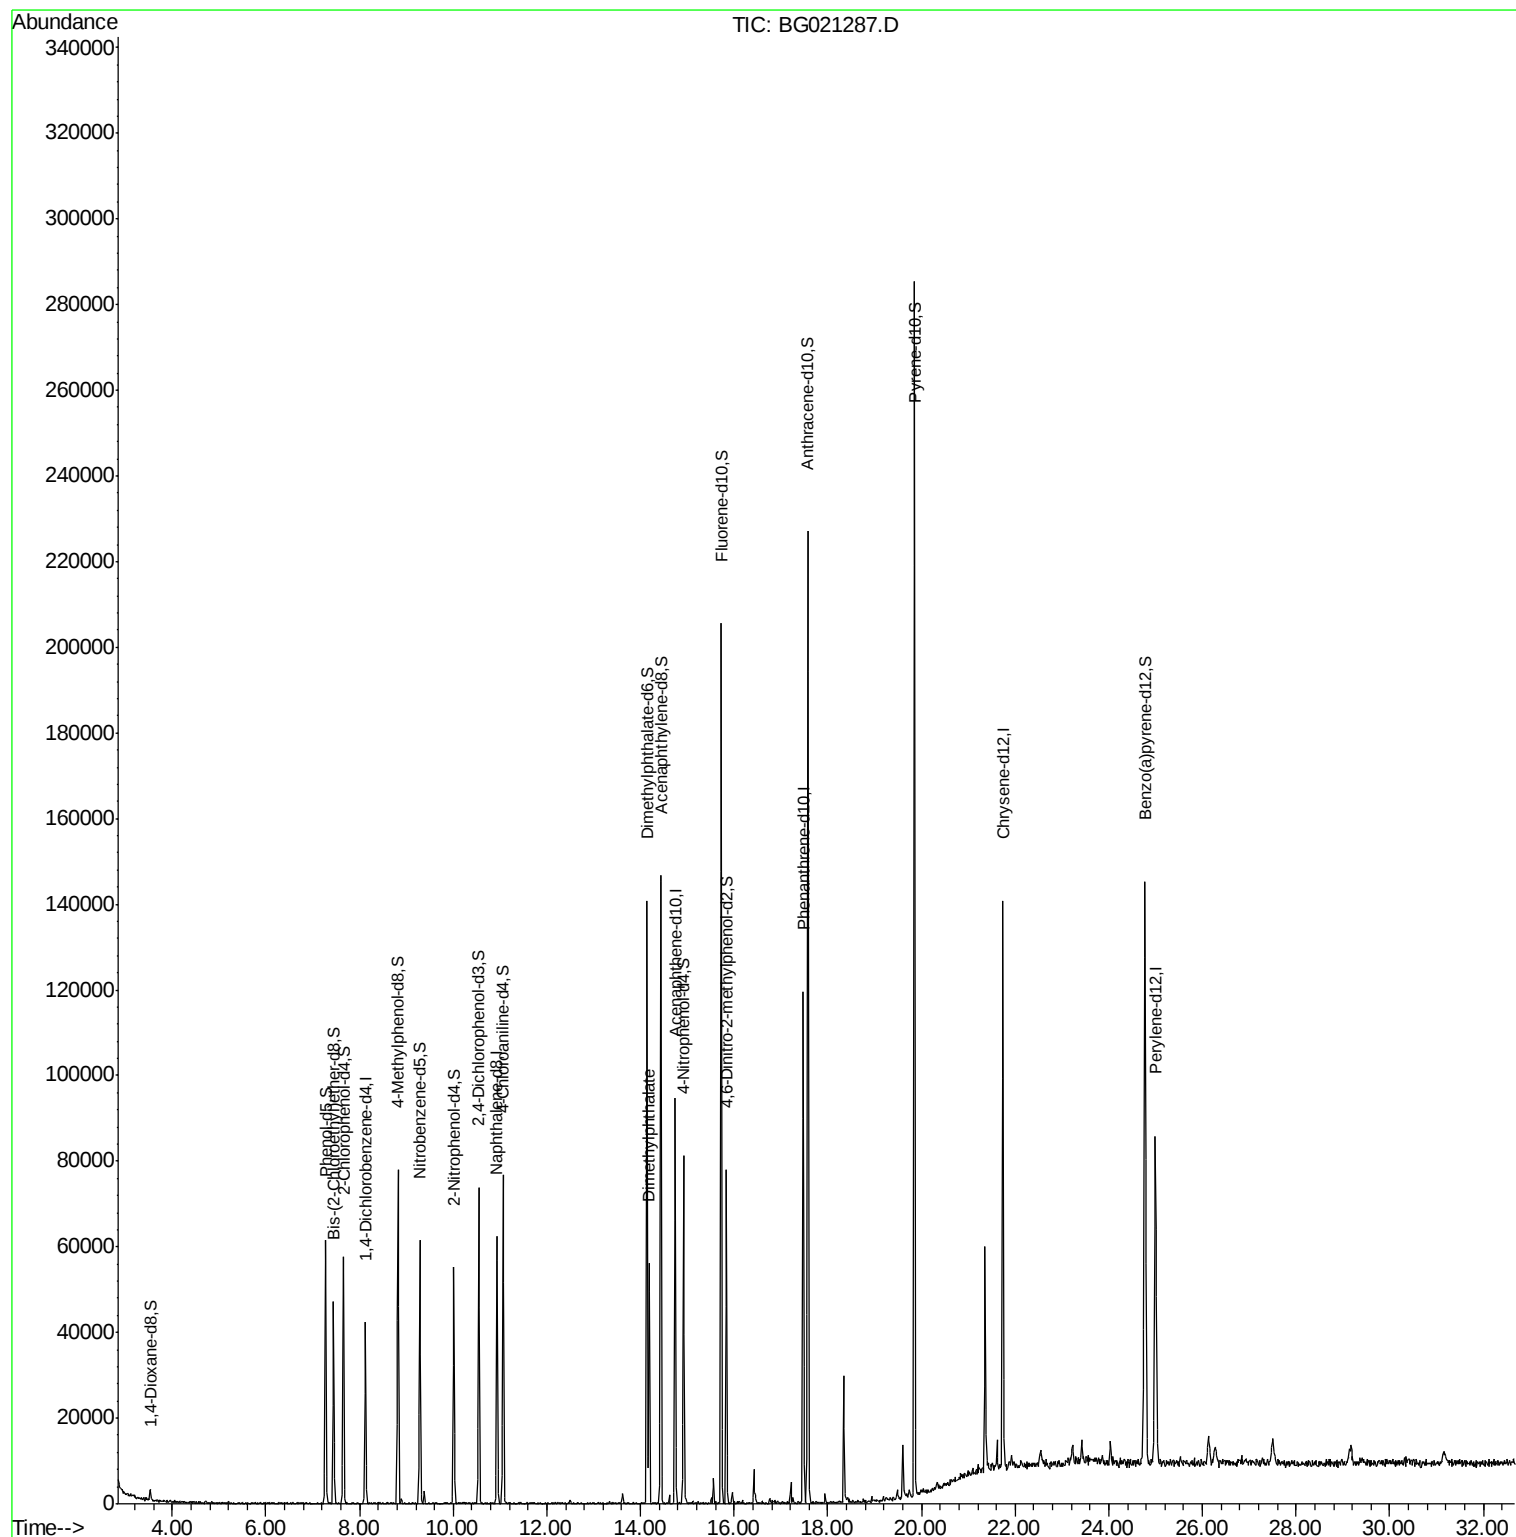

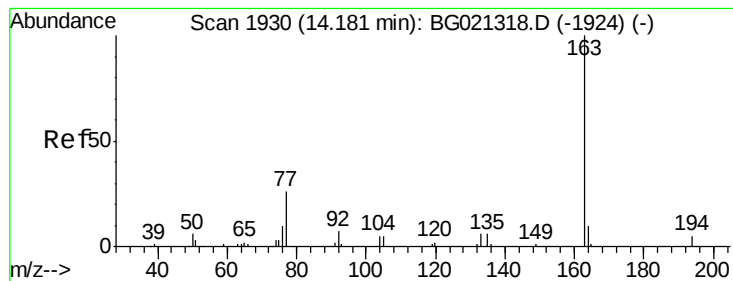

#45

Dimethylphthalate

Concen: 11.86 ng/ul

RT: 14.18 min Scan# 1931

Delta R.T. -0.00 min

Lab File: BG021287.D

Acq: 5 Mar 2016 2:13

Instrument :

BNA_G

ClientSampleId :

JHFK1


Tgt Ion:163 Resp: 31371

Ion Ratio Lower Upper

163 100

194 4.3 2.8 4.2#

164 11.5 8.2 12.2

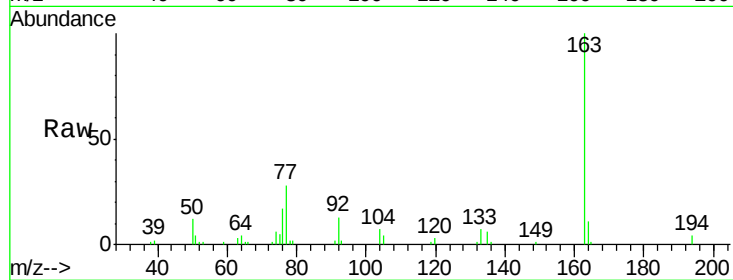

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

