

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030416\
 Data File : BG021276.D
 Acq On : 4 Mar 2016 18:53
 Operator : UM/SJ
 Sample : PB88596BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK96

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.194	55	60	66	rBV	11529	20554	5.83%	0.560%
2	3.270	70	73	75	rVB3	1453	1530	0.43%	0.042%
3	3.535	114	118	126	rVB	3201	4836	1.37%	0.132%
4	3.593	126	128	131	rVV2	720	644	0.18%	0.018%
5	3.623	131	133	136	rVB	966	770	0.22%	0.021%
6	3.664	136	140	143	rBV3	500	844	0.24%	0.023%
7	3.811	163	165	168	rBV2	511	471	0.13%	0.013%
8	3.852	170	172	174	rVV2	547	494	0.14%	0.013%
9	3.916	182	183	186	rVV3	746	508	0.14%	0.014%
10	3.940	186	187	190	rVB2	583	497	0.14%	0.014%
11	4.175	224	227	229	rBV	540	665	0.19%	0.018%
12	4.234	235	237	241	rVB	416	474	0.13%	0.013%
13	4.298	247	248	253	rBV3	421	426	0.12%	0.012%
14	4.451	272	274	277	rVB2	526	435	0.12%	0.012%
15	4.475	277	278	281	rBV2	575	476	0.14%	0.013%
16	4.504	281	283	284	rVV2	650	454	0.13%	0.012%
17	4.569	290	294	298	rVB3	524	583	0.17%	0.016%
18	4.774	327	329	331	rVB2	548	413	0.12%	0.011%
19	4.915	351	353	357	rBV2	299	438	0.12%	0.012%
20	5.062	377	378	380	rBV	469	412	0.12%	0.011%
21	5.409	435	437	439	rBV	463	508	0.14%	0.014%
22	5.503	449	453	454	rVB2	507	449	0.13%	0.012%
23	5.744	491	494	497	rBV2	421	507	0.14%	0.014%
24	5.820	505	507	510	rBV	301	457	0.13%	0.012%
25	5.891	517	519	520	rBV	641	521	0.15%	0.014%
26	6.173	563	567	569	rVV2	345	452	0.13%	0.012%
27	6.214	572	574	577	rBV2	565	702	0.20%	0.019%
28	6.590	636	638	641	rVB	502	550	0.16%	0.015%
29	7.019	708	711	713	rBV	388	409	0.12%	0.011%
30	7.218	742	745	746	rBV	533	422	0.12%	0.011%
31	7.277	749	755	764	rVB	56096	93233	26.45%	2.540%
32	7.453	778	785	792	rVB	43490	71633	20.32%	1.951%
33	7.583	803	807	809	rVB	482	507	0.14%	0.014%
34	7.659	813	820	828	rBV	54465	90999	25.82%	2.479%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030416\
 Data File : BG021276.D
 Acq On : 4 Mar 2016 18:53
 Operator : UM/SJ
 Sample : PB88596BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK96

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
 Title : SVOA CALIBRATION

35	7.824	846	848	851	rVB	518	505	0.14%	0.014%
36	7.882	854	858	862	rBV	206	498	0.14%	0.014%
37	8.129	893	900	907	rBB	37555	61878	17.55%	1.686%
38	8.822	1012	1018	1027	rVB	69722	115322	32.72%	3.142%
39	9.292	1091	1098	1106	rBV	57734	100467	28.50%	2.737%
40	10.015	1214	1221	1228	rBB	50222	84834	24.07%	2.311%
41	10.550	1306	1312	1319	rBB2	65667	111713	31.69%	3.043%
42	10.938	1371	1378	1385	rBB	61419	100947	28.64%	2.750%
43	11.067	1394	1400	1411	rBB	70015	122472	34.75%	3.336%
44	12.518	1643	1647	1649	rBB	697	767	0.22%	0.021%
45	13.617	1830	1834	1838	rBB2	1185	1819	0.52%	0.050%
46	14.140	1916	1923	1930	rBB	134954	190196	53.96%	5.181%
47	14.434	1965	1973	1981	rBV	139279	214714	60.91%	5.849%
48	14.739	2018	2025	2032	rBB2	93320	142720	40.49%	3.888%
49	14.915	2050	2055	2067	rBV	69427	112525	31.92%	3.065%
50	15.726	2187	2193	2200	rVB	187045	274269	77.81%	7.472%
51	15.838	2206	2212	2219	rVB	65873	98991	28.08%	2.697%
52	15.961	2229	2233	2235	rBV2	1302	1197	0.34%	0.033%
53	17.230	2446	2449	2452	rBB	426	505	0.14%	0.014%
54	17.271	2452	2456	2459	rBB	527	725	0.21%	0.020%
55	17.477	2485	2491	2498	rVV2	122980	179526	50.93%	4.891%
56	17.577	2501	2508	2514	rVV	206647	309645	87.85%	8.436%
57	17.706	2527	2530	2533	rVB	443	493	0.14%	0.013%
58	17.871	2555	2558	2561	rVB	464	648	0.18%	0.018%
59	17.906	2561	2564	2566	rBV	412	553	0.16%	0.015%
60	17.935	2566	2569	2571	rVV	481	621	0.18%	0.017%
61	17.965	2571	2574	2578	rVV	382	594	0.17%	0.016%
62	18.035	2582	2586	2587	rVV	332	417	0.12%	0.011%
63	18.529	2669	2670	2674	rBV	417	458	0.13%	0.012%
64	18.999	2749	2750	2753	rBV	529	480	0.14%	0.013%
65	19.052	2756	2759	2762	rBV	407	495	0.14%	0.013%
66	19.204	2780	2785	2787	rBV2	695	652	0.18%	0.018%
67	19.304	2801	2802	2808	rVB2	570	837	0.24%	0.023%
68	19.392	2815	2817	2818	rBV	684	576	0.16%	0.016%
69	19.445	2824	2826	2827	rBV2	555	566	0.16%	0.015%
70	19.486	2830	2833	2838	rVB2	2013	2901	0.82%	0.079%
71	19.533	2838	2841	2843	rBV	615	740	0.21%	0.020%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030416\
 Data File : BG021276.D
 Acq On : 4 Mar 2016 18:53
 Operator : UM/SJ
 Sample : PB88596BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK96

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
 Title : SVOA CALIBRATION

72	19.551	2843	2844	2847	rBV2	778	622	0.18%	0.017%
73	19.604	2852	2853	2855	rVV2	673	434	0.12%	0.012%
74	19.645	2859	2860	2862	rVV	850	412	0.12%	0.011%
75	19.669	2862	2864	2865	rVB	769	451	0.13%	0.012%
76	19.733	2871	2875	2878	rBV	1160	1800	0.51%	0.049%
77	19.780	2880	2883	2884	rVB2	793	552	0.16%	0.015%
78	19.851	2886	2895	2904	rBV	258760	352485	100.00%	9.603%
79	19.980	2914	2917	2918	rBV2	1086	851	0.24%	0.023%
80	20.033	2924	2926	2928	rBV2	745	583	0.17%	0.016%
81	20.280	2966	2968	2969	rVB2	888	439	0.12%	0.012%
82	20.303	2969	2972	2975	rBV3	1176	977	0.28%	0.027%
83	20.567	3015	3017	3019	rVB3	1024	819	0.23%	0.022%
84	20.603	3021	3023	3024	rVB2	1027	502	0.14%	0.014%
85	20.632	3024	3028	3029	rBV3	1102	1572	0.45%	0.043%
86	20.914	3074	3076	3079	rVB3	1129	740	0.21%	0.020%
87	21.208	3124	3126	3127	rBV2	1267	801	0.23%	0.022%
88	21.414	3159	3161	3162	rBV2	1615	864	0.25%	0.024%
89	21.737	3210	3216	3223	rVB	133314	207619	58.90%	5.656%
90	21.831	3230	3232	3233	rBV	1392	1037	0.29%	0.028%
91	22.230	3299	3300	3304	rBV3	1539	1866	0.53%	0.051%
92	22.283	3307	3309	3311	rBV3	1616	1350	0.38%	0.037%
93	22.524	3348	3350	3351	rBV2	2113	1941	0.55%	0.053%
94	23.223	3465	3469	3476	rVB6	5005	9994	2.84%	0.272%
95	23.446	3506	3507	3510	rBV3	1910	932	0.26%	0.025%
96	24.040	3604	3608	3612	rVB6	4660	7609	2.16%	0.207%
97	24.774	3723	3733	3743	rVB2	120048	320577	90.95%	8.733%
98	24.998	3762	3771	3782	rVB2	75711	198514	56.32%	5.408%
99	25.979	3936	3938	3939	rBV2	1669	1340	0.38%	0.037%
100	26.132	3961	3964	3974	rVB9	7553	18507	5.25%	0.504%


Sum of corrected areas: 3670729

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030416\
Data File : BG021276.D
Acq On : 4 Mar 2016 18:53
Operator : UM/SJ
Sample : PB88596BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK96

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

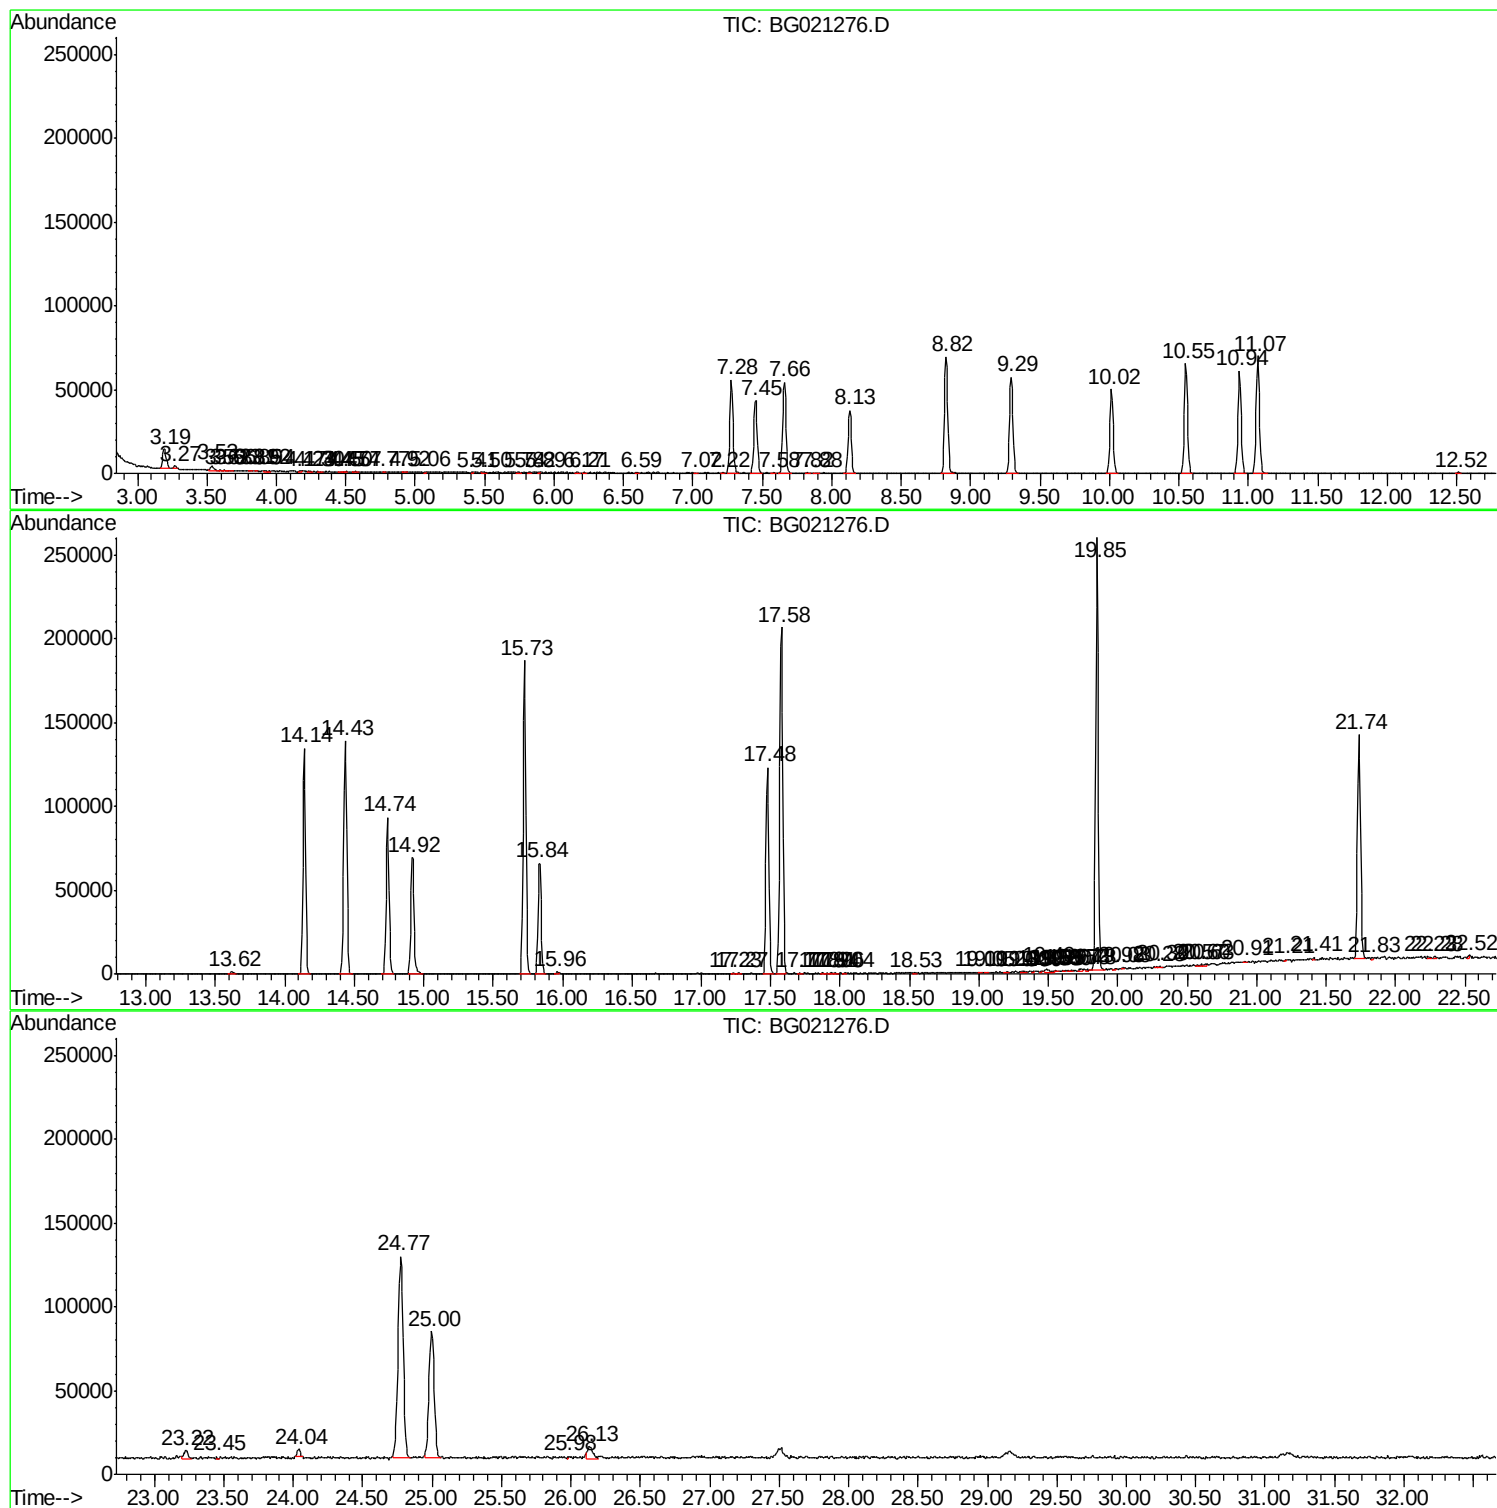

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030416\
Data File : BG021276.D
Acq On : 4 Mar 2016 18:53
Operator : UM/SJ
Sample : PB88596BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK96

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030416\
Data File : BG021276.D
Acq On : 4 Mar 2016 18:53
Operator : UM/SJ
Sample : PB88596BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK96

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc