


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030416\
Data File : BG021272.D
Acq On : 4 Mar 2016 16:20
Operator : UM/SJ
Sample : DFTPP02
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP02

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
Title : SVOA CALIBRATION
Last Update : Mon Mar 07 04:51:57 2016

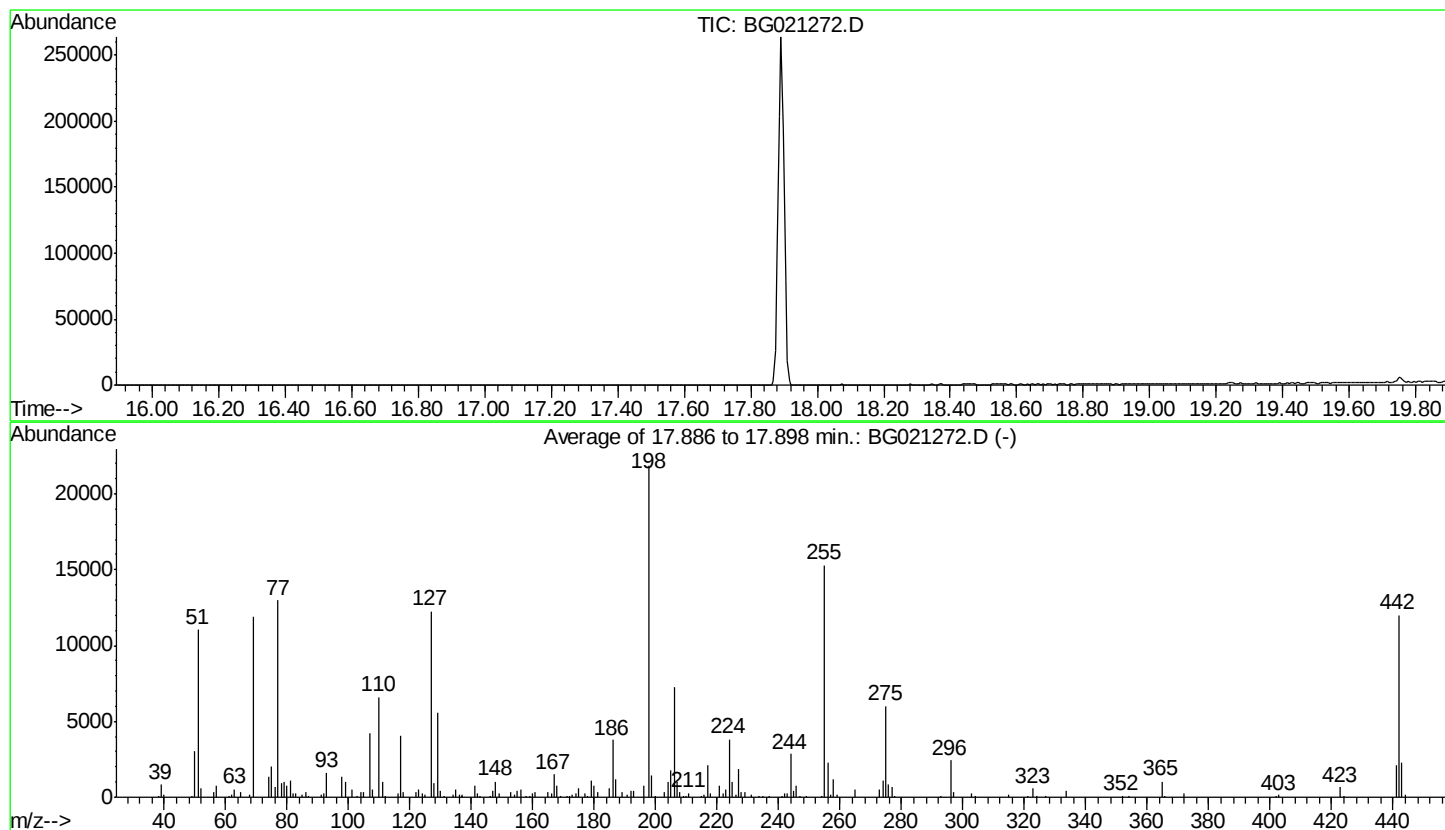

AutoFind: Scans 2561, 2562, 2563; Background Corrected with Scan 2556

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.4	11027	PASS
68	69	0.00	2	1.6	191	PASS
69	198	0.00	100	54.4	11898	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	56.1	12262	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	21861	PASS
199	198	5	9	6.7	1469	PASS
275	198	10	60	27.5	6013	PASS
365	198	1	100	4.7	1031	PASS
441	442	0.01	100	17.4	2090	PASS
442	198	50	100	54.9	12007	PASS
443	442	15	24	18.7	2247	PASS

m/z	Abundance
206.90	236.0

Instrument :
BNA_G
ClientSampleId :
DFTPP02

m/z	Abundance
38.00	162.0
39.00	908.0
39.90	179.0
49.00	166.0
50.00	3228.0
51.00	11115.0
52.00	564.0
55.90	363.0
56.90	829.0
61.90	156.0
63.00	460.0
65.00	289.0
67.90	163.0
68.90	12293.0
74.00	1360.0
74.90	2072.0
76.00	692.0
77.00	13519.0
78.00	1018.0
78.90	1018.0
79.90	828.0
80.90	901.0
82.00	299.0
83.00	196.0
85.00	215.0
85.90	357.0
86.90	177.0
90.90	262.0
91.90	270.0
92.90	1745.0
97.90	1563.0
98.90	1067.0
100.90	550.0
103.00	211.0
103.80	286.0
104.90	340.0
106.90	4195.0
107.90	535.0
109.90	6451.0
110.90	892.0
115.90	178.0
116.90	3985.0
117.90	358.0
121.90	287.0
122.90	497.0
123.90	267.0
125.00	232.0
126.90	12007.0
127.90	1023.0
128.90	5103.0
129.90	508.0
133.90	222.0
134.90	454.0
135.90	179.0
136.80	162.0
140.90	845.0
141.90	219.0
145.90	185.0
146.80	476.0
147.90	860.0
148.90	222.0
153.00	312.0
154.00	210.0
154.80	347.0
155.90	521.0
159.90	192.0
160.80	332.0
164.90	335.0
165.90	356.0
166.90	1331.0
167.90	834.0
170.90	169.0
172.90	182.0
173.90	200.0
174.90	602.0
176.90	307.0
178.90	1029.0
179.90	731.0
180.90	267.0
184.90	705.0
185.90	3312.0
186.90	1027.0
188.80	273.0
190.90	220.0
191.90	357.0
192.90	347.0
195.90	672.0
197.80	19312.0
198.80	1378.0
202.90	283.0
203.90	848.0

Instrument :
BNA_G
ClientSampleId :
DFTPP02

204.90	1661.0
205.90	6723.0
206.90	1055.0
207.90	376.0
209.90	171.0
210.80	313.0
215.80	214.0
216.90	1892.0
217.80	221.0
220.90	835.0
221.80	259.0
222.80	452.0
223.90	3347.0
224.90	758.0
225.90	186.0
226.90	1726.0
227.90	278.0
228.90	318.0
230.90	165.0
234.90	156.0
236.90	155.0
241.90	160.0
242.80	218.0
243.90	2372.0
244.90	458.0
245.90	653.0
253.80	151.0
254.90	12885.0
255.90	2163.0
257.80	1188.0
264.90	427.0
272.90	345.0
273.90	1023.0
274.90	4964.0
275.90	766.0
276.90	528.0
292.90	163.0
295.90	2148.0
296.80	264.0
302.80	184.0
322.90	450.0
333.80	325.0
364.80	850.0
365.80	172.0
371.90	157.0
402.70	151.0
422.90	424.0
440.90	1403.0
441.90	8680.0
442.90	1535.0

Instrument :
BNA_G
ClientSampleId :
DFTPP02

m/z	Abundance
39.00	962.0
39.90	220.0
50.00	3584.0
51.00	12903.0
52.00	625.0
55.90	473.0
56.90	931.0
60.90	190.0
62.00	191.0
63.00	656.0
64.90	379.0
68.00	236.0
68.90	14294.0
74.00	1486.0
74.90	2303.0
76.00	909.0
77.00	15372.0
78.00	1007.0
79.00	1149.0
79.90	835.0
80.90	1280.0
81.90	218.0
82.90	262.0
84.90	203.0
85.90	370.0
90.90	247.0
91.90	295.0
92.90	1862.0
97.90	1310.0
98.90	1184.0
100.90	606.0
102.90	171.0
103.90	432.0
104.90	455.0
106.90	4908.0
107.90	627.0
109.90	8165.0
110.90	1239.0
112.00	151.0
115.90	469.0
116.90	5003.0
118.00	384.0
121.90	437.0
122.90	605.0
123.90	223.0
124.90	173.0
126.90	14218.0
127.90	1113.0
128.90	7132.0
129.90	554.0
130.90	173.0
133.90	251.0
134.90	541.0
135.90	279.0
137.00	315.0
140.90	930.0
141.90	266.0
142.90	195.0
145.90	158.0
146.90	485.0
147.90	1274.0
148.90	329.0
152.80	309.0
153.90	192.0
154.90	508.0
155.90	661.0
157.80	230.0
158.90	152.0
159.90	270.0
160.90	386.0
164.90	434.0
165.90	243.0
166.90	1670.0
167.90	850.0
171.90	213.0
172.80	171.0
173.90	372.0
174.90	779.0
176.80	297.0
177.80	155.0
178.90	1227.0
179.90	909.0
180.90	455.0
185.00	630.0
185.90	4481.0
186.90	1265.0
188.90	358.0
190.80	219.0
191.90	519.0
192.90	486.0
195.90	871.0

Instrument :
BNA_G
ClientSampleId :
DFTPP02

197.80	26432.0
198.80	1837.0
199.90	167.0
202.80	393.0
203.90	1147.0
204.90	2041.0
205.90	8450.0
206.90	1405.0
207.90	354.0
209.80	177.0
210.90	336.0
214.90	191.0
215.90	179.0
216.90	2708.0
217.90	296.0
220.90	944.0
221.60	277.0
222.90	635.0
223.90	4568.0
224.90	1196.0
225.90	205.0
226.90	2258.0
227.90	360.0
228.80	408.0
230.90	209.0
233.80	153.0
236.90	195.0
240.90	207.0
241.80	355.0
242.80	303.0
243.90	3335.0
244.90	570.0
245.90	948.0
246.90	175.0
248.90	220.0
253.90	220.0
254.90	18448.0
255.90	2736.0
256.80	217.0
257.90	1085.0
258.80	166.0
264.90	621.0
272.80	565.0
273.90	1364.0
274.90	7297.0
275.90	919.0
276.90	898.0
277.90	159.0
292.90	165.0
295.90	2806.0
296.80	399.0
302.90	269.0
304.00	166.0
314.90	327.0
320.90	161.0
322.90	687.0
323.80	221.0
326.90	157.0
333.80	432.0
351.80	260.0
364.80	1285.0
371.90	282.0
402.80	174.0
422.80	805.0
424.00	184.0
440.90	2332.0
441.90	14141.0
442.90	2564.0
443.80	349.0

Instrument :
BNA_G
ClientSampleId :
DFTPP02

m/z	Abundance
39.00	655.0
39.90	160.0
50.00	2251.0
51.00	9065.0
52.00	494.0
55.90	299.0
56.90	537.0
61.90	180.0
62.90	419.0
65.00	289.0
68.00	176.0
68.90	9109.0
74.00	1133.0
75.00	1672.0
76.00	558.0
77.00	10018.0
78.00	707.0
78.90	852.0
79.90	581.0
81.00	996.0
81.90	179.0
82.90	232.0
84.90	197.0
85.90	251.0
91.80	171.0
92.90	1286.0
97.90	1234.0
98.90	824.0
101.00	441.0
103.80	395.0
104.90	347.0
106.90	3467.0
107.90	488.0
109.90	5137.0
110.90	849.0
115.90	247.0
116.90	3276.0
117.90	206.0
121.90	362.0
122.90	321.0
123.90	215.0
126.90	10562.0
127.90	750.0
128.90	4386.0
129.90	338.0
134.90	420.0
136.90	190.0
140.90	598.0
142.00	218.0
142.90	178.0
146.90	439.0
147.90	946.0
148.90	163.0
152.80	285.0
154.90	423.0
155.90	374.0
159.90	196.0
160.80	185.0
164.80	217.0
165.90	199.0
166.90	1478.0
167.90	582.0
168.90	206.0
172.90	178.0
173.80	275.0
174.90	450.0
176.90	275.0
178.90	1047.0
179.90	680.0
180.90	360.0
184.80	376.0
185.90	3489.0
186.90	1158.0
188.80	296.0
190.90	158.0
191.90	365.0
192.90	499.0
195.90	650.0
197.80	19840.0
198.80	1194.0
202.80	310.0
203.90	1161.0
204.90	1614.0
205.90	6601.0
206.90	1251.0
207.80	348.0
208.90	159.0
210.90	213.0
215.90	164.0
216.90	1758.0
217.90	242.0

Instrument :
BNA_G
ClientSampleId :
DFTPP02

220.80	633.0
221.80	214.0
222.90	433.0
223.90	3517.0
224.90	989.0
226.90	1643.0
227.80	280.0
228.80	410.0
230.90	154.0
234.80	176.0
241.80	185.0
242.90	209.0
243.90	2888.0
244.90	346.0
245.80	611.0
254.90	14603.0
255.90	1906.0
256.80	216.0
257.90	1177.0
258.90	269.0
264.80	508.0
272.90	507.0
273.80	1018.0
274.90	5778.0
275.80	836.0
276.90	641.0
295.90	2276.0
296.90	287.0
302.90	207.0
314.90	245.0
322.90	525.0
323.90	159.0
326.90	155.0
333.80	463.0
353.90	168.0
364.80	960.0
365.80	167.0
371.90	307.0
401.90	155.0
402.90	163.0
422.90	679.0
423.90	197.0
440.90	2535.0
441.90	13201.0
442.90	2642.0
443.90	219.0

Instrument :
BNA_G
ClientSampleId :
DFTPP02