
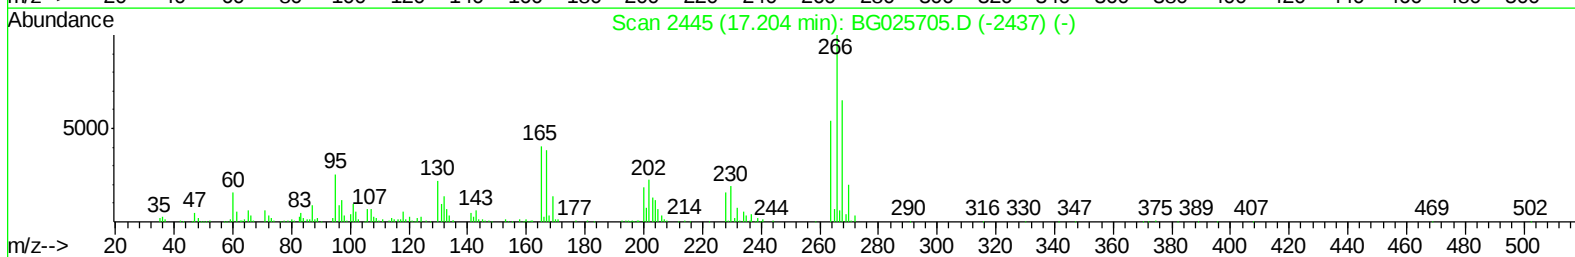
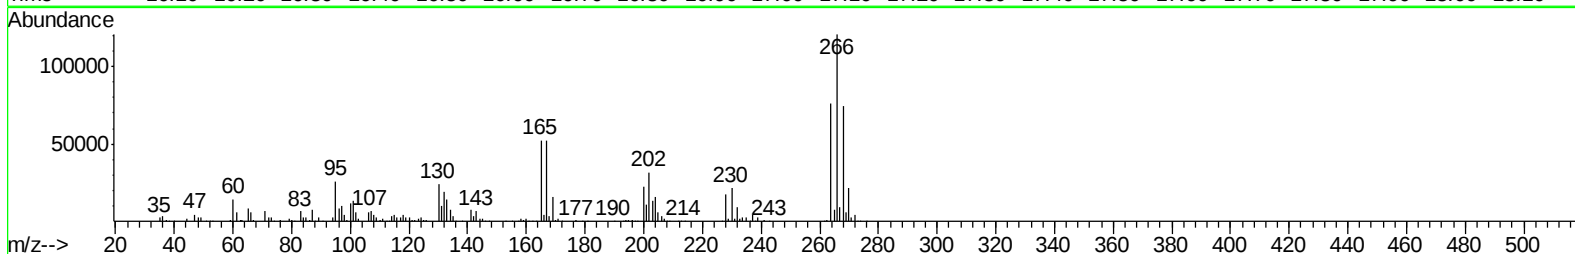


Data Path : Z:\HPCHEM1\BNA_G\Data\BG030417\
Data File : BG026064.D
Acq On : 3 Mar 2017 15:11
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 04 04:36:27 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG021717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 28 15:36:56 2017
Response via : Initial Calibration

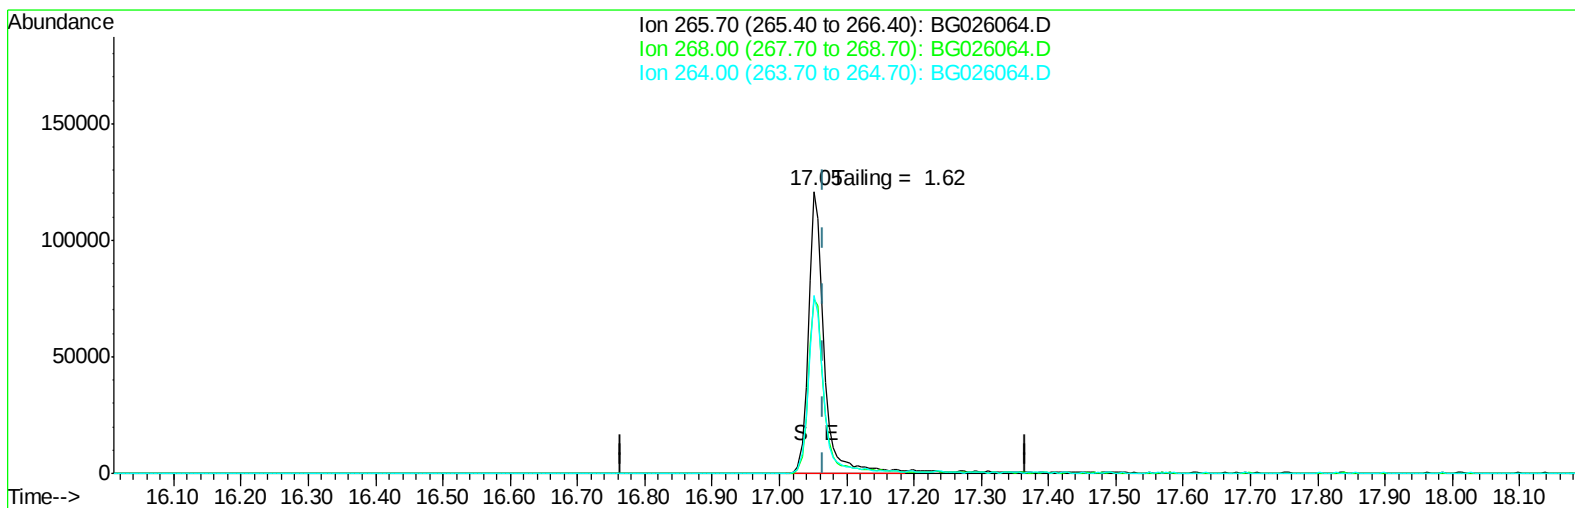

TIC: BG026064.D

(69) Pentachlorophenol (C)




17.051min (-0.015) 469193.36ng

response 196966

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	62.06
264.00	62.60	63.14
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG030417\
Data File : BG026064.D
Acq On : 3 Mar 2017 15:11
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 04 04:36:27 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG021717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 28 15:36:56 2017
Response via : Initial Calibration

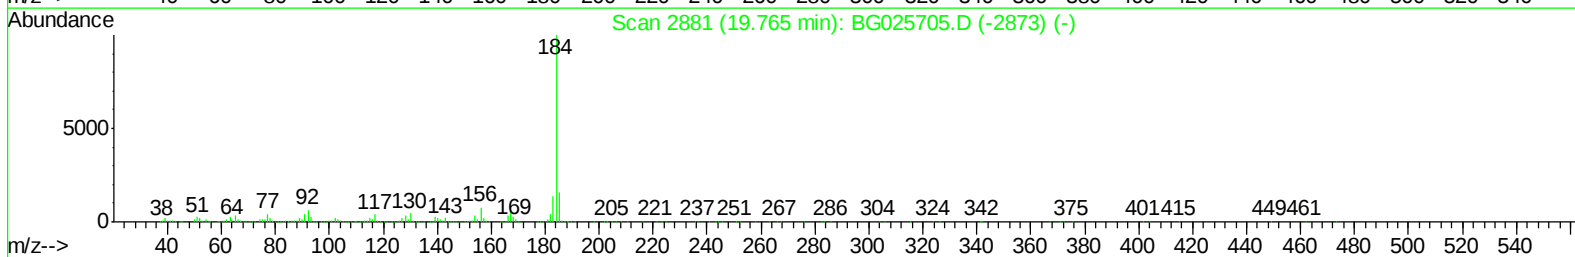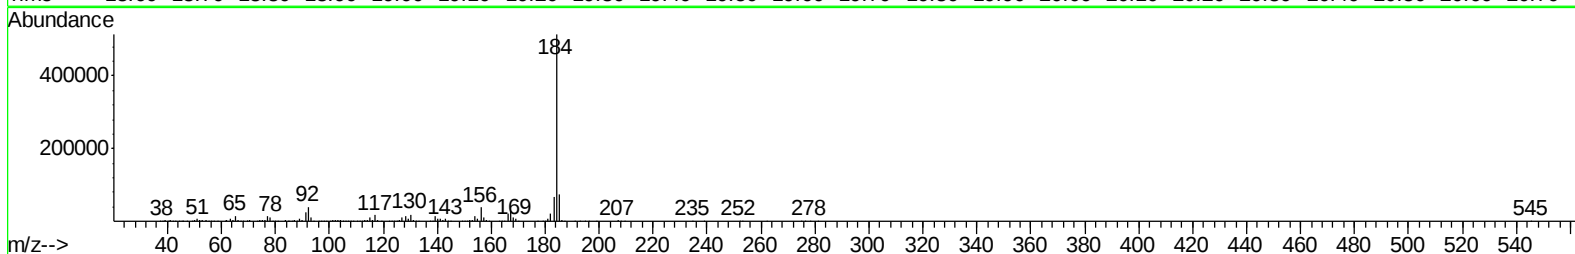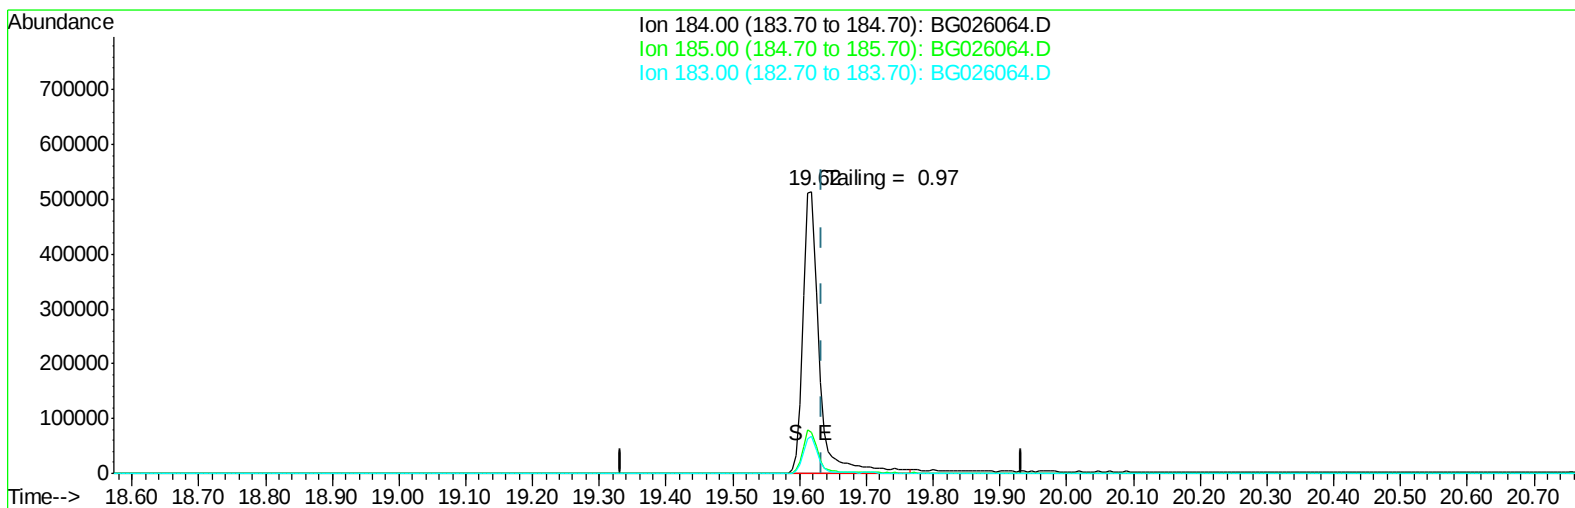

TIC: BG026064.D

(76) Benzidine

19.619min (-0.015) 14685.40ng

response 846032

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	14.73
183.00	13.80	13.16
0.00	0.00	0.00