

Data Path : Z:\HPCHEM1\BNA G\DATA\BG030417\
 Data File : BG026070.D
 Acq On : 3 Mar 2017 19:08
 Operator : SJ/MA
 Sample : I2081-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 022717-PRRT-F-U-M

Quant Time: Mar 03 22:56:43 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG021717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 28 15:36:56 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.07	152	117315	20.00	ng	-0.02
21) Naphthalene-d8	10.87	136	490889	20.00	ng	-0.02
38) Acenaphthene-d10	14.67	164	277400	20.00	ng	-0.02
63) Phenanthrene-d10	17.40	188	644805	20.00	ng	-0.01
75) Chrysene-d12	21.65	240	624481	20.00	ng	-0.03
86) Perylene-d12	24.84	264	585121	20.00	ng	-0.04
System Monitoring Compounds						
5) 2-Fluorophenol	5.64	112	293025	43.49	ng	-0.01
7) Phenol-d6	7.22	99	246448	24.72	ng	-0.01
23) Nitrobenzene-d5	9.22	82	731985	94.10	ng	-0.02
41) 2,4,6-Tribromophenol	16.15	330	282418	110.20	ng	-0.01
44) 2-Fluorobiphenyl	13.30	172	1780610	112.16	ng	-0.02
78) Terphenyl-d14	20.00	244	2238049	87.16	ng	-0.02
Target Compounds						
49) Dimethylphthalate	14.11	163	63258	3.32	ng	Qvalue # 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG030417\
Data File : BG026070.D
Acq On : 3 Mar 2017 19:08
Operator : SJ/MA
Sample : I2081-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
022717-PRRT-F-U-M

Quant Time: Mar 03 22:56:43 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG021717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 28 15:36:56 2017
Response via : Initial Calibration

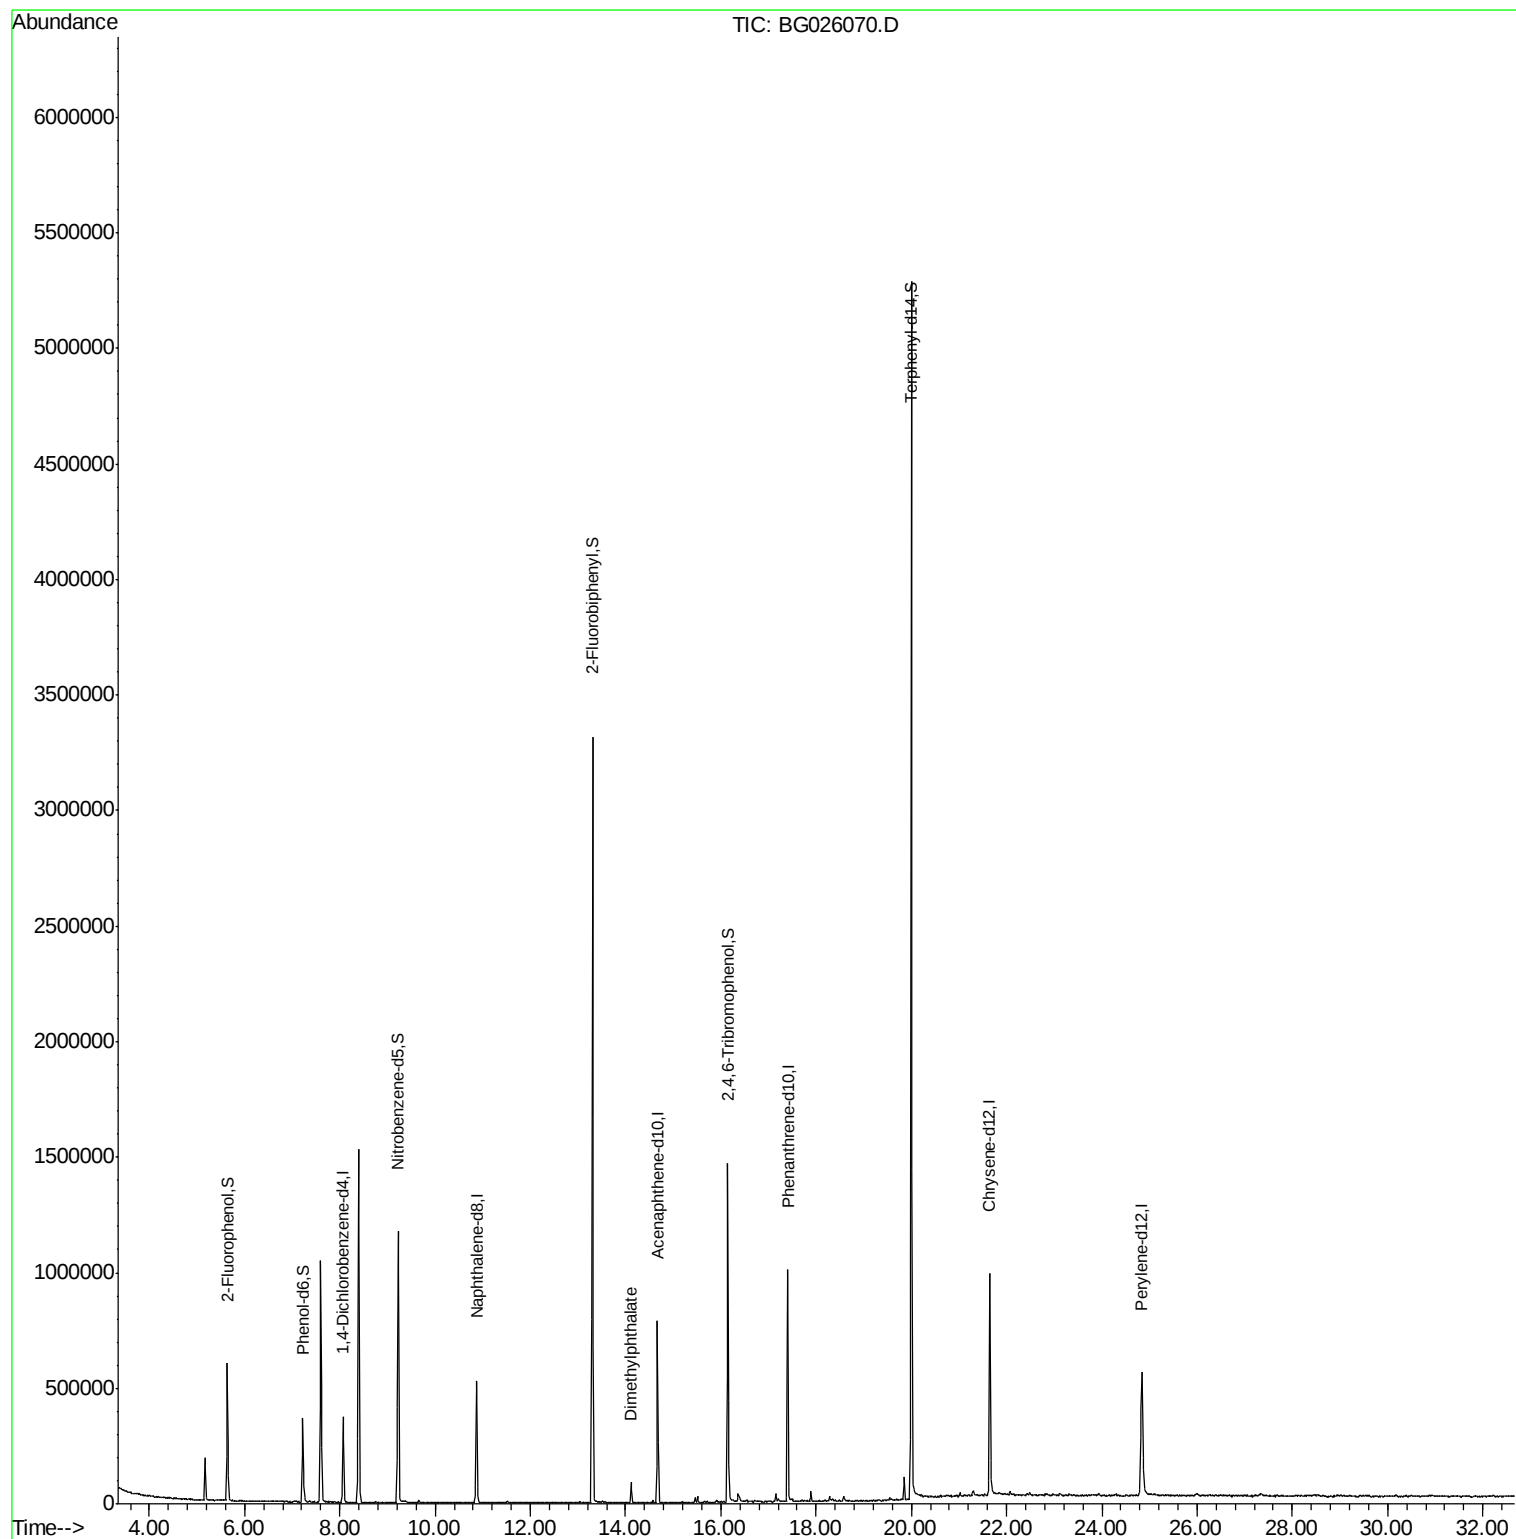

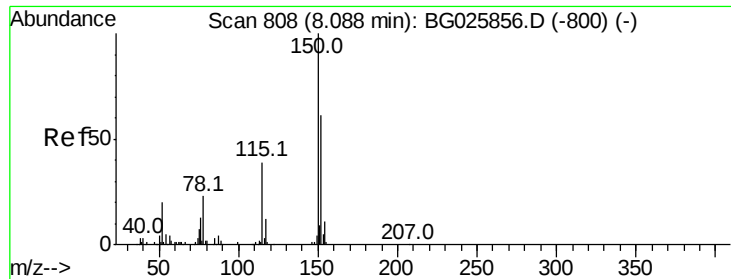


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 8.07 min Scan# 805
Delta R.T. -0.02 min
Lab File: BG026070.D
Acq: 3 Mar 2017 19:08

Instrument :
BNA_G
ClientSampleId :
022717-PRRT-F-U-M

Tot Ion	Ratio	Lower	Upper
152	100		
150	155.3	114.0	171.0
115	57.4	48.1	72.1

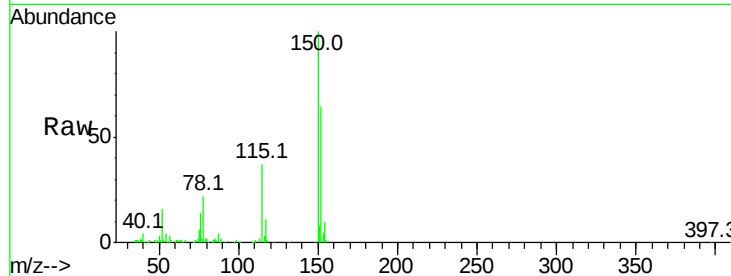


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

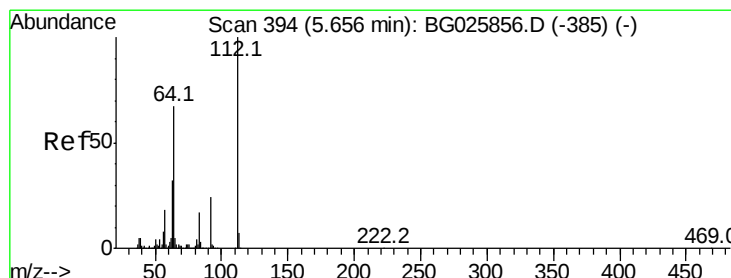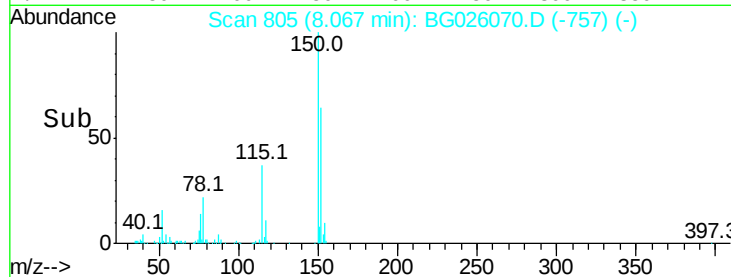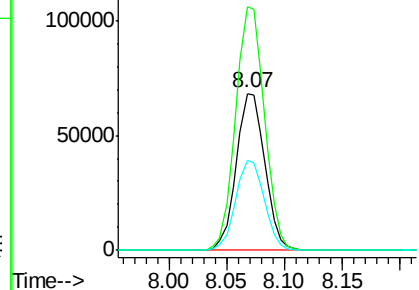



#5


2-Fluorophenol
Concen: 43.49 ng
RT: 5.64 min Scan# 392
Delta R.T. -0.01 min
Lab File: BG026070.D
Acq: 3 Mar 2017 19:08

Tgt Ion	Ratio	Lower	Upper
112	100		
64	59.8	61.8	92.6#
63	29.1	37.2	55.8#

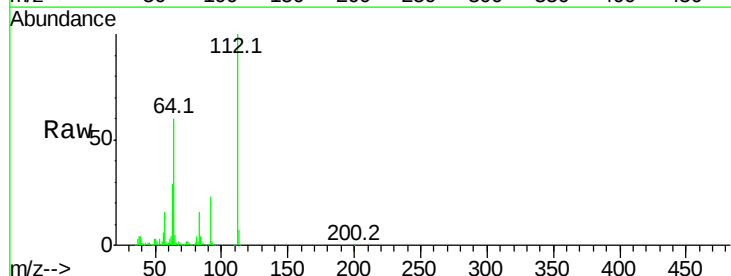

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

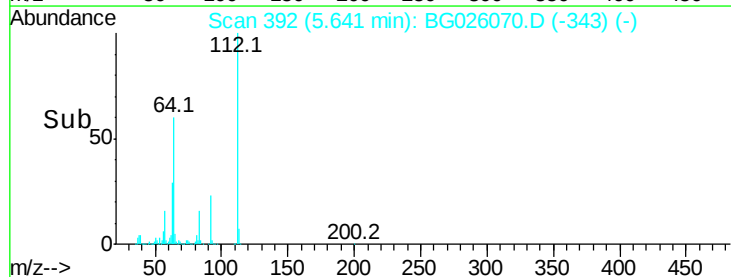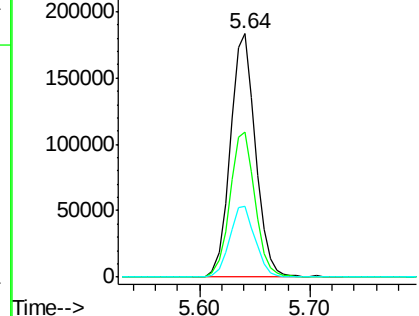

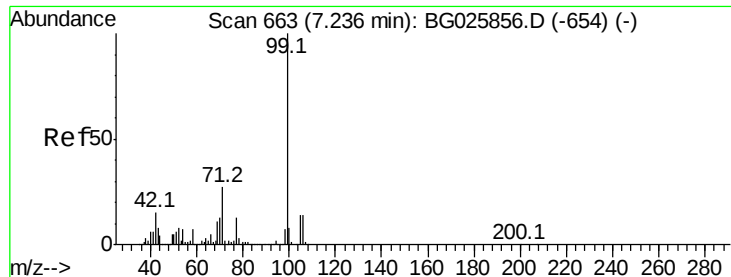

#7

Phenol-d6

Concen: 24.72 ng

RT: 7.22 min Scan# 661

Delta R.T. -0.01 min

Lab File: BG026070.D

Acq: 3 Mar 2017 19:08

Instrument :

BNA_G

ClientSampleId :

022717-PRRT-F-U-M


Tot Ion: 99 Resp: 246448

Ion Ratio Lower Upper




99 100

42 11.8 20.5 30.7#

71 26.5 37.6 56.4#

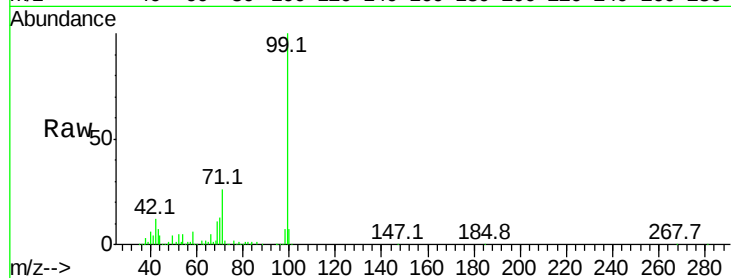

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

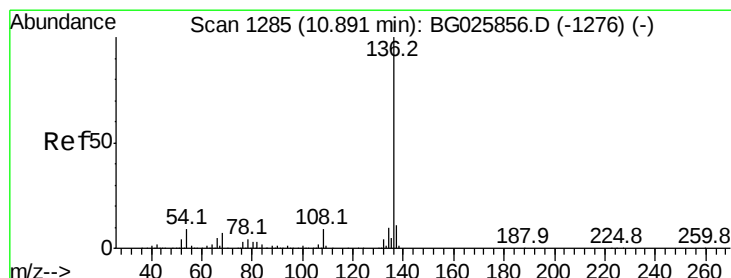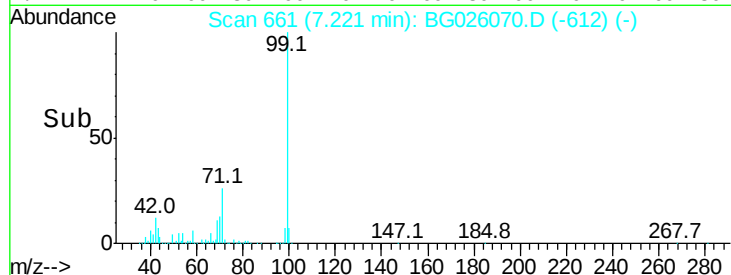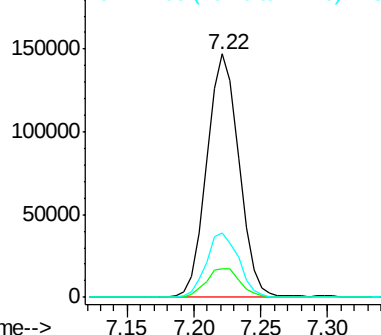

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.87 min Scan# 1282

Delta R.T. -0.02 min

Lab File: BG026070.D

Acq: 3 Mar 2017 19:08

Tgt Ion: 136 Resp: 490889


Ion Ratio Lower Upper

136 100



137 11.2 8.9 13.3


54 6.7 9.3 13.9#

68 6.7 5.1 7.7

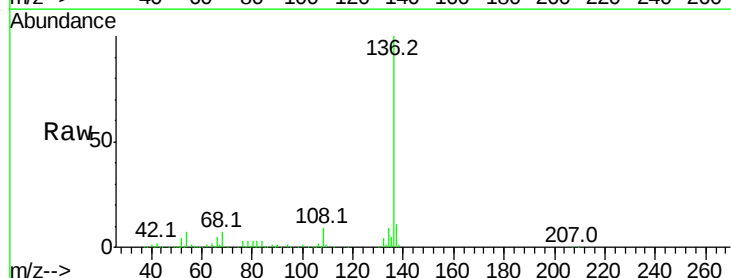

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



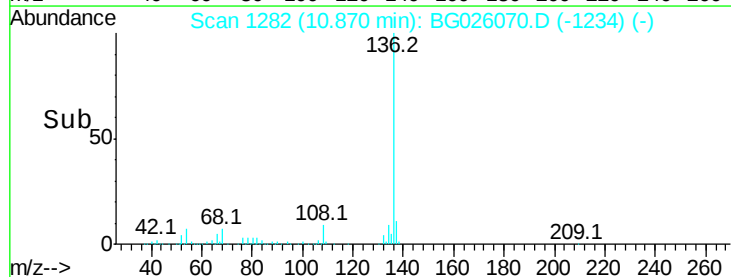
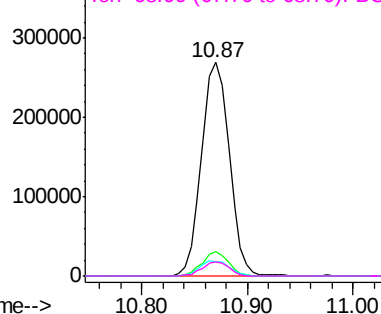


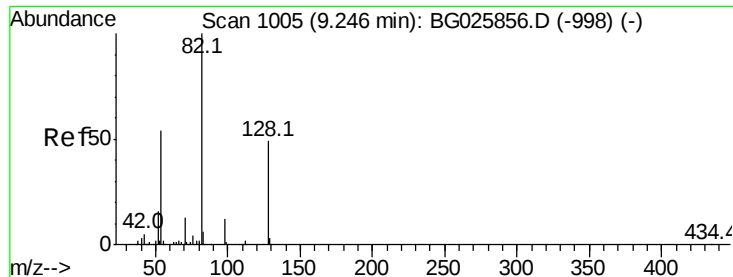

#23
 Nitrobenzene-d5
 Concen: 94.10 ng
 RT: 9.22 min Scan# 1002
 Delta R.T. -0.02 min
 Lab File: BG026070.D
 Acq: 3 Mar 2017 19:08




Instrument :
 BNA_G
 ClientSampleId :
 022717-PRRT-F-U-M


Tot Ion	Ratio	Lower	Upper
82	100		
128	48.1	26.4	39.6#
54	45.7	49.4	74.2#

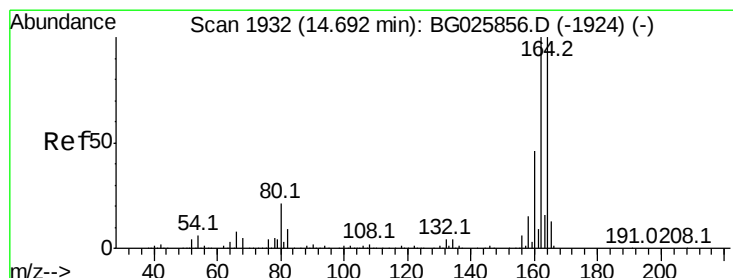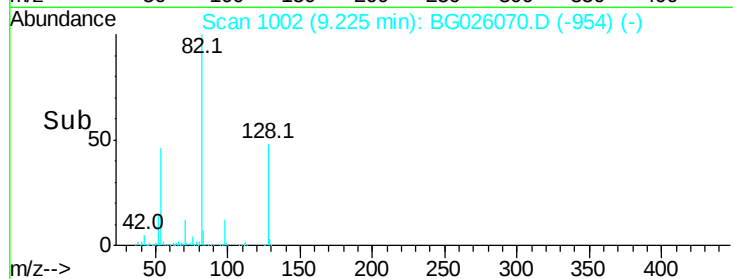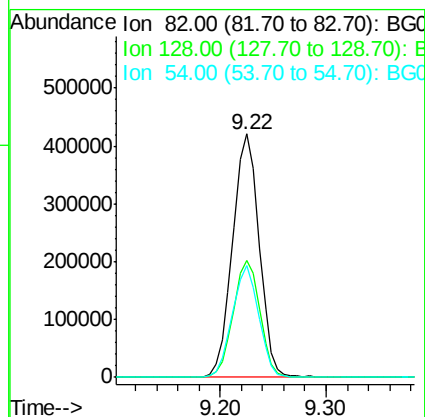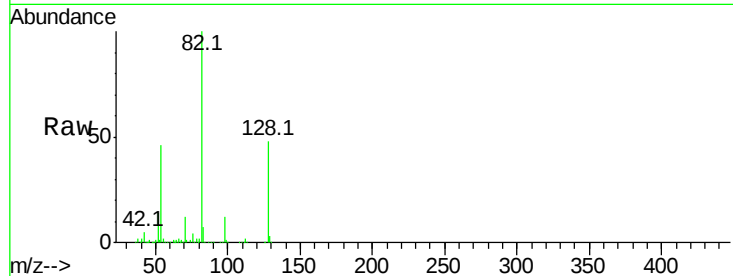

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.67 min Scan# 1929
 Delta R.T. -0.02 min
 Lab File: BG026070.D
 Acq: 3 Mar 2017 19:08

Tgt Ion	Ratio	Lower	Upper
164	100		
162	98.5	85.1	127.7
160	44.8	34.7	52.1

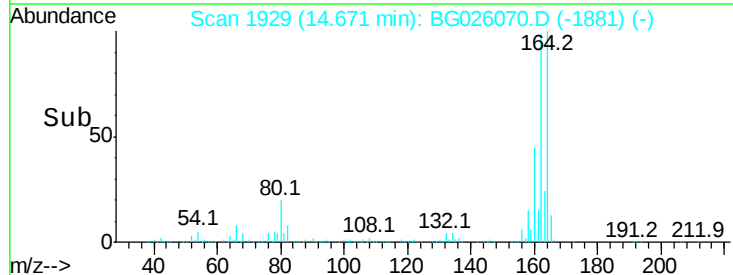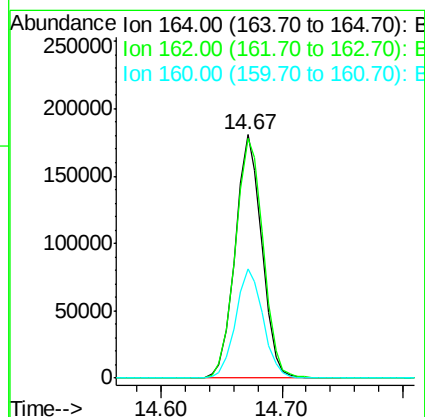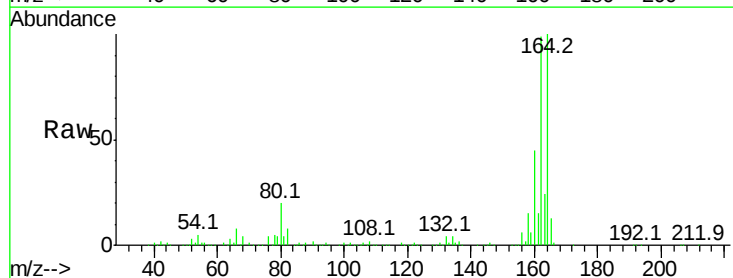


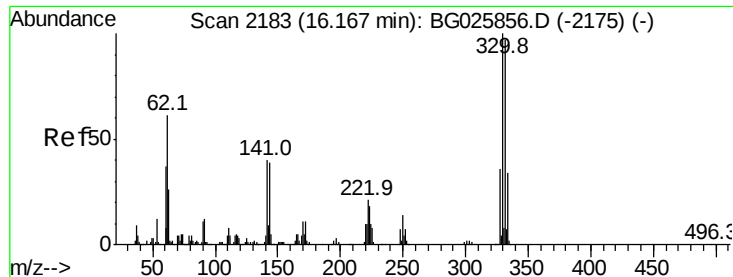




#41
2,4,6-Tribromophenol
Concen: 110.20 ng
RT: 16.15 min Scan# 2181
Delta R.T. -0.01 min
Lab File: BG026070.D
Acq: 3 Mar 2017 19:08

Instrument :
BNA_G
ClientSampleId :
022717-PRRT-F-U-M

Tot Ion:330 Resp: 282418
Ion Ratio Lower Upper
330 100
332 97.1 77.3 115.9
141 36.4 32.1 48.1

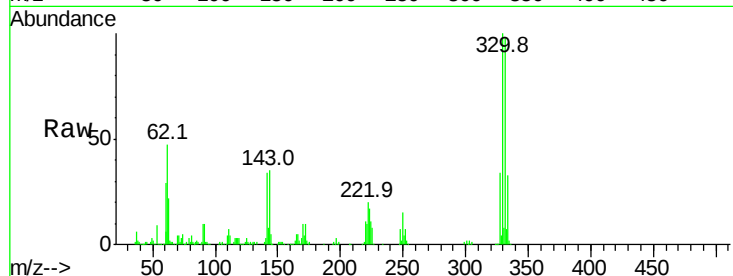


Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

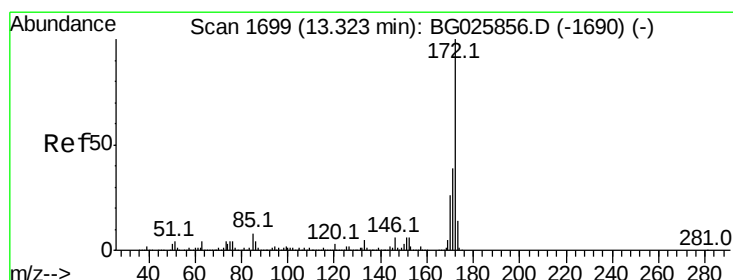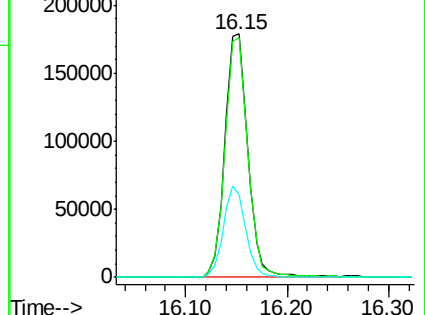
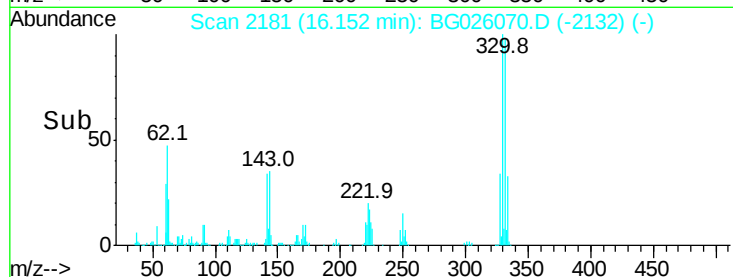



#44
2-Fluorobiphenyl
Concen: 112.16 ng
RT: 13.30 min Scan# 1696
Delta R.T. -0.02 min
Lab File: BG026070.D
Acq: 3 Mar 2017 19:08

Tgt Ion:172 Resp: 1780610
Ion Ratio Lower Upper
172 100
171 38.0 32.2 48.2
170 26.0 21.8 32.6

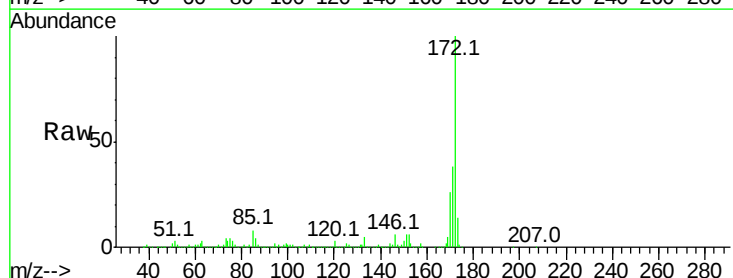

Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

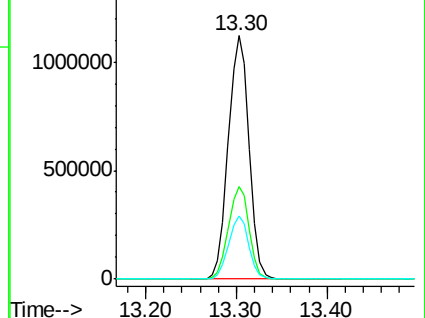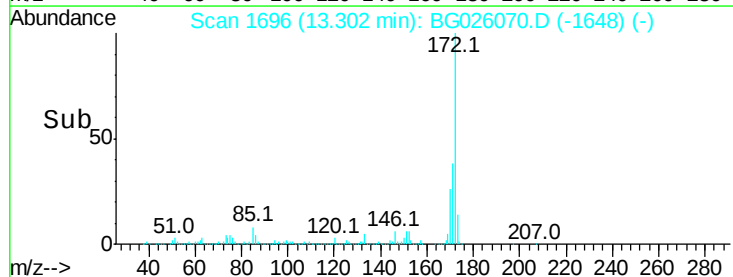

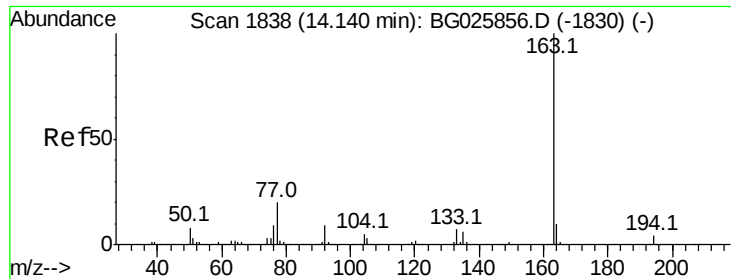

#49

Dimethylphthalate

Concen: 3.32 ng

RT: 14.11 min Scan# 1834

Delta R.T. -0.03 min

Lab File: BG026070.D

Acq: 3 Mar 2017 19:08

Instrument :

BNA_G

ClientSampleId :

022717-PRRT-F-U-M


Tot Ion:163 Resp: 63258

Ion Ratio Lower Upper

163 100

194 3.3 3.8 5.6#




164 7.8 9.3 13.9#

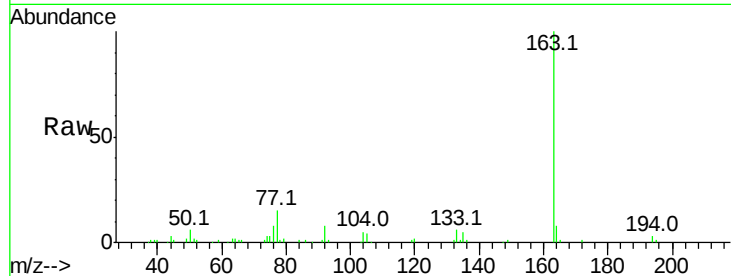

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

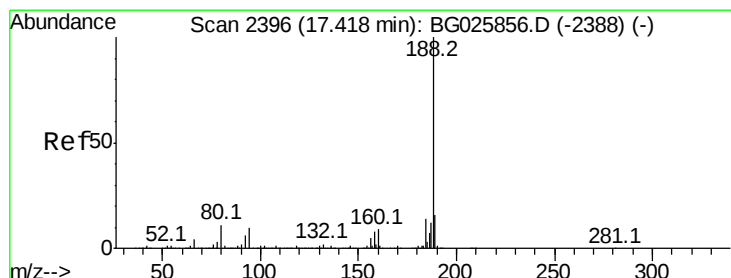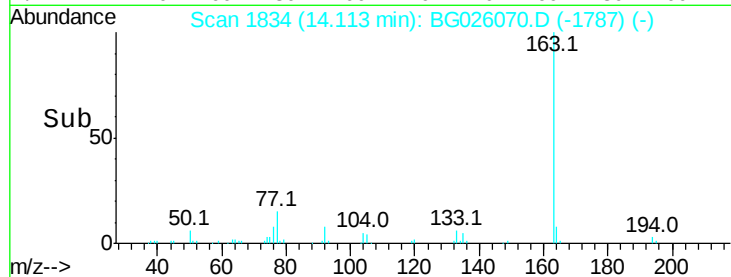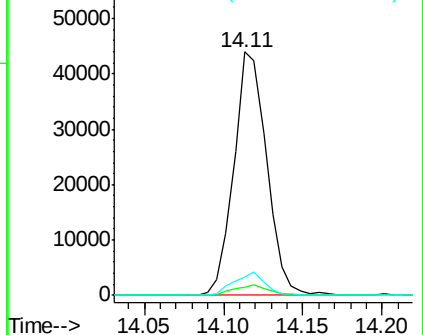

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 17.40 min Scan# 2394

Delta R.T. -0.01 min

Lab File: BG026070.D

Acq: 3 Mar 2017 19:08


Tgt Ion:188 Resp: 644805

Ion Ratio Lower Upper

188 100

94 9.9 5.8 8.8#



80 9.5 7.5 11.3

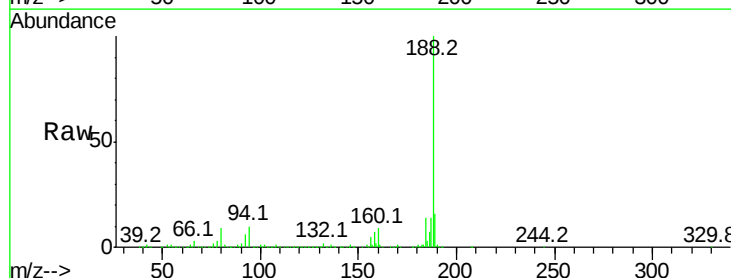


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

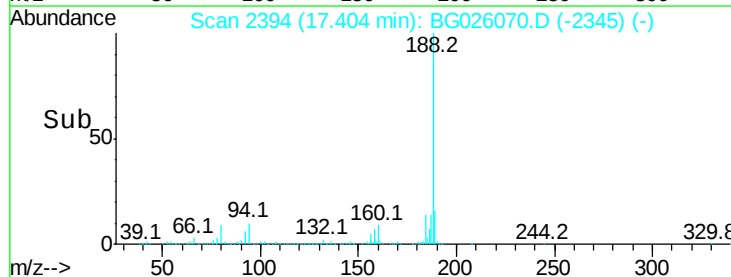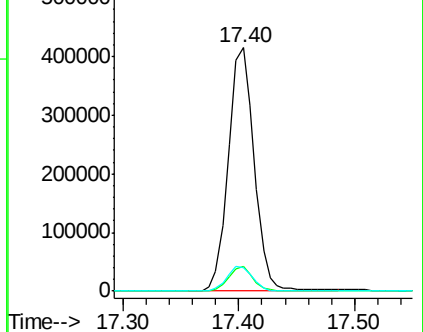

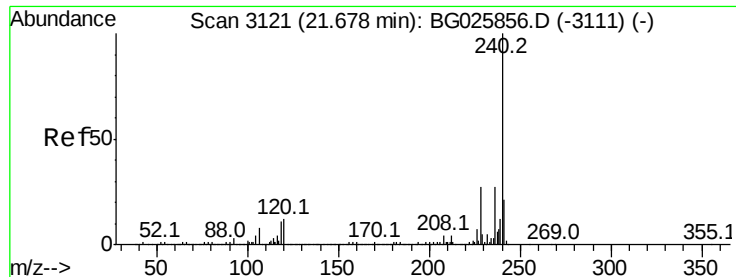

#75

Chrysene-d12

Concen: 20.00 ng

RT: 21.65 min Scan# 3116

Delta R.T. -0.03 min

Lab File: BG026070.D

Acq: 3 Mar 2017 19:08

Instrument :

BNA_G

ClientSampleId :

022717-PRRT-F-U-M


Tot Ion:240 Resp: 624481

Ion Ratio Lower Upper

240 100

120 12.2 5.7 8.5#




236 26.2 22.2 33.4

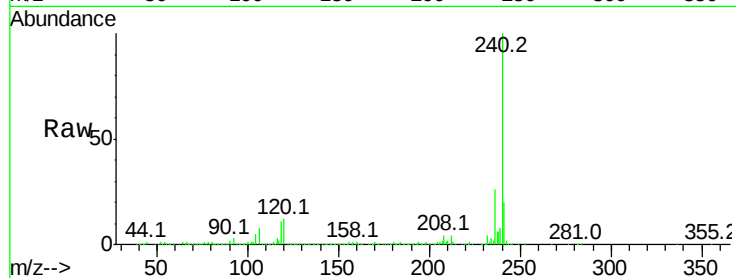

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

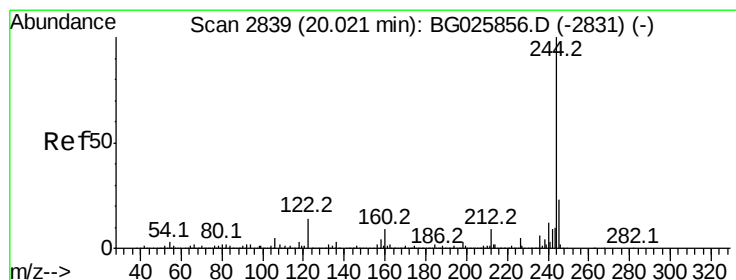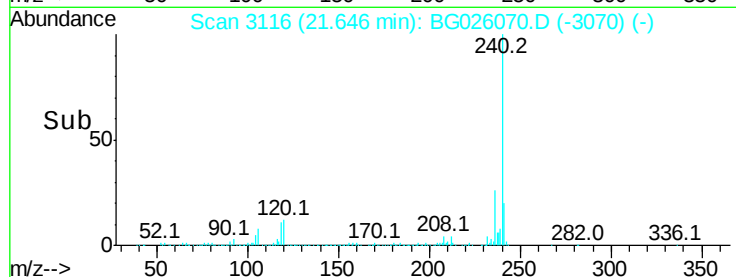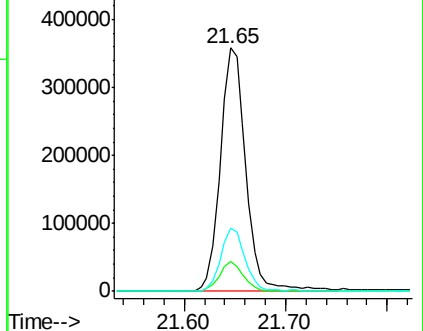

#78

Terphenyl-d14

Concen: 87.16 ng

RT: 20.00 min Scan# 2836

Delta R.T. -0.02 min

Lab File: BG026070.D

Acq: 3 Mar 2017 19:08


Tgt Ion:244 Resp: 2238049

Ion Ratio Lower Upper

244 100

212 8.4 10.0 15.0#



122 13.2 8.6 12.8#

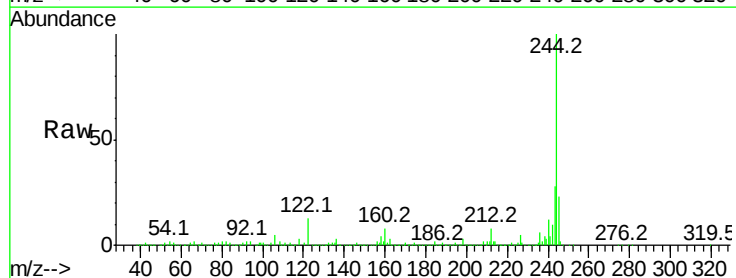


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

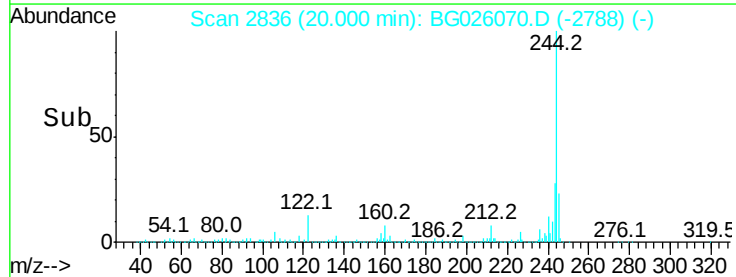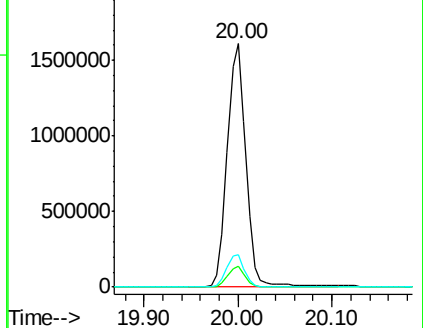

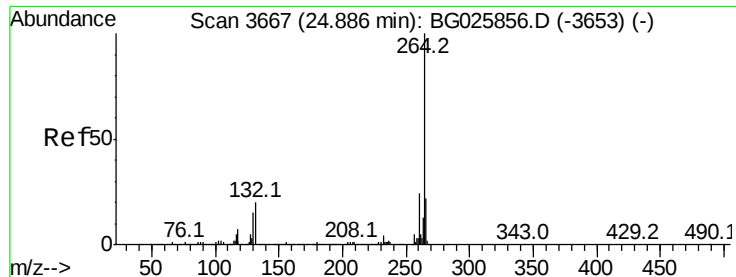

#86
Pervlene-d12
Concen: 20.00 ng
RT: 24.84 min Scan# 3660
Delta R.T. -0.04 min
Lab File: BG026070.D
Acq: 3 Mar 2017 19:08

Instrument :
BNA_G
ClientSampleId :
022717-PRRT-F-U-M

Tot Ion	Ratio	Lower	Upper
264	100		
260	25.2	21.8	32.8
265	21.4	18.2	27.4

