


Data Path : Z:\HPCHEM1\BNA G\Data\BG030417\
 Data File : BG026064.D
 Acq On : 3 Mar 2017 15:11
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG021717.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Mar 04 04:44:17 2017

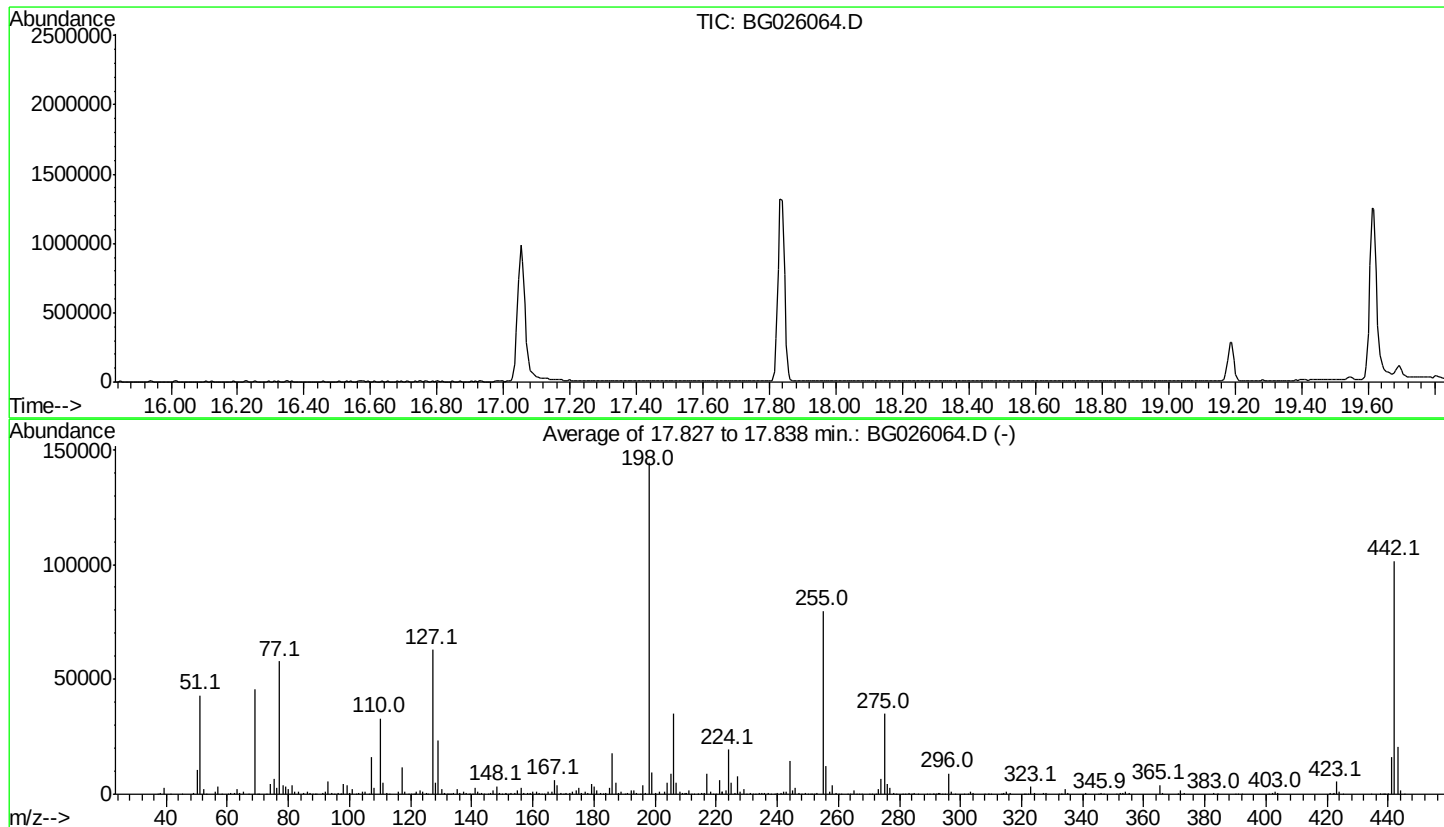

AutoFind: Scans 2466, 2467, 2468; Background Corrected with Scan 2460

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.8	42997	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	31.6	45650	PASS
70	69	0.00	2	0.5	241	PASS
127	198	10	80	43.5	62717	PASS
197	198	0.00	2	0.4	586	PASS
198	198	100	100	100.0	144333	PASS
199	198	5	9	6.5	9450	PASS
275	198	10	60	24.2	34997	PASS
365	198	1	100	2.9	4178	PASS
441	442	0.01	24	16.0	16248	PASS
442	198	50	100	70.4	101672	PASS
443	442	15	24	20.3	20671	PASS