

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030516\
 Data File : BG021311.D
 Acq On : 5 Mar 2016 18:35
 Operator : UM/SJ
 Sample : H1650-06
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MS-DS-B70

Quant Time: Mar 07 03:51:12 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Mar 07 03:50:11 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.13	152	8640	20.00	ng/ul	0.00
18) Naphthalene-d8	10.94	136	40867	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.73	164	25386	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.47	188	61621	20.00	ng/ul	0.00
78) Chrysene-d12	21.73	240	64576	20.00	ng/ul	0.00
86) Perylene-d12	24.98	264	59222	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.53	96	803	3.77	ng/uL	0.00
5) Phenol-d5	7.27	99	18083	19.76	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.45	67	12927	21.18	ng/ul	0.00
9) 2-Chlorophenol-d4	7.66	132	13257	20.76	ng/ul	0.00
13) 4-Methylphenol-d8	8.82	113	14909	20.64	ng/ul	0.00
19) Nitrobenzene-d5	9.28	128	7111	21.48	ng/ul	0.00
22) 2-Nitrophenol-d4	10.01	143	7283	20.64	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.55	165	12731	20.19	ng/ul	0.00
29) 4-Chloroaniline-d4	11.06	131	2618	3.27	ng/ul	0.00
44) Dimethylphthalate-d6	14.13	166	48325	22.72	ng/ul	0.00
47) Acenaphthylene-d8	14.43	160	59840	22.60	ng/ul	0.00
52) 4-Nitrophenol-d4	14.91	143	7733	18.65	ng/ul	0.00
58) Fluorene-d10	15.72	176	43324	23.19	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.83	200	6980	15.78	ng/ul	0.00
71) Anthracene-d10	17.57	188	68607	22.39	ng/ul	0.00
79) Pyrene-d10	19.84	212	75095	22.97	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.75	264	71427	22.34	ng/ul	-0.01


Target Compounds					Qvalue
45) Dimethylphthalate	14.18	163	14686	6.42 ng/ul#	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030516\
Data File : BG021311.D
Acq On : 5 Mar 2016 18:35
Operator : UM/SJ
Sample : H1650-06
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MS-DS-B70

Quant Time: Mar 07 03:51:12 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Mar 07 03:50:11 2016
Response via : Initial Calibration

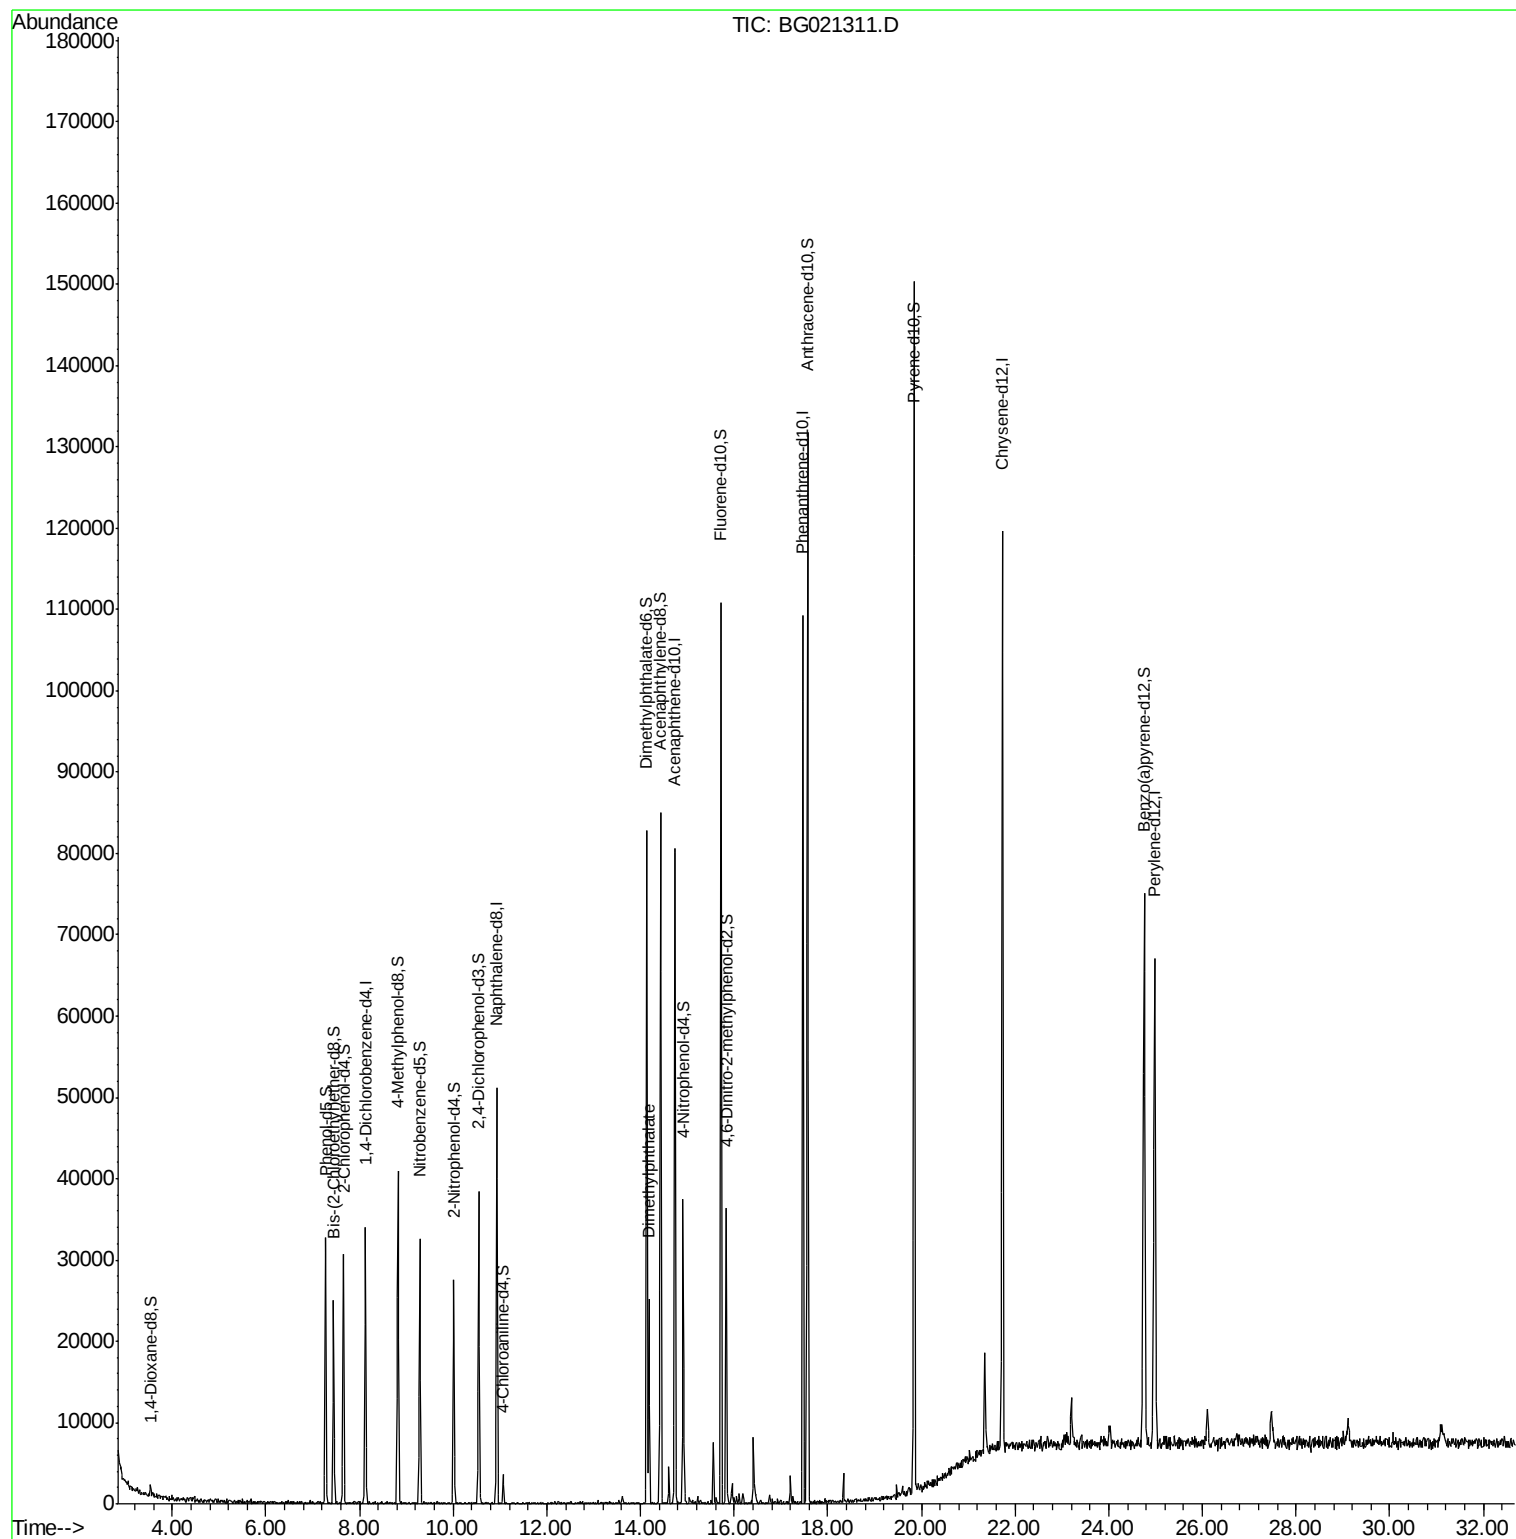

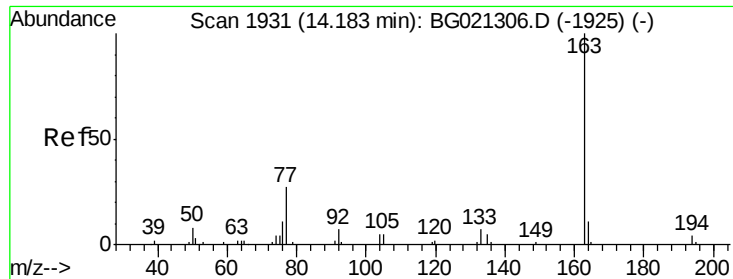

#45

Dimethylphthalate

Concen: 6.42 ng/ul

RT: 14.18 min Scan# 1930

Delta R.T. -0.00 min

Lab File: BG021311.D

Acq: 5 Mar 2016 18:35

Instrument :

BNA_G

ClientSampleId :

MS-DS-B70


Tgt Ion:163 Resp: 14686

Ion Ratio Lower Upper

163 100

194 4.5 2.8 4.2#

164 11.5 8.2 12.2

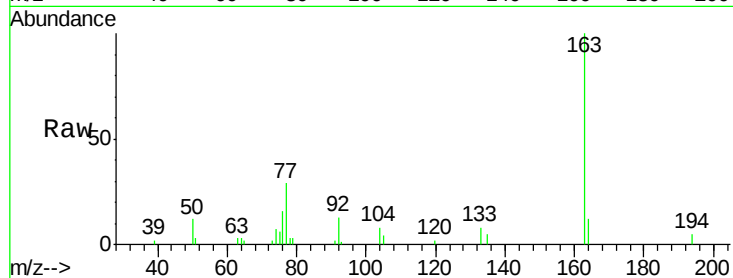

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

