

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030516\
 Data File : BG021316.D
 Acq On : 5 Mar 2016 21:51
 Operator : UM/SJ
 Sample : H1650-17
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MS-SS-B210

Quant Time: Mar 07 03:51:37 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Mar 07 03:50:11 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.12	152	9713	20.00	ng/ul	0.00
18) Naphthalene-d8	10.93	136	47725	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.74	164	28526	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.47	188	61987	20.00	ng/ul	0.00
78) Chrysene-d12	21.73	240	67449	20.00	ng/ul	0.00
86) Perylene-d12	24.98	264	61436	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.54	96	683	2.86	ng/uL	0.00
5) Phenol-d5	7.27	99	19054	18.52	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.44	67	13444	19.60	ng/ul	0.00
9) 2-Chlorophenol-d4	7.66	132	13506	18.82	ng/ul	0.00
13) 4-Methylphenol-d8	8.82	113	14550	17.91	ng/ul	0.00
19) Nitrobenzene-d5	9.28	128	7483	19.36	ng/ul	0.00
22) 2-Nitrophenol-d4	10.01	143	7511	18.22	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.54	165	13088	17.77	ng/ul	0.00
29) 4-Chloroaniline-d4	11.06	131	11564	12.38	ng/ul	0.00
44) Dimethylphthalate-d6	14.13	166	48317	20.21	ng/ul	0.00
47) Acenaphthylene-d8	14.43	160	60416	20.31	ng/ul	0.00
52) 4-Nitrophenol-d4	14.91	143	7154	15.35	ng/ul	0.00
58) Fluorene-d10	15.72	176	42799	20.39	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.83	200	6461	14.52	ng/ul	0.00
71) Anthracene-d10	17.57	188	64846	21.04	ng/ul	0.00
79) Pyrene-d10	19.84	212	72246	21.16	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.75	264	67617	20.39	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.18	163	12891	5.01	ng/ul#	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030516\
Data File : BG021316.D
Acq On : 5 Mar 2016 21:51
Operator : UM/SJ
Sample : H1650-17
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MS-SS-B210

Quant Time: Mar 07 03:51:37 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Mar 07 03:50:11 2016
Response via : Initial Calibration

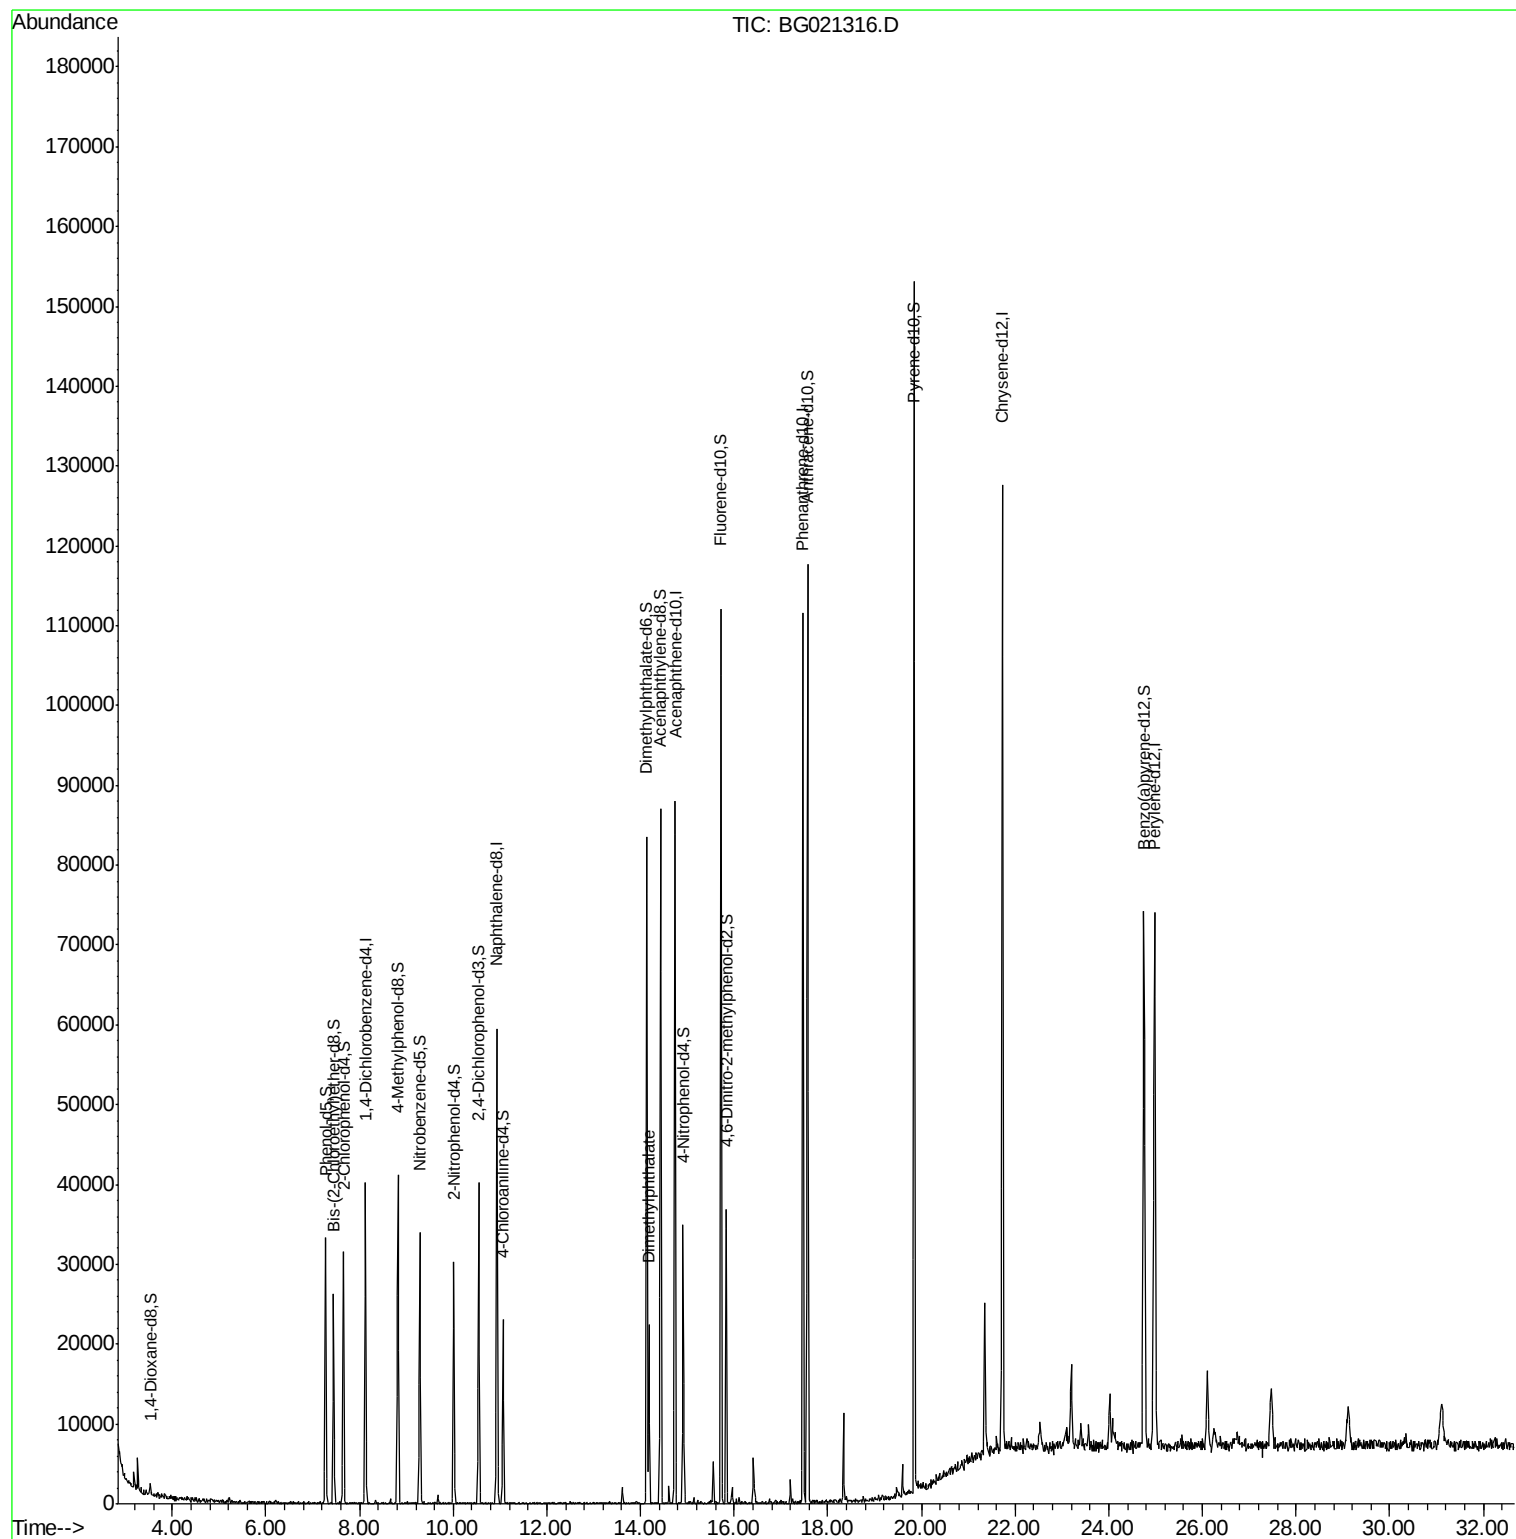


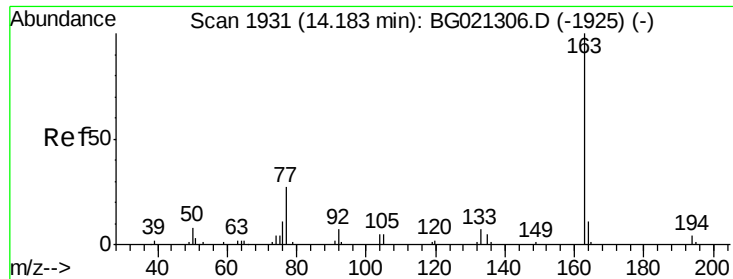

#45
 Dimethylphthalate
 Concen: 5.01 ng/ul
 RT: 14.18 min Scan# 1930
 Delta R.T. -0.00 min
 Lab File: BG021316.D
 Acq: 5 Mar 2016 21:51

Instrument :
 BNA_G
 ClientSampleId :
 MS-SS-B210

Tgt Ion:163 Resp: 12891
 Ion Ratio Lower Upper
 163 100
 194 5.2 2.8 4.2#
 164 11.4 8.2 12.2

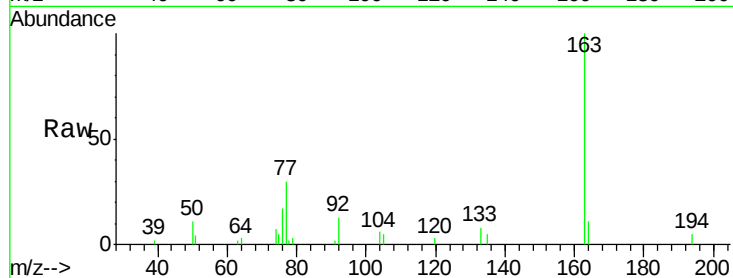

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

