

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030516\
 Data File : BG021324.D
 Acq On : 6 Mar 2016 3:44
 Operator : UM/SJ
 Sample : H1650-21
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MS-SS-C280

Quant Time: Mar 07 04:53:08 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Mar 07 04:51:57 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.12	152	11253	20.00	ng/ul	0.00
18) Naphthalene-d8	10.93	136	53582	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.73	164	32258	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.47	188	75787	20.00	ng/ul	0.00
78) Chrysene-d12	21.73	240	77955	20.00	ng/ul	0.00
86) Perylene-d12	24.98	264	73390	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.53	96	822	2.97	ng/uL	0.00
5) Phenol-d5	7.27	99	22666	19.02	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.45	67	16142	20.31	ng/ul	0.00
9) 2-Chlorophenol-d4	7.65	132	16990	20.43	ng/ul	0.00
13) 4-Methylphenol-d8	8.82	113	17166	18.24	ng/ul	0.00
19) Nitrobenzene-d5	9.29	128	8693	20.03	ng/ul	0.00
22) 2-Nitrophenol-d4	10.01	143	9070	19.60	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.55	165	16357	19.78	ng/ul	0.00
29) 4-Chloroaniline-d4	11.07	131	9974	9.51	ng/ul	0.00
44) Dimethylphthalate-d6	14.13	166	54814	20.28	ng/ul	0.00
47) Acenaphthylene-d8	14.43	160	69715	20.72	ng/ul	0.00
52) 4-Nitrophenol-d4	14.91	143	7713	14.64	ng/ul	0.00
58) Fluorene-d10	15.72	176	49841	20.99	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.83	200	8192	15.06	ng/ul	0.00
71) Anthracene-d10	17.57	188	75813	20.12	ng/ul	0.00
79) Pyrene-d10	19.84	212	82958	21.02	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.76	264	81384	20.54	ng/ul	0.00

Target Compounds


						Qvalue
45) Dimethylphthalate	14.18	163	16553	5.69	ng/ul	97
50) Acenaphthene	14.80	153	8144	3.41	ng/ul	97
54) Dibenzofuran	15.13	168	7372	2.27	ng/ul	98
59) Fluorene	15.78	166	11172	3.95	ng/ul	91
70) Phenanthrene	17.51	178	116941	25.65	ng/ul	100
72) Anthracene	17.60	178	28372	6.16	ng/ul	99
75) Carbazole	17.87	167	9411	2.34	ng/ul#	94
77) Fluoranthene	19.51	202	114677	21.50	ng/ul	99
80) Pyrene	19.87	202	95944	18.37	ng/ul	99
83) Benzo(a)anthracene	21.71	228	57838	11.45	ng/ul	98
84) Bis(2-ethylhexyl)phthalate	21.60	149	28376	8.06	ng/ul	97
85) Chrysene	21.78	228	51500	10.92	ng/ul	98
88) Benzo(b)fluoranthene	23.94	252	49177	9.68	ng/ul	99
89) Benzo(k)fluoranthene	23.94	252	49177	10.03	ng/ul	99
91) Benzo(a)pyrene	24.83	252	37916	7.73	ng/ul	98
92) Indeno(1,2,3-cd)pyrene	28.68	276	19650	3.69	ng/ul	94
94) Benzo(g,h,i)perylene	29.83	276	9993	2.24	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030516\
Data File : BG021324.D
Acq On : 6 Mar 2016 3:44
Operator : UM/SJ
Sample : H1650-21
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MS-SS-C280

Quant Time: Mar 07 04:53:08 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Mar 07 04:51:57 2016
Response via : Initial Calibration




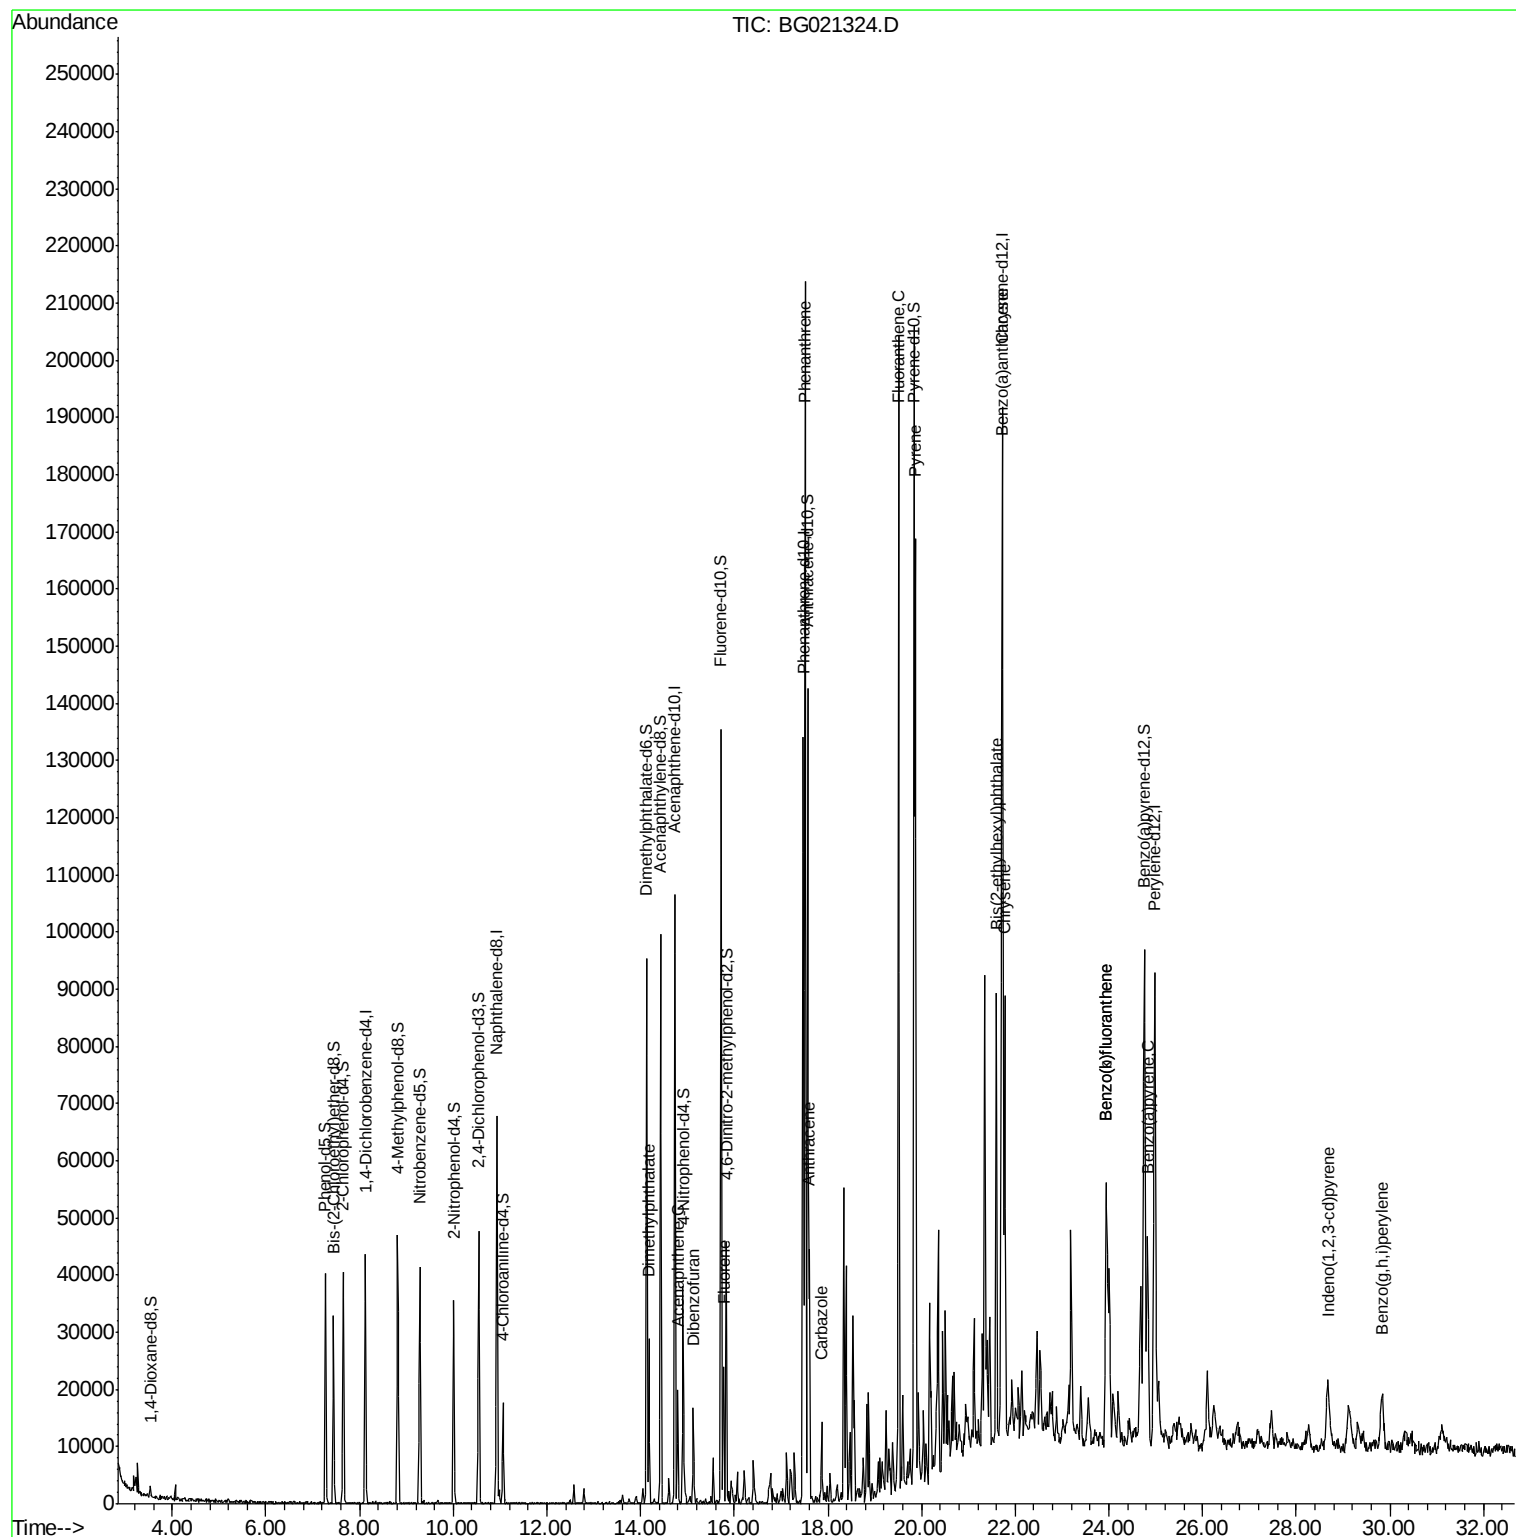


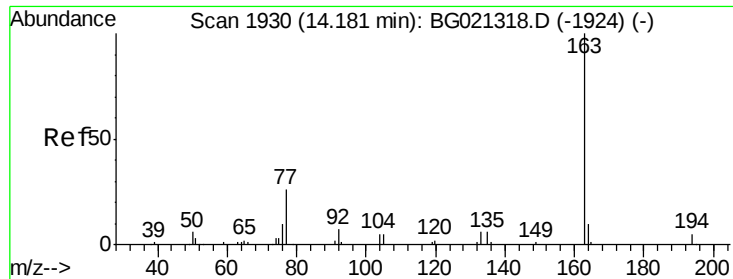

#45
Dimethylphthalate
Concen: 5.69 ng/ul
RT: 14.18 min Scan# 1930
Delta R.T. -0.00 min
Lab File: BG021324.D
Acq: 6 Mar 2016 3:44




Instrument :
BNA_G
ClientSampleId :
MS-SS-C280


Tgt Ion:163 Resp: 16553
Ion Ratio Lower Upper
163 100
194 4.0 2.8 4.2
164 11.6 8.2 12.2

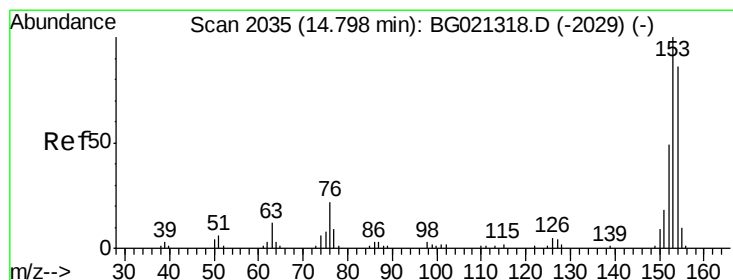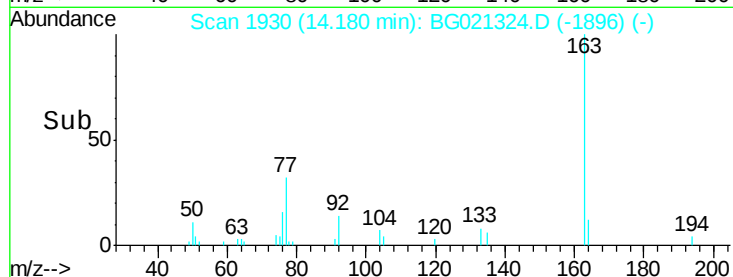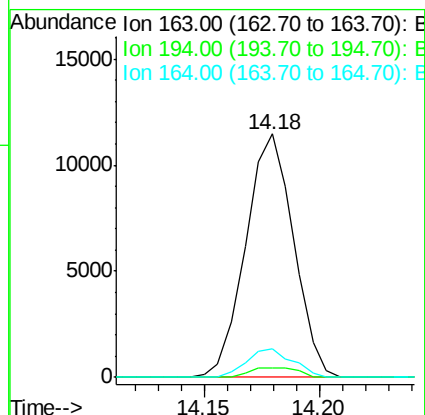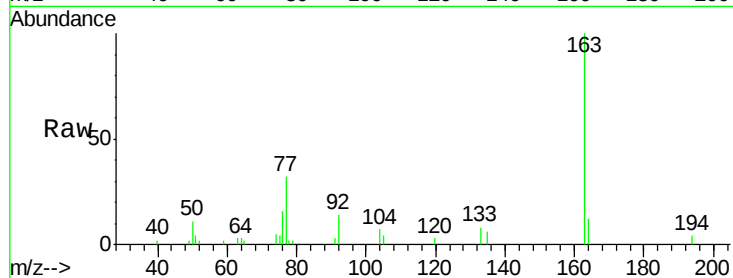

#50
Acenaphthene
Concen: 3.41 ng/ul
RT: 14.80 min Scan# 2035
Delta R.T. -0.00 min
Lab File: BG021324.D
Acq: 6 Mar 2016 3:44

Tgt Ion:153 Resp: 8144
Ion Ratio Lower Upper
153 100
152 48.1 39.0 58.6
154 87.4 66.8 100.2


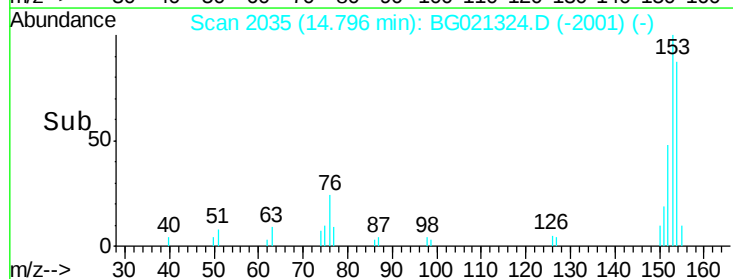
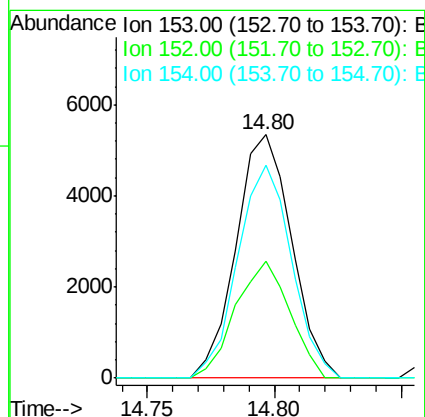
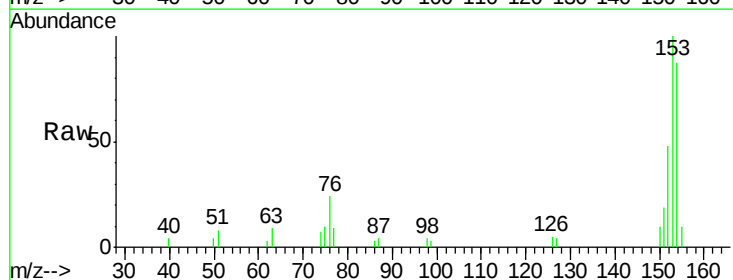


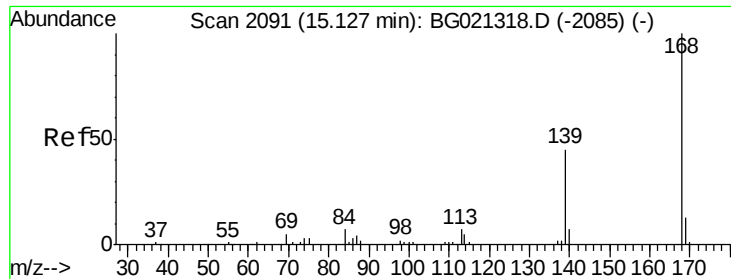

#54
Dibenzenofuran
Concen: 2.27 ng/ul
RT: 15.13 min Scan# 2091
Delta R.T. -0.00 min
Lab File: BG021324.D
Acq: 6 Mar 2016 3:44




Instrument :
BNA_G
ClientSampleId :
MS-SS-C280


Tgt Ion:168 Resp: 7372
Ion Ratio Lower Upper
168 100
139 43.6 35.7 53.5

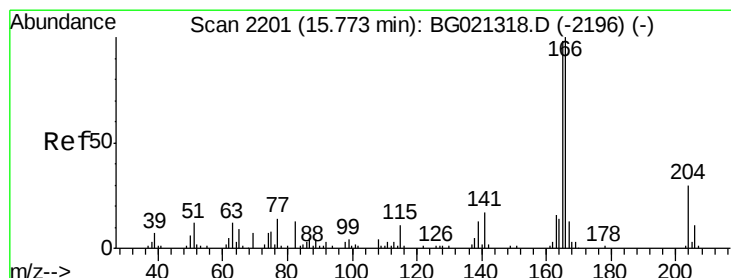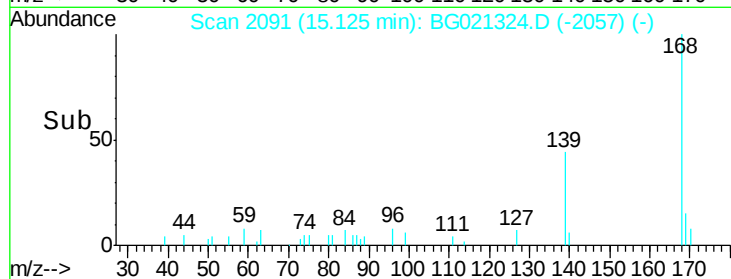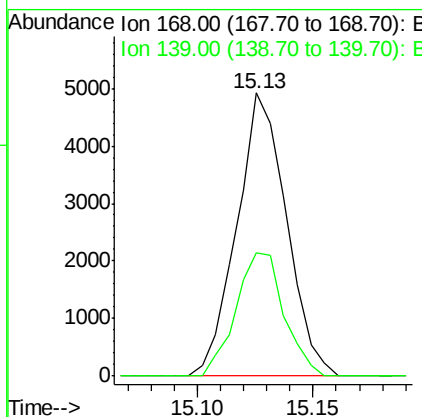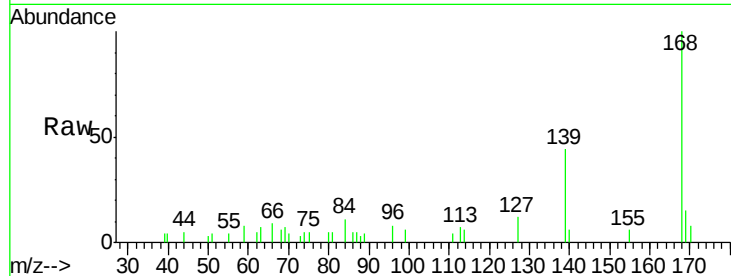

#59
Fluorene
Concen: 3.95 ng/ul
RT: 15.78 min Scan# 2202
Delta R.T. 0.00 min
Lab File: BG021324.D
Acq: 6 Mar 2016 3:44

Tgt Ion:166 Resp: 11172
Ion Ratio Lower Upper
166 100
165 95.0 83.8 125.8
167 11.6 11.5 17.3

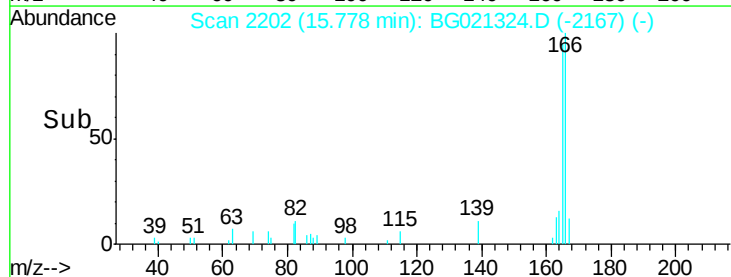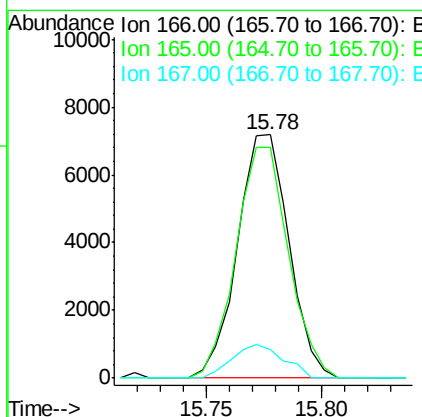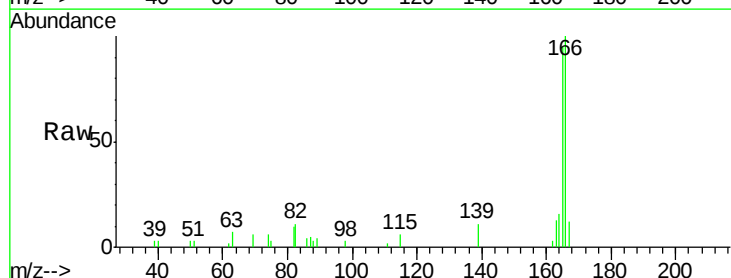

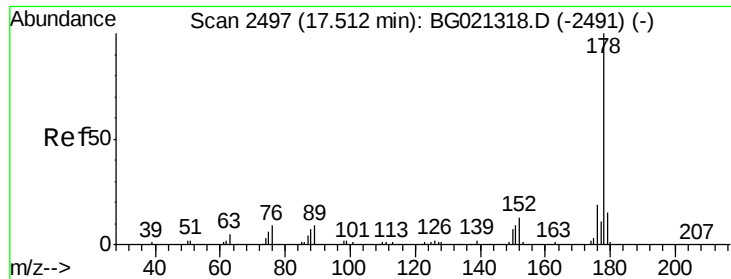

#70

Phenanthrene

Concen: 25.65 ng/ul

RT: 17.51 min Scan# 2497

Delta R.T. -0.00 min

Lab File: BG021324.D

Acq: 6 Mar 2016 3:44

Instrument :

BNA_G

ClientSampleId :

MS-SS-C280


Tgt Ion:178 Resp: 116941

Ion Ratio Lower Upper

178 100

179 15.1 12.3 18.5




176 18.9 15.1 22.7

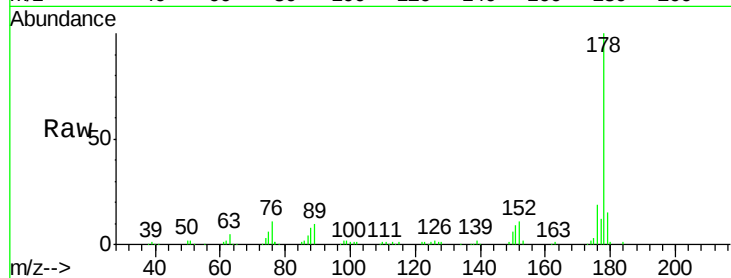

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

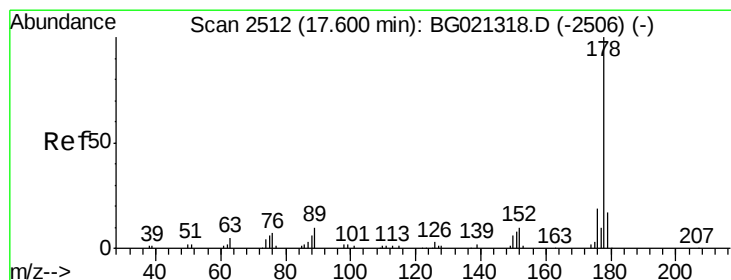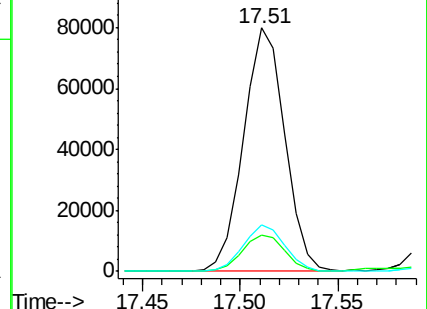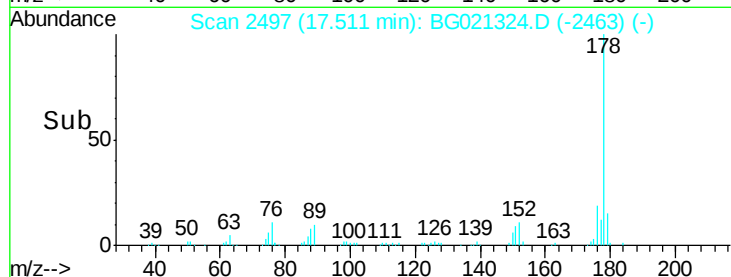

#72

Anthracene

Concen: 6.16 ng/ul

RT: 17.60 min Scan# 2513

Delta R.T. 0.00 min

Lab File: BG021324.D

Acq: 6 Mar 2016 3:44


Tgt Ion:178 Resp: 28372

Ion Ratio Lower Upper

178 100

179 14.9 11.8 17.8



176 18.3 15.2 22.8

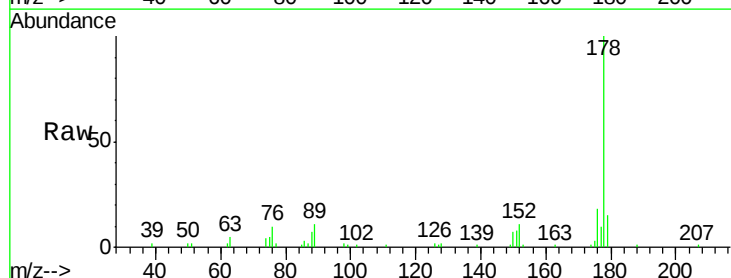


Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

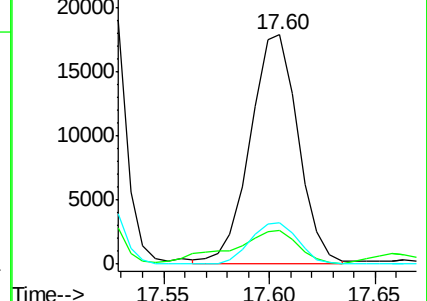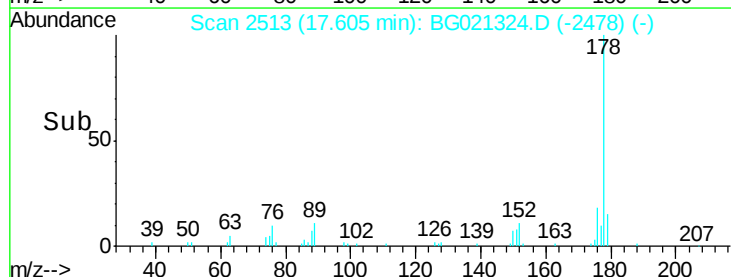

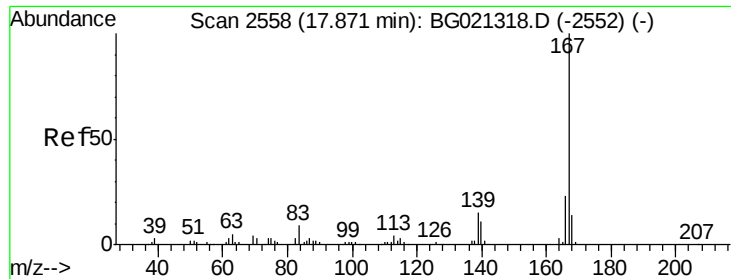

#75

Carbazole

Concen: 2.34 ng/ul

RT: 17.87 min Scan# 2558

Delta R.T. -0.00 min

Lab File: BG021324.D

Acq: 6 Mar 2016 3:44

Instrument :

BNA_G

ClientSampleId :

MS-SS-C280


Tgt Ion:167 Resp: 9411

Ion Ratio Lower Upper

167 100

166 22.1 17.4 26.0




139 8.7 11.8 17.6#

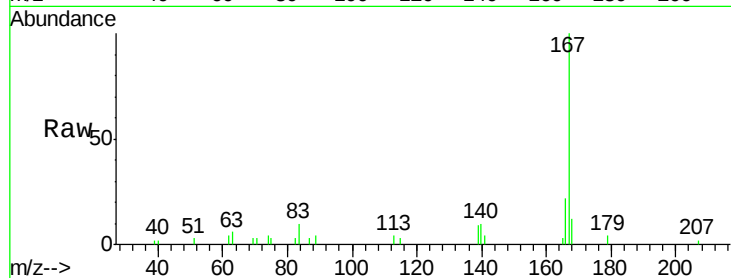

Abundance Ion 167.00 (166.70 to 167.70): E

Ion 166.00 (165.70 to 166.70): E

Ion 139.00 (138.70 to 139.70): E

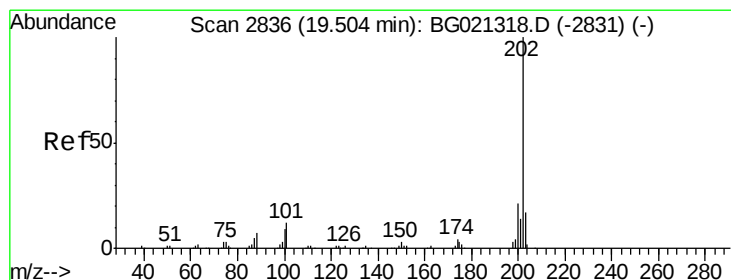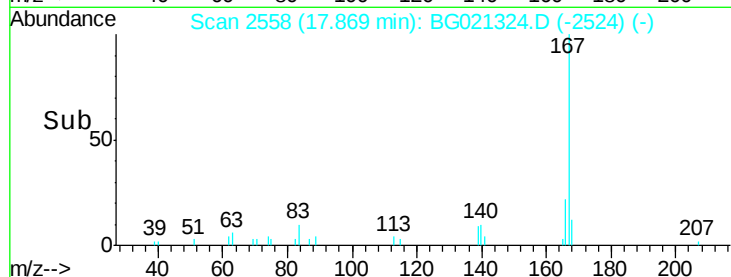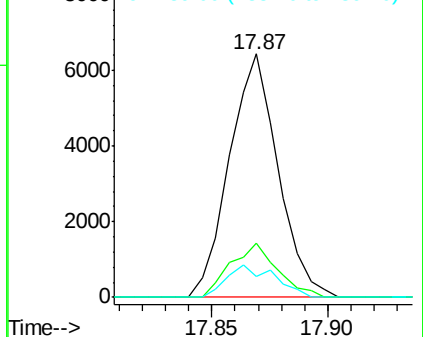

#77

Fluoranthene

Concen: 21.50 ng/ul

RT: 19.51 min Scan# 2837

Delta R.T. 0.00 min

Lab File: BG021324.D

Acq: 6 Mar 2016 3:44


Tgt Ion:202 Resp: 114677

Ion Ratio Lower Upper

202 100

101 11.6 9.9 14.9



100 9.5 7.4 11.0

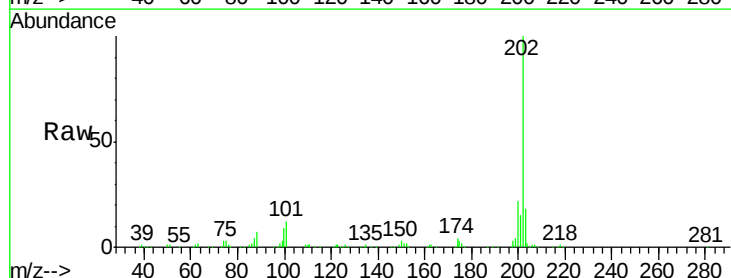


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B



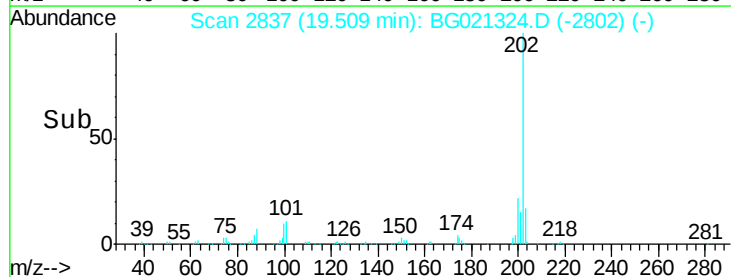
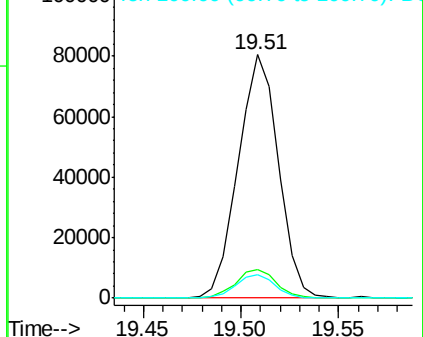


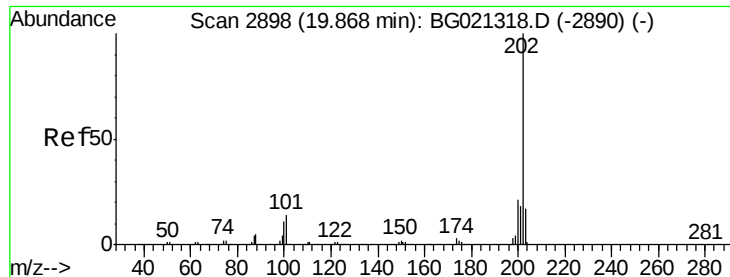

#80
 Pyrene
 Concen: 18.37 ng/ul
 RT: 19.87 min Scan# 2899
 Delta R.T. 0.00 min
 Lab File: BG021324.D
 Acq: 6 Mar 2016 3:44




Instrument :
 BNA_G
 ClientSampleId :
 MS-SS-C280


Tgt Ion:202 Resp: 95944
 Ion Ratio Lower Upper
 202 100
 101 13.3 11.0 16.4
 100 10.7 8.1 12.1

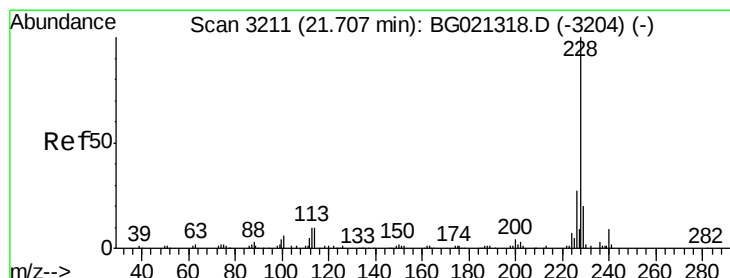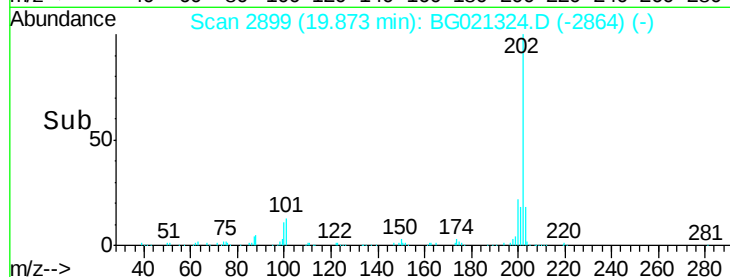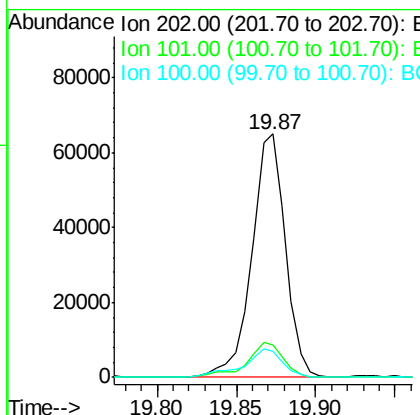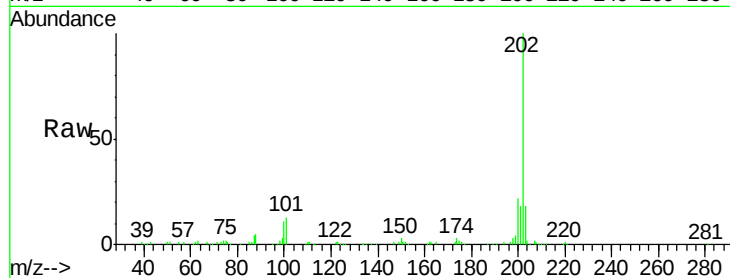

#83
 Benzo(a)anthracene
 Concen: 11.45 ng/ul
 RT: 21.71 min Scan# 3212
 Delta R.T. 0.00 min
 Lab File: BG021324.D
 Acq: 6 Mar 2016 3:44

Tgt Ion:228 Resp: 57838
 Ion Ratio Lower Upper
 228 100
 229 18.5 15.7 23.5
 226 25.3 21.1 31.7

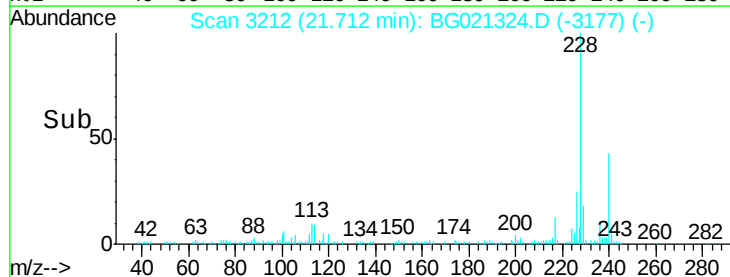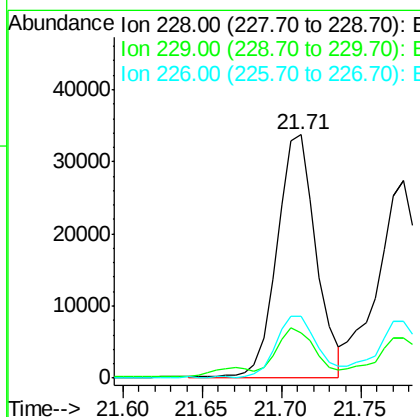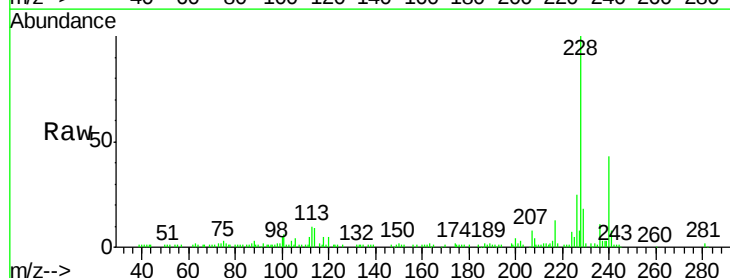


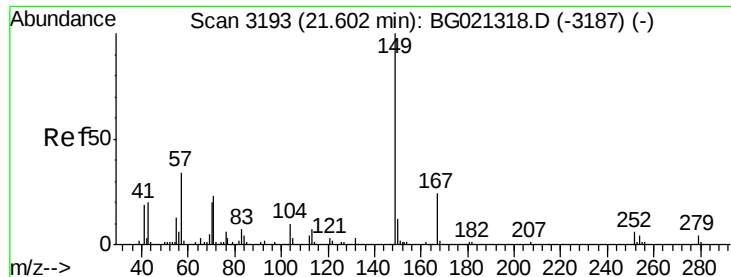




#84
 Bis(2-ethylhexyl)phthalate
 Concen: 8.06 ng/ul
 RT: 21.60 min Scan# 3193
 Delta R.T. -0.00 min
 Lab File: BG021324.D
 Acq: 6 Mar 2016 3:44

Instrument :
 BNA_G
 ClientSampleId :
 MS-SS-C280

Tgt Ion:149 Resp: 28376
 Ion Ratio Lower Upper
 149 100
 167 24.7 21.2 31.8
 279 4.6 3.4 5.0

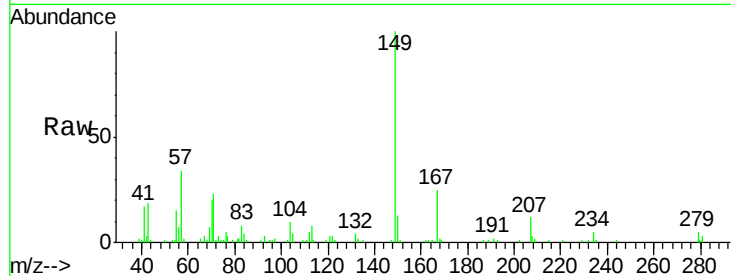


Abundance Ion 149.00 (148.70 to 149.70): E
 Ion 167.00 (166.70 to 167.70): E
 Ion 279.00 (278.70 to 279.70): E

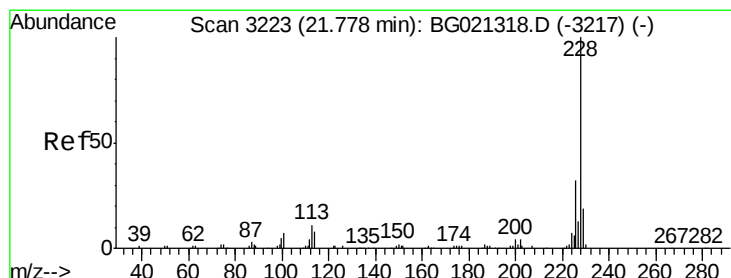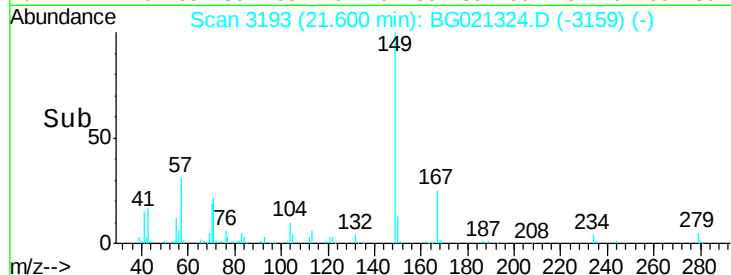
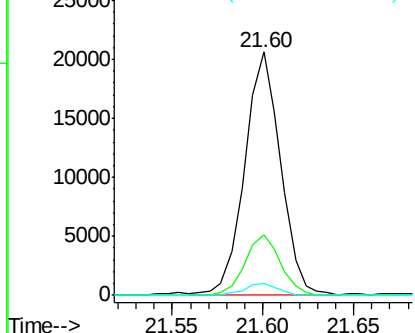



#85
 Chrysene
 Concen: 10.92 ng/ul
 RT: 21.78 min Scan# 3223
 Delta R.T. -0.00 min
 Lab File: BG021324.D
 Acq: 6 Mar 2016 3:44

Tgt Ion:228 Resp: 51500
 Ion Ratio Lower Upper
 228 100
 226 29.0 24.5 36.7
 229 20.3 15.8 23.8

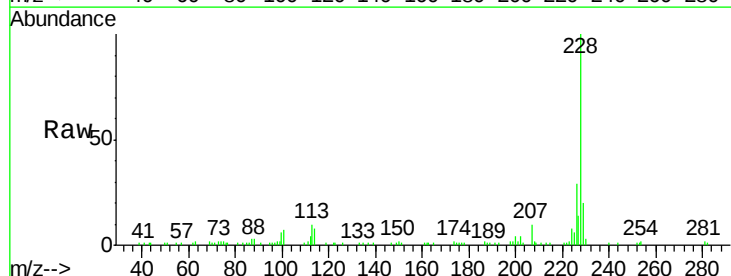

Abundance Ion 228.00 (227.70 to 228.70): E
 Ion 226.00 (225.70 to 226.70): E
 Ion 229.00 (228.70 to 229.70): E



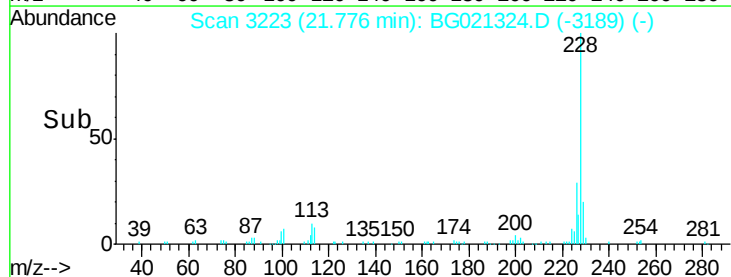
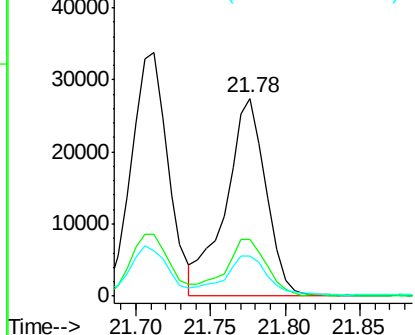


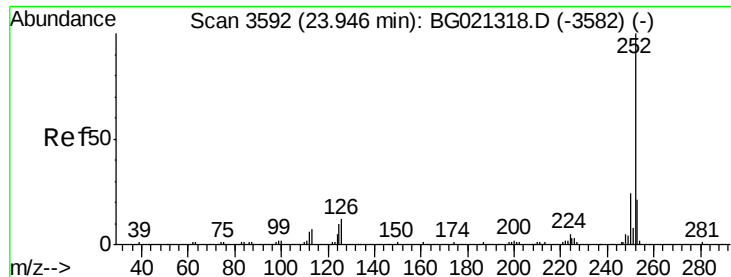

#88
Benzo(b)fluoranthene
Concen: 9.68 ng/u1
RT: 23.94 min Scan# 3592
Delta R.T. -0.00 min
Lab File: BG021324.D
Acq: 6 Mar 2016 3:44




Instrument :
BNA_G
ClientSampleId :
MS-SS-C280


Tgt Ion	Ratio	Lower	Upper
252	100		
253	22.9	18.0	27.0
125	10.6	8.0	12.0

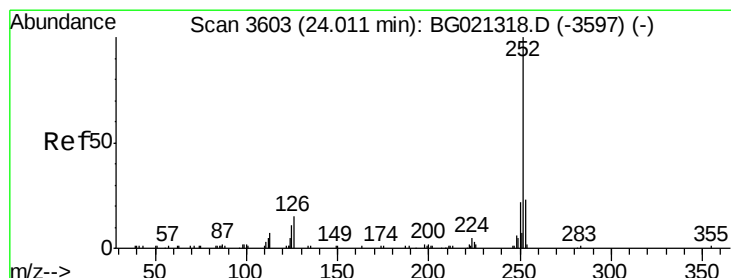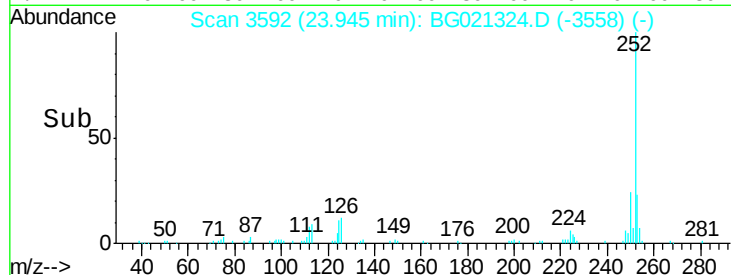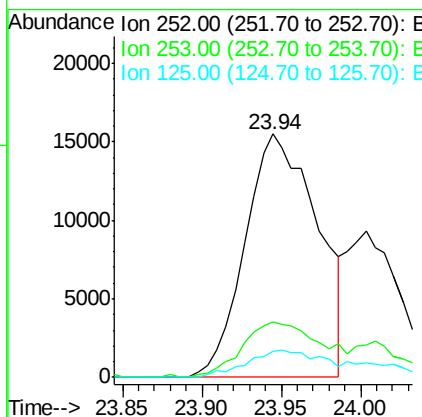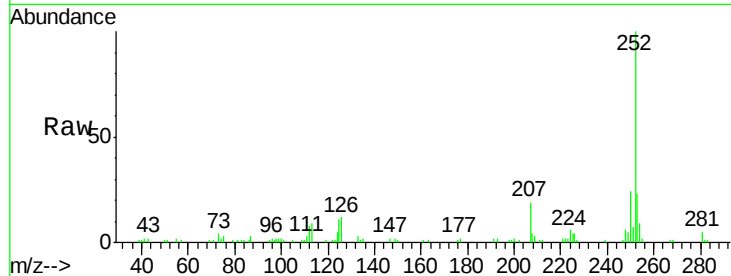

#89
Benzo(k)fluoranthene
Concen: 10.03 ng/u1
RT: 23.94 min Scan# 3592
Delta R.T. -0.07 min
Lab File: BG021324.D
Acq: 6 Mar 2016 3:44

Tgt Ion	Ratio	Lower	Upper
252	100		
253	22.9	18.0	27.0
125	10.6	8.1	12.1

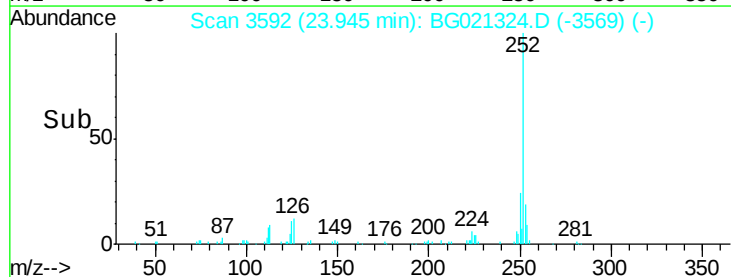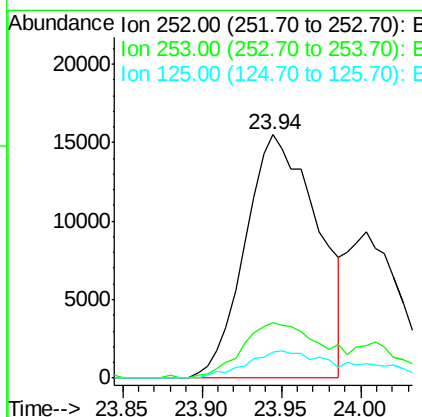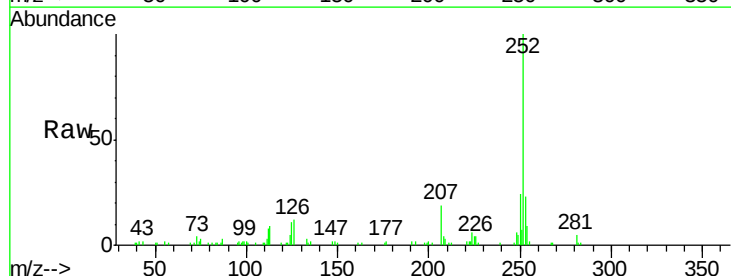

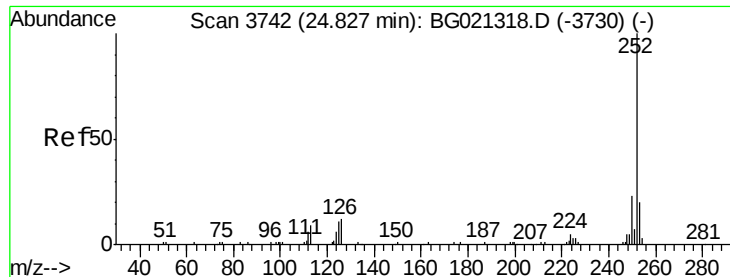

#91

Benzo(a)pyrene

Concen: 7.73 ng/ul

RT: 24.83 min Scan# 3742

Delta R.T. -0.00 min

Lab File: BG021324.D

Acq: 6 Mar 2016 3:44





Instrument :

BNA_G

ClientSampleId :

MS-SS-C280

Tgt Ion:	252	Resp:	37916
Ion	Ratio	Lower	Upper
252	100		
253	23.1	17.2	25.8
125	10.1	8.2	12.4

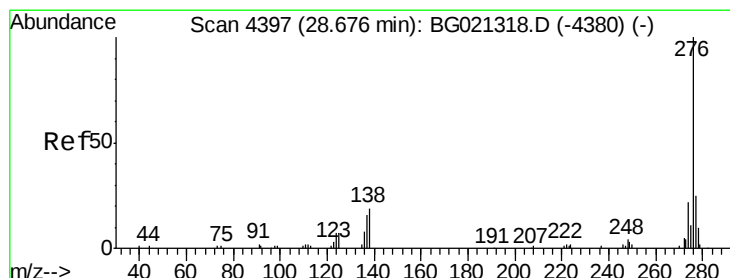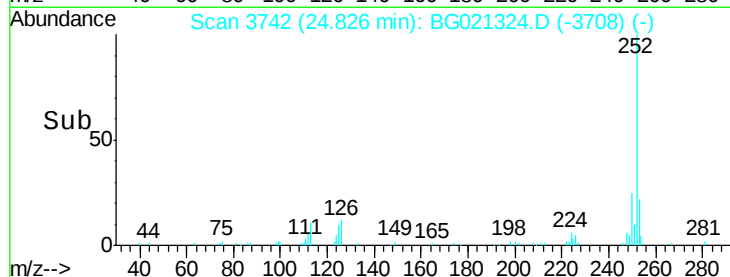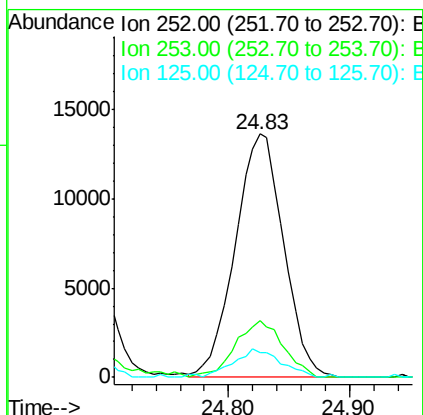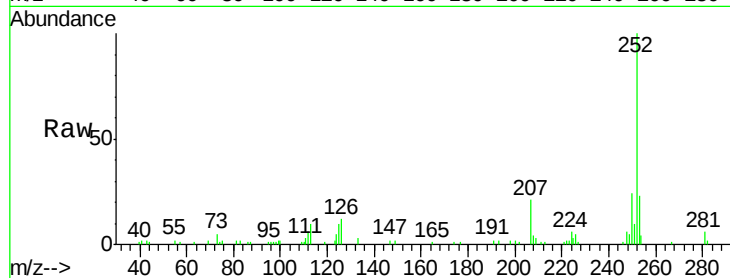

#92

Indeno(1,2,3-cd)pyrene

Concen: 3.69 ng/ul




RT: 28.68 min Scan# 4398


Delta R.T. 0.00 min

Lab File: BG021324.D

Acq: 6 Mar 2016 3:44

Tgt Ion:	276	Resp:	19650
Ion	Ratio	Lower	Upper
276	100		
138	19.7	14.4	21.6
277	19.1	18.0	27.0

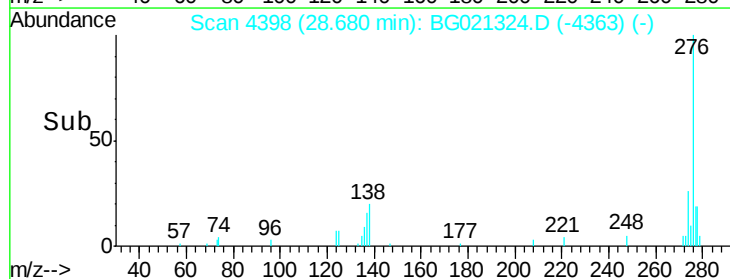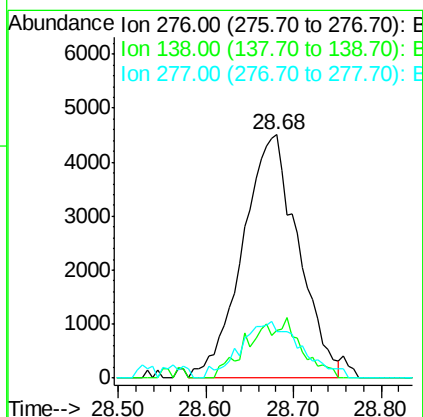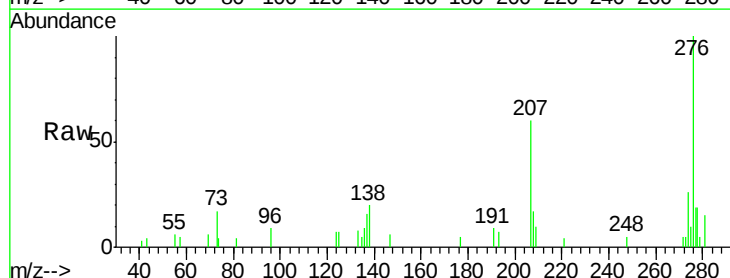

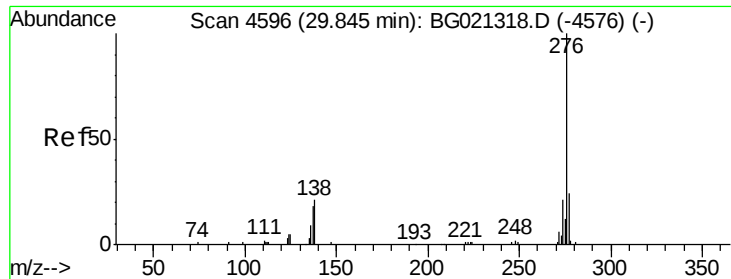

#94

Benzo(g,h,i)perylene

Concen: 2.24 ng/ul

RT: 29.83 min Scan# 4593

Delta R.T. -0.02 min

Lab File: BG021324.D

Acq: 6 Mar 2016 3:44

Instrument :

BNA_G

ClientSampleId :

MS-SS-C280


Tgt Ion: 276 Resp: 9993

Ion Ratio Lower Upper

276 100

138 19.1 15.3 22.9

277 26.8 19.0 28.4

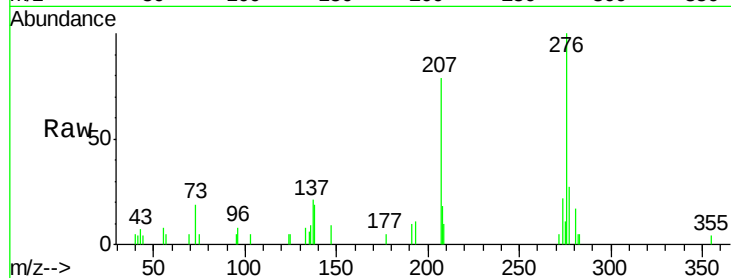

Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

