

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030516\
 Data File : BG021327.D
 Acq On : 6 Mar 2016 5:41
 Operator : UM/SJ
 Sample : H1650-20
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MS-DS-C210

Quant Time: Mar 07 04:53:37 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Mar 07 04:51:57 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.13	152	11807	20.00	ng/ul	0.00
18) Naphthalene-d8	10.93	136	55501	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.74	164	31722	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.47	188	74530	20.00	ng/ul	0.00
78) Chrysene-d12	21.73	240	79561	20.00	ng/ul	0.00
86) Perylene-d12	24.98	264	75334	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.53	96	1696	5.83	ng/uL	0.00
5) Phenol-d5	7.27	99	39312	31.44	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.44	67	27621	33.12	ng/ul	0.00
9) 2-Chlorophenol-d4	7.66	132	28400	32.55	ng/ul	0.00
13) 4-Methylphenol-d8	8.82	113	31822	32.23	ng/ul	0.00
19) Nitrobenzene-d5	9.29	128	15297	34.02	ng/ul	0.00
22) 2-Nitrophenol-d4	10.01	143	16575	34.58	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.55	165	27738	32.39	ng/ul	0.00
29) 4-Chloroaniline-d4	11.06	131	19785	18.22	ng/ul	0.00
44) Dimethylphthalate-d6	14.14	166	94931	35.71	ng/ul	0.00
47) Acenaphthylene-d8	14.43	160	119637	36.16	ng/ul	0.00
52) 4-Nitrophenol-d4	14.91	143	17383	33.55	ng/ul	0.00
58) Fluorene-d10	15.72	176	85083	36.45	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.83	200	16476	30.80	ng/ul	0.00
71) Anthracene-d10	17.57	188	136514	36.83	ng/ul	0.00
79) Pyrene-d10	19.84	212	155712	38.66	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.76	264	149859	36.85	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.18	163	26583	9.29	ng/ul#	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030516\
Data File : BG021327.D
Acq On : 6 Mar 2016 5:41
Operator : UM/SJ
Sample : H1650-20
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MS-DS-C210

Quant Time: Mar 07 04:53:37 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Mar 07 04:51:57 2016
Response via : Initial Calibration

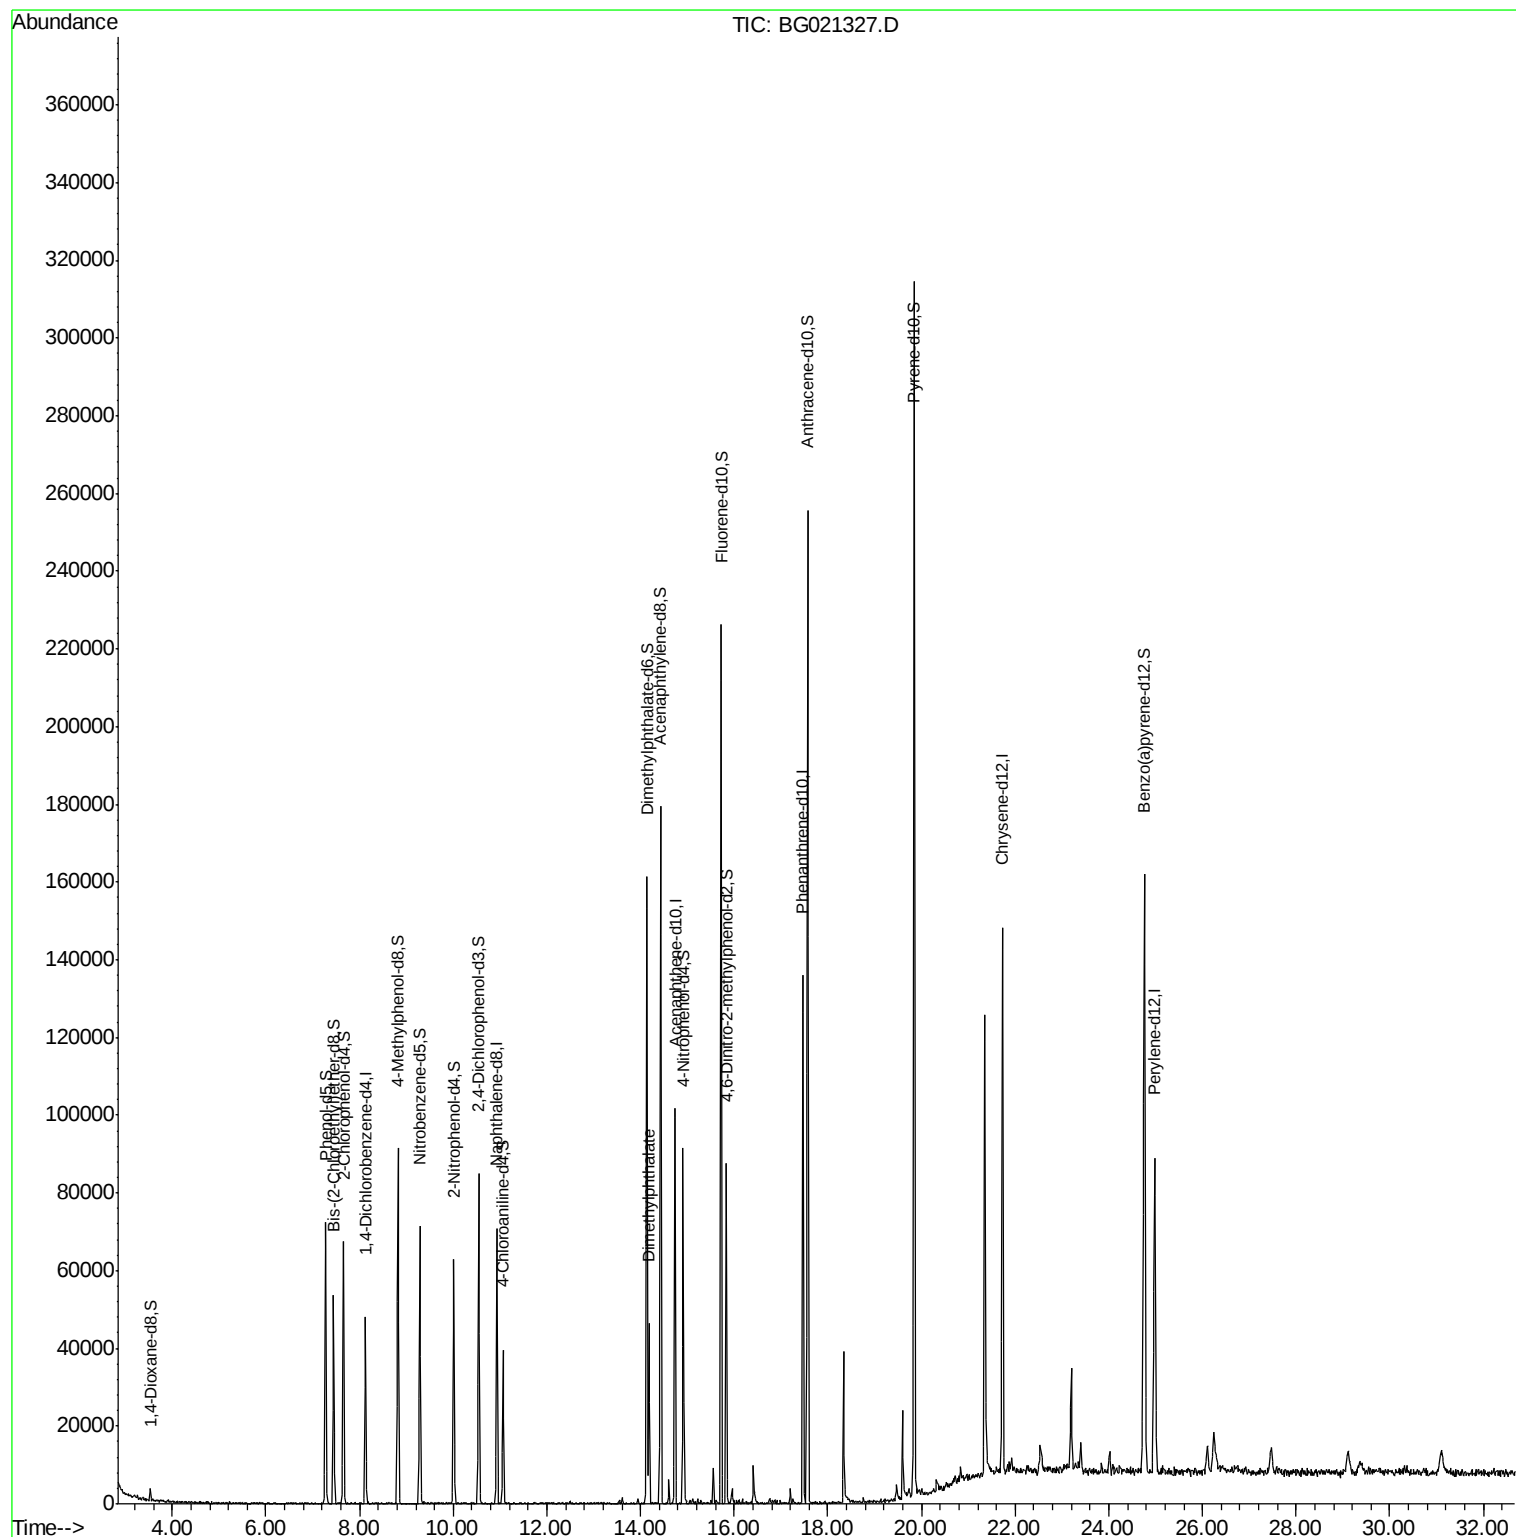

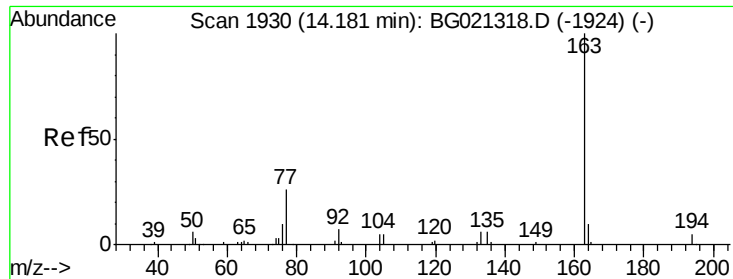

#45

Dimethylphthalate

Concen: 9.29 ng/ul

RT: 14.18 min Scan# 1930

Delta R.T. -0.00 min

Lab File: BG021327.D


Acq: 6 Mar 2016 5:41

Instrument :

BNA_G

ClientSampleId :

MS-DS-C210

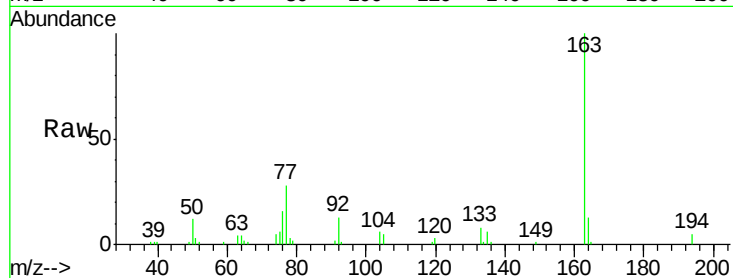

Tgt Ion:	163	Resp:	26583
Ion	Ratio	Lower	Upper
163	100		
194	5.0	2.8	4.2#
164	13.4	8.2	12.2#

