




Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030516\
Data File : BG021321.D
Acq On : 6 Mar 2016 1:46
Operator : UM/SJ
Sample : H1650-07
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MS-SS-C350

Manual Integrations
APPROVED

UMANGI
3/7/2016 12:34:27 PM

Quant Time: Mar 07 04:52:42 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Mar 07 04:51:57 2016
Response via : Initial Calibration

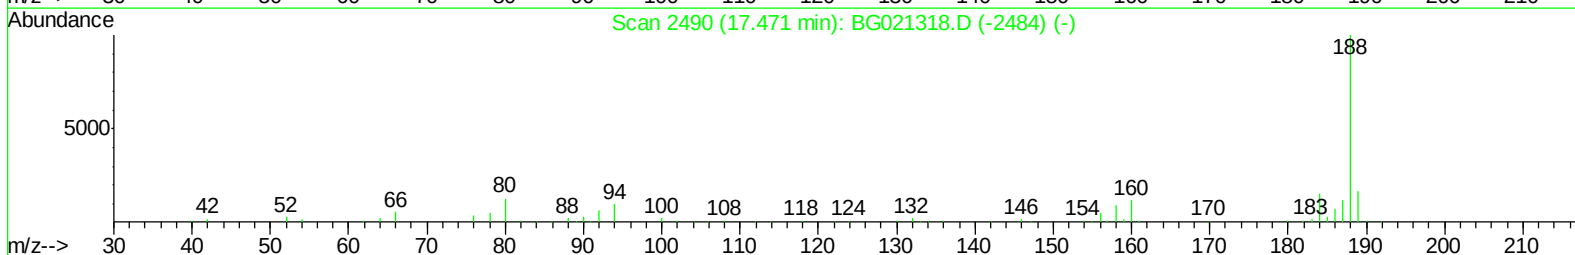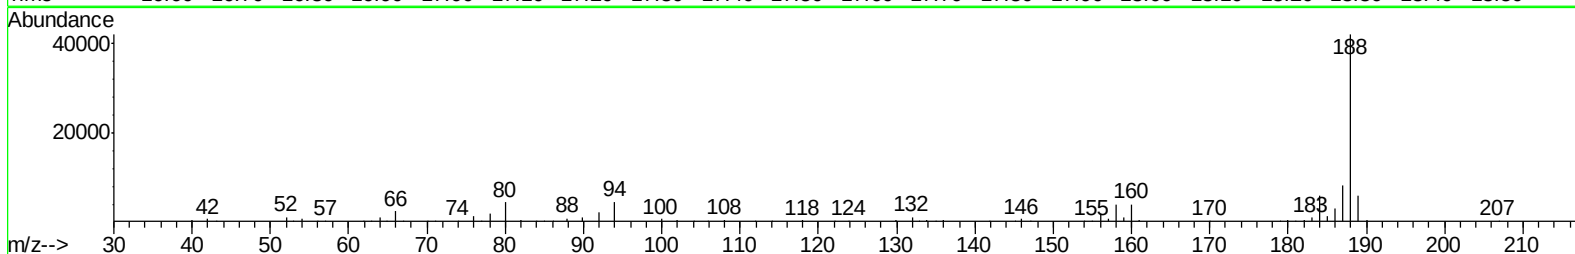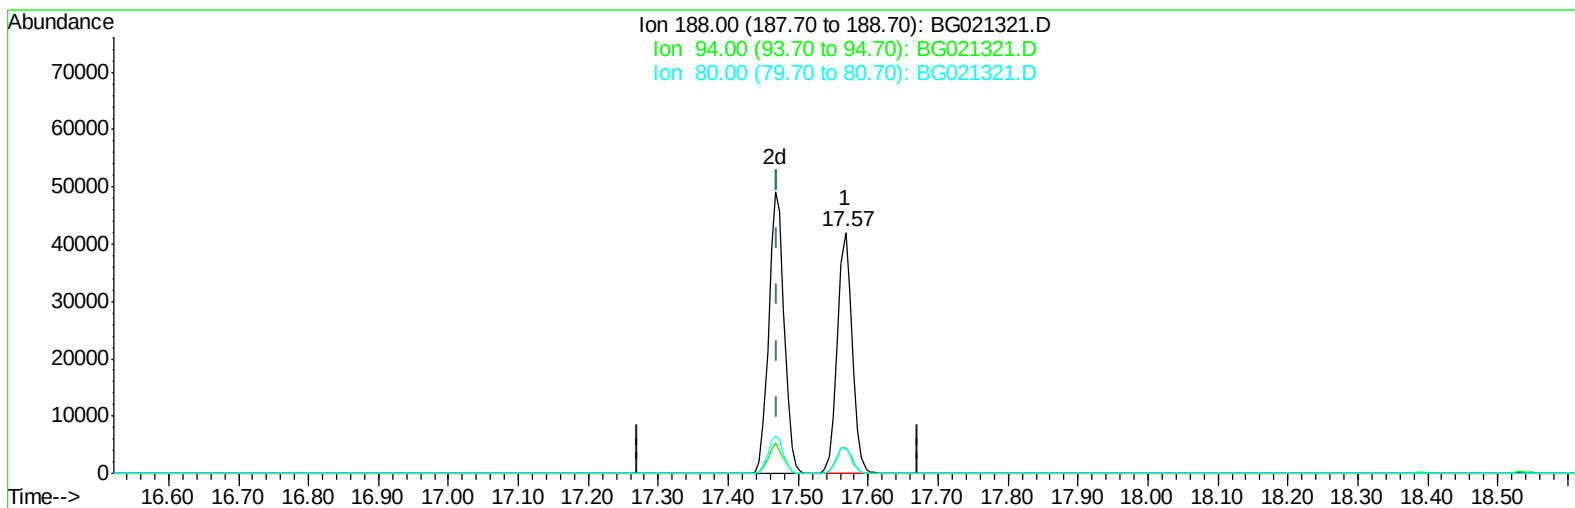

TIC: BG021321.D

(62) Phenanthrene-d10 (I)

17.567min (+0.096) 20.00ng/ul

response 61647

Ion	Exp%	Act%
188.00	100	100
94.00	9.30	10.67
80.00	10.60	10.31
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030516\
Data File : BG021321.D
Acq On : 6 Mar 2016 1:46
Operator : UM/SJ
Sample : H1650-07
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MS-SS-C350

Manual Integrations
APPROVED

UMANGI
3/7/2016 12:34:27 PM

Quant Time: Mar 07 04:52:42 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Mar 07 04:51:57 2016
Response via : Initial Calibration

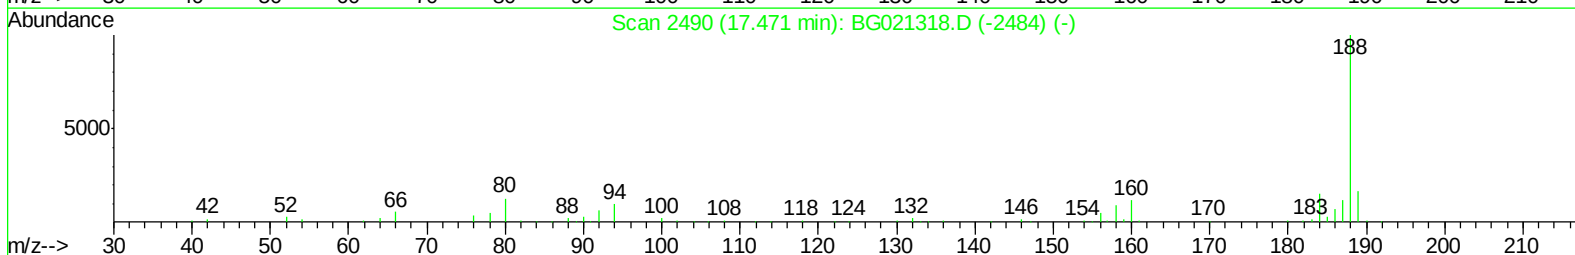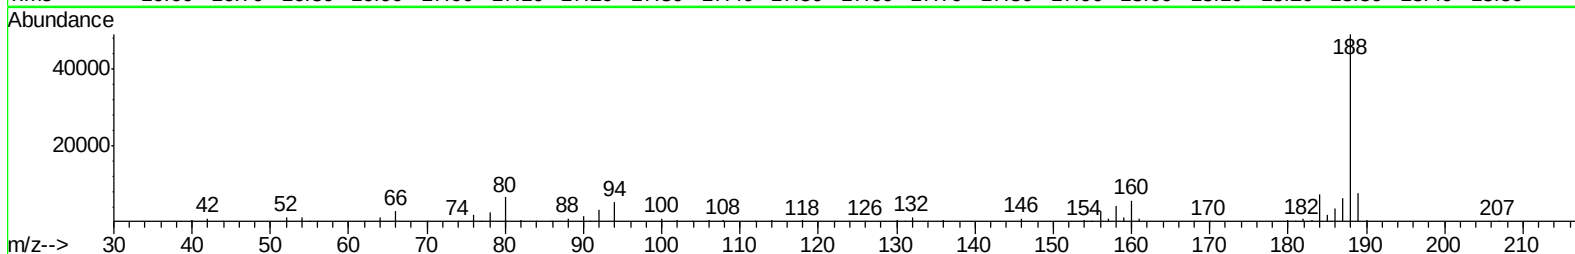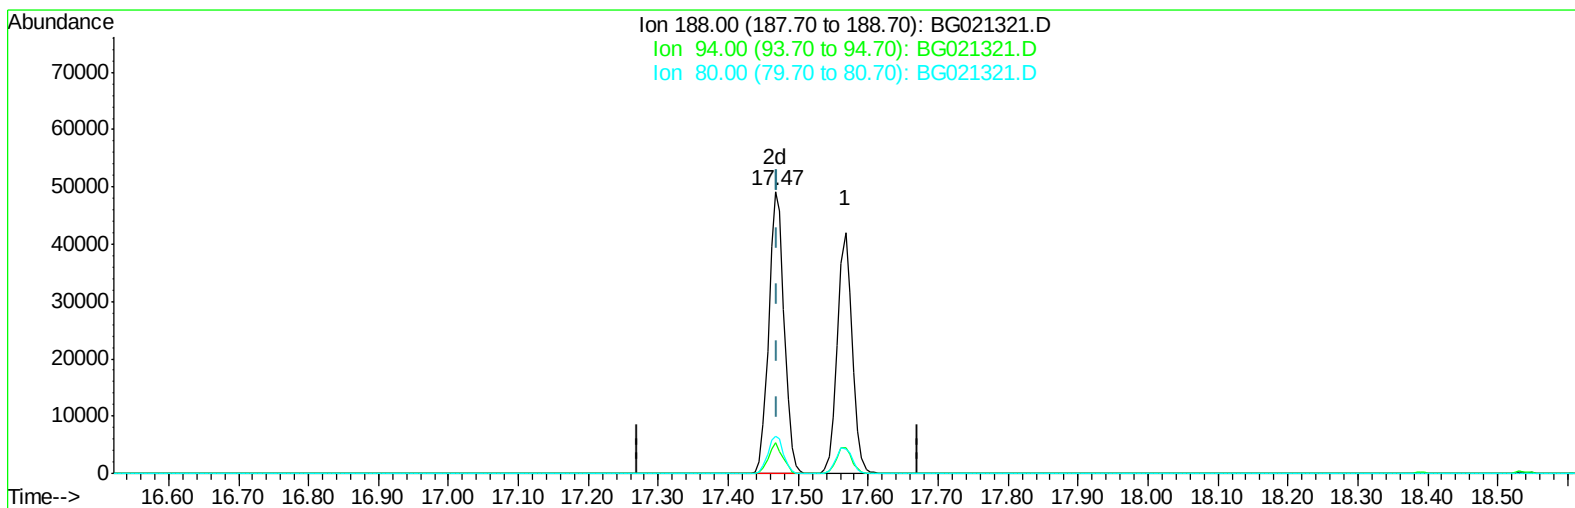

TIC: BG021321.D

(62) Phenanthrene-d10 (I)

17.467min (-0.004) 20.00ng/ul m

response 75538

Ion	Exp%	Act%
188.00	100	100
94.00	9.30	10.85
80.00	10.60	13.02#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030516\
Data File : BG021321.D
Acq On : 6 Mar 2016 1:46
Operator : UM/SJ
Sample : H1650-07
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MS-SS-C350

Manual Integrations
APPROVED

UMANGI
3/7/2016 12:34:27 PM

Quant Time: Mar 07 05:42:44 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Mar 07 04:51:57 2016
Response via : Initial Calibration

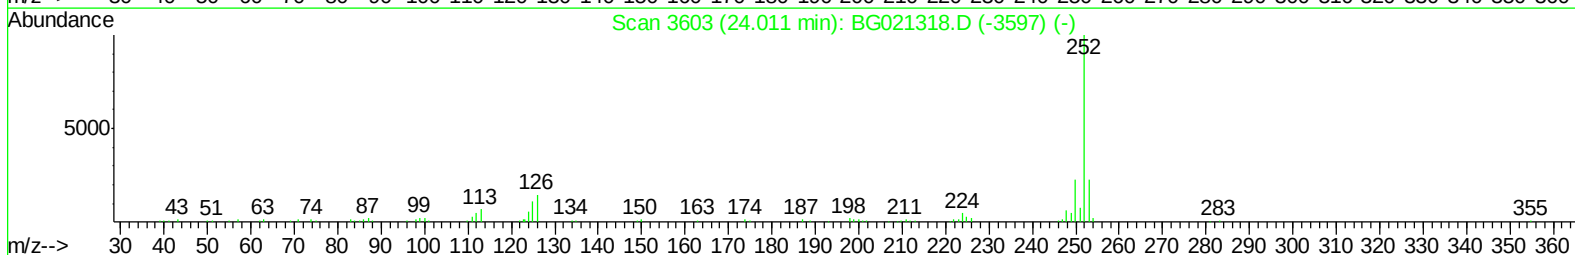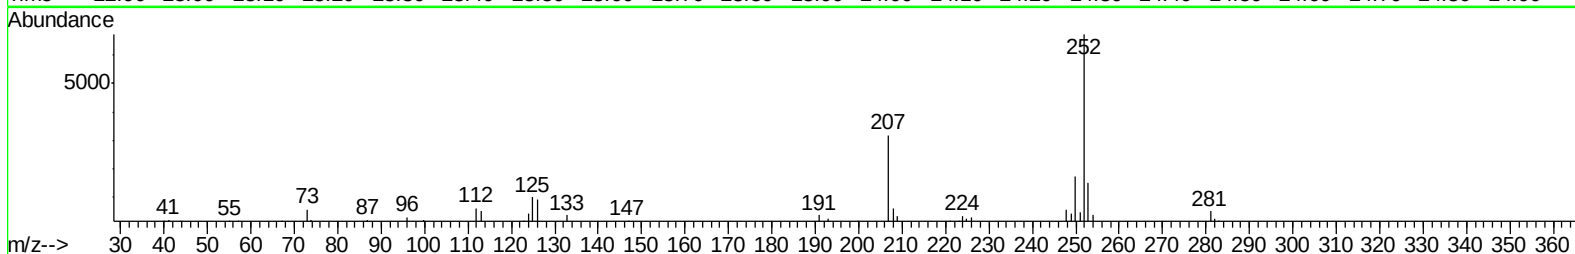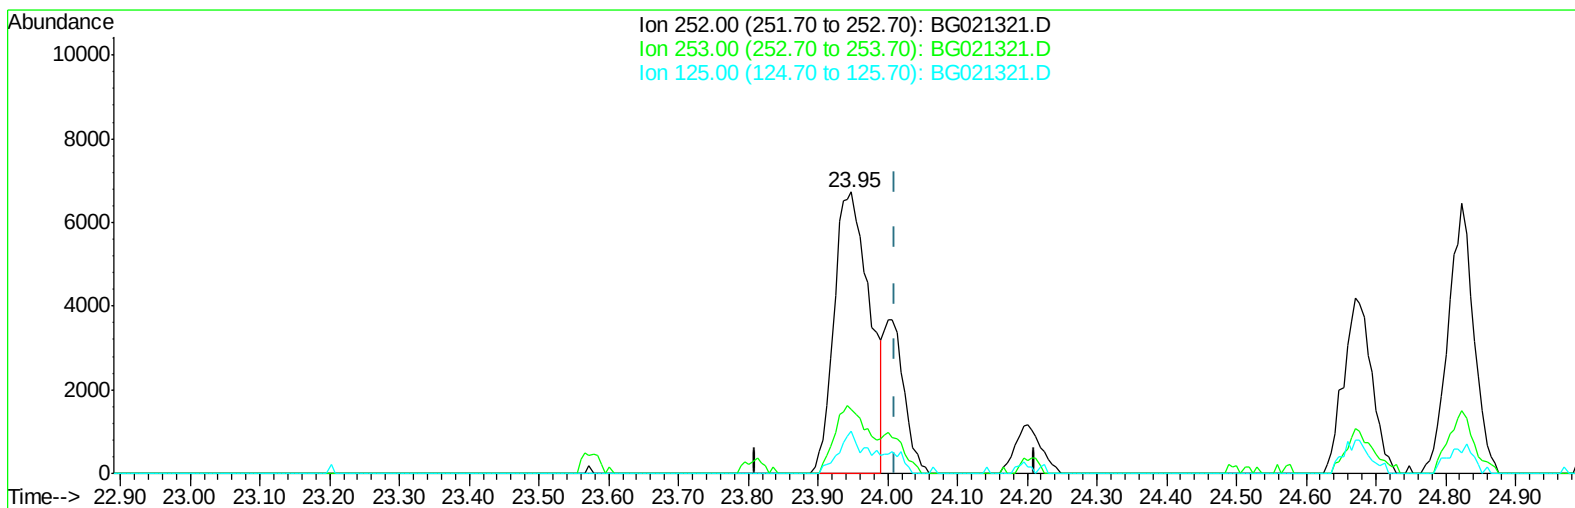

TIC: BG021321.D

(89) Benzo(k)fluoranthene
23.948min (-0.062) 4.46ng/ul
response 23651

Ion	Exp%	Act%
252.00	100	100
253.00	22.50	22.64
125.00	10.10	14.85#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030516\
Data File : BG021321.D
Acq On : 6 Mar 2016 1:46
Operator : UM/SJ
Sample : H1650-07
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MS-SS-C350

Manual Integrations
APPROVED

UMANGI
3/7/2016 12:34:27 PM

Quant Time: Mar 07 05:42:44 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Mar 07 04:51:57 2016
Response via : Initial Calibration

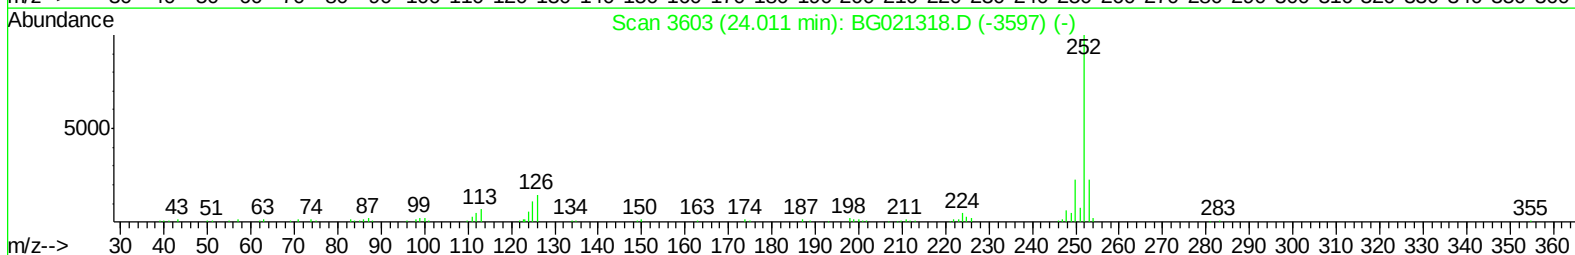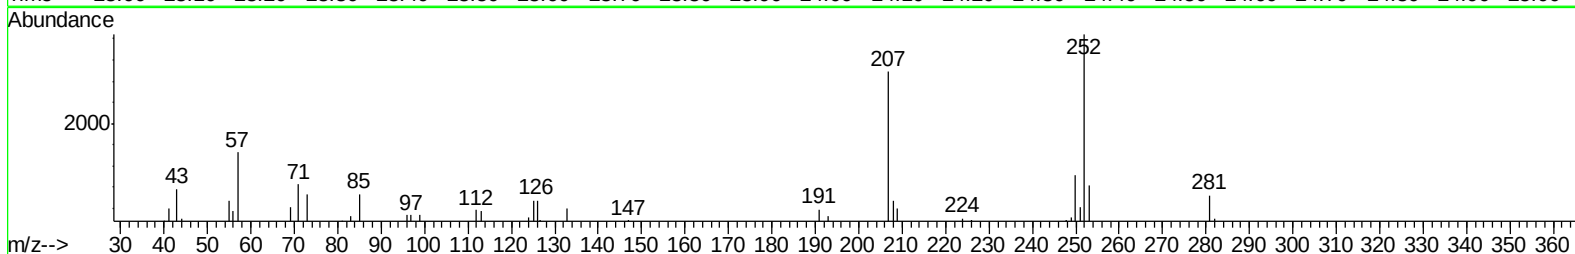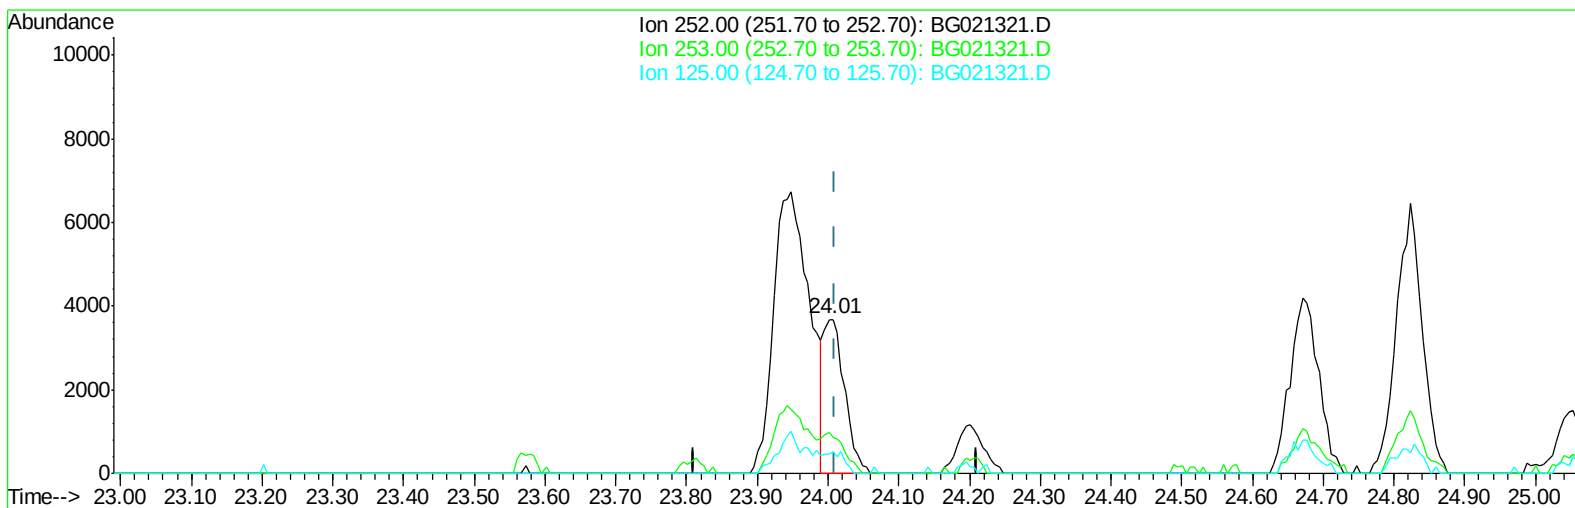

TIC: BG021321.D

(89) Benzo(k)fluoranthene

24.007min (-0.004) 1.40ng/ul m

response 7444

Ion	Exp%	Act%
252.00	100	100
253.00	22.50	22.90
125.00	10.10	14.48#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030516\
Data File : BG021321.D
Acq On : 6 Mar 2016 1:46
Operator : UM/SJ
Sample : H1650-07
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MS-SS-C350

Manual Integrations
APPROVED

UMANGI
3/7/2016 12:34:27 PM

Quant Time: Mar 07 05:42:44 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Mar 07 04:51:57 2016
Response via : Initial Calibration

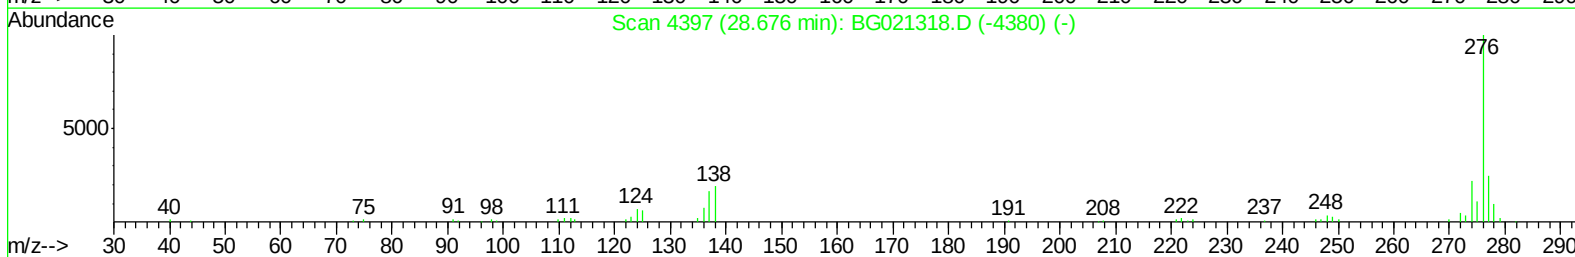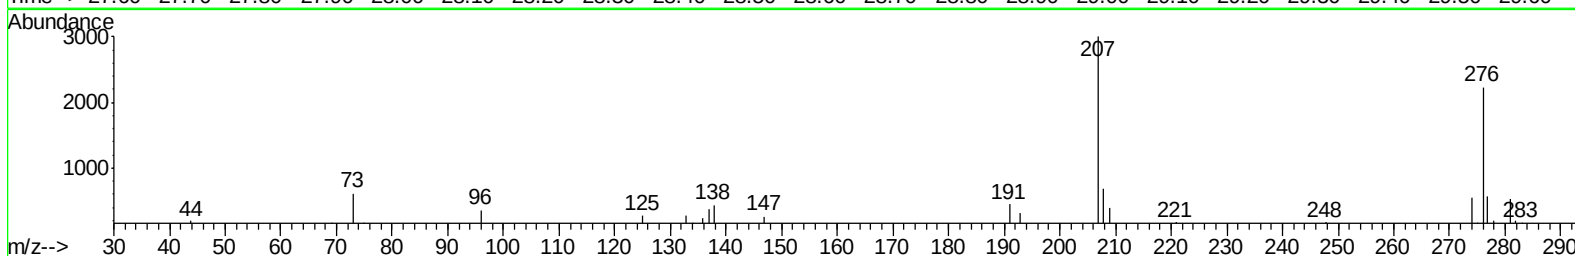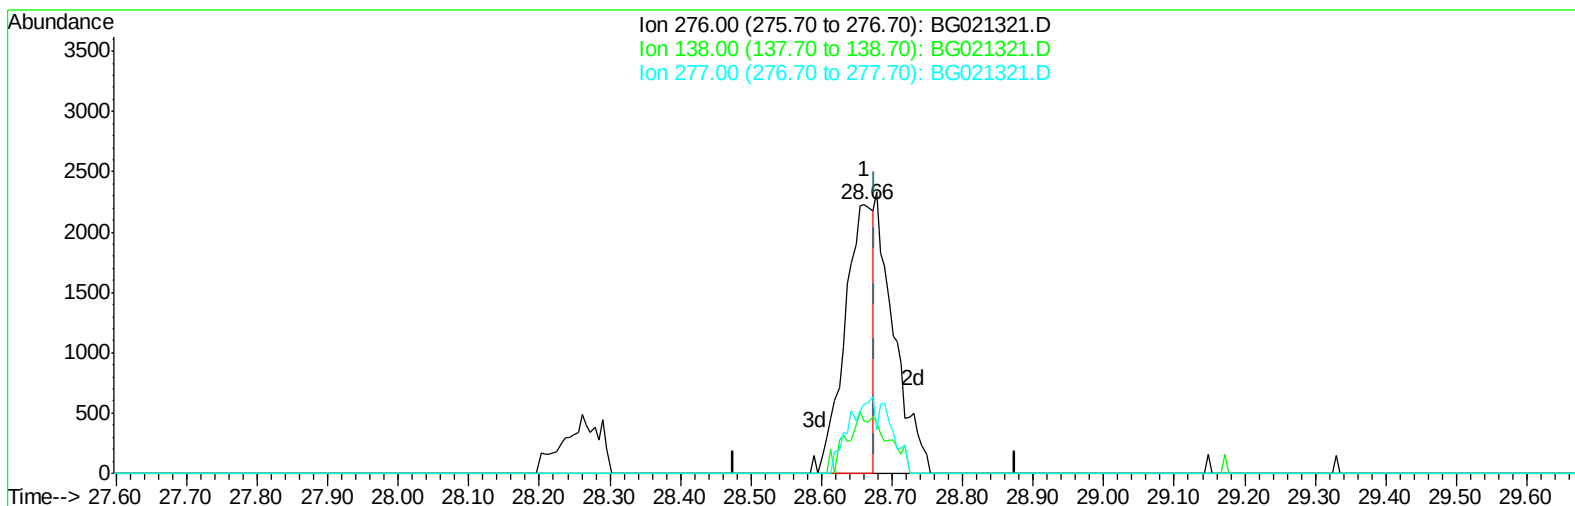

TIC: BG021321.D

(92) Indeno(1,2,3-cd)pyrene

28.660min (-0.015) 1.06ng/ul

response 6104

Ion	Exp%	Act%
276.00	100	100
138.00	18.00	19.44
277.00	22.50	25.68
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030516\
Data File : BG021321.D
Acq On : 6 Mar 2016 1:46
Operator : UM/SJ
Sample : H1650-07
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MS-SS-C350

Manual Integrations
APPROVED

UMANGI
3/7/2016 12:34:27 PM

Quant Time: Mar 07 05:42:44 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Mar 07 04:51:57 2016
Response via : Initial Calibration

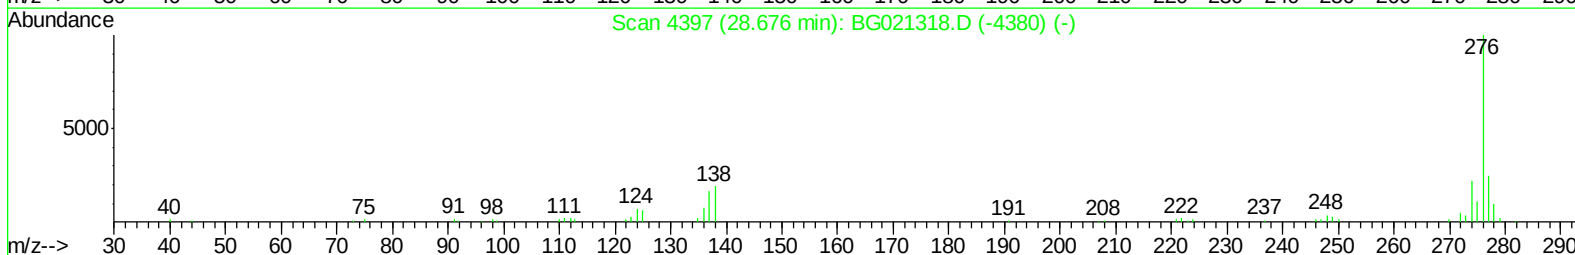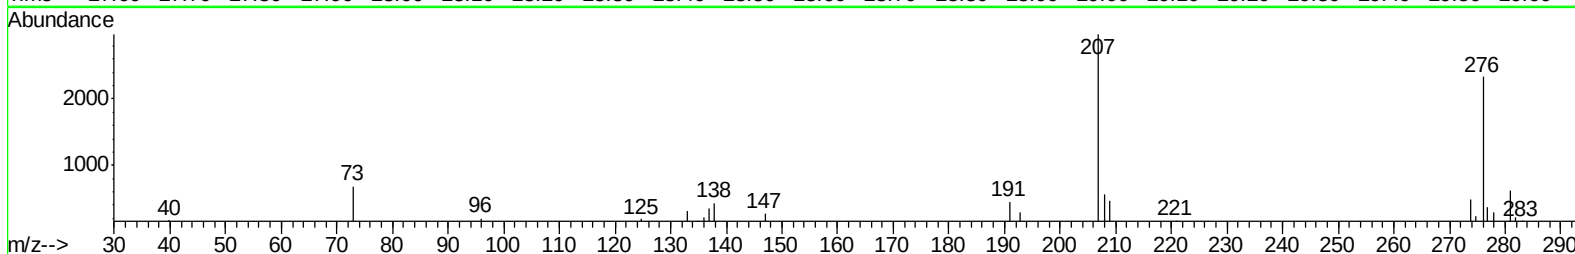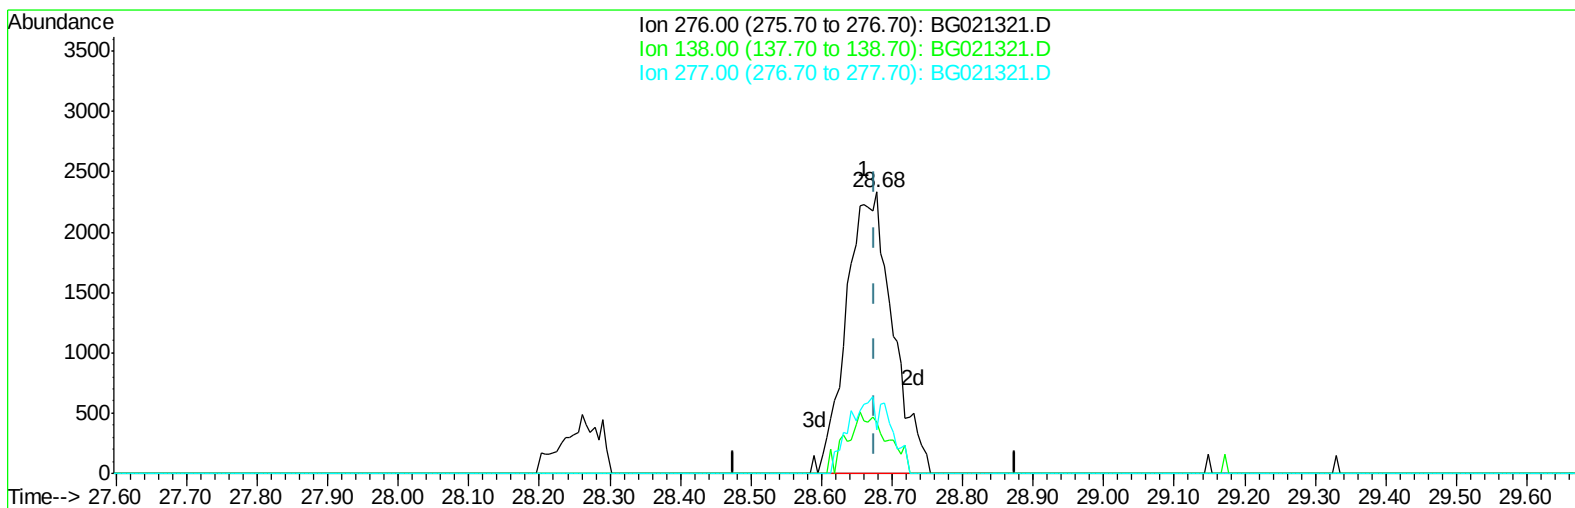

TIC: BG021321.D

(92) Indeno(1,2,3-cd)pyrene

28.678min (+0.002) 1.84ng/ul m

response 10594

Ion	Exp%	Act%
276.00	100	100
138.00	18.00	18.29
277.00	22.50	15.51#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030516\
Data File : BG021321.D
Acq On : 6 Mar 2016 1:46
Operator : UM/SJ
Sample : H1650-07
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MS-SS-C350

Manual Integrations
APPROVED

UMANGI
3/7/2016 12:34:27 PM

Quant Time: Mar 07 05:42:44 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Mar 07 04:51:57 2016
Response via : Initial Calibration

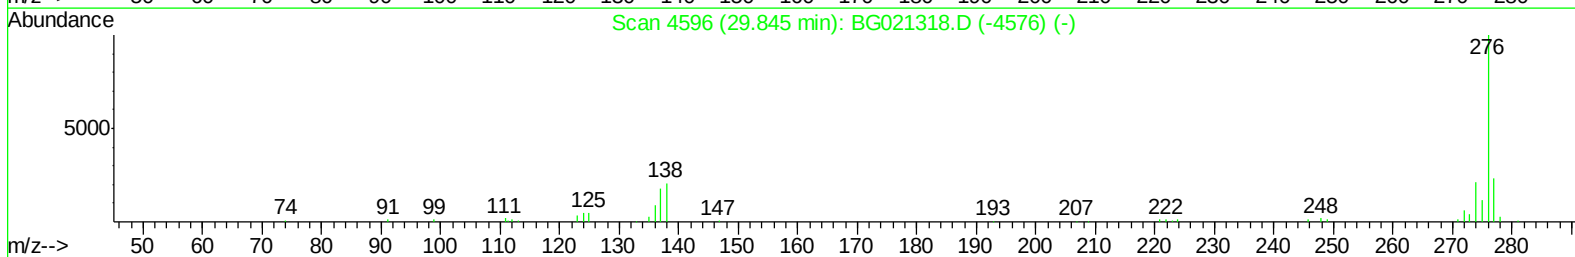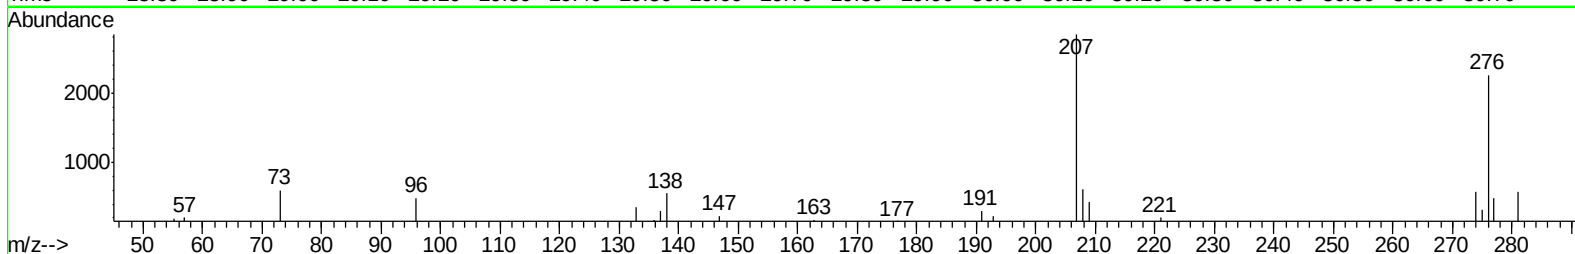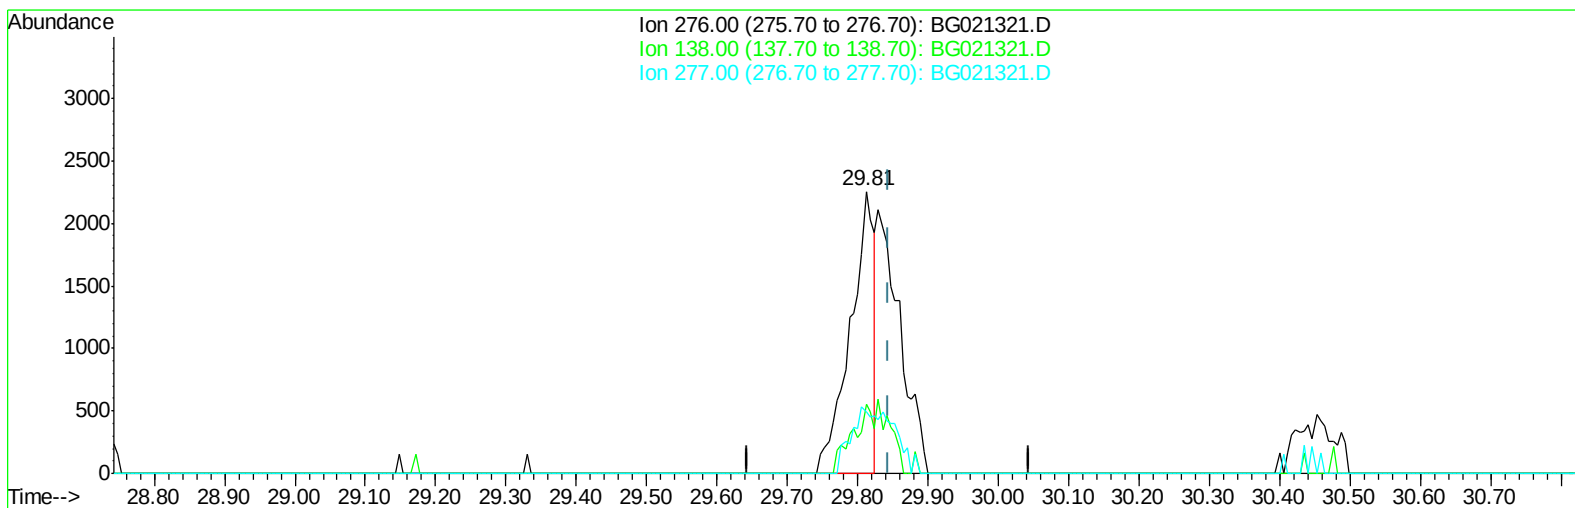

TIC: BG021321.D

(94) Benzo(g,h,i)perylene

29.812min (-0.033) 1.10ng/ul

response 5294

Ion	Exp%	Act%
276.00	100	100
138.00	19.10	24.41#
277.00	23.70	21.75
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030516\
Data File : BG021321.D
Acq On : 6 Mar 2016 1:46
Operator : UM/SJ
Sample : H1650-07
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MS-SS-C350

Manual Integrations
APPROVED

UMANGI
3/7/2016 12:34:27 PM

Quant Time: Mar 07 05:42:44 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Mar 07 04:51:57 2016
Response via : Initial Calibration

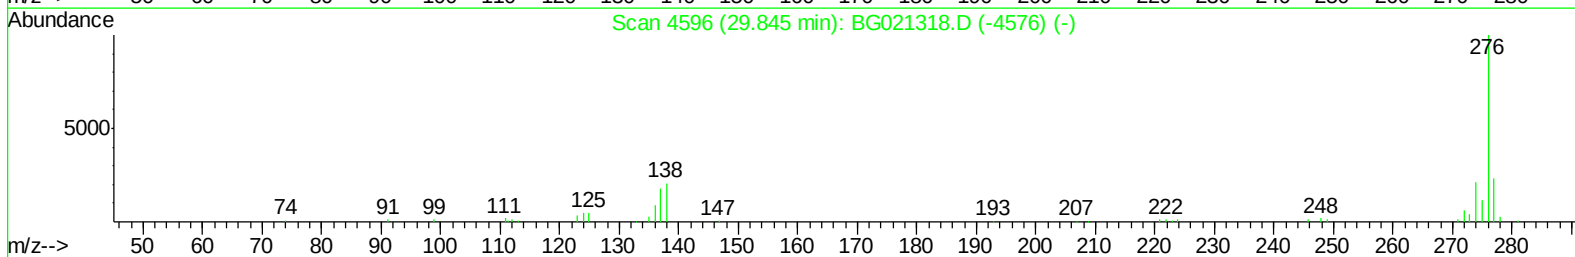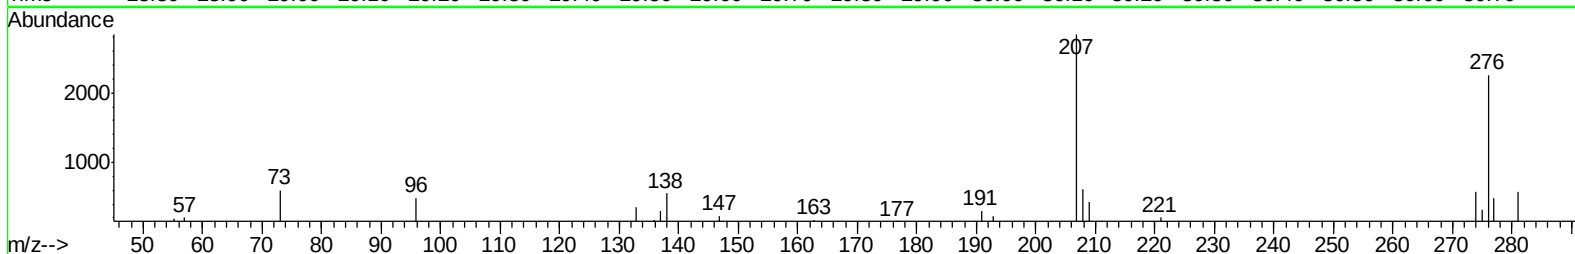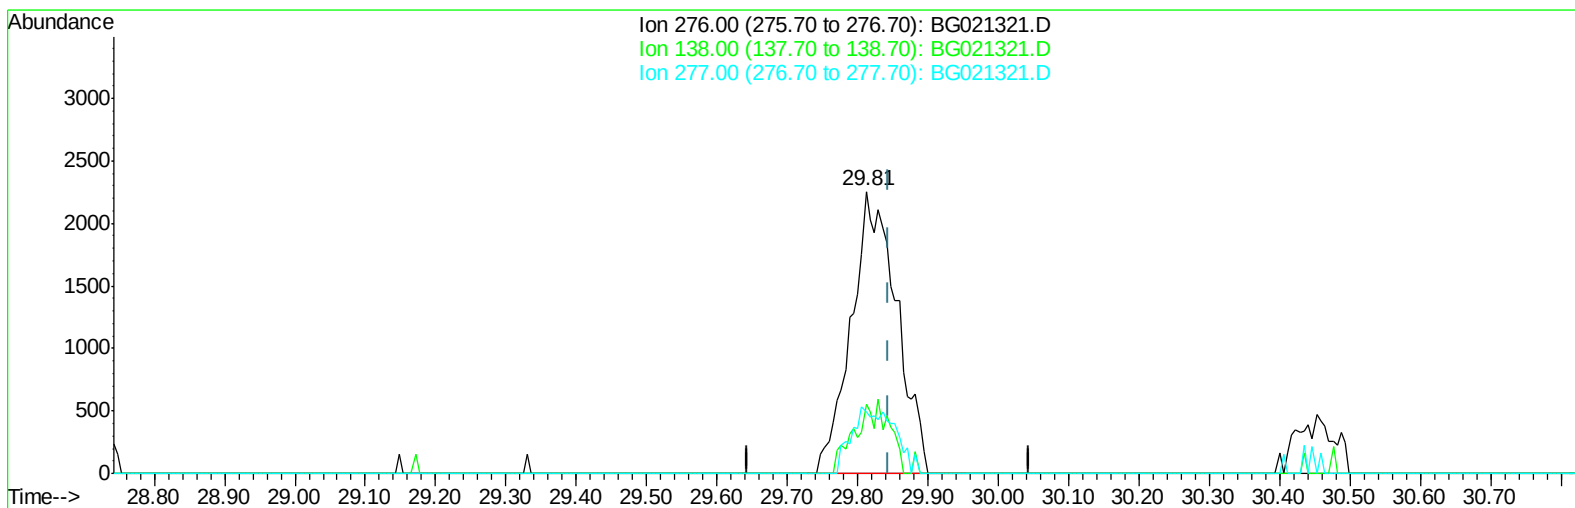

TIC: BG021321.D

(94) Benzo(g,h,i)perylene

29.812min (-0.033) 2.08ng/ul m

response 10030

Ion	Exp%	Act%
276.00	100	100
138.00	19.10	24.41#
277.00	23.70	21.75
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030516\
 Data File : BG021321.D
 Acq On : 6 Mar 2016 1:46
 Operator : UM/SJ
 Sample : H1650-07
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MS-SS-C350

Manual Integrations
 APPROVED

UMANGI
 3/7/2016 12:34:27 PM

Quant Time: Mar 07 05:44:19 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Mar 07 04:51:57 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.13	152	12337	20.00	ng/ul	0.00
18) Naphthalene-d8	10.93	136	60789	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.74	164	34836	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.47	188	75538m	20.00	ng/ul	0.00
78) Chrysene-d12	21.73	240	84640	20.00	ng/ul	0.00
86) Perylene-d12	24.98	264	79376	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.53	96	770	2.53	ng/uL	0.00
5) Phenol-d5	7.27	99	19340	14.80	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.44	67	14414	16.54	ng/ul	0.00
9) 2-Chlorophenol-d4	7.66	132	14111	15.48	ng/ul	0.00
13) 4-Methylphenol-d8	8.82	113	13806	13.38	ng/ul	0.00
19) Nitrobenzene-d5	9.29	128	7850	15.94	ng/ul	0.00
22) 2-Nitrophenol-d4	10.01	143	7976	15.19	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.54	165	13461	14.35	ng/ul	0.00
29) 4-Chloroaniline-d4	11.06	131	30770	25.86	ng/ul	0.00
44) Dimethylphthalate-d6	14.13	166	46421	15.90	ng/ul	0.00
47) Acenaphthylene-d8	14.43	160	59406	16.35	ng/ul	0.00
52) 4-Nitrophenol-d4	14.91	143	5921	10.41	ng/ul	0.00
58) Fluorene-d10	15.72	176	40812	15.92	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.83	200	6029	11.12	ng/ul	0.00
71) Anthracene-d10	17.57	188	61647	16.41	ng/ul	0.00
79) Pyrene-d10	19.84	212	72067	16.82	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.75	264	69496	16.22	ng/ul	0.00

Target Compounds

					Qvalue
45) Dimethylphthalate	14.18	163	17582	5.60 ng/ul#	97
77) Fluoranthene	19.51	202	37680	7.09 ng/ul	98
80) Pyrene	19.87	202	32549	5.74 ng/ul#	95
83) Benzo(a)anthracene	21.71	228	19133	3.49 ng/ul	99
85) Chrysene	21.77	228	17486	3.41 ng/ul	97
88) Benzo(b)fluoranthene	23.95	252	23651	4.30 ng/ul#	96
89) Benzo(k)fluoranthene	24.01	252	7444m	1.40 ng/ul	
91) Benzo(a)pyrene	24.82	252	16390	3.09 ng/ul#	95
92) Indeno(1,2,3-cd)pyrene	28.68	276	10594m	1.84 ng/ul	
94) Benzo(g,h,i)perylene	29.81	276	10030m	2.08 ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030516\
Data File : BG021321.D
Acq On : 6 Mar 2016 1:46
Operator : UM/SJ
Sample : H1650-07
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MS-SS-C350

Manual Integrations
APPROVED

UMANGI
3/7/2016 12:34:27 PM

Quant Time: Mar 07 05:44:19 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Mar 07 04:51:57 2016
Response via : Initial Calibration

