

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030516\
 Data File : BG021315.D
 Acq On : 5 Mar 2016 21:12
 Operator : UM/SJ
 Sample : H1650-16
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MS-DS-C140

Manual Integrations
 APPROVED

UMANGI
 3/7/2016 12:34:18 PM

Quant Time: Mar 07 04:43:48 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Mar 07 03:50:11 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.13	152	9430	20.00	ng/ul	0.00
18) Naphthalene-d8	10.94	136	46195	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.73	164	26948	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.47	188	63458m	20.00	ng/ul	0.00
78) Chrysene-d12	21.73	240	69031	20.00	ng/ul	0.00
86) Perylene-d12	24.98	264	63246	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.53	96	1171	5.04	ng/uL	0.00
5) Phenol-d5	7.27	99	29167	29.20	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.45	67	21135	31.73	ng/ul	0.00
9) 2-Chlorophenol-d4	7.65	132	21546	30.92	ng/ul	0.00
13) 4-Methylphenol-d8	8.82	113	24470	31.03	ng/ul	0.00
19) Nitrobenzene-d5	9.28	128	11211	29.96	ng/ul	0.00
22) 2-Nitrophenol-d4	10.01	143	11785	29.54	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.55	165	20366	28.57	ng/ul	0.00
29) 4-Chloroaniline-d4	11.06	131	18695	20.68	ng/ul	0.00
44) Dimethylphthalate-d6	14.14	166	74537	33.01	ng/ul	0.00
47) Acenaphthylene-d8	14.43	160	93830	33.39	ng/ul	0.00
52) 4-Nitrophenol-d4	14.91	143	13317	30.25	ng/ul	0.00
58) Fluorene-d10	15.72	176	66994	33.78	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.83	200	11434	25.11	ng/ul	0.00
71) Anthracene-d10	17.57	188	107011	33.91	ng/ul	0.00
79) Pyrene-d10	19.84	212	119888	34.31	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.76	264	116161	34.02	ng/ul	0.00

Target Compounds					Qvalue
45) Dimethylphthalate	14.18	163	21754	8.95 ng/ul#	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030516\
Data File : BG021315.D
Acq On : 5 Mar 2016 21:12
Operator : UM/SJ
Sample : H1650-16
Misc :
ALS Vial : 11 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
MS-DS-C140

Manual Integrations
APPROVED

UMANGI
3/7/2016 12:34:18 PM

Quant Time: Mar 07 04:43:48 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Mar 07 03:50:11 2016
Response via : Initial Calibration

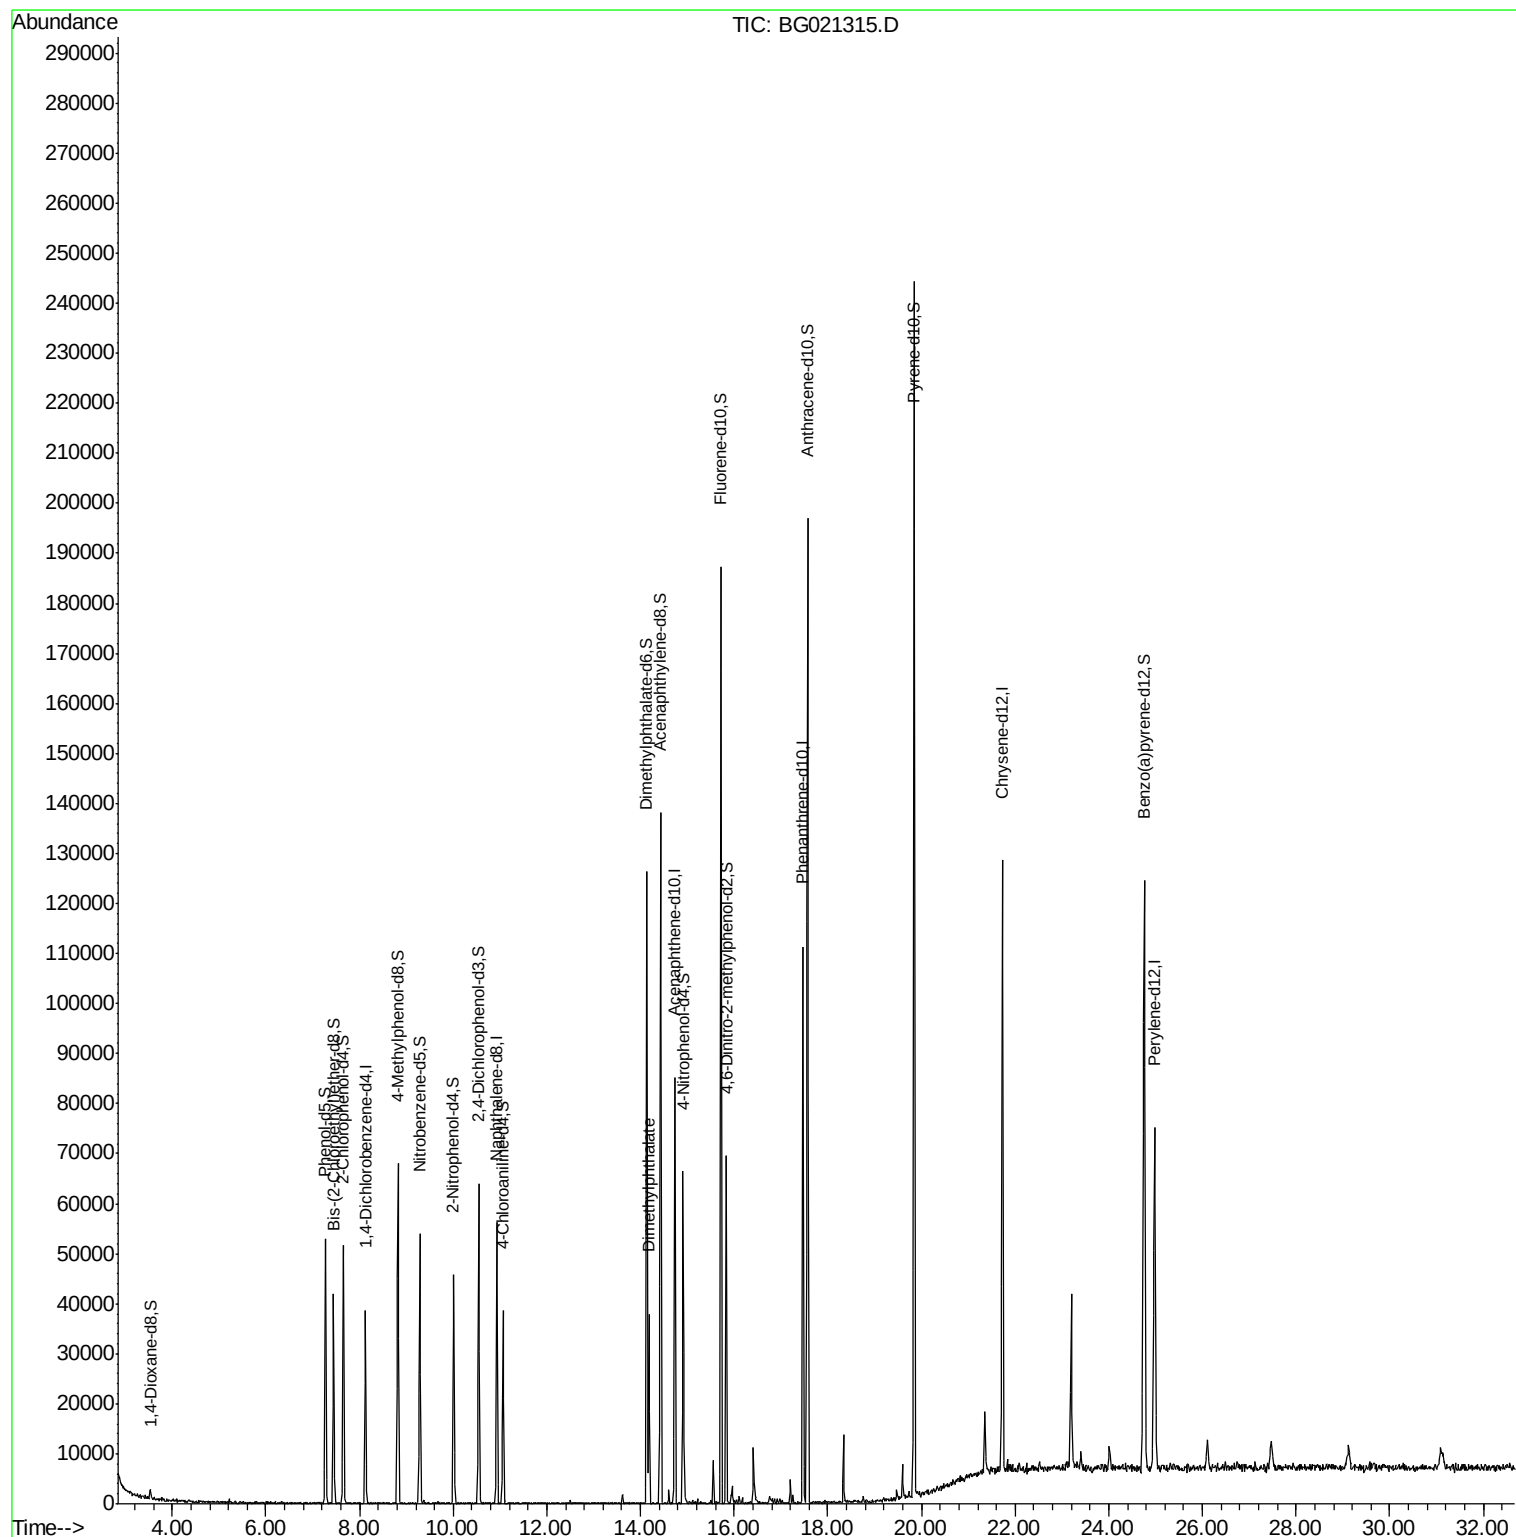

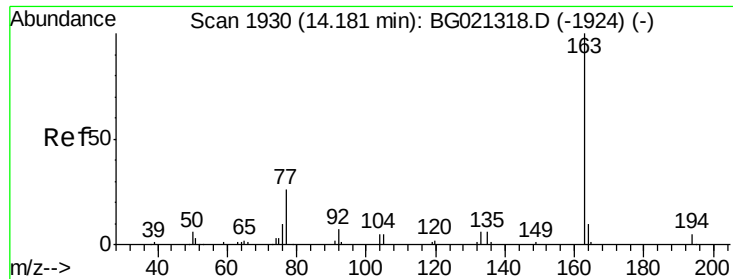


#45
 Dimethylphthalate
 Concen: 8.95 ng/ul
 RT: 14.18 min Scan# 1930
 Delta R.T. -0.00 min
 Lab File: BG021315.D
 Acq: 5 Mar 2016 21:12

Instrument :
 BNA_G
 ClientSampleId :
 MS-DS-C140

Tgt Ion	Ratio	Resp Lower	Resp Upper
163	100		
194	5.1	2.8	4.2#
164	11.0	8.2	12.2

Manual Integrations
 APPROVED

UMANGI
 3/7/2016 12:34:18 PM

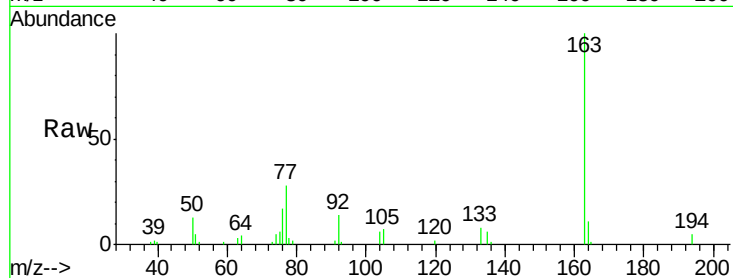

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

