

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030516\
 Data File : BG021317.D
 Acq On : 5 Mar 2016 22:30
 Operator : UM/SJ
 Sample : H1650-18
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MS-DS-B210

Quant Time: Mar 07 03:51:42 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Mar 07 03:50:11 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.12	152	10841	20.00	ng/ul	0.00
18) Naphthalene-d8	10.93	136	54058	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.73	164	32065	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.47	188	69456	20.00	ng/ul	0.00
78) Chrysene-d12	21.73	240	74045	20.00	ng/ul	0.00
86) Perylene-d12	24.98	264	68255	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.53	96	1195	4.48	ng/uL	0.00
5) Phenol-d5	7.28	99	31135	27.12	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.45	67	22753	29.72	ng/ul	0.00
9) 2-Chlorophenol-d4	7.65	132	22139	27.64	ng/ul	0.00
13) 4-Methylphenol-d8	8.82	113	25275	27.88	ng/ul	0.00
19) Nitrobenzene-d5	9.29	128	12016	27.44	ng/ul	0.00
22) 2-Nitrophenol-d4	10.01	143	13140	28.15	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.55	165	21788	26.12	ng/ul	0.00
29) 4-Chloroaniline-d4	11.07	131	21814	20.62	ng/ul	0.00
44) Dimethylphthalate-d6	14.13	166	78104	29.07	ng/ul	0.00
47) Acenaphthylene-d8	14.43	160	99523	29.76	ng/ul	0.00
52) 4-Nitrophenol-d4	14.91	143	12594	24.05	ng/ul	0.00
58) Fluorene-d10	15.72	176	68152	28.88	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.83	200	11993	24.06	ng/ul	0.00
71) Anthracene-d10	17.57	188	105270	30.48	ng/ul	0.00
79) Pyrene-d10	19.84	212	118504	31.62	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.76	264	113264	30.74	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.18	163	21070	7.29	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030516\
Data File : BG021317.D
Acq On : 5 Mar 2016 22:30
Operator : UM/SJ
Sample : H1650-18
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MS-DS-B210

Quant Time: Mar 07 03:51:42 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Mar 07 03:50:11 2016
Response via : Initial Calibration

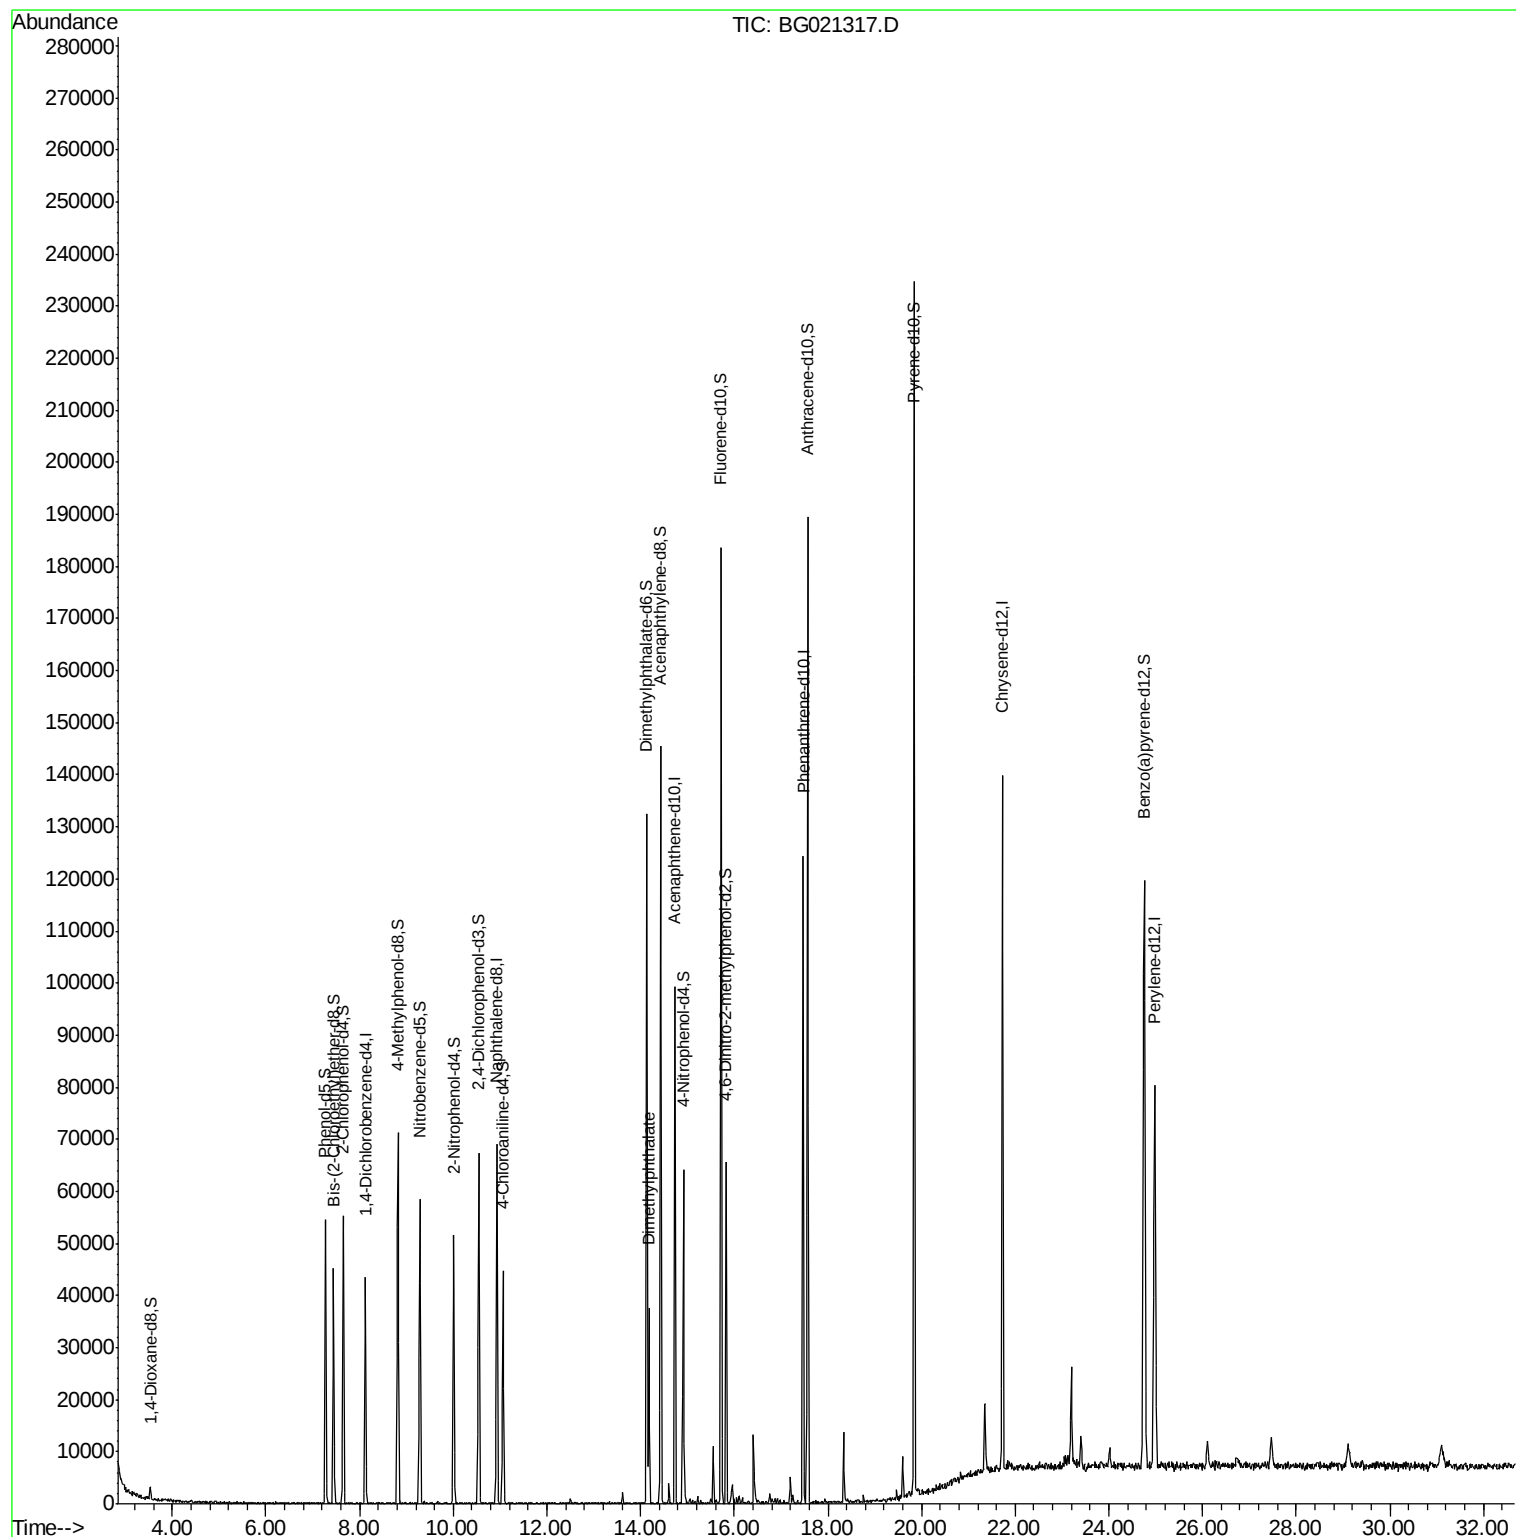

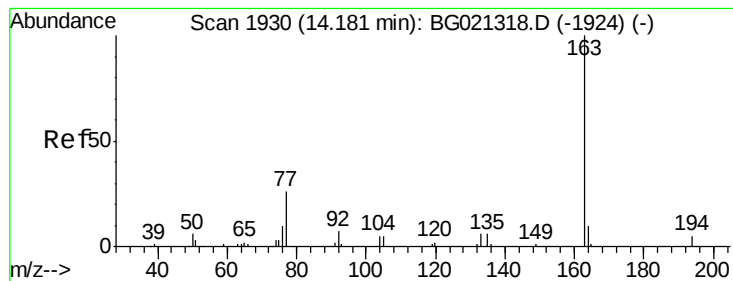

#45

Dimethylphthalate

Concen: 7.29 ng/ul

RT: 14.18 min Scan# 1930

Delta R.T. -0.00 min

Lab File: BG021317.D


Acq: 5 Mar 2016 22:30

Instrument :

BNA_G

ClientSampleId :

MS-DS-B210

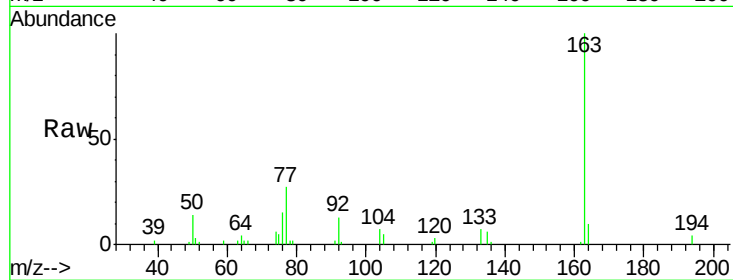


Tgt Ion:163 Resp: 21070

Ion Ratio Lower Upper

163 100

194 3.8 2.8 4.2

164 10.3 8.2 12.2

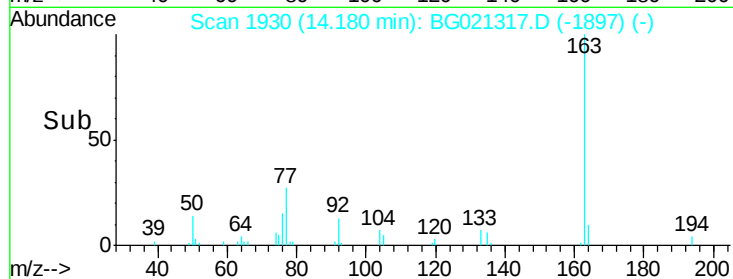

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

