


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA G\Data\BG030518\
 Data File : BG033000.D
 Acq On : 5 Mar 2018 22:15
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG022118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 01 17:38:52 2018

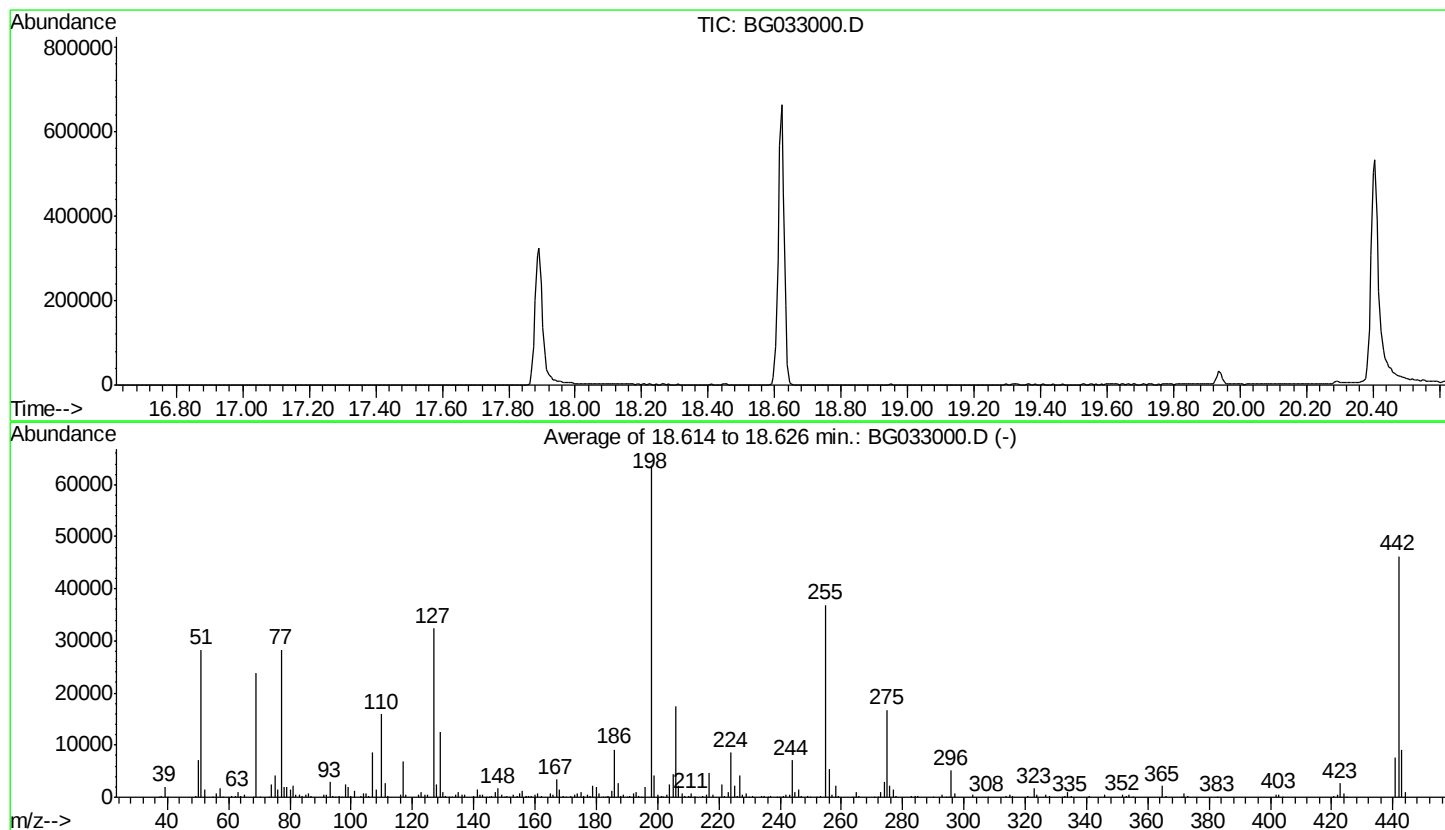

AutoFind: Scans 2609, 2610, 2611; Background Corrected with Scan 2602

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.5	28296	PASS
68	69	0.00	2	0.5	120	PASS
69	198	0.00	100	37.3	23720	PASS
70	69	0.00	2	0.3	66	PASS
127	198	10	80	50.8	32338	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	63640	PASS
199	198	5	9	6.7	4289	PASS
275	198	10	60	26.3	16756	PASS
365	198	1	100	3.5	2209	PASS
441	442	0.01	24	16.5	7615	PASS
442	198	50	100	72.6	46218	PASS
443	442	15	24	19.7	9106	PASS