
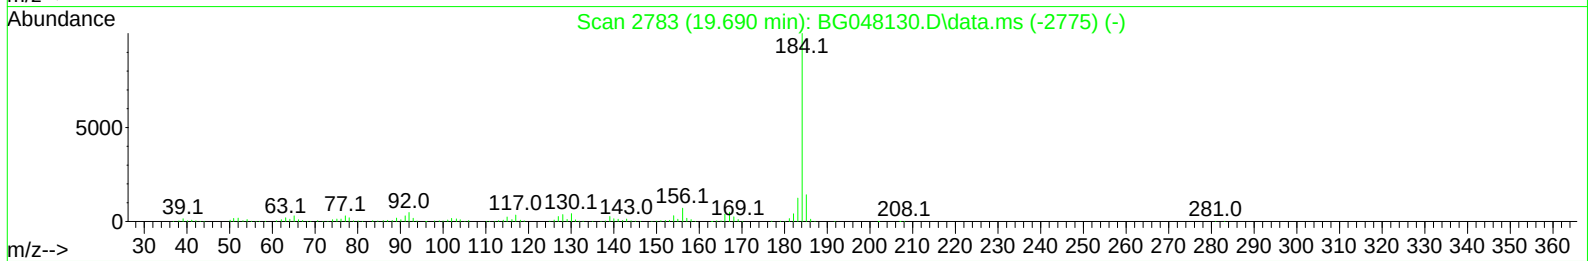
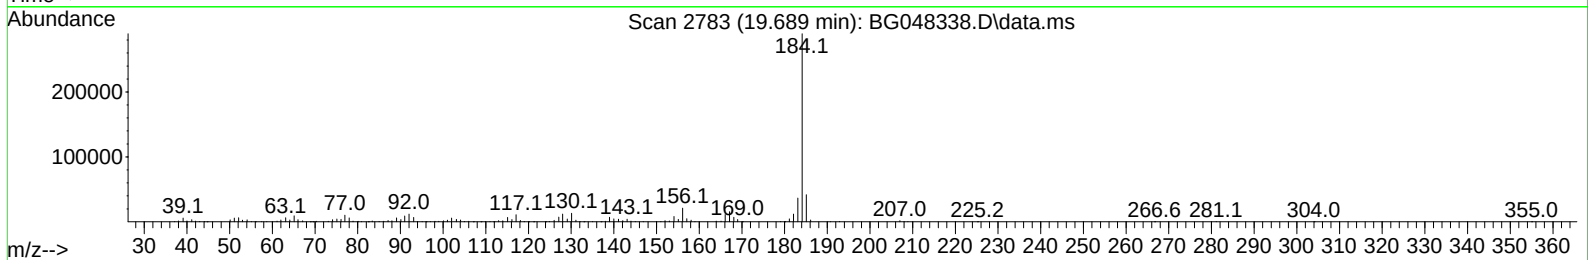


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030521\
 Data File : BG048338.D
 Acq On : 5 Mar 2021 13:33
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 05 14:39:17 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG021021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 03 16:40:27 2021
 Response via : Initial Calibration

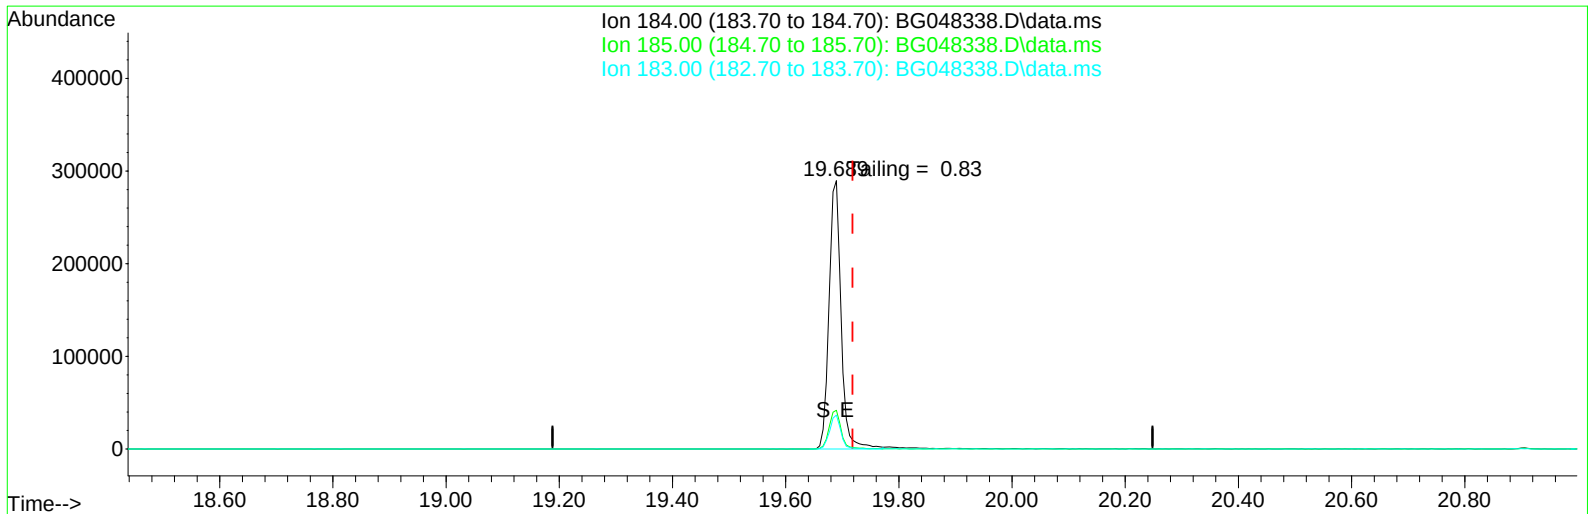




TIC: BG048338.D\data.ms

(77) Benzidine**19.689min (-0.028) 220189.64 ng****response 431673**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.45
183.00	13.20	12.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030521\
Data File : BG048338.D
Acq On : 5 Mar 2021 13:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 05 14:39:17 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG021021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 03 16:40:27 2021
Response via : Initial Calibration

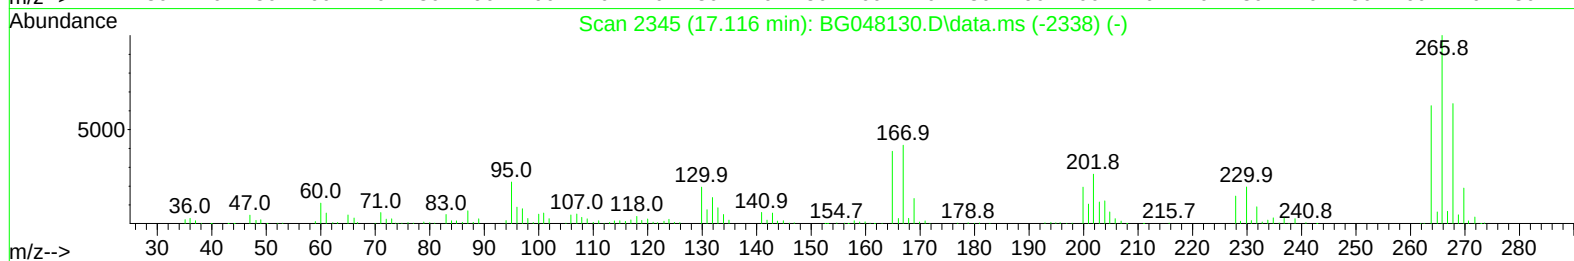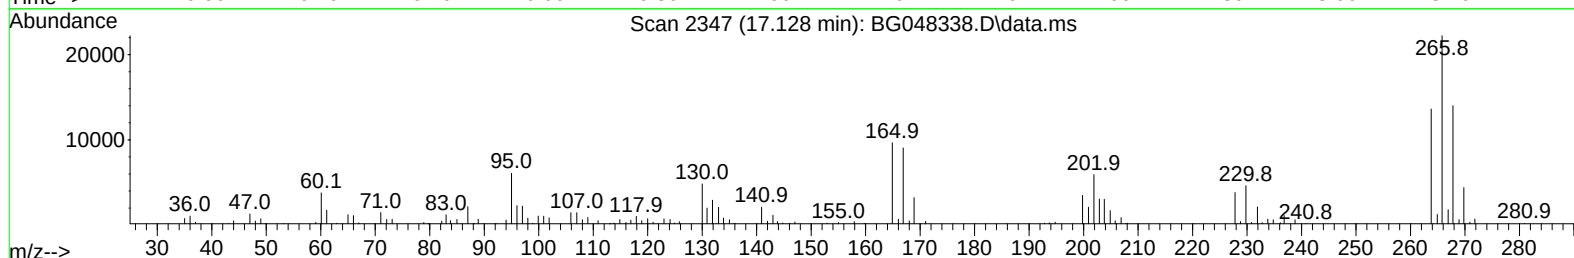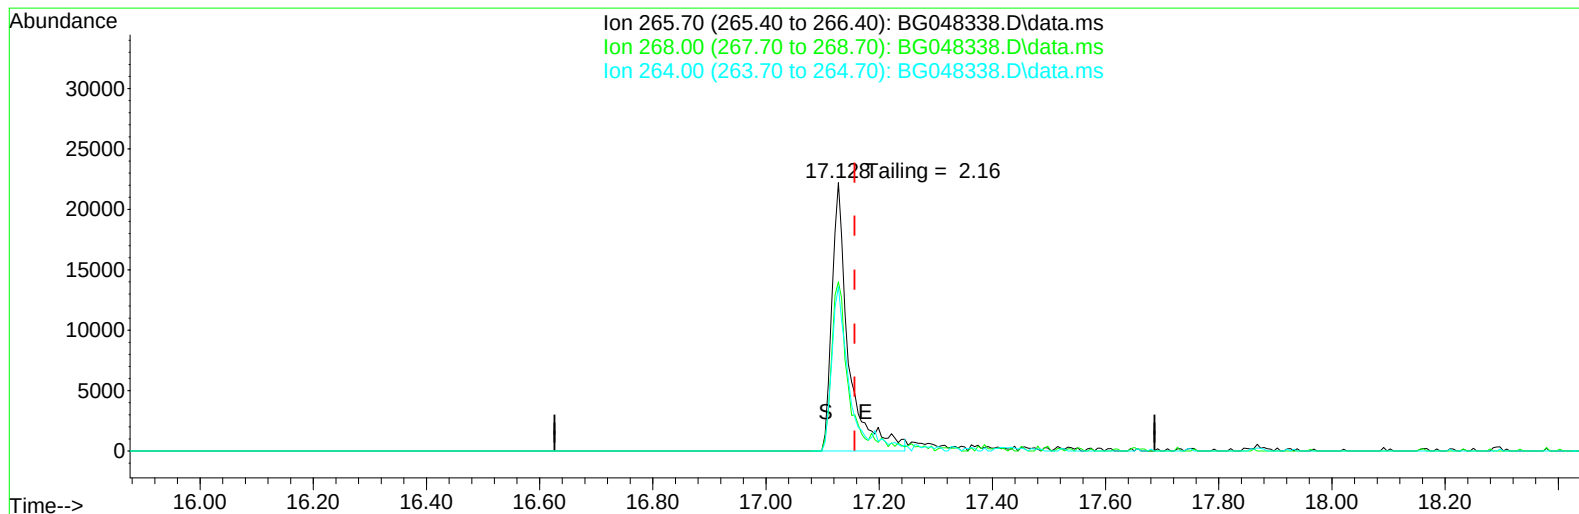

TIC: BG048338.D\data.ms

(70) Pentachlorophenol (C)

17.128min (-0.028) 83192.68 ng

response 43418

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.06
264.00	61.60	61.28
0.00	0.00	0.00