


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030521\
 Data File : BG048338.D
 Acq On : 5 Mar 2021 13:33
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG021021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 05 16:23:55 2021

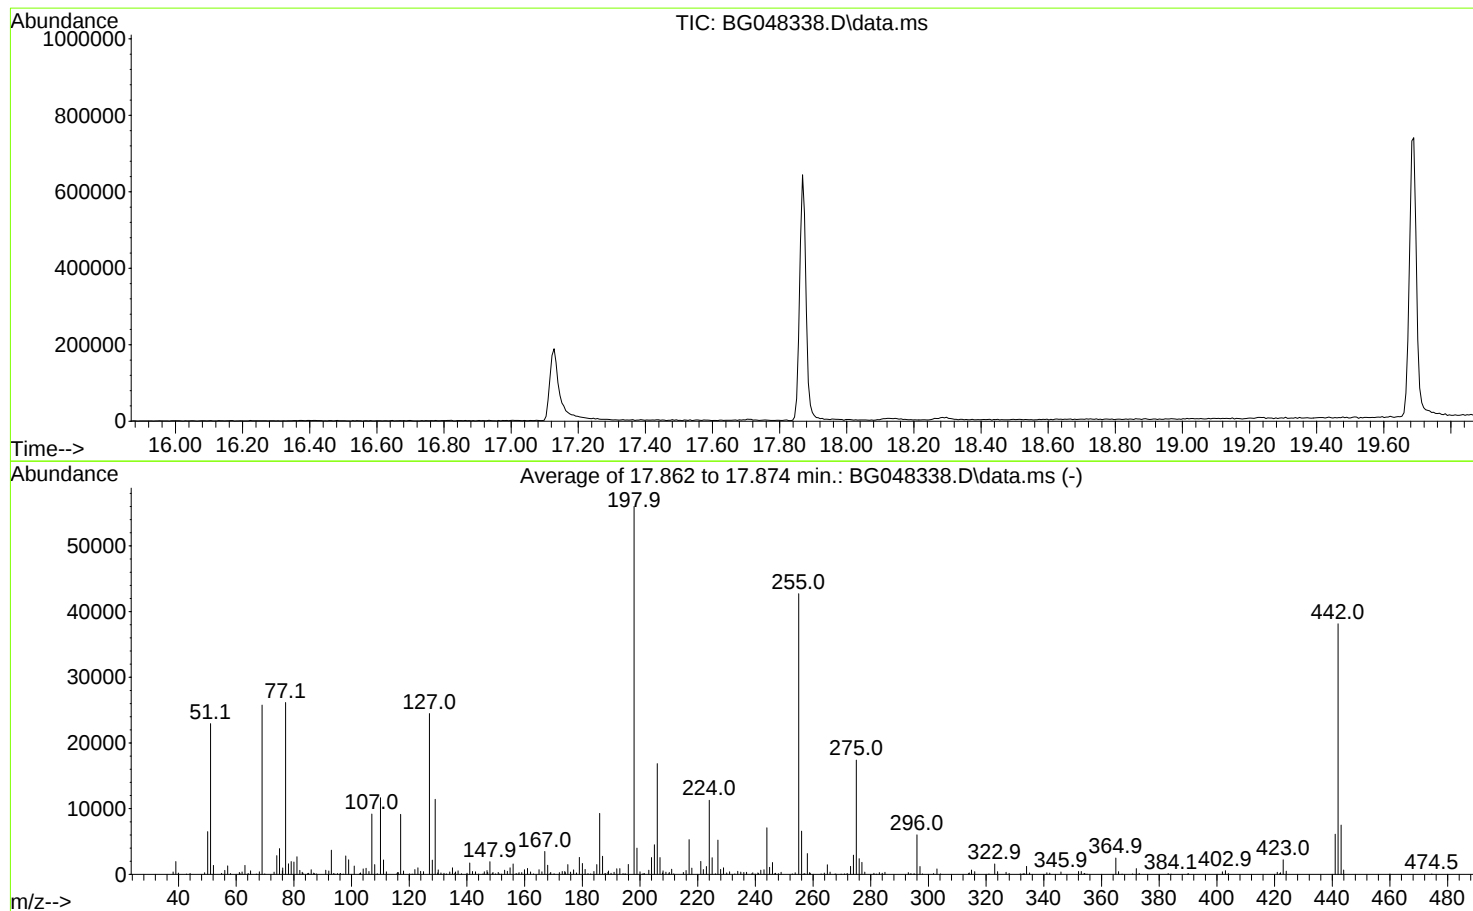

AutoFind: Scans 2472, 2473, 2474; Background Corrected with Scan 2466

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.0	22944	PASS
68	69	0.00	2	1.5	388	PASS
69	198	0.00	100	46.0	25773	PASS
70	69	0.00	2	0.3	84	PASS
127	198	10	80	43.7	24480	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	56000	PASS
199	198	5	9	7.1	4002	PASS
275	198	10	60	31.1	17389	PASS
365	198	1	100	4.4	2491	PASS
441	198	0.01	100	10.9	6124	PASS
442	198	50	100	68.1	38141	PASS
443	442	15	24	19.6	7493	PASS




	DDT Breakdown	
Date	Instrument Name	DFTPP Data File
3/5/2021	BNA_G	<u>BG048338.D</u>
Compound Name	Response	Retention Time
DDT	241225	20.9
DDD	984	20.51
DDE	322	19.95
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1306	242531	0.54

Instrument :
 BNA_G
ClientSampleId :
 DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030521\
Data File : BG048338.D
Acq On : 5 Mar 2021 13:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 05 14:39:17 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG021021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 03 16:40:27 2021
Response via : Initial Calibration

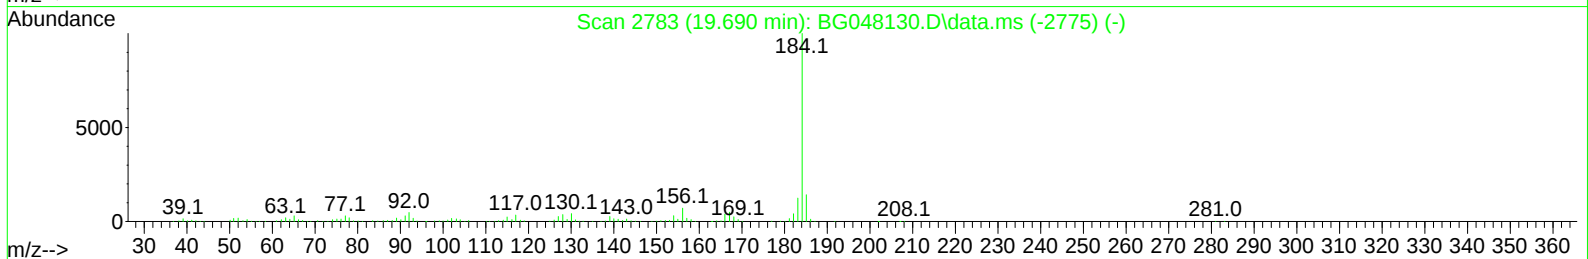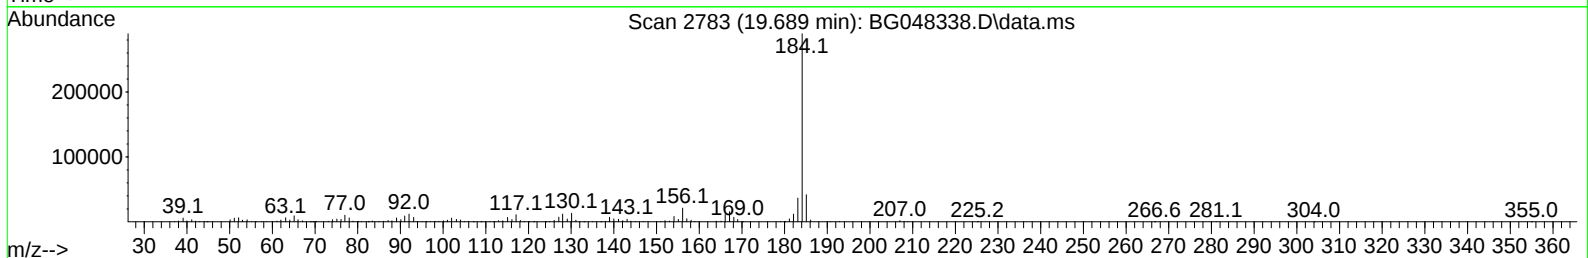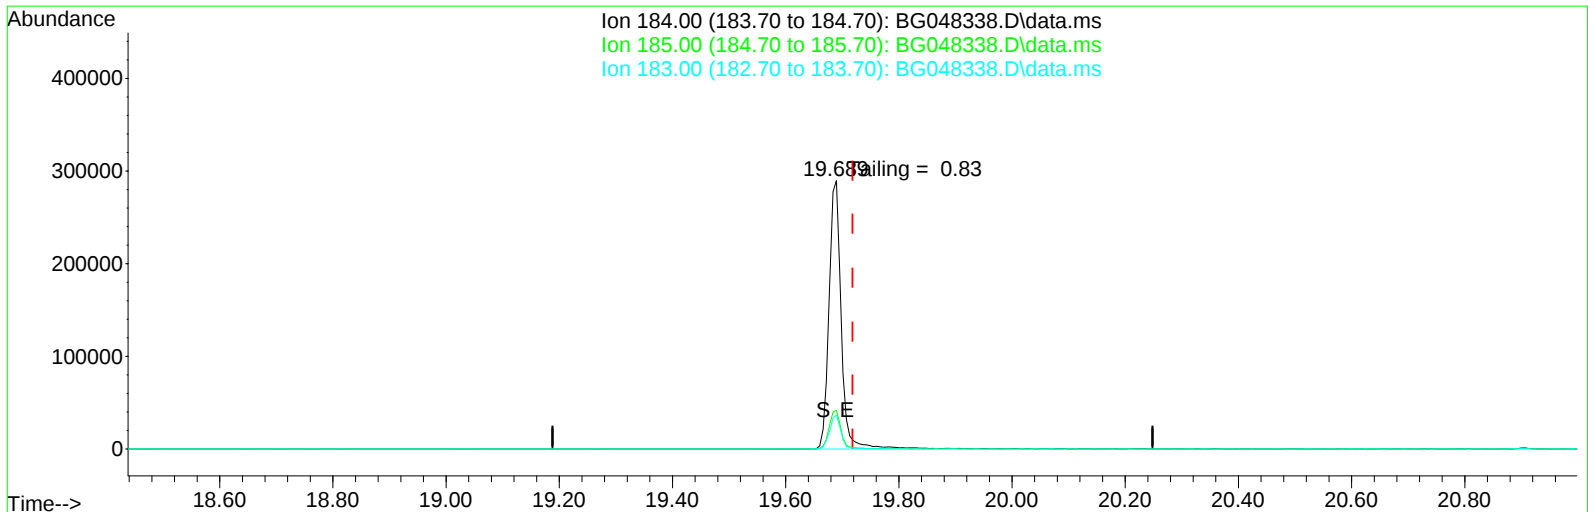

TIC: BG048338.D\data.ms

(77) Benzidine

19.689min (-0.028) 220189.64 ng




response 431673

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.45
183.00	13.20	12.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030521\
Data File : BG048338.D
Acq On : 5 Mar 2021 13:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 05 14:39:17 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG021021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 03 16:40:27 2021
Response via : Initial Calibration

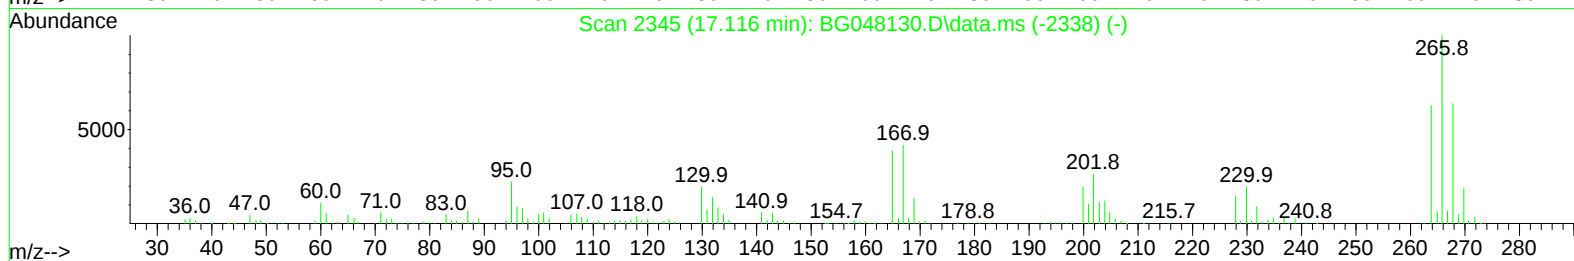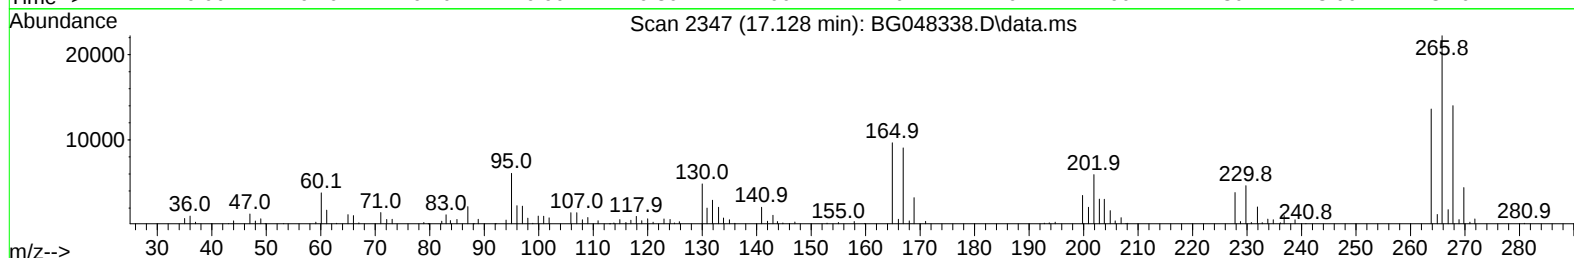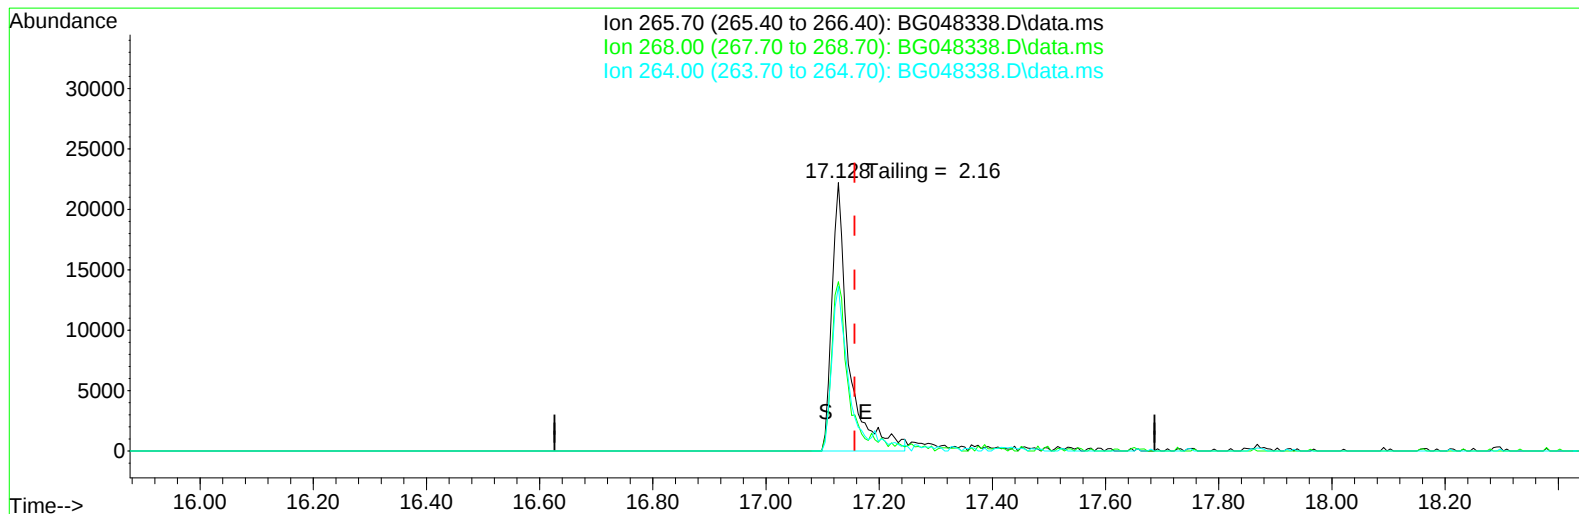

TIC: BG048338.D\data.ms

(70) Pentachlorophenol (C)

17.128min (-0.028) 83192.68 ng

response 43418

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.06
264.00	61.60	61.28
0.00	0.00	0.00