
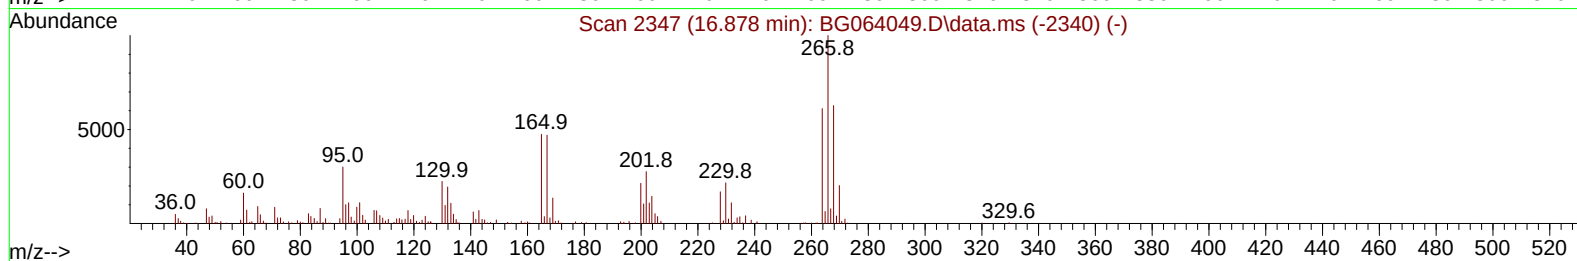
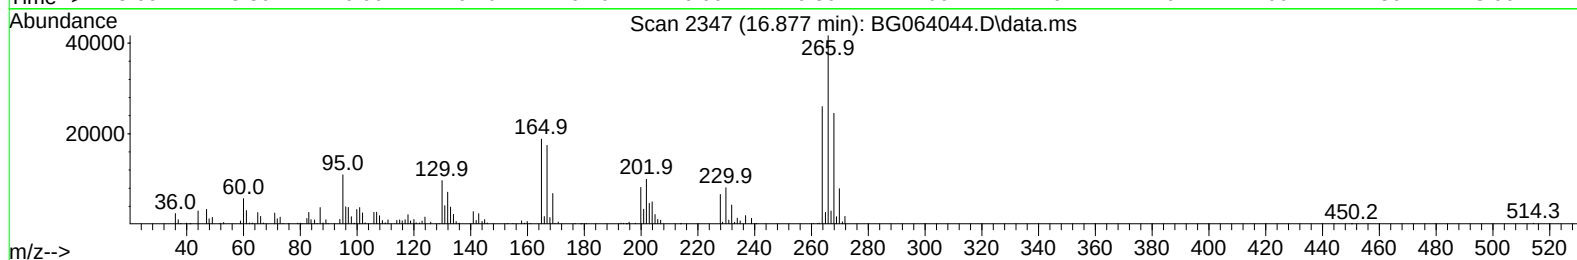


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030525\
Data File : BG064044.D
Acq On : 5 Mar 2025 8:15
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 05 15:40:12 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 05 15:39:19 2025
Response via : Initial Calibration

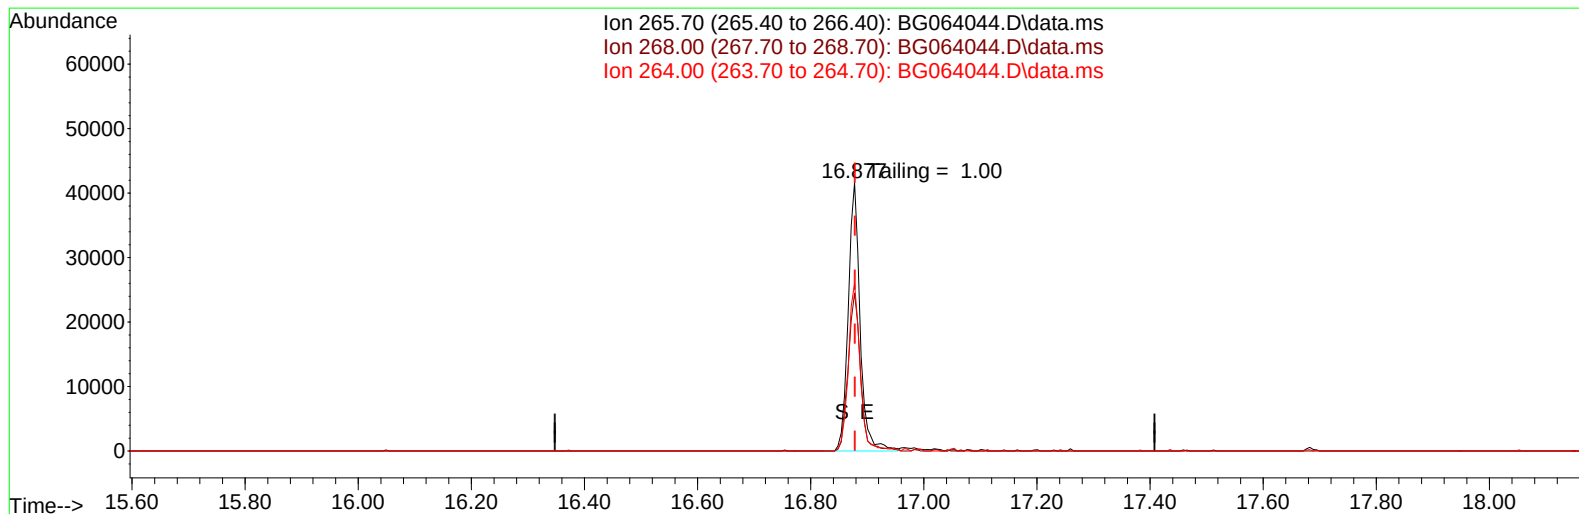

TIC: BG064044.D\data.ms

(70) Pentachlorophenol (C)




16.877min (-0.001) 14067.66 ng

response 60892

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.80	58.85
264.00	61.10	62.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030525\
Data File : BG064044.D
Acq On : 5 Mar 2025 8:15
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 05 15:40:12 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 05 15:39:19 2025
Response via : Initial Calibration

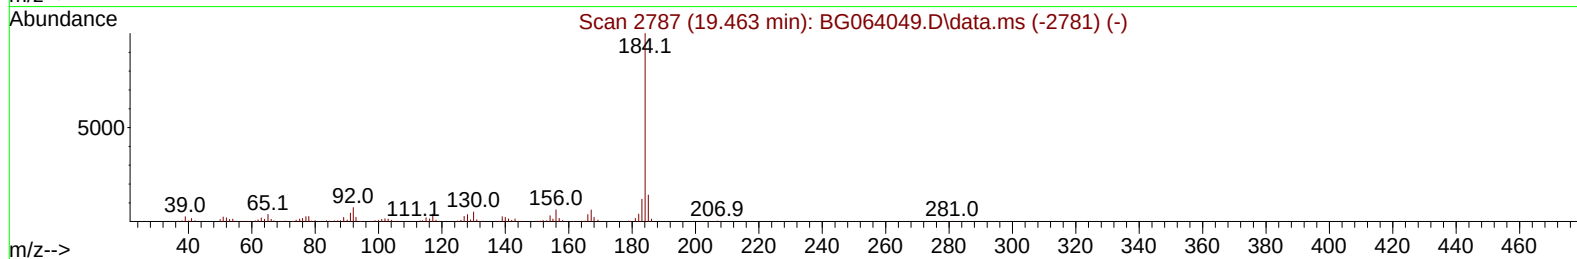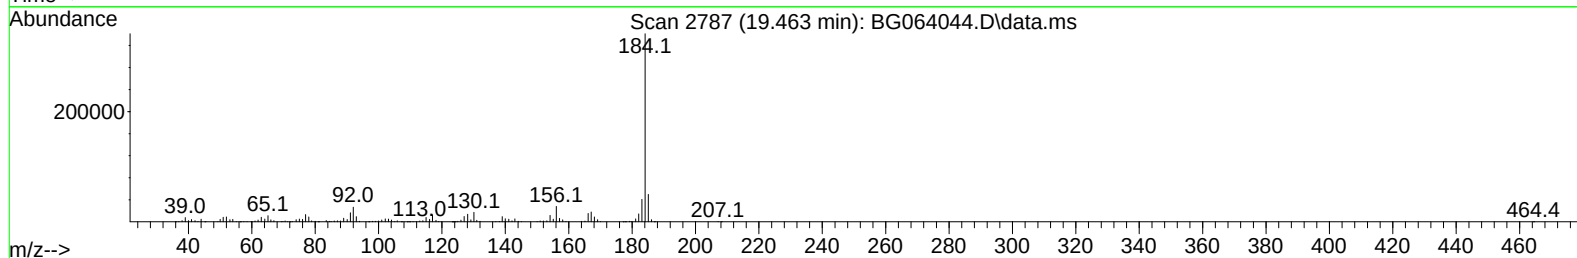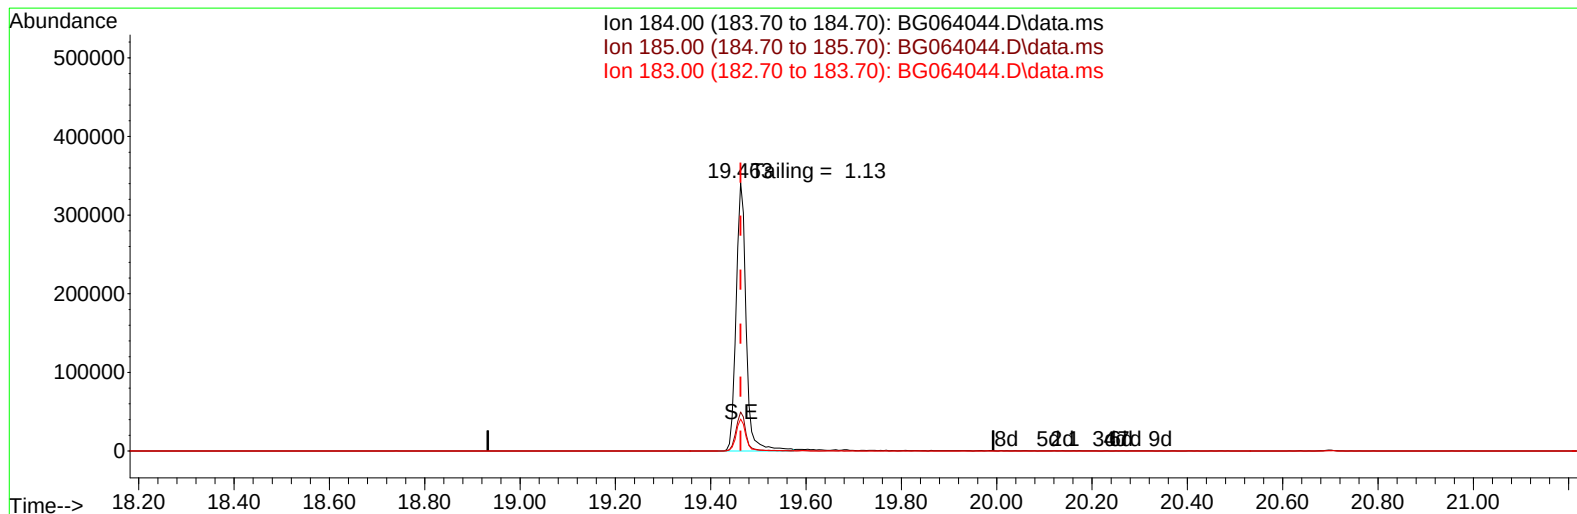

TIC: BG064044.D\data.ms

(77) Benzidine

19.463min (-0.000) 687177.88 ng m

response 523350

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.57
183.00	11.90	11.97
0.00	0.00	0.00