
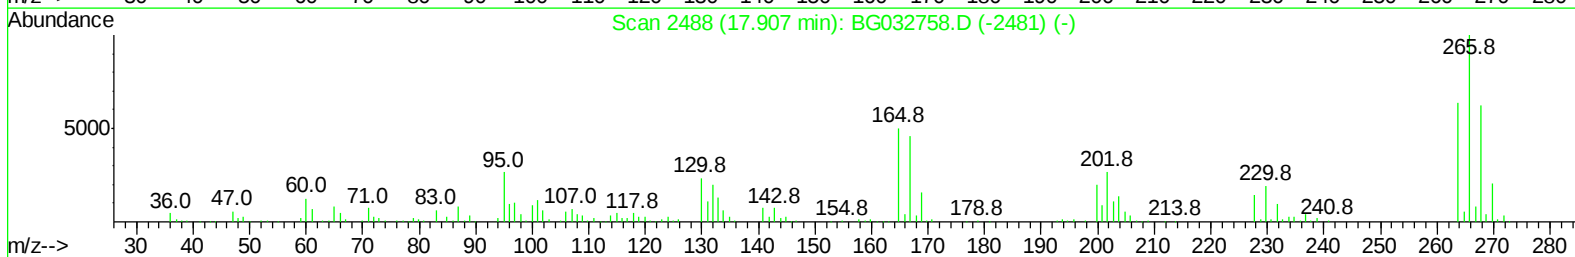
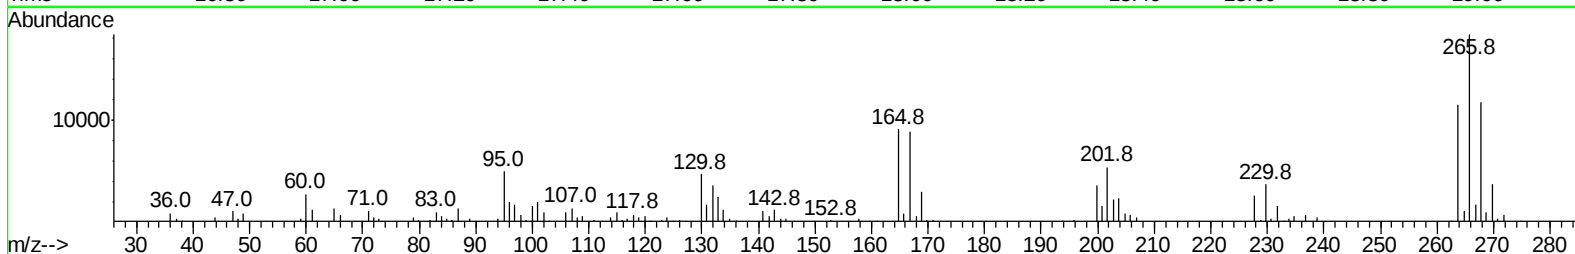


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG030618\  
Data File : BG033033.D  
Acq On : 6 Mar 2018 23:02  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 07 03:19:26 2018  
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022118.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Mar 06 17:38:59 2018  
Response via : Initial Calibration

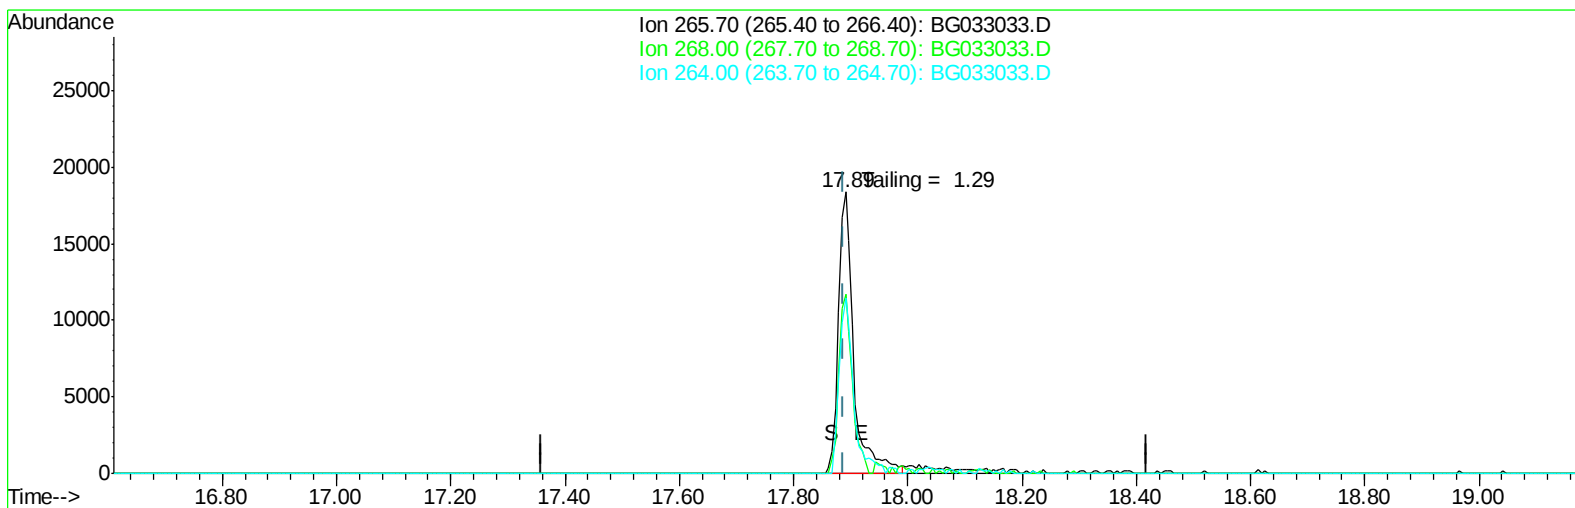

TIC: BG033033.D

(69) Pentachlorophenol (C)




17.891min (+0.001) 73121.21ng

response 34209

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 63.90 | 63.86 |
| 264.00 | 62.00 | 62.45 |
| 0.00   | 0.00  | 0.00  |

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG030618\  
Data File : BG033033.D  
Acq On : 6 Mar 2018 23:02  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 07 03:19:26 2018  
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022118.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Mar 06 17:38:59 2018  
Response via : Initial Calibration

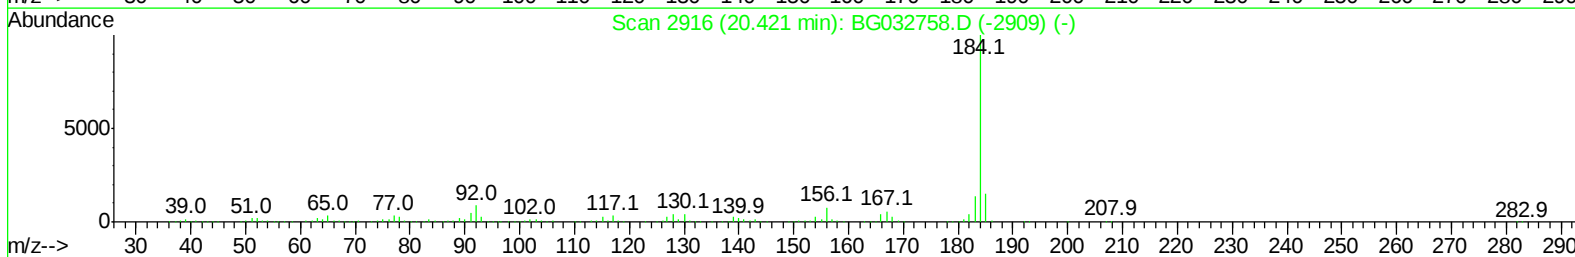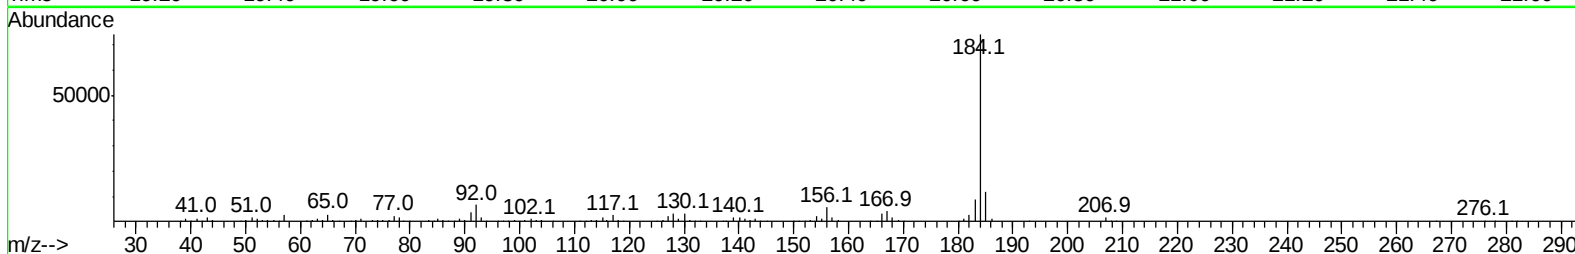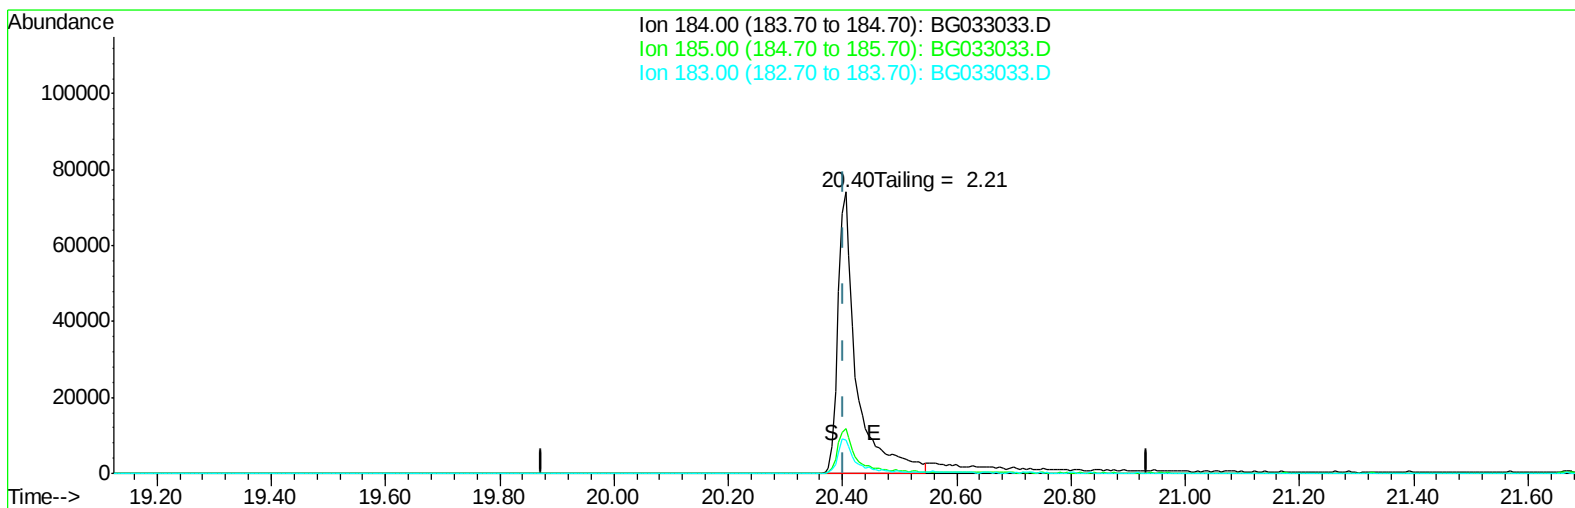

TIC: BG033033.D

(76) Benzidine

20.405min (+0.001) 0.00ng

response 168904

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 13.90 | 15.98 |
| 183.00 | 13.30 | 11.81 |
| 0.00   | 0.00  | 0.00  |