

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG030618\
 Data File : BG033031.D
 Acq On : 6 Mar 2018 21:09
 Operator : SJ/JU
 Sample : PB107125BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB107125BL

Quant Time: Mar 07 03:02:13 2018
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 06 17:38:59 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.91	152	52969	20.00	ng	0.00
21) Naphthalene-d8	11.79	136	225687	20.00	ng	0.00
38) Acenaphthene-d10	15.52	164	127487	20.00	ng	0.00
63) Phenanthrene-d10	18.25	188	282958	20.00	ng	0.00
75) Chrysene-d12	22.61	240	255514	20.00	ng	0.00
86) Perylene-d12	26.40	264	212150	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	6.33	112	395821	119.55	ng	0.00
7) Phenol-d6	8.01	99	525987	113.98	ng	0.00
23) Nitrobenzene-d5	10.11	82	308933	93.83	ng	0.00
41) 2,4,6-Tribromophenol	16.99	330	159144	118.72	ng	0.00
44) 2-Fluorobiphenyl	14.16	172	674209	76.27	ng	0.00
78) Terphenyl-d14	20.77	244	988532	86.92	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG030618\
Data File : BG033031.D
Acq On : 6 Mar 2018 21:09
Operator : SJ/JU
Sample : PB107125BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB107125BL

Quant Time: Mar 07 03:02:13 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 06 17:38:59 2018
Response via : Initial Calibration

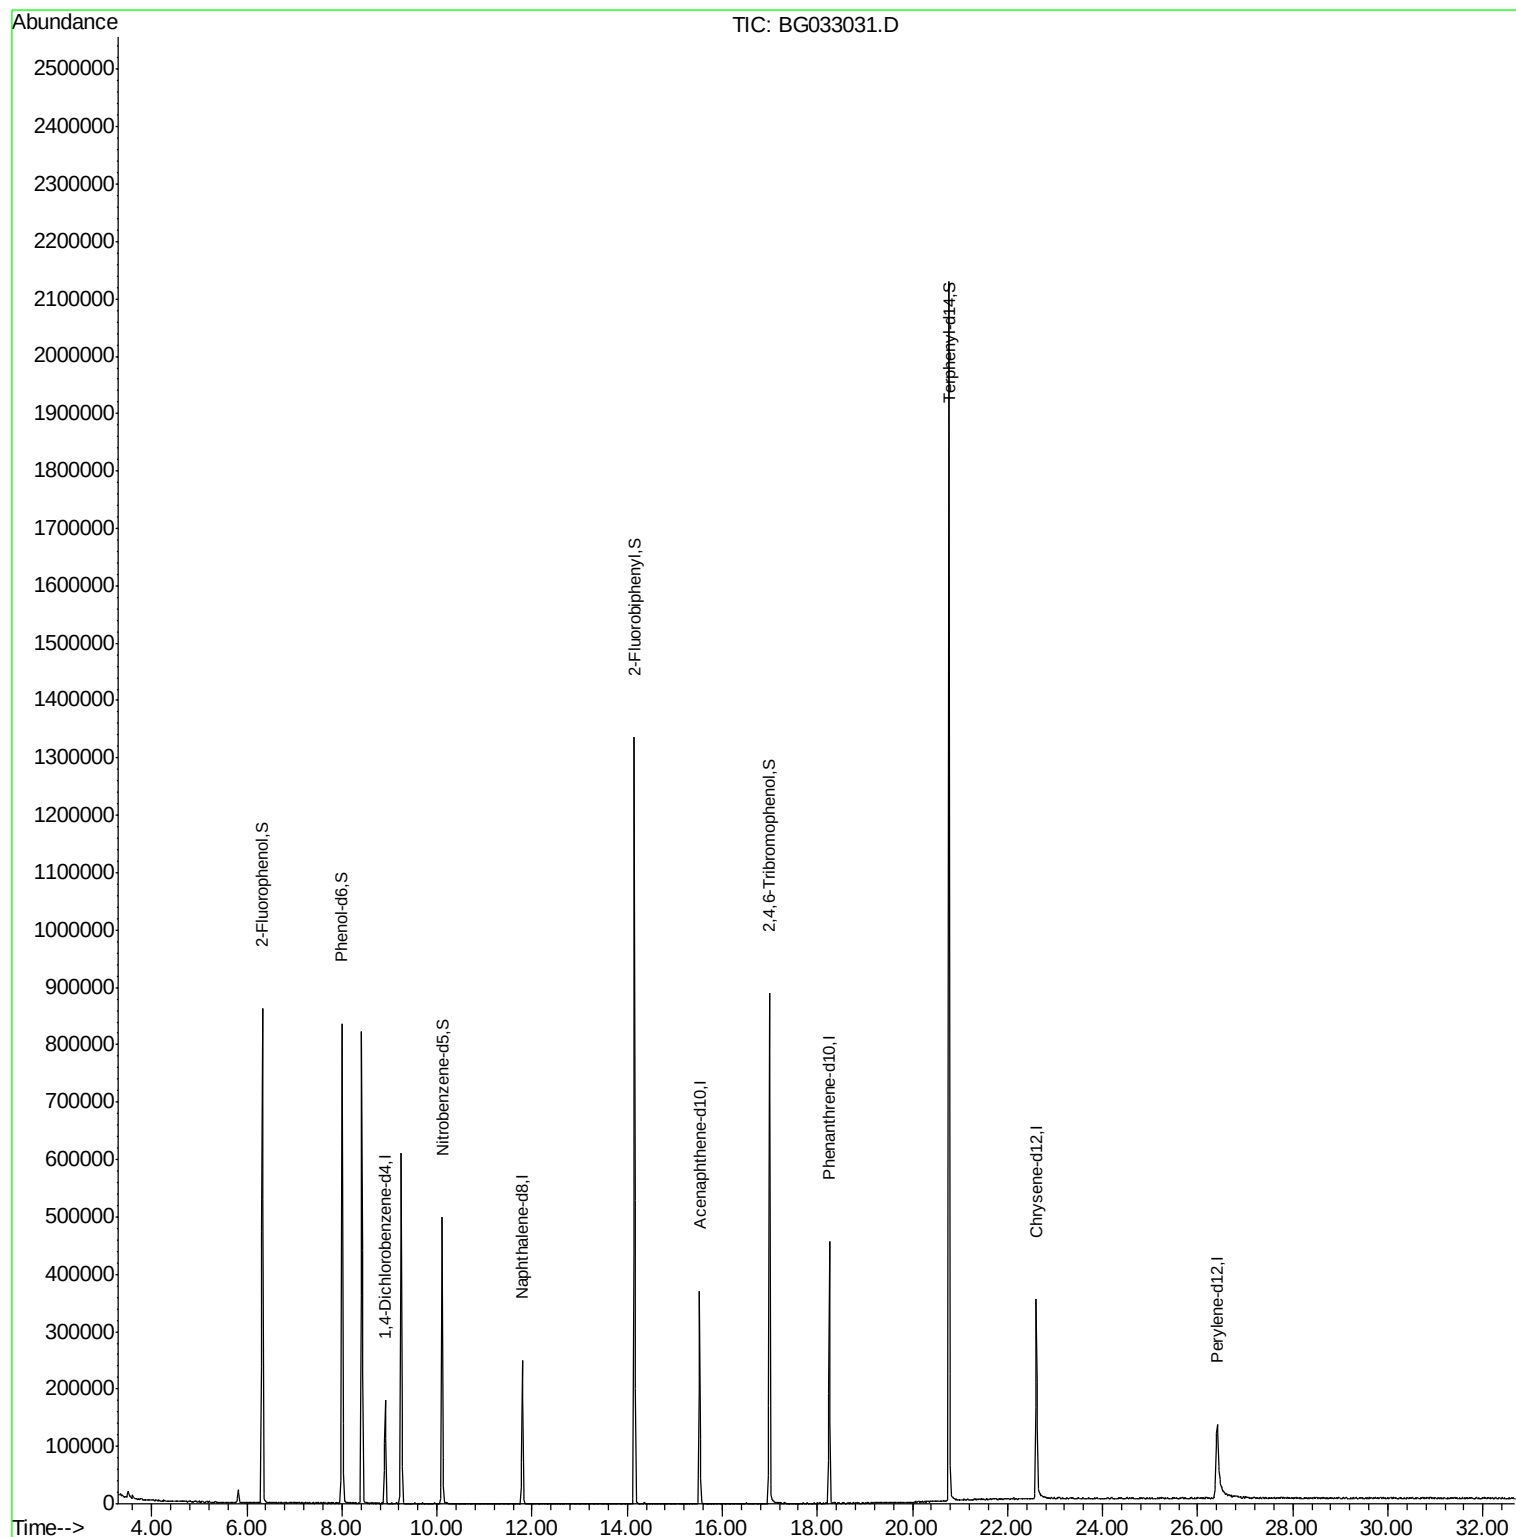

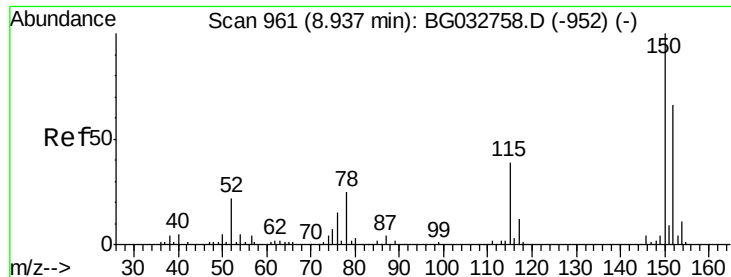


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.91 min Scan# 957
Delta R.T. -0.00 min
Lab File: BG033031.D
Acq: 6 Mar 2018 21:09

Instrument :
BNA_G
ClientSampleId :
PB107125BL

Tot Ion:152 Resp: 52969
Ion Ratio Lower Upper
152 100
150 153.6 126.6 189.8
115 60.7 53.0 79.4

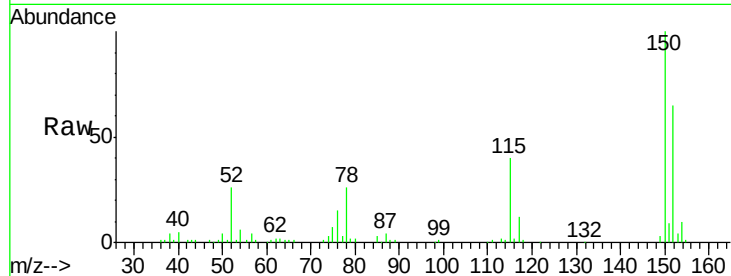


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

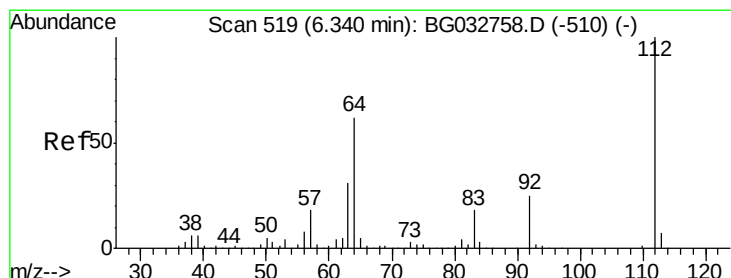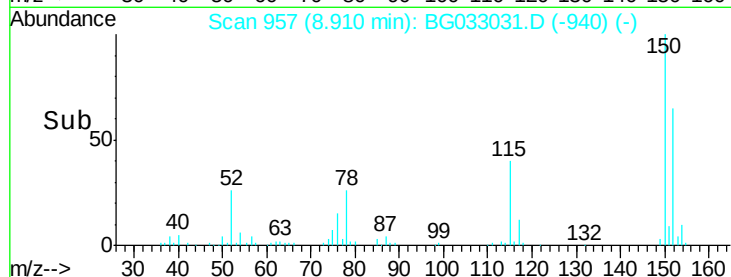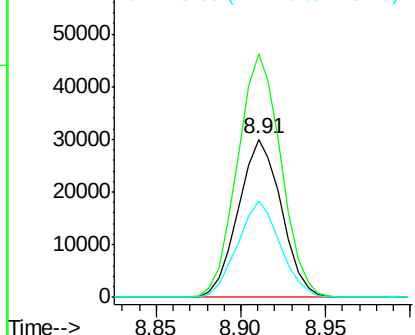



#5


2-Fluorophenol
Concen: 119.552 ng
RT: 6.33 min Scan# 517
Delta R.T. 0.00 min
Lab File: BG033031.D
Acq: 6 Mar 2018 21:09

Tgt Ion:112 Resp: 395821
Ion Ratio Lower Upper
112 100
64 68.5 56.3 84.5
63 34.4 30.1 45.1

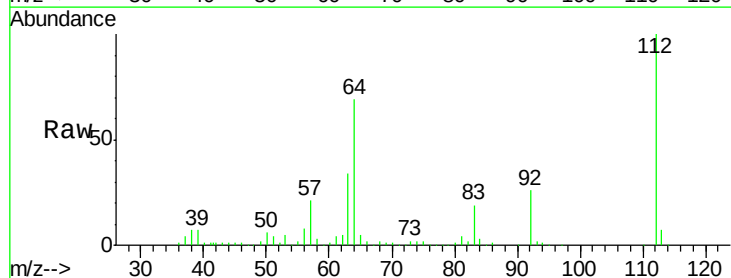

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

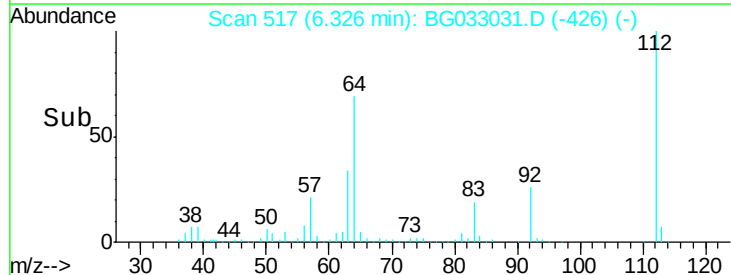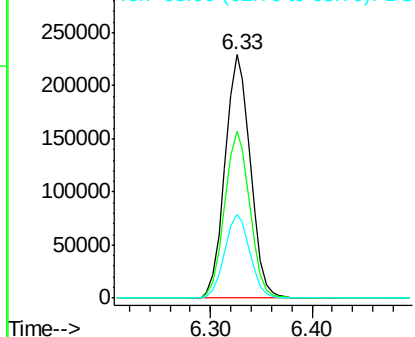

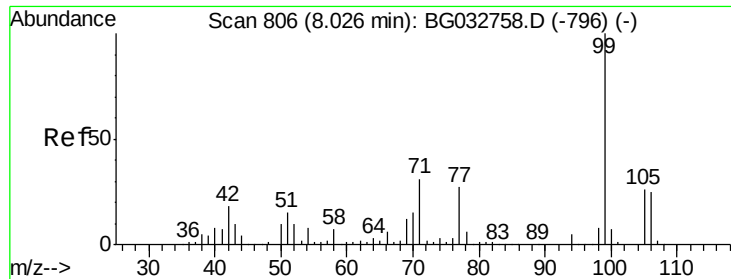

#7

Phenol-d6

Concen: 113.976 ng

RT: 8.01 min Scan# 803

Delta R.T. -0.00 min

Lab File: BG033031.D

Acq: 6 Mar 2018 21:09

Instrument :

BNA_G

ClientSampleId :

PB107125BL


Tot Ion: 99 Resp: 525987

Ion Ratio Lower Upper




99 100

42 21.6 14.1 21.1#

71 33.7 26.1 39.1

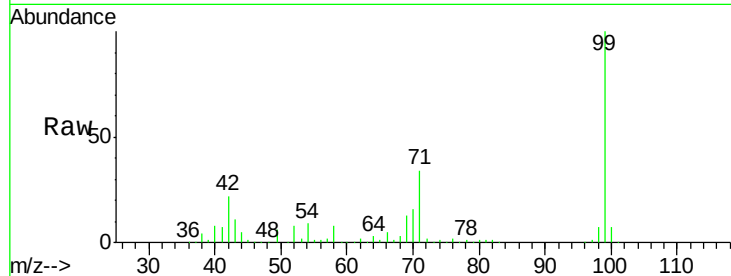

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

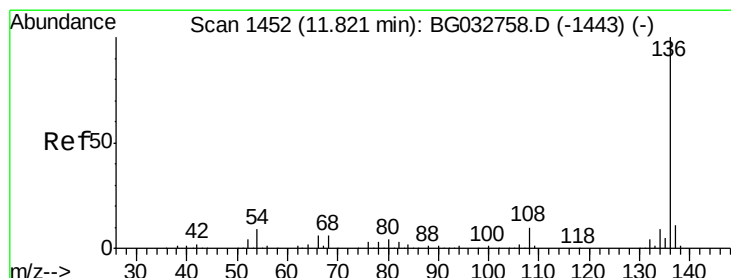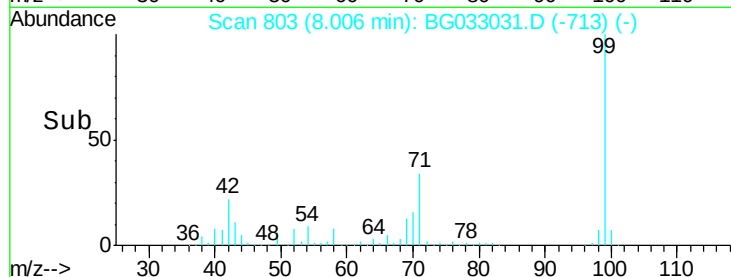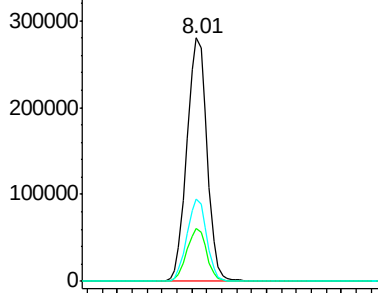

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 11.79 min Scan# 1448

Delta R.T. -0.00 min

Lab File: BG033031.D

Acq: 6 Mar 2018 21:09

Tgt Ion: 136 Resp: 225687


Ion Ratio Lower Upper

136 100



137 11.1 9.2 13.8


54 10.4 10.3 15.5

68 6.4 4.5 6.7

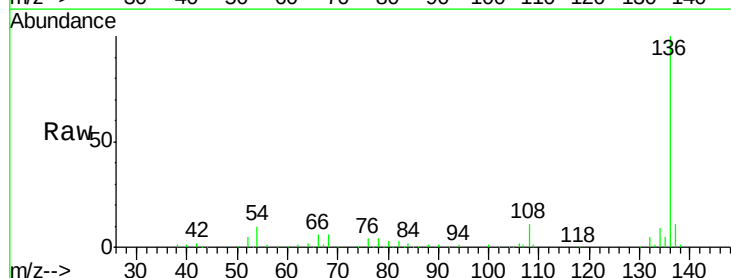

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



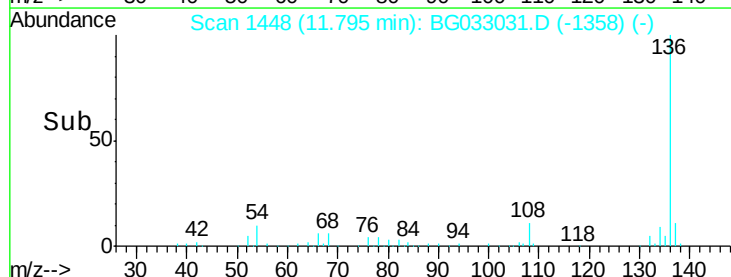
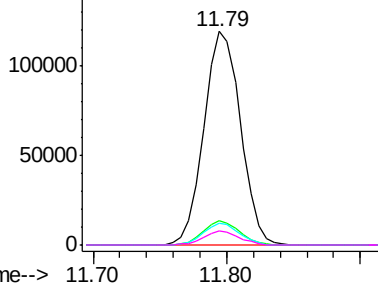


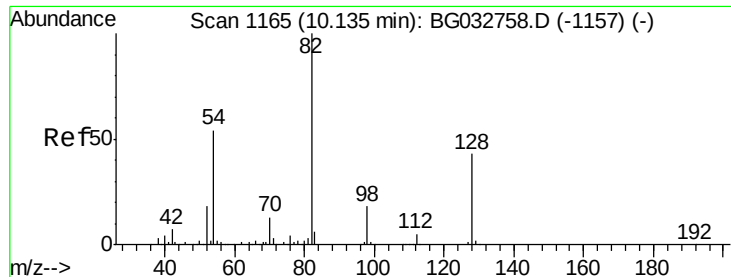

#23
 Nitrobenzene-d5
 Concen: 93.827 ng
 RT: 10.11 min Scan# 1161
 Delta R.T. -0.00 min
 Lab File: BG033031.D
 Acq: 6 Mar 2018 21:09




Instrument :
 BNA_G
 ClientSampleId :
 PB107125BL


Tot Ion	82	Resp	308933
Ion Ratio	Lower	Upper	
82	100		
128	43.5	29.7	44.5
54	58.3	43.1	64.7

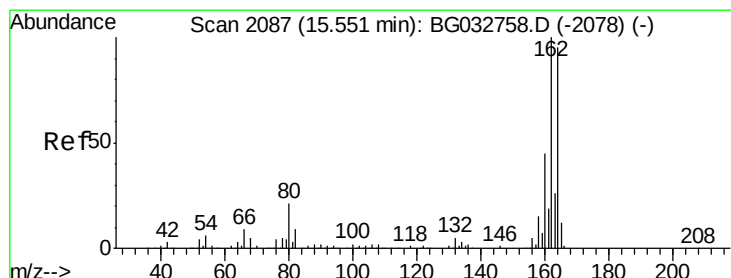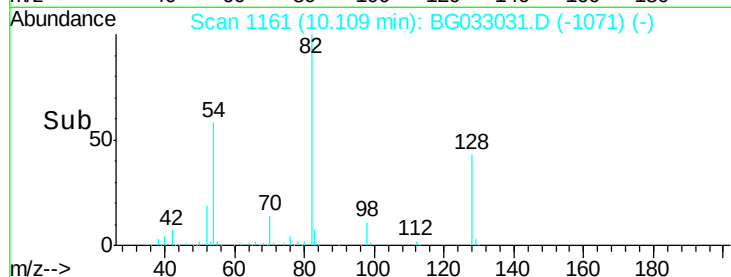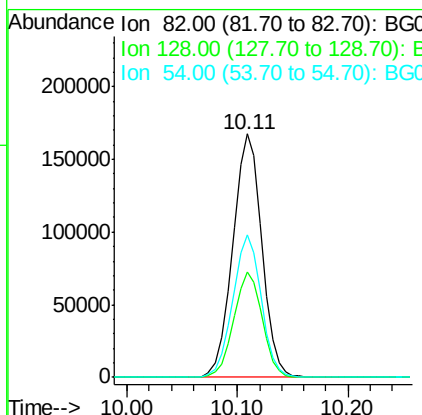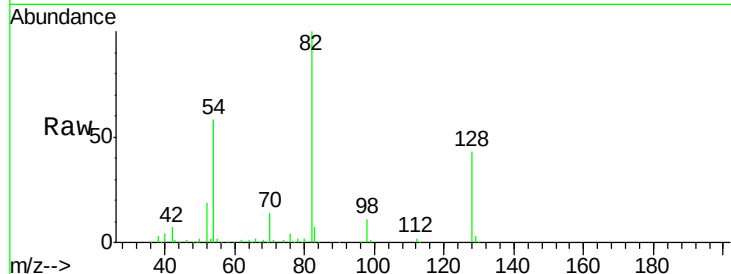

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 15.52 min Scan# 2083
 Delta R.T. -0.00 min
 Lab File: BG033031.D
 Acq: 6 Mar 2018 21:09

Tgt Ion	164	Resp	127487
Ion Ratio	Lower	Upper	
164	100		
162	99.5	78.8	118.2
160	46.2	35.4	53.0

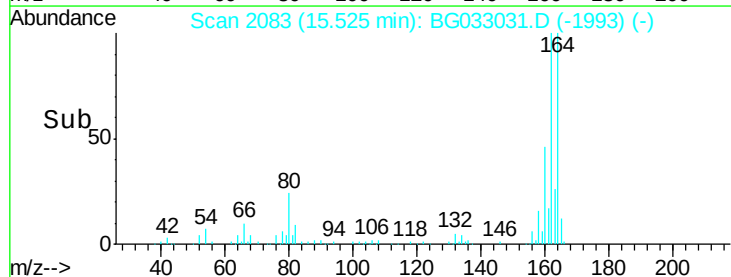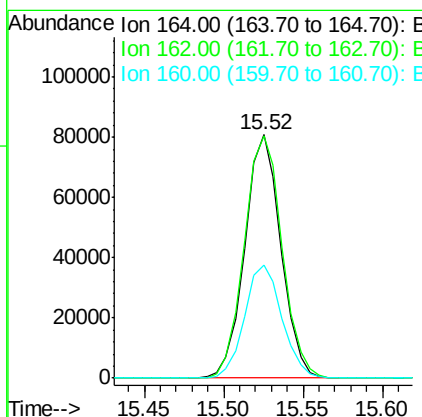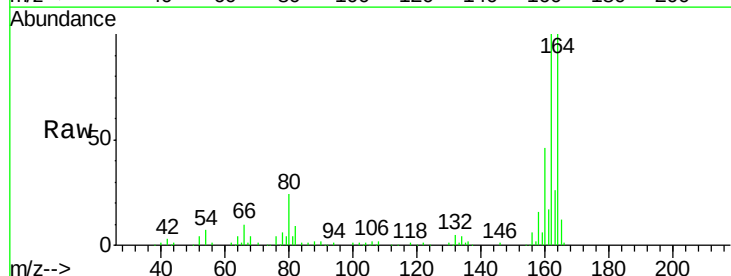

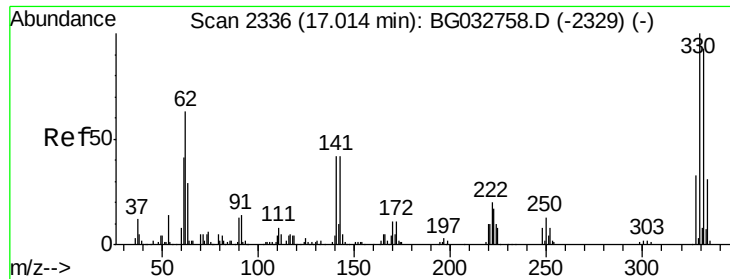

#41

2,4,6-Tribromophenol

Concen: 118.721 ng

RT: 16.99 min Scan# 2333

Delta R.T. -0.00 min

Lab File: BG033031.D

Acq: 6 Mar 2018 21:09

Instrument :

BNA_G

ClientSampleId :

PB107125BL


Tot Ion:330 Resp: 159144

Ion Ratio Lower Upper




330 100

332 94.8 77.0 115.6

141 42.8 25.2 37.8#

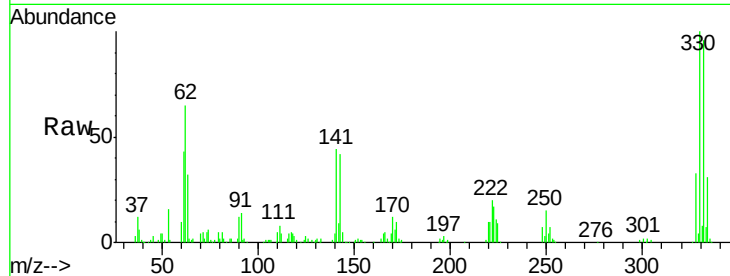

Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

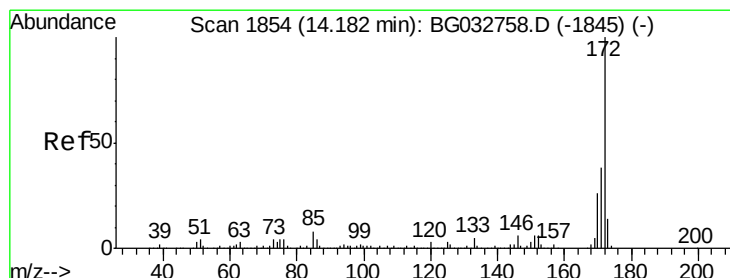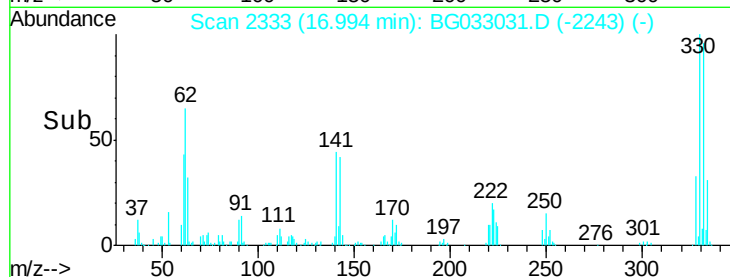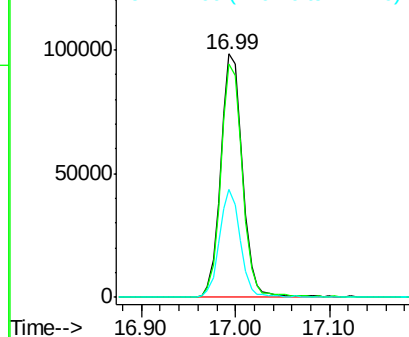

#44

2-Fluorobiphenyl

Concen: 76.273 ng

RT: 14.16 min Scan# 1850

Delta R.T. 0.00 min

Lab File: BG033031.D

Acq: 6 Mar 2018 21:09


Tgt Ion:172 Resp: 674209

Ion Ratio Lower Upper



172 100


171 37.1 30.0 45.0

170 24.5 19.5 29.3

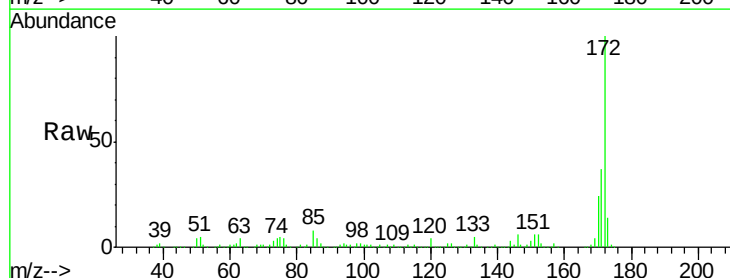

Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

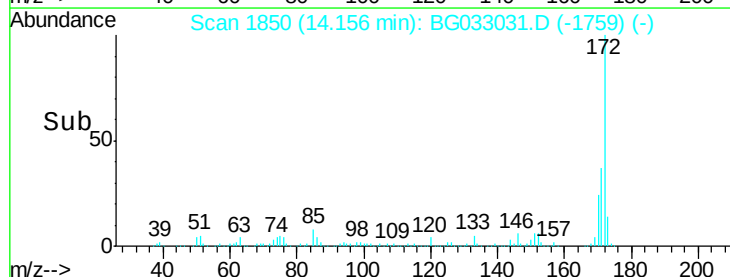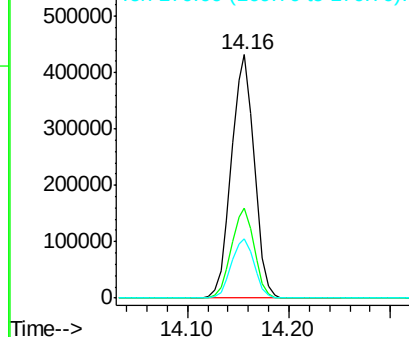

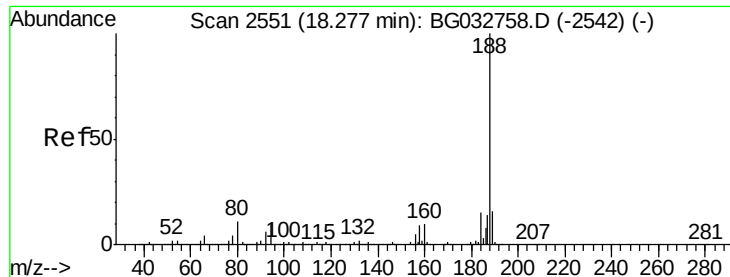

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 18.25 min Scan# 2547

Delta R.T. -0.00 min

Lab File: BG033031.D

Acq: 6 Mar 2018 21:09

Instrument :

BNA_G

ClientSampleId :

PB107125BL


Tot Ion:188 Resp: 282958

Ion Ratio Lower Upper

188 100

94 10.4 6.9 10.3#




80 12.2 7.7 11.5#

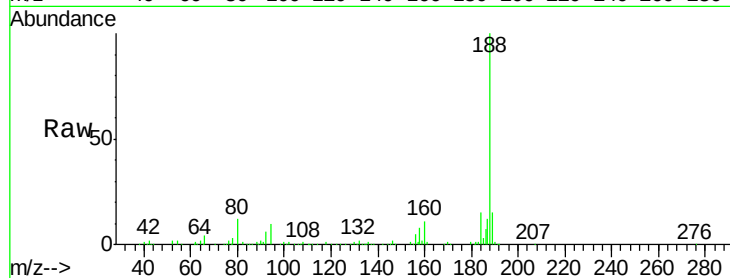

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

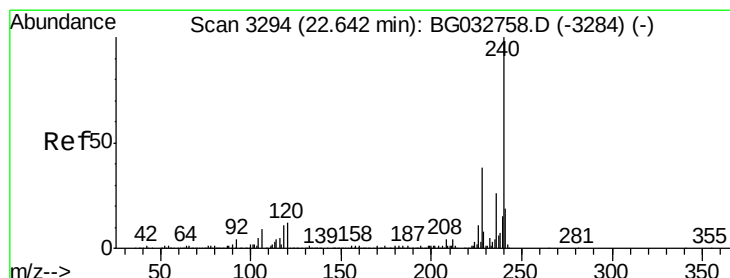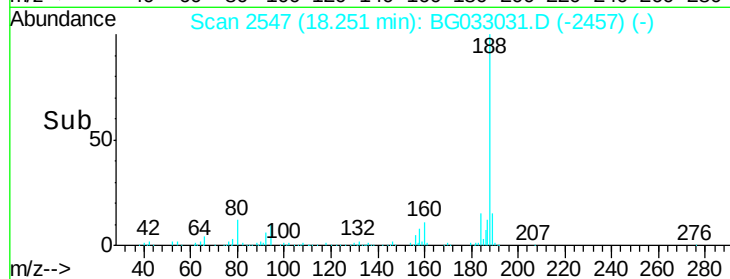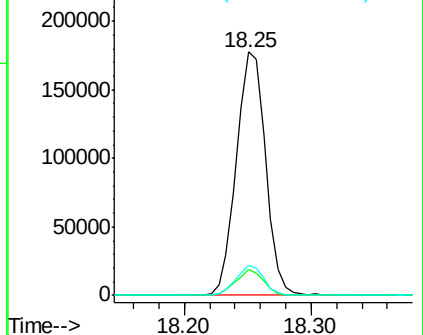

#75

Chrysene-d12

Concen: 20.000 ng

RT: 22.61 min Scan# 3289

Delta R.T. -0.00 min

Lab File: BG033031.D

Acq: 6 Mar 2018 21:09


Tgt Ion:240 Resp: 255514

Ion Ratio Lower Upper

240 100

120 12.6 6.8 10.2#



236 27.0 20.9 31.3

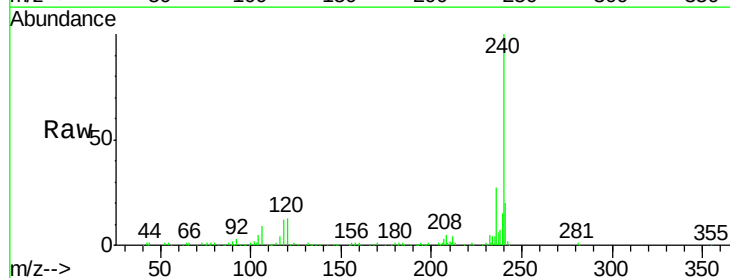


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

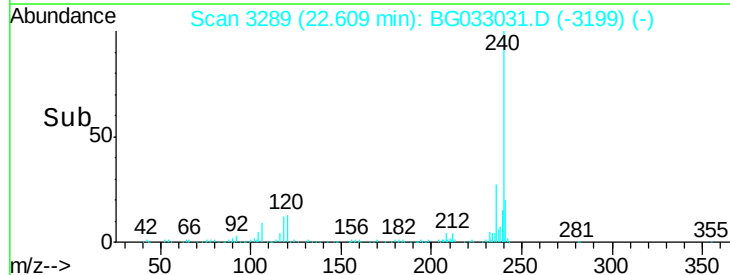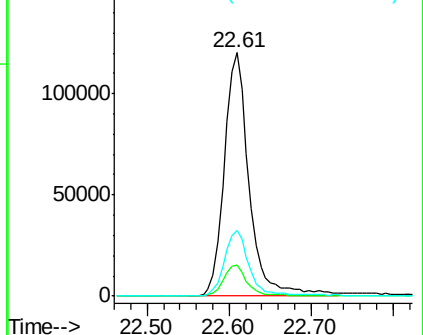

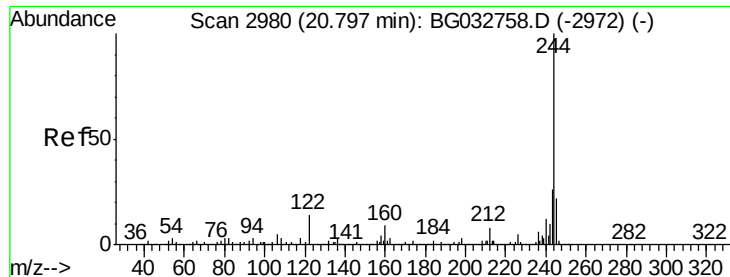

#78

Terphenyl-d14

Concen: 86.921 ng

RT: 20.77 min Scan# 2976

Delta R.T. 0.00 min

Lab File: BG033031.D

Acq: 6 Mar 2018 21:09

Instrument :

BNA_G

ClientSampleId :

PB107125BL


Tot Ion:244 Resp: 988532

Ion Ratio Lower Upper

244 100

212 7.9 5.8 8.8




122 12.8 7.0 10.4#

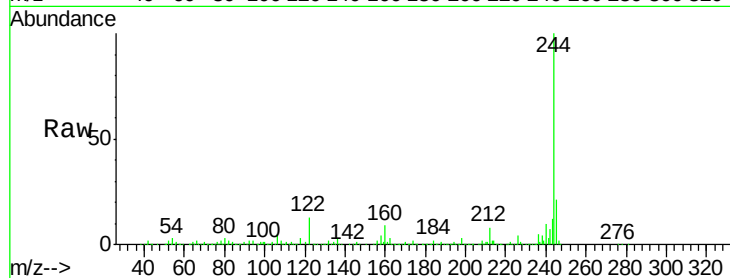

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

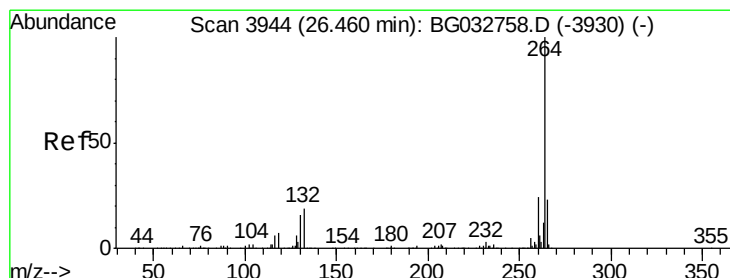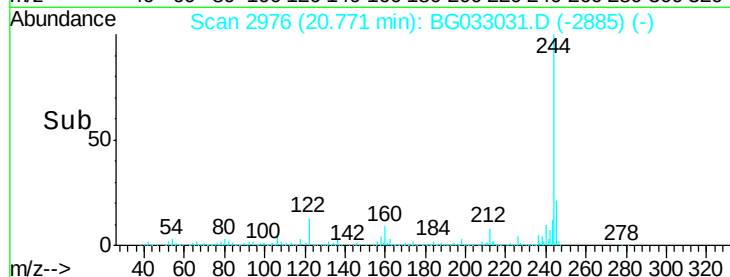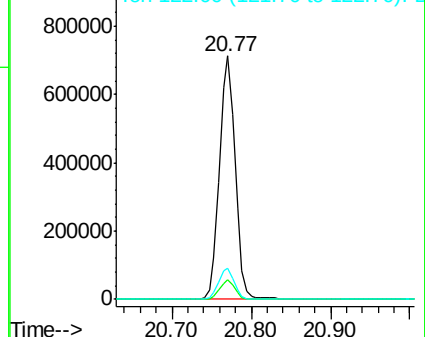

#86

Perylene-d12

Concen: 20.000 ng

RT: 26.40 min Scan# 3935

Delta R.T. -0.00 min

Lab File: BG033031.D

Acq: 6 Mar 2018 21:09


Tgt Ion:264 Resp: 212150

Ion Ratio Lower Upper

264 100

260 23.2 17.4 26.0

265 21.4 17.7 26.5

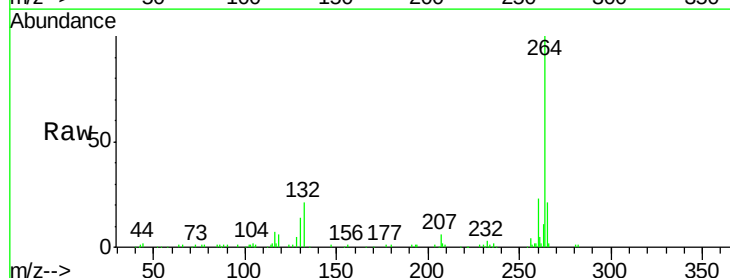

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

