


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA G\Data\BG030618\
 Data File : BG033033.D
 Acq On : 6 Mar 2018 23:02
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG022118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 06 17:38:59 2018

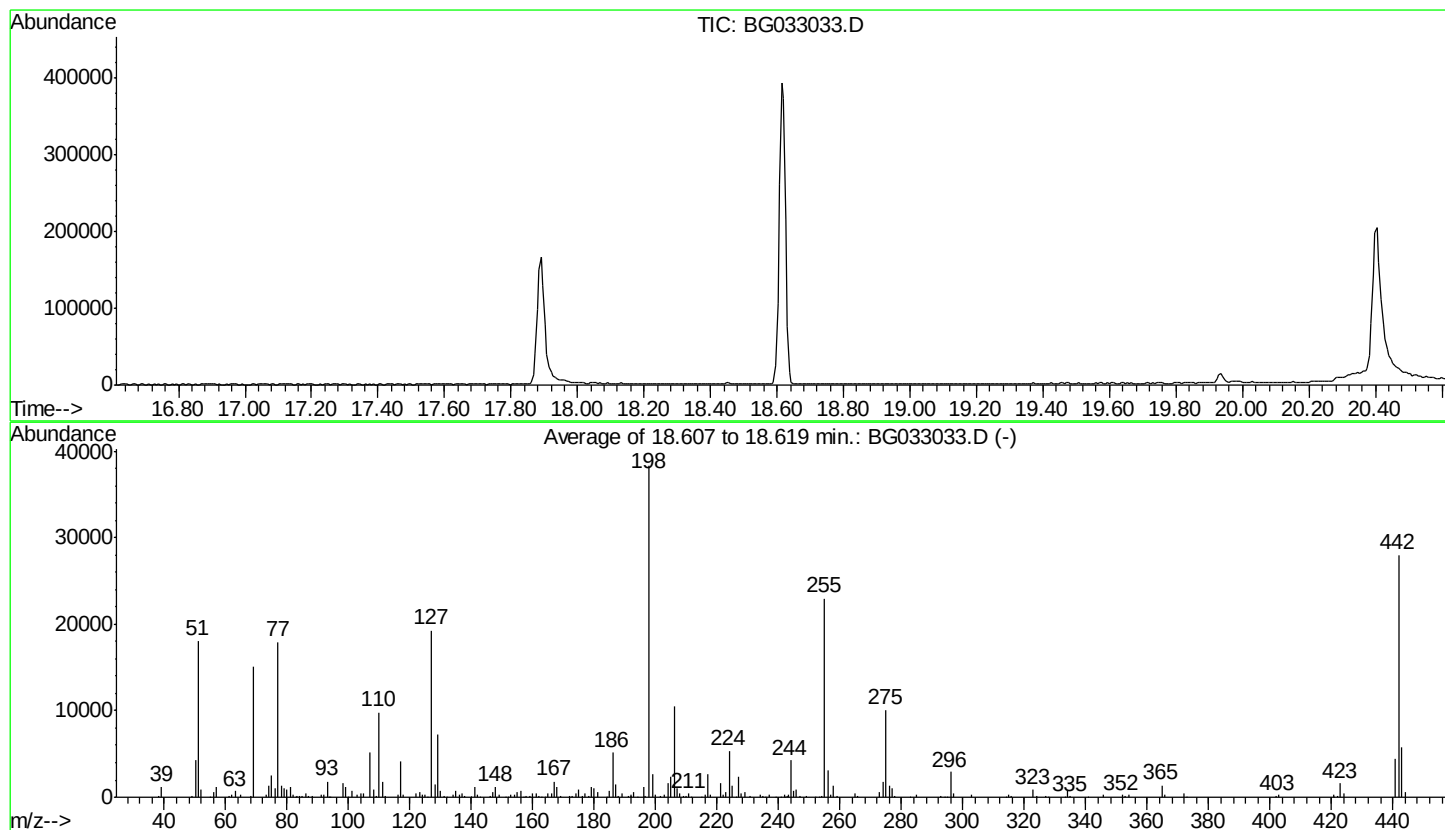

AutoFind: Scans 2608, 2609, 2610; Background Corrected with Scan 2602

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.2	18089	PASS
68	69	0.00	2	0.8	121	PASS
69	198	0.00	100	39.3	15046	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.3	19280	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	38314	PASS
199	198	5	9	7.0	2664	PASS
275	198	10	60	26.4	10101	PASS
365	198	1	100	3.7	1408	PASS
441	442	0.01	24	15.6	4377	PASS
442	198	50	100	73.1	28010	PASS
443	442	15	24	20.8	5835	PASS