

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030623\
 Data File : BG056843.D
 Acq On : 6 Mar 2023 16:02
 Operator : CG/JU
 Sample : 01712-15
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBZX7

Quant Time: Mar 06 16:53:42 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 02 00:12:28 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.414	152	17034	20.000	ng/ul	0.00
20) Naphthalene-d8	11.252	136	81187	20.000	ng/ul	0.00
38) Acenaphthene-d10	15.024	164	58628	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.756	188	130597	20.000	ng/ul	0.00
79) Chrysene-d12	22.063	240	111709	20.000	ng/ul	0.00
88) Perylene-d12	25.588	264	121643	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.702	96	950	3.094	ng/uL	0.00
4) Pyridine-d5	4.137	84	125	0.101	ng/ul	0.00
7) Phenol-d5	7.545	99	26188	15.363	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.721	67	16631	15.995	ng/ul	0.00
11) 2-Chlorophenol-d4	7.938	132	17918	15.829	ng/ul	0.00
15) 4-Methylphenol-d8	9.108	113	19140	14.695	ng/ul	0.00
21) Nitrobenzene-d5	9.589	128	10076	14.809	ng/ul	0.00
24) 2-Nitrophenol-d4	10.324	143	11873	14.660	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.858	165	22954	15.044	ng/ul	0.00
31) 4-Chloroaniline-d4	11.375	131	19566	9.832	ng/ul	0.00
46) Dimethylphthalate-d6	14.407	166	81074	17.139	ng/ul	0.00
49) Acenaphthylene-d8	14.719	160	89959	16.733	ng/ul	0.00
54) 4-Nitrophenol-d4	15.183	143	11041	13.538	ng/ul	0.00
60) Fluorene-d10	16.005	176	72260	16.514	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	16.105	200	9477	10.846	ng/ul	0.00
73) Anthracene-d10	17.850	188	119892	18.923	ng/ul	0.00
81) Pyrene-d10	20.112	212	102611	13.574	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.336	264	58149	8.856	ng/ul	-0.01
Target Compounds						
					Qvalue	
16) Acetophenone	9.243	105	4498	2.017	ng/ul	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030623\
Data File : BG056843.D
Acq On : 6 Mar 2023 16:02
Operator : CG/JU
Sample : 01712-15
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBZX7

Quant Time: Mar 06 16:53:42 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 02 00:12:28 2023
Response via : Initial Calibration

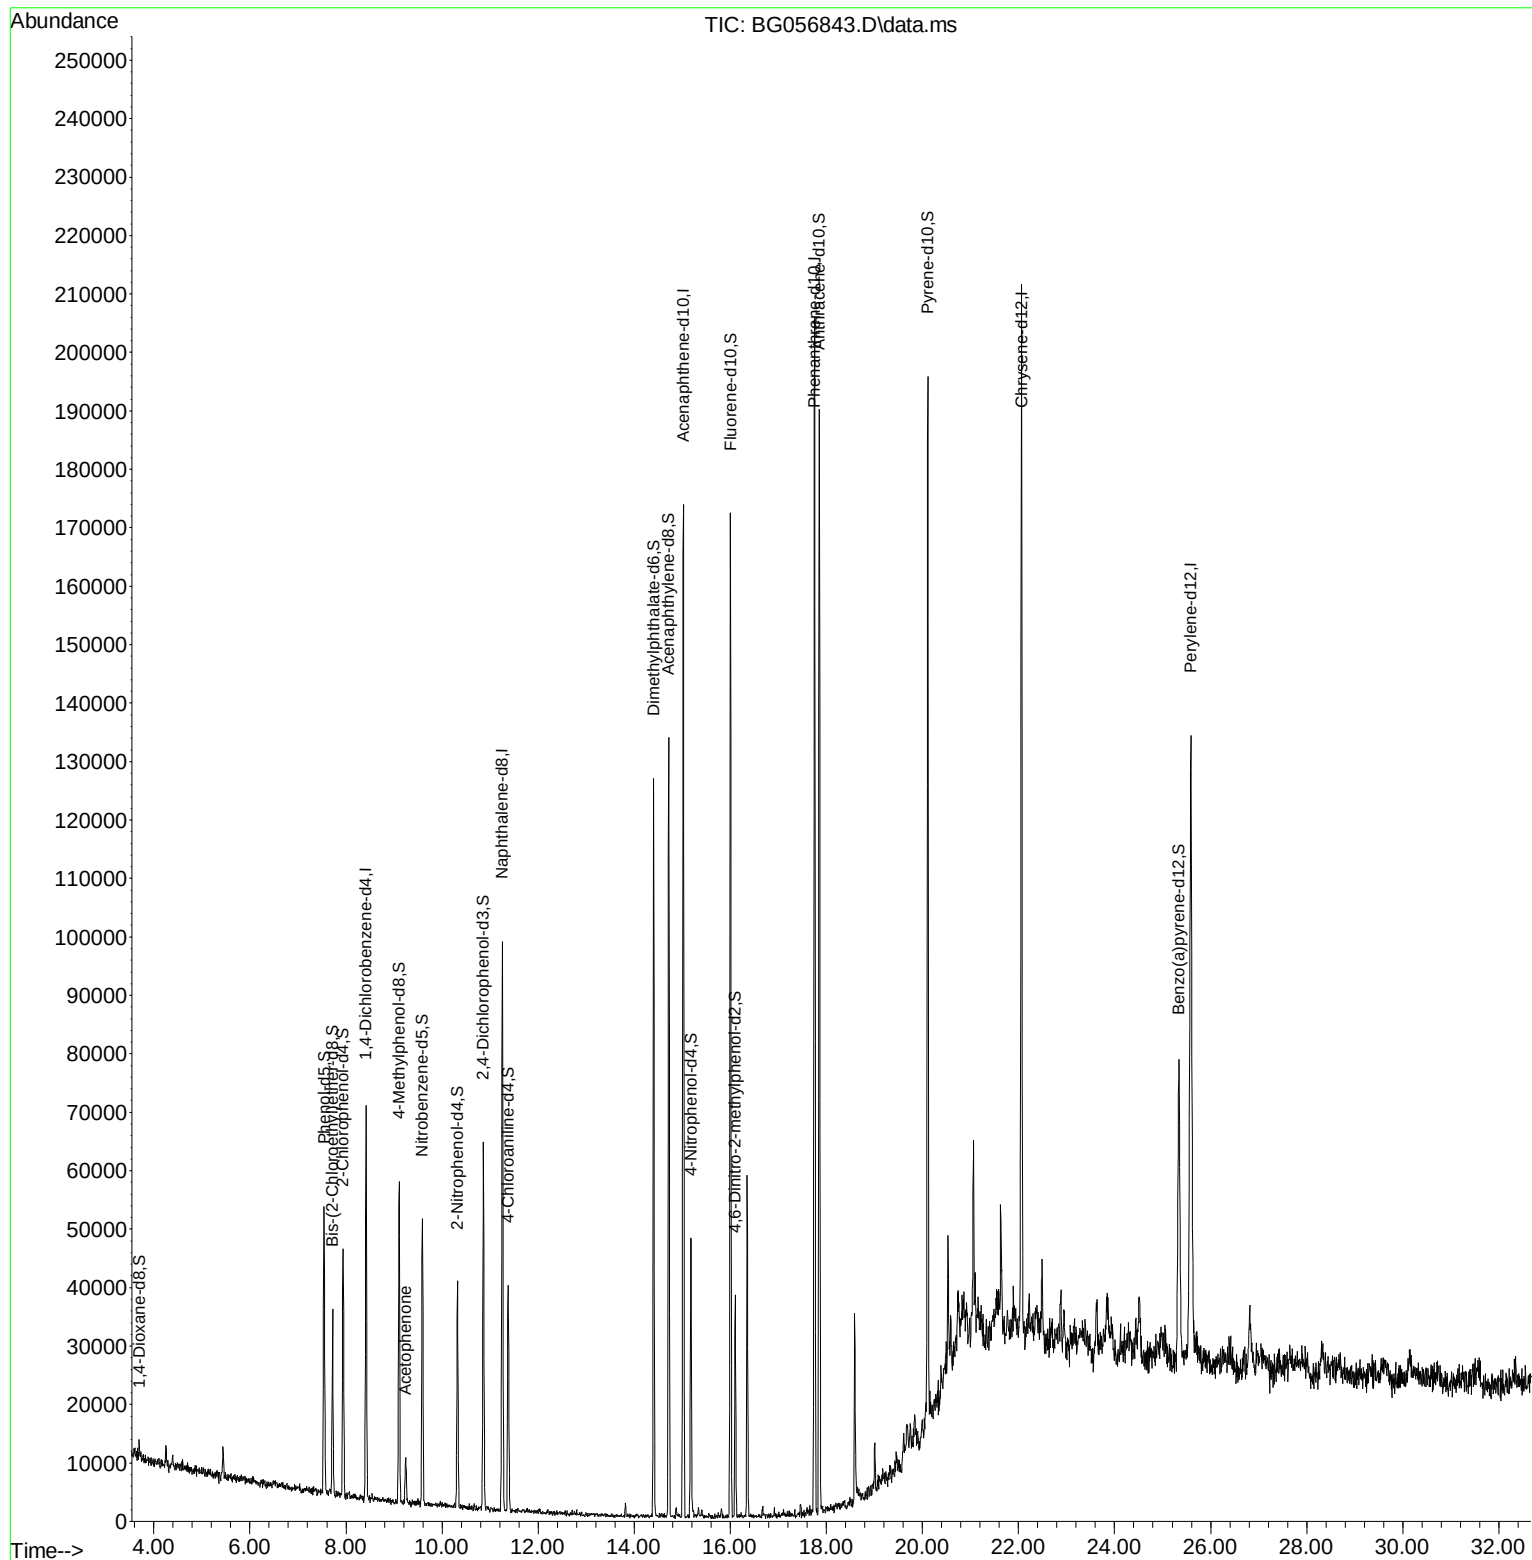

Abundance Scan 970 (9.240 min): BG056835.D\data.ms (-964) #16

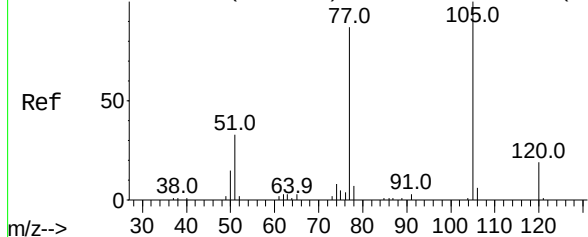

Acetophenone

Concen: 2.017 ng/ul

RT: 9.243 min Scan# 16

Delta R.T. 0.003 min

Lab File: BG056843.D

Acq: 6 Mar 2023 16:02


Instrument :

BNA_G

ClientSampleId :

DBZX7

Abundance Scan 971 (9.243 min): BG056843.D\data.ms

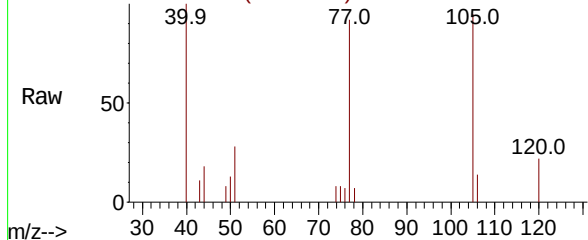


Tgt Ion:105 Resp: 4498

Ion Ratio Lower Upper

105 100

77 96.1 71.4 107.0

51 29.3 23.6 35.4

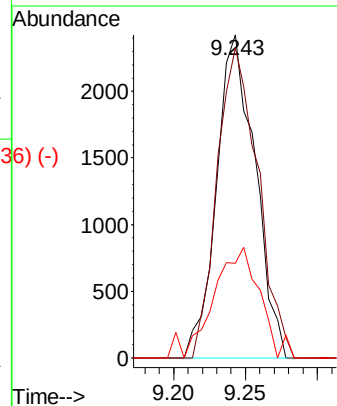

Abundance Scan 971 (9.243 min): BG056843.D\data.ms (-936) (-)

